


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040220\
 Data File : VV015363.D
 Acq On : 02 Apr 2020 08:52
 Operator : SY/MD
 Sample : BFB77
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB77

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis
 Last Update : Fri Apr 03 15:05:50 2020

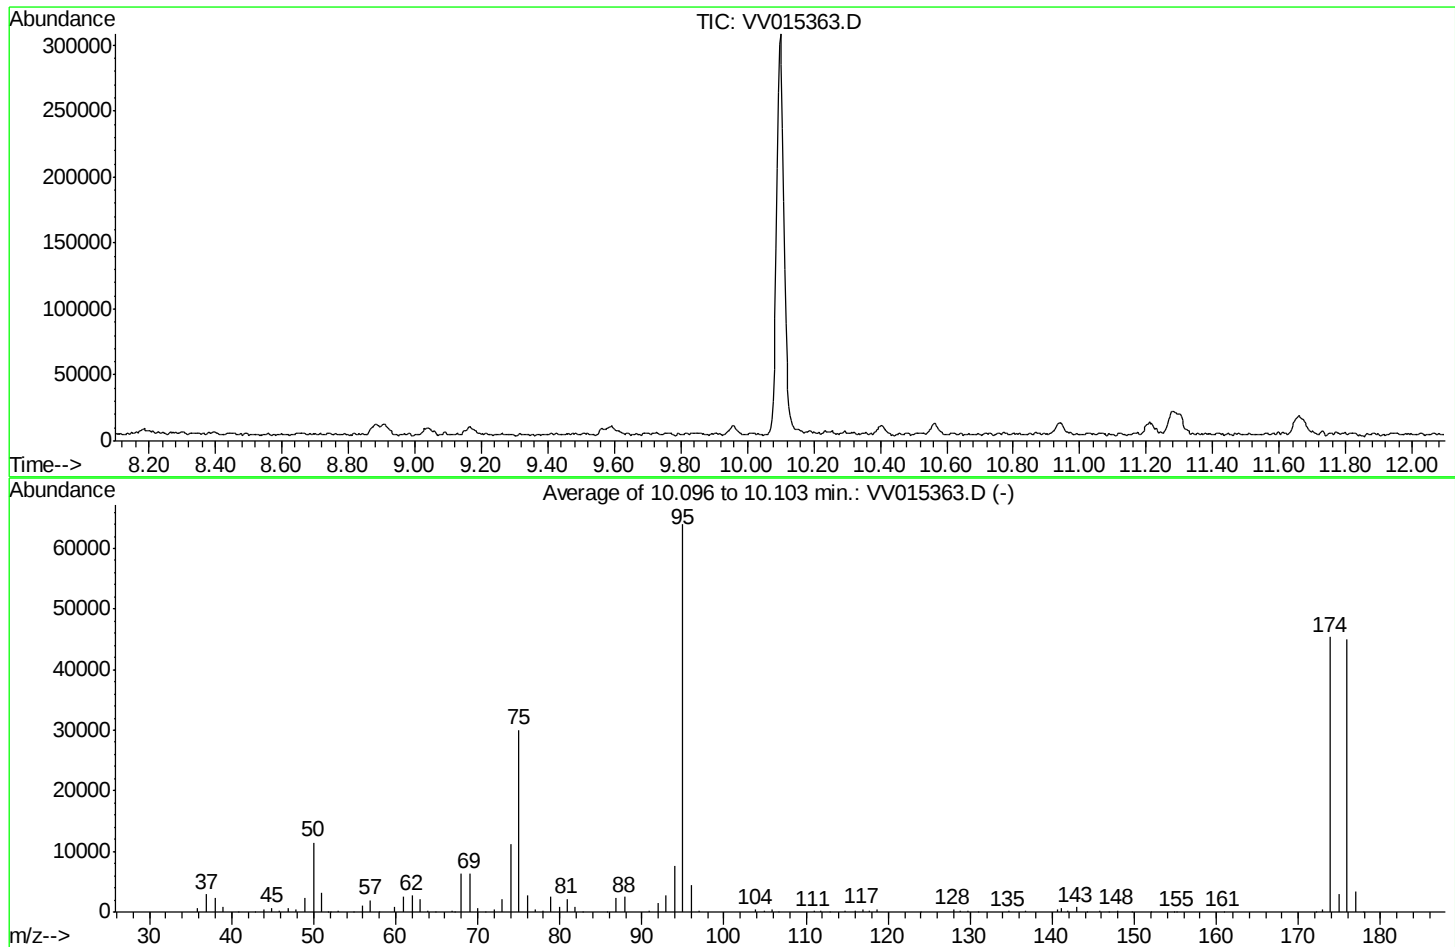

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	11446	PASS
75	95	30	80	47.0	30077	PASS
95	95	100	100	100.0	63976	PASS
96	95	5	9	7.1	4512	PASS
173	174	0.00	2	1.0	441	PASS
174	95	50	120	70.9	45333	PASS
175	174	5	9	6.7	3023	PASS
176	174	95	101	99.2	44986	PASS
177	176	5	9	7.6	3432	PASS

m/z	Abundance
35.50	146.0
38.20	182.0
38.70	139.0
39.20	172.0
39.90	900.0
42.00	159.0
42.90	164.0
43.90	1039.0
46.00	104.0
46.60	171.0
50.40	111.0
54.80	179.0
57.40	278.0
61.20	114.0
64.80	101.0
65.50	123.0
73.10	143.0
75.00	123.0
76.20	101.0
77.20	111.0
125.70	159.0
150.60	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	618.0
37.00	3277.0
38.00	2580.0
39.00	1041.0
39.90	647.0
40.80	121.0
41.90	105.0
42.90	241.0
44.00	1450.0
44.90	758.0
45.90	200.0
46.90	775.0
47.90	456.0
49.00	2160.0
50.00	11484.0
51.00	3203.0
52.10	153.0
53.00	193.0
55.00	232.0
56.00	1056.0
57.00	1986.0
59.90	768.0
61.00	2930.0
62.00	2598.0
63.00	2154.0
63.80	288.0
64.80	137.0
66.80	237.0
68.00	6300.0
69.00	6399.0
70.00	647.0
70.90	126.0
71.90	463.0
73.00	2476.0
74.00	10780.0
75.00	30504.0
76.00	2880.0
76.90	367.0
77.90	293.0
78.90	2565.0
79.90	728.0
80.90	2224.0
81.90	781.0
82.70	171.0
85.70	121.0
86.90	2544.0
87.90	2658.0
90.90	371.0
92.00	1657.0
92.90	2385.0
94.00	7855.0
95.00	64608.0
96.00	4853.0
97.00	152.0
103.90	447.0
104.90	185.0
105.80	353.0
106.70	107.0
111.00	160.0
112.90	114.0
114.80	232.0
115.90	238.0
116.90	405.0
117.70	333.0
118.70	370.0
127.90	348.0
128.90	213.0
129.70	192.0
131.00	130.0
134.70	201.0
136.80	131.0
140.70	605.0
141.10	548.0
141.90	137.0
142.90	722.0
145.80	125.0
147.90	247.0
149.70	137.0
152.10	111.0
154.90	154.0
173.00	674.0
173.90	44936.0
174.90	2918.0
175.90	44672.0
176.90	3468.0
177.90	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	637.0
37.00	3016.0
38.00	2656.0
39.00	1105.0
39.90	587.0
41.90	125.0
42.90	242.0
44.00	1414.0
45.00	744.0
45.80	276.0
46.90	628.0
47.80	478.0
49.00	2372.0
50.00	12025.0
51.00	3414.0
53.10	180.0
55.00	207.0
56.00	1036.0
56.90	2051.0
58.00	120.0
59.90	826.0
61.00	2856.0
62.00	2762.0
63.00	2268.0
63.80	320.0
64.90	163.0
66.80	236.0
68.00	6405.0
69.00	6579.0
70.00	588.0
70.90	112.0
71.90	344.0
73.00	2462.0
74.00	11652.0
75.00	31352.0
76.00	2978.0
76.90	385.0
77.90	249.0
78.80	2540.0
80.00	772.0
80.90	2281.0
81.90	813.0
82.80	155.0
86.90	2417.0
87.90	2607.0
90.80	293.0
91.90	1423.0
92.90	2780.0
94.00	7895.0
95.00	66128.0
96.00	4628.0
97.00	224.0
103.90	428.0
104.90	197.0
105.80	384.0
110.90	155.0
111.80	174.0
112.90	116.0
114.80	214.0
115.90	277.0
116.90	454.0
117.80	292.0
118.70	371.0
128.00	348.0
128.90	172.0
129.70	197.0
131.00	102.0
134.70	185.0
136.70	178.0
140.70	577.0
141.10	596.0
141.90	155.0
142.90	751.0
145.80	117.0
146.90	103.0
147.90	245.0
152.10	115.0
155.10	137.0
160.90	150.0
172.10	107.0
173.90	46792.0
175.00	3116.0
175.90	46696.0
176.90	3614.0
177.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	623.0
36.90	2533.0
38.00	2339.0
39.00	1027.0
39.90	558.0
41.90	129.0
43.00	213.0
43.90	1266.0
45.00	652.0
45.90	331.0
46.90	500.0
47.80	437.0
49.00	2337.0
50.00	10829.0
51.00	3183.0
51.80	113.0
53.10	127.0
55.00	152.0
56.00	964.0
56.90	1944.0
58.00	145.0
59.90	748.0
61.00	2469.0
62.00	2617.0
63.00	2137.0
63.90	277.0
64.90	132.0
67.20	328.0
68.00	6096.0
69.00	5876.0
70.10	577.0
72.00	297.0
73.00	2165.0
74.00	10999.0
75.00	28744.0
76.00	2691.0
77.00	336.0
77.90	164.0
78.80	2287.0
80.00	813.0
80.90	2157.0
81.90	720.0
86.90	2163.0
87.80	2154.0
90.80	262.0
91.90	1244.0
92.90	2883.0
94.00	6802.0
95.00	61192.0
96.00	4056.0
97.00	246.0
103.90	364.0
104.90	205.0
105.80	389.0
110.90	126.0
111.80	218.0
114.80	140.0
116.00	257.0
116.90	465.0
117.80	218.0
118.70	333.0
124.00	109.0
128.00	311.0
128.80	145.0
129.70	171.0
134.70	165.0
136.70	161.0
141.00	661.0
142.00	170.0
142.90	783.0
144.20	113.0
145.90	129.0
146.90	143.0
147.90	221.0
150.40	116.0
155.20	145.0
160.90	120.0
172.10	146.0
172.80	650.0
173.90	44272.0
175.00	3036.0
175.90	43592.0
176.90	3216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77