


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040320\
 Data File : VV015394.D
 Acq On : 03 Apr 2020 08:57
 Operator : SY/MD
 Sample : BFB78
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB78

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis
 Last Update : Sat Apr 04 00:09:13 2020

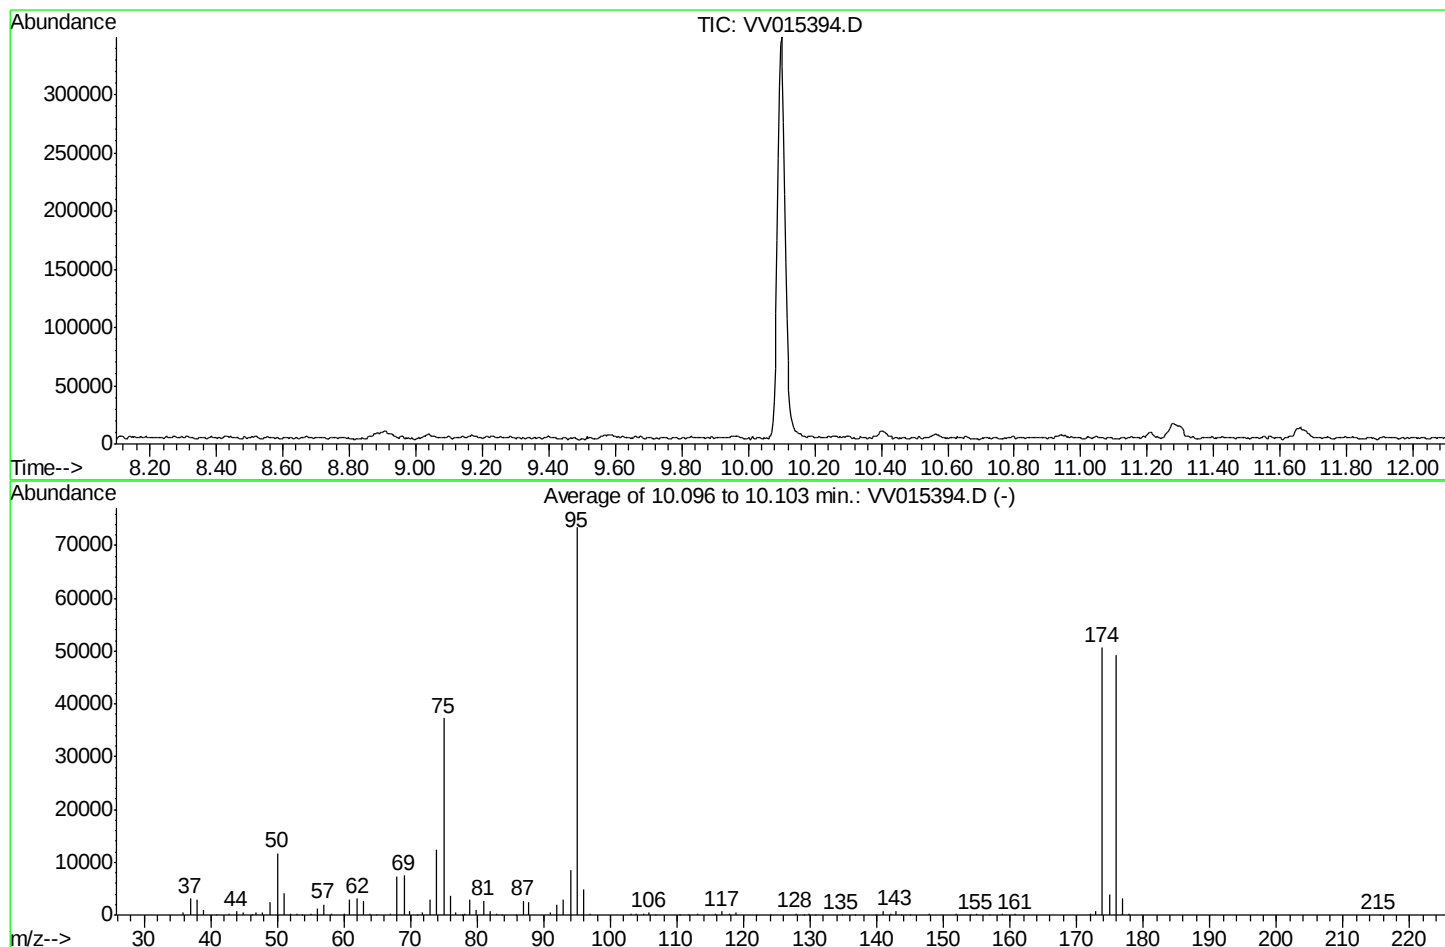

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	11706	PASS
75	95	30	80	50.7	37250	PASS
95	95	100	100	100.0	73442	PASS
96	95	5	9	6.7	4917	PASS
173	174	0.00	2	1.2	619	PASS
174	95	50	120	68.9	50570	PASS
175	174	5	9	7.5	3783	PASS
176	174	95	101	97.2	49149	PASS
177	176	5	9	6.2	3043	PASS

m/z	Abundance
36.70	176.0
37.30	149.0
39.00	210.0
39.90	583.0
41.10	198.0
42.00	212.0
42.70	150.0
43.90	802.0
45.50	131.0
46.80	139.0
48.50	168.0
48.80	167.0
49.50	126.0
50.20	124.0
51.00	133.0
51.80	108.0
55.00	160.0
56.10	180.0
57.00	142.0
60.00	184.0
61.30	105.0
63.90	105.0
68.50	140.0
77.80	130.0
120.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	745.0
37.00	3564.0
38.00	3182.0
39.00	1412.0
40.00	506.0
40.80	145.0
41.90	144.0
42.80	309.0
44.00	1520.0
45.00	454.0
46.20	112.0
46.90	742.0
47.80	497.0
48.90	2901.0
50.00	12170.0
51.00	4369.0
52.00	471.0
53.00	181.0
55.10	322.0
55.90	1686.0
57.00	2099.0
58.20	296.0
60.00	511.0
60.90	2944.0
62.00	3066.0
63.00	2673.0
64.00	335.0
65.00	116.0
67.00	302.0
68.00	7655.0
69.00	7849.0
69.90	802.0
71.00	114.0
71.80	483.0
72.90	2978.0
74.00	12708.0
75.00	38280.0
76.00	3456.0
76.80	480.0
77.60	168.0
78.10	332.0
78.80	2638.0
79.90	915.0
80.90	2642.0
81.90	681.0
82.90	233.0
83.60	178.0
85.80	137.0
86.90	2677.0
87.80	2613.0
91.00	366.0
92.00	1885.0
93.00	3139.0
94.00	8376.0
95.00	75168.0
96.00	4861.0
97.00	183.0
103.00	179.0
103.80	283.0
105.00	139.0
105.80	371.0
110.30	147.0
113.10	199.0
115.80	270.0
116.80	694.0
117.90	248.0
118.80	513.0
121.90	215.0
124.00	109.0
127.80	345.0
129.00	109.0
129.80	373.0
130.80	154.0
134.80	185.0
140.90	884.0
142.00	122.0
142.80	847.0
143.70	101.0
147.80	189.0
151.90	166.0
154.00	127.0
154.90	252.0
158.90	214.0
160.80	154.0
172.10	262.0
172.90	683.0
173.90	49928.0
174.90	3852.0
175.90	47856.0
176.90	3112.0
177.90	195.0
215.50	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.90	593.0
37.00	3139.0
38.00	3035.0
39.00	1347.0
39.90	550.0
41.00	137.0
41.90	167.0
42.80	298.0
44.00	1571.0
45.00	528.0
46.30	110.0
46.90	747.0
47.80	430.0
48.90	2728.0
50.00	12275.0
51.00	4317.0
52.00	434.0
53.00	190.0
55.10	296.0
55.90	1477.0
56.90	2199.0
58.10	245.0
60.00	518.0
60.90	2868.0
62.00	3267.0
63.00	2715.0
64.00	383.0
66.90	373.0
68.00	7404.0
69.00	7624.0
69.90	902.0
71.80	425.0
73.00	2894.0
73.90	12692.0
75.00	38664.0
76.00	3793.0
76.90	557.0
77.60	165.0
78.10	299.0
78.90	2929.0
79.90	929.0
80.90	2797.0
81.90	706.0
82.90	146.0
83.60	135.0
85.80	105.0
87.00	2847.0
87.80	2429.0
91.00	436.0
92.00	1988.0
93.00	3071.0
94.00	8839.0
95.00	75760.0
96.00	4889.0
97.00	154.0
103.00	165.0
103.80	306.0
105.00	169.0
105.80	430.0
106.70	122.0
110.30	119.0
111.80	102.0
113.10	183.0
115.90	261.0
116.70	717.0
117.90	293.0
118.90	526.0
121.90	146.0
127.80	380.0
129.00	103.0
129.80	366.0
130.80	123.0
134.80	160.0
136.80	145.0
139.80	102.0
141.00	888.0
142.00	148.0
142.80	877.0
144.90	108.0
147.80	207.0
151.90	159.0
154.90	252.0
156.90	119.0
158.90	182.0
160.80	203.0
172.10	255.0
172.90	647.0
173.90	52080.0
174.90	3870.0
175.90	50560.0
176.90	3187.0
177.90	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

215.50

127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.80	417.0
36.90	2452.0
38.00	2618.0
39.00	1114.0
39.90	645.0
41.00	174.0
41.90	206.0
42.80	281.0
43.90	1438.0
44.90	583.0
46.80	613.0
47.80	297.0
48.90	2480.0
50.00	11047.0
51.00	3799.0
52.00	305.0
53.00	201.0
53.80	147.0
55.00	306.0
56.00	1207.0
56.90	2080.0
58.00	186.0
60.00	537.0
60.90	2742.0
62.00	3051.0
63.00	2569.0
64.00	382.0
64.80	101.0
66.90	356.0
68.00	6610.0
69.00	6806.0
69.90	796.0
71.80	381.0
73.00	2764.0
74.00	11894.0
75.00	34808.0
76.00	3485.0
76.90	576.0
77.60	144.0
78.10	198.0
78.90	3001.0
79.90	901.0
80.90	2632.0
81.90	682.0
82.80	100.0
87.00	2559.0
87.80	2197.0
91.00	407.0
91.90	1837.0
93.00	2879.0
94.00	8351.0
95.00	69400.0
95.90	5003.0
97.00	112.0
103.00	121.0
103.90	414.0
104.90	166.0
105.80	417.0
106.70	104.0
111.80	105.0
113.00	111.0
115.90	255.0
116.80	590.0
117.90	307.0
118.90	478.0
127.80	339.0
129.80	300.0
136.70	168.0
139.80	106.0
141.00	793.0
142.10	140.0
142.90	849.0
144.90	138.0
147.80	166.0
151.90	132.0
154.90	204.0
156.80	130.0
158.90	138.0
160.80	197.0
172.00	222.0
172.90	527.0
173.90	49704.0
174.90	3627.0
175.90	49032.0
176.90	2832.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78