




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034946.D
Acq On : 03 Apr 2024 10:21
Operator : SY/MD
Sample : VV0403WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Manual IntegrationsAPPROVED

Quant Time: Apr 04 05:01:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 04 02:49:59 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/09/2024
Supervised By :Semsettin Yesilyurt 04/09/2024

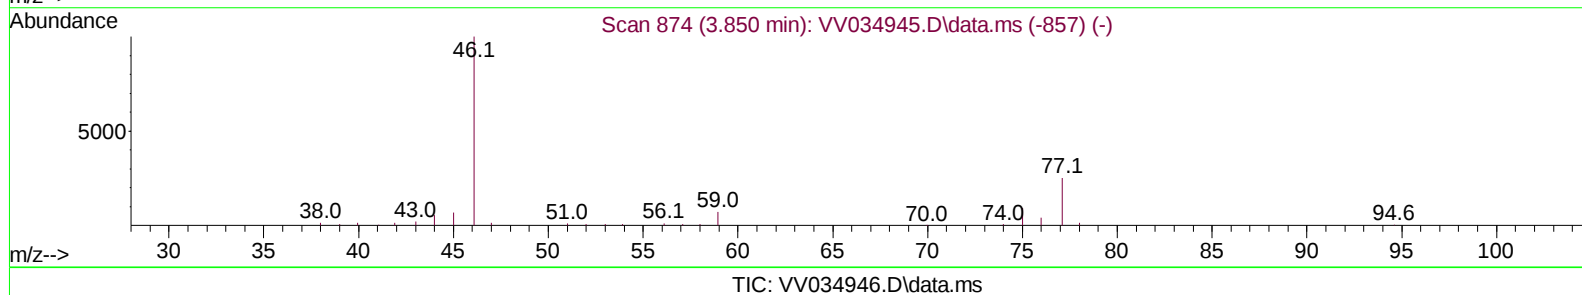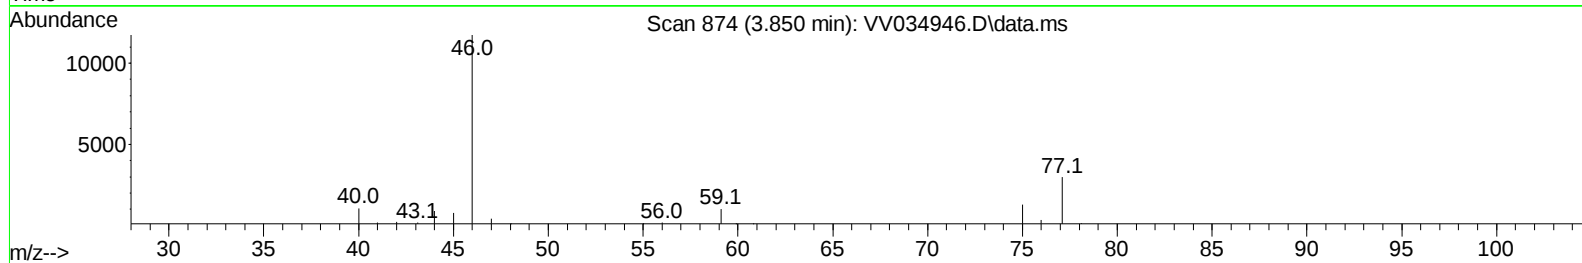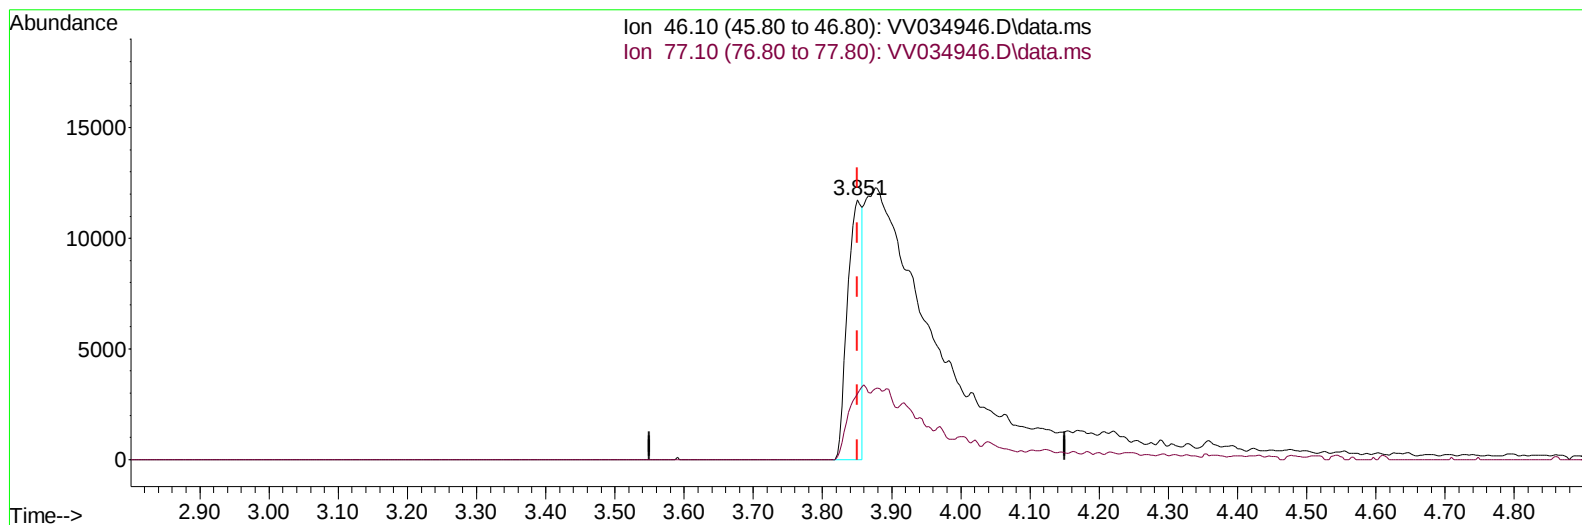

(20) 2-Butanone-d5 (S)

3.850min (+ 0.000) 7.17 ug/L

response 17121

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	17.20	40.77#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034946.D
Acq On : 03 Apr 2024 10:21
Operator : SY/MD
Sample : VV0403WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Manual IntegrationsAPPROVED

Quant Time: Apr 04 05:01:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 04 02:49:59 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/09/2024
Supervised By :Semsettin Yesilyurt 04/09/2024

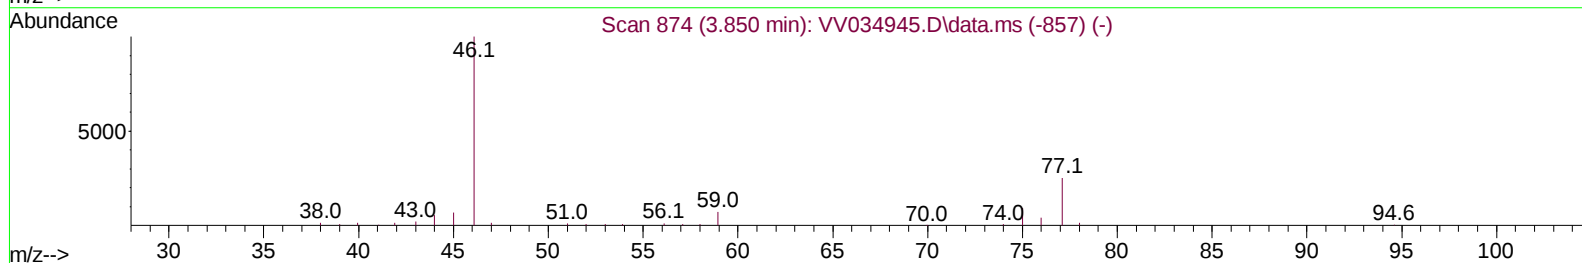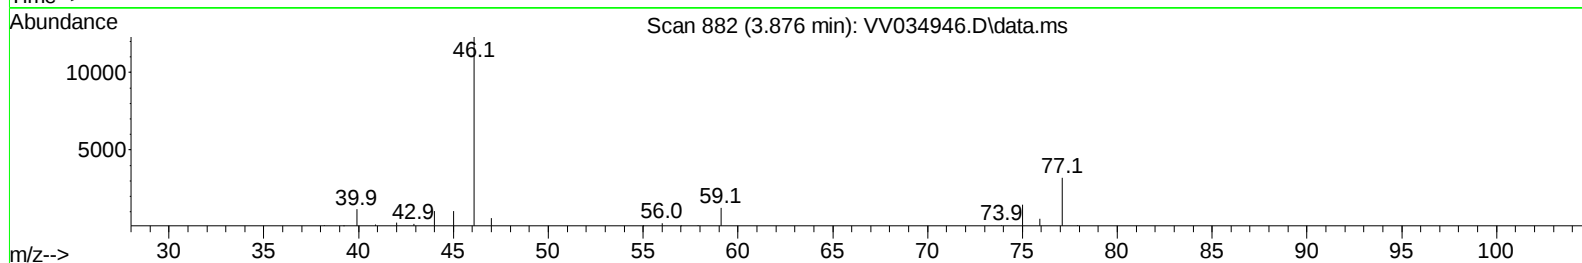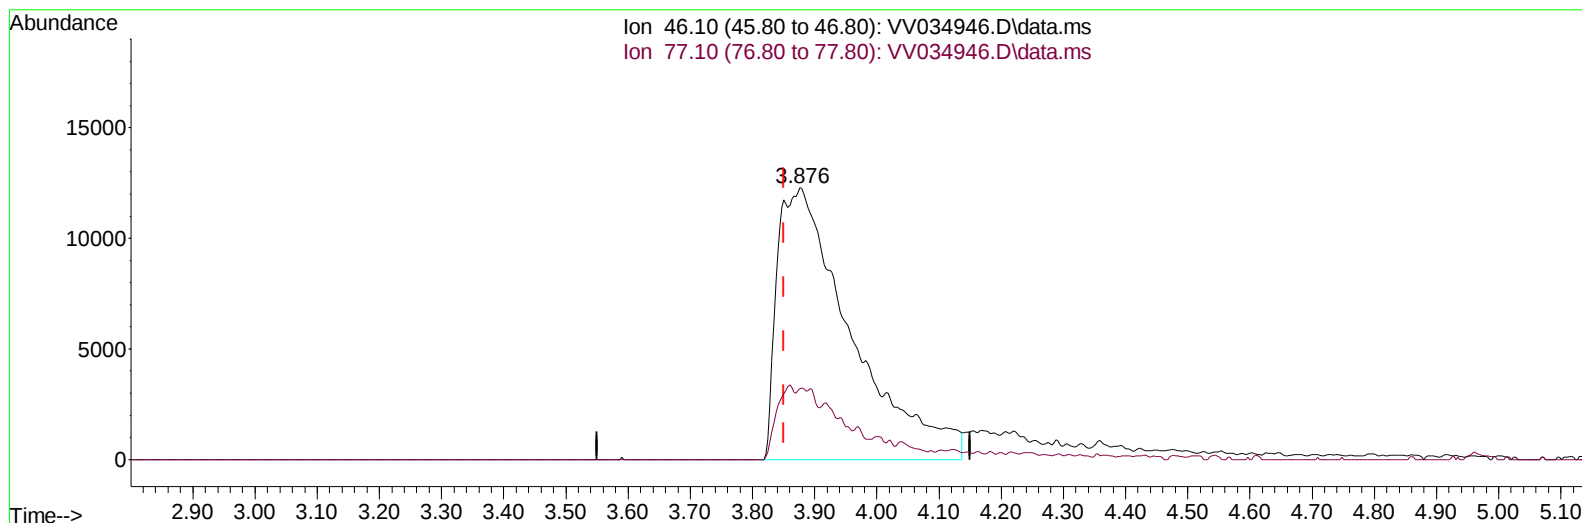

TIC: VV034946.D\data.ms

(20) 2-Butanone-d5 (S)

3.876min (+ 0.026) 42.34 ug/L m

response 101082

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	17.20	6.91#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
 Data File : VV034946.D
 Acq On : 03 Apr 2024 10:21
 Operator : SY/MD
 Sample : VV0403WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Manual IntegrationsAPPROVED

Quant Time: Apr 04 05:01:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 04 02:49:59 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/09/2024
 Supervised By :Semsettin Yesilyurt 04/09/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		185146	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		184405	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		77918	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		71525	4.688	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	93.800%	
7) Chloroethane-d5	1.532	69		60968	4.846	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	97.000%	
11) 1,1-Dichloroethene-d2	2.060	65		32340	4.667	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	93.400%	
20) 2-Butanone-d5	3.876	46		101082m	42.339	ug/L	0.03
Spiked Amount 50.000	Range 40	- 130		Recovery	=	84.680%	
24) Chloroform-d	4.249	84		118352	4.794	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	95.800%	
26) 1,2-Dichloroethane-d4	4.944	65		56247	5.045	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	100.800%	
32) Benzene-d6	4.960	84		237223	4.918	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	98.400%	
36) 1,2-Dichloropropane-d6	5.989	67		73475	5.190	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	103.800%	
41) Toluene-d8	7.243	98		195839	4.469	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	89.400%	
43) trans-1,3-Dichloroprop...	7.561	79		20722	4.120	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	82.400%	
46) 2-Hexanone-d5	8.034	63		66801	38.700	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	77.400%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84		46181	4.675	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	93.400%	
66) 1,2-Dichlorobenzene-d4	11.561	152		63174	5.147	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	103.000%	
Target Compounds							
65) 1,4-Dichlorobenzene	11.214	146		3635	0.146	ug/L	96
70) 1,2,4-trichlorobenzene	13.207	180		4952	0.342	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034946.D
Acq On : 03 Apr 2024 10:21
Operator : SY/MD
Sample : VV0403WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/09/2024
Supervised By :Semsettin Yesilyurt 04/09/2024

Quant Time: Apr 04 05:01:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 04 02:49:59 2024
Response via : Initial Calibration

