

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
 Data File : VV034946.D
 Acq On : 03 Apr 2024 10:21
 Operator : SY/MD
 Sample : VV0403WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	110862	116050	18.00%	2.313%
2	1.535	146	154	165	rVB	96194	110396	17.13%	2.201%
3	2.060	306	317	333	rBV	185625	272850	42.33%	5.439%
4	3.860	862	877	880	rBV2	22284	47667	7.39%	0.950%
5	4.249	982	998	1023	rBV	104972	277423	43.04%	5.530%
6	4.960	1204	1219	1252	rBV2	250238	644626	100.00%	12.850%
7	5.535	1387	1398	1430	rBV	207528	446726	69.30%	8.905%
8	5.838	1482	1492	1511	rVB8	4878	12787	1.98%	0.255%
9	5.989	1525	1539	1562	rBV	143077	304752	47.28%	6.075%
10	6.918	1814	1828	1859	rBV	51900	112218	17.41%	2.237%
11	7.243	1917	1929	1949	rBV	282447	508588	78.90%	10.138%
12	7.561	2019	2028	2048	rBV	29262	60441	9.38%	1.205%
13	8.034	2166	2175	2222	rBV2	172735	484445	75.15%	9.657%
14	8.783	2397	2408	2434	rBV	322817	559752	86.83%	11.158%
15	10.153	2824	2834	2848	rBV	90973	147777	22.92%	2.946%
16	11.185	3144	3155	3178	rBV	292491	478574	74.24%	9.540%
17	11.561	3257	3272	3298	rBV	241522	397653	61.69%	7.927%
18	13.204	3772	3783	3799	rBV2	14102	24487	3.80%	0.488%
19	13.455	3850	3861	3874	rBV2	5240	9321	1.45%	0.186%




Sum of corrected areas: 5016533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034946.D
Acq On : 03 Apr 2024 10:21
Operator : SY/MD
Sample : VV0403WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

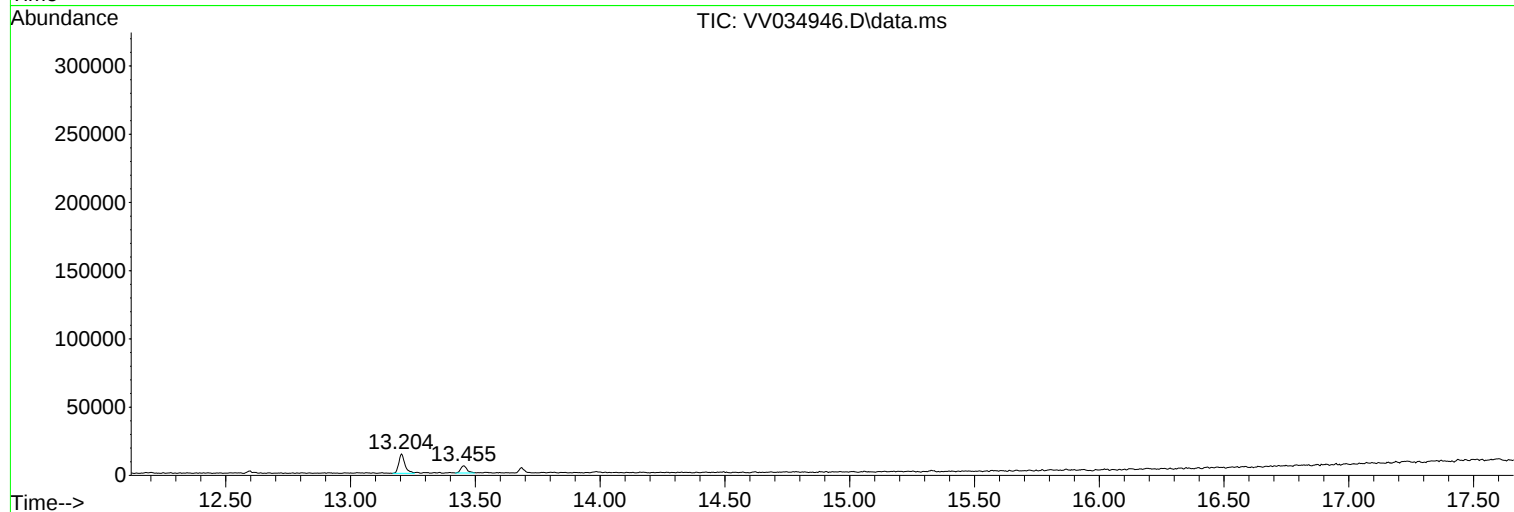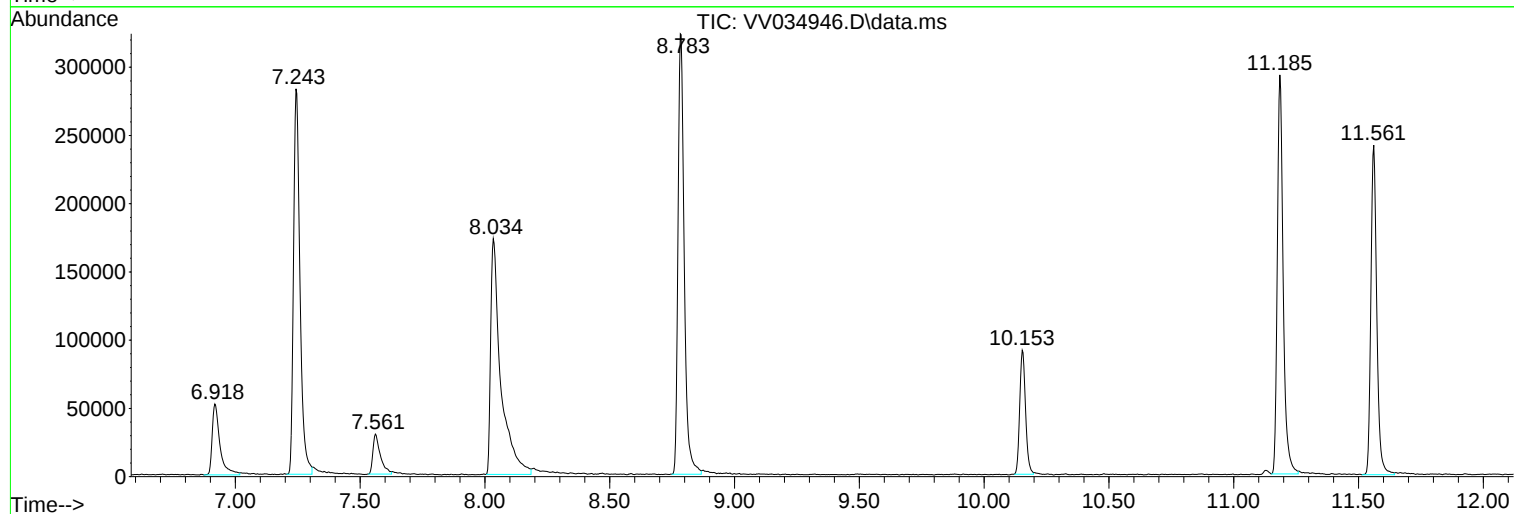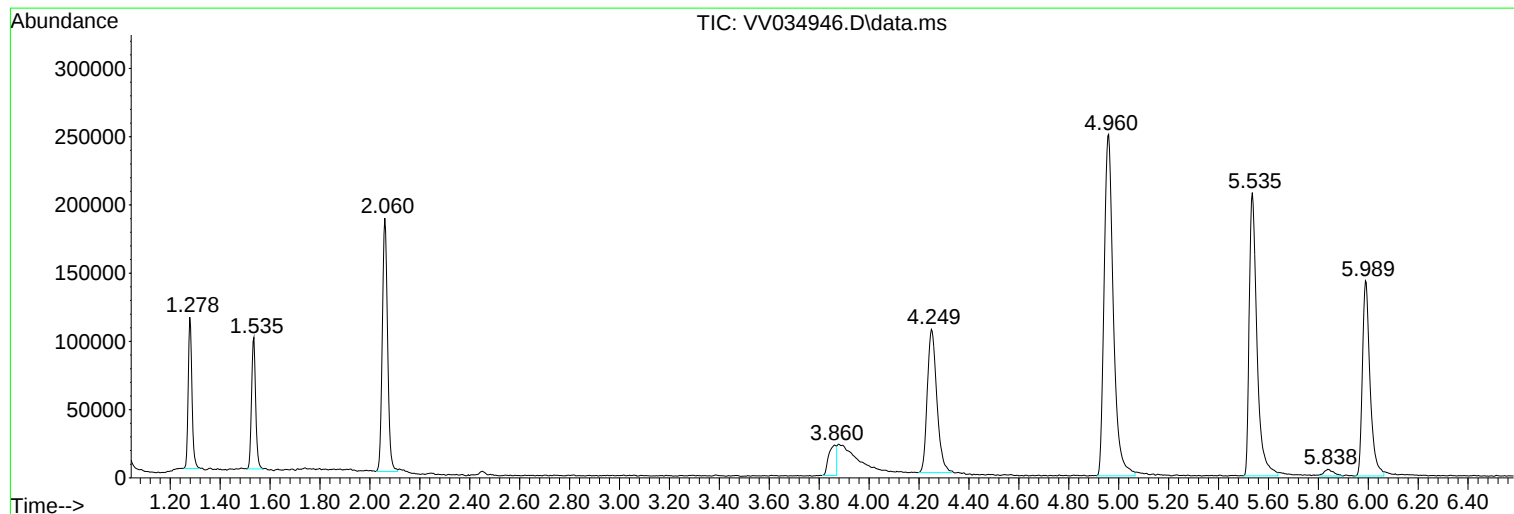

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034946.D
Acq On : 03 Apr 2024 10:21
Operator : SY/MD
Sample : VV0403WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034946.D
Acq On : 03 Apr 2024 10:21
Operator : SY/MD
Sample : VV0403WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc