

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
 Data File : VV034948.D
 Acq On : 03 Apr 2024 11:31
 Operator : SY/MD
 Sample : P1925-01DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-6(20240326)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rBV	109217	114721	12.96%	1.915%
2	1.532	146	153	168	rVB	92717	108855	12.30%	1.817%
3	2.056	306	316	333	rBV	190465	280172	31.65%	4.678%
4	2.446	428	437	448	rVB2	12163	19869	2.24%	0.332%
5	3.841	854	871	904	rBV3	33986	181765	20.53%	3.035%
6	4.249	981	998	1030	rBV	104973	278662	31.48%	4.652%
7	4.957	1201	1218	1255	rBV2	254642	661928	74.77%	11.051%
8	5.532	1387	1397	1430	rBV	199531	435074	49.15%	7.264%
9	5.989	1524	1539	1568	rBV	139598	307930	34.78%	5.141%
10	6.918	1818	1828	1859	rBV2	57590	125646	14.19%	2.098%
11	7.243	1918	1929	1951	rBV	281450	522234	58.99%	8.719%
12	7.561	2015	2028	2059	rBV	32676	71168	8.04%	1.188%
13	8.030	2165	2174	2216	rBV2	183407	498754	56.34%	8.327%
14	8.783	2396	2408	2413	rBV	345645	545378	61.61%	9.105%
15	10.153	2819	2834	2855	rBV	94560	157734	17.82%	2.633%
16	11.117	3125	3134	3145	rBV	91518	146014	16.49%	2.438%
17	11.185	3145	3155	3183	rVB2	346717	885245	100.00%	14.779%
18	11.561	3259	3272	3293	rBV	269434	476079	53.78%	7.948%
19	13.197	3770	3781	3801	rBV	90993	151382	17.10%	2.527%
20	14.728	4246	4257	4266	rBV5	12579	21156	2.39%	0.353%




Sum of corrected areas: 5989766

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034948.D
Acq On : 03 Apr 2024 11:31
Operator : SY/MD
Sample : P1925-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6(20240326)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

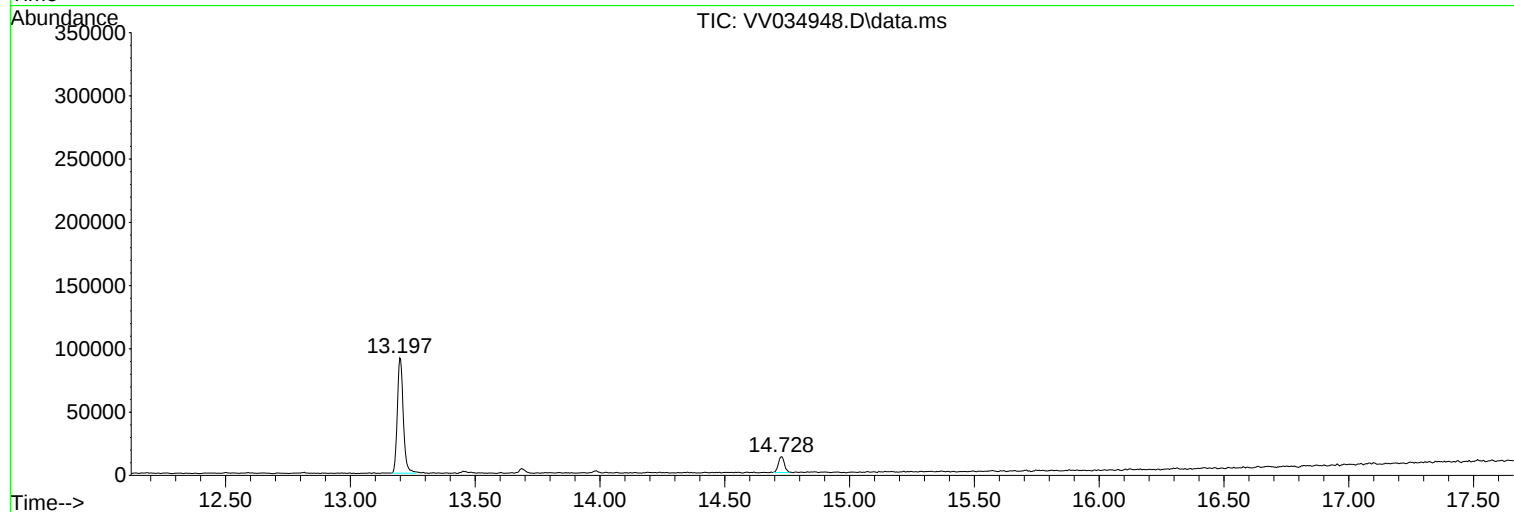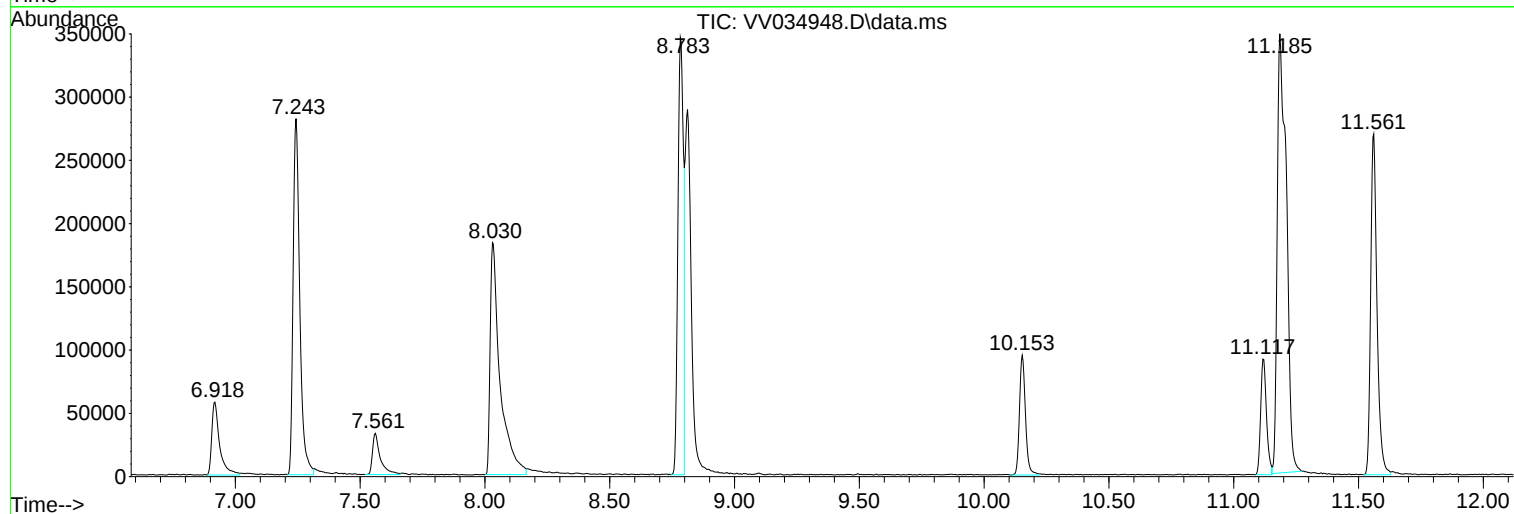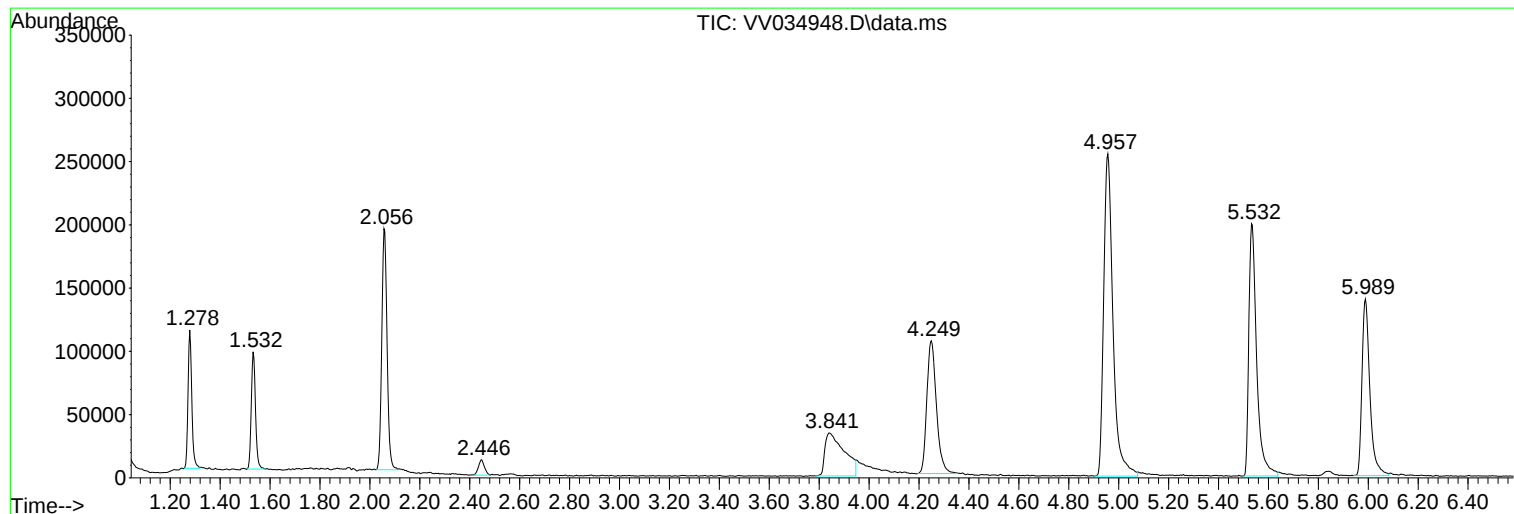

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034948.D
Acq On : 03 Apr 2024 11:31
Operator : SY/MD
Sample : P1925-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6(20240326)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034948.D
Acq On : 03 Apr 2024 11:31
Operator : SY/MD
Sample : P1925-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6(20240326)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------