

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
 Data File : VV034953.D
 Acq On : 03 Apr 2024 13:54
 Operator : SY/MD
 Sample : P1925-12DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9S(20240327)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	99374	107689	3.50%	1.117%
2	1.535	146	154	165	rBV	87184	103146	3.36%	1.070%
3	2.060	307	317	331	rBV	175068	253884	8.26%	2.633%
4	3.831	855	868	913	rBV3	40114	221994	7.22%	2.302%
5	4.252	983	999	1034	rBV	103642	276443	8.99%	2.867%
6	4.960	1204	1219	1257	rBV3	244180	637468	20.74%	6.610%
7	5.535	1388	1398	1431	rBV	196292	425367	13.84%	4.411%
8	5.989	1527	1539	1567	rBV	139692	300877	9.79%	3.120%
9	6.918	1816	1828	1851	rBV2	55983	116377	3.79%	1.207%
10	7.243	1919	1929	1956	rBV	272264	504344	16.41%	5.230%
11	7.561	2018	2028	2054	rBV2	30319	65592	2.13%	0.680%
12	8.030	2166	2174	2212	rBV2	191987	500314	16.28%	5.188%
13	8.786	2397	2409	2412	rBV	358771	510743	16.62%	5.296%
14	8.812	2413	2417	2442	rVB	467999	734244	23.89%	7.614%
15	10.152	2821	2834	2858	rBV	92979	155042	5.04%	1.608%
16	11.114	3122	3133	3146	rBV	688235	1071501	34.86%	11.111%
17	11.207	3146	3162	3189	rVB2	1695332	3073888	100.00%	31.875%
18	11.561	3260	3272	3295	rBV2	287800	550789	17.92%	5.711%
19	13.204	3773	3783	3807	rBV4	18675	34004	1.11%	0.353%




Sum of corrected areas: 9643706

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034953.D
Acq On : 03 Apr 2024 13:54
Operator : SY/MD
Sample : P1925-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9S(20240327)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

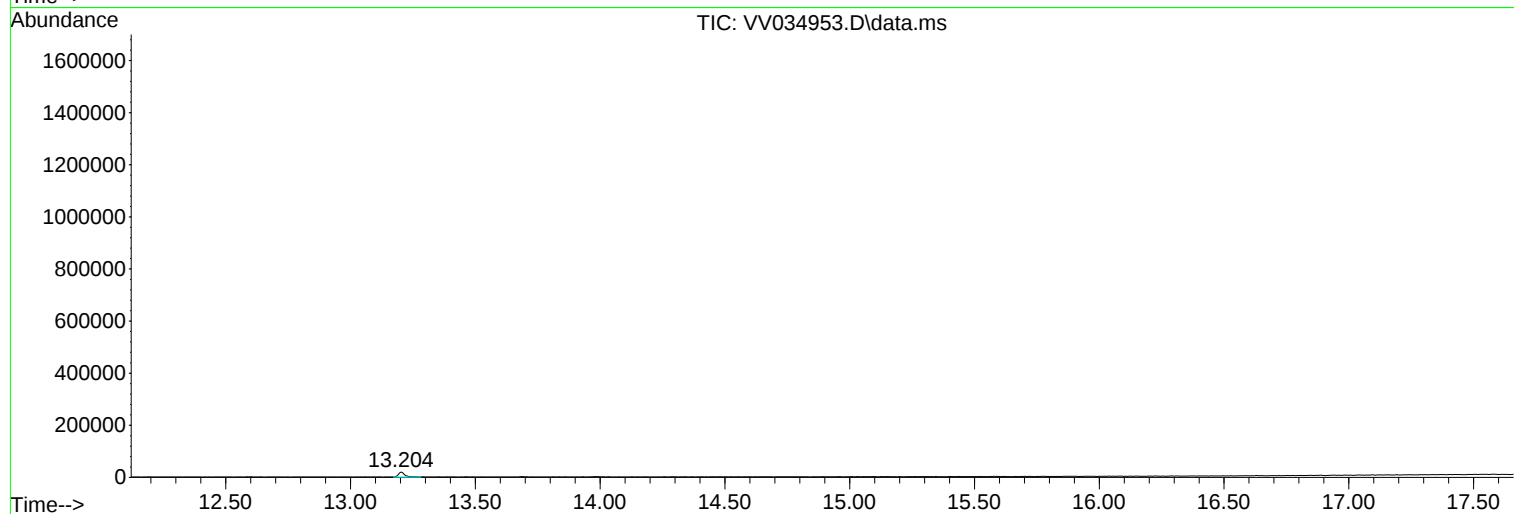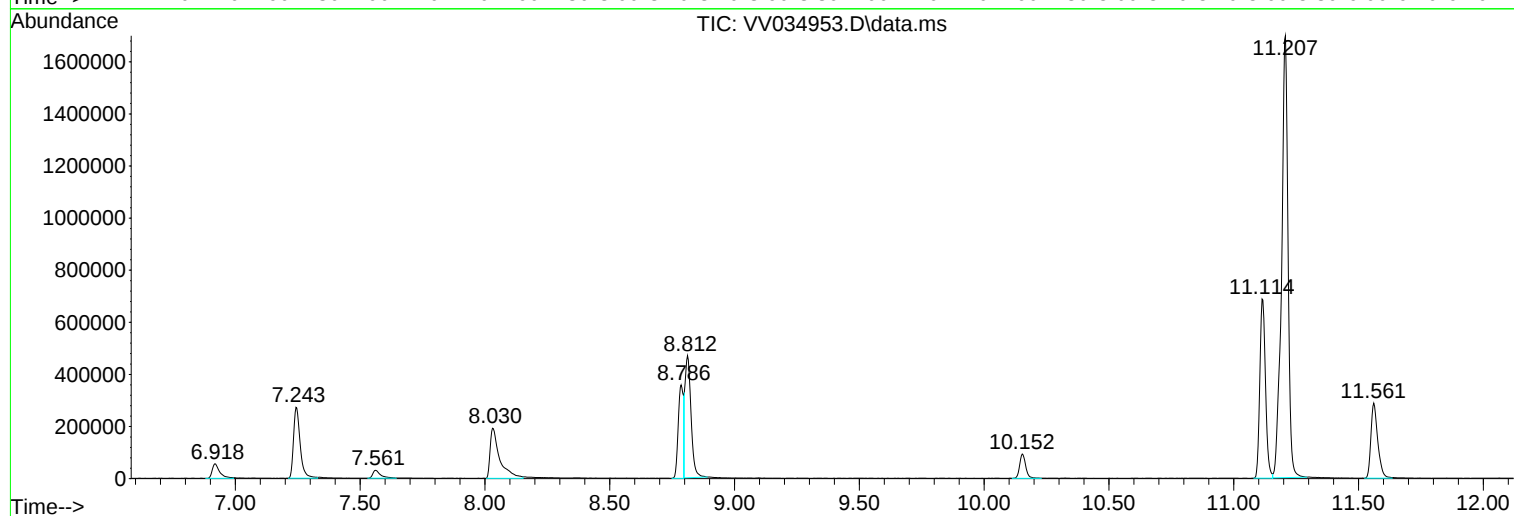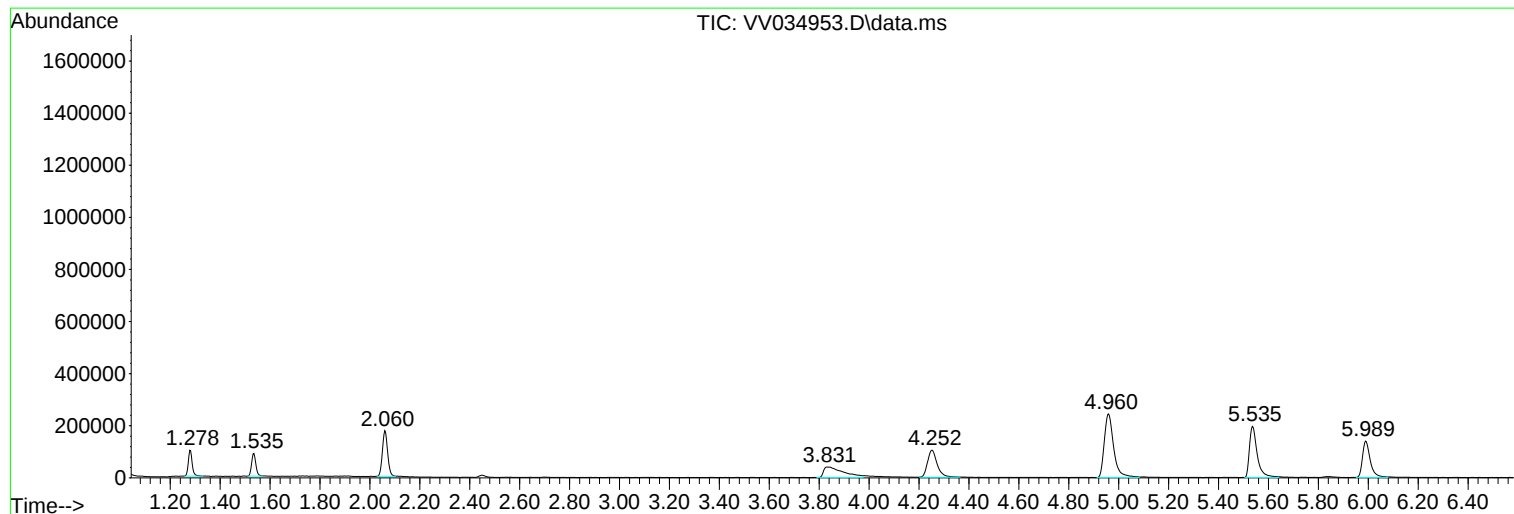

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034953.D
Acq On : 03 Apr 2024 13:54
Operator : SY/MD
Sample : P1925-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9S(20240327)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034953.D
Acq On : 03 Apr 2024 13:54
Operator : SY/MD
Sample : P1925-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9S(20240327)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc