
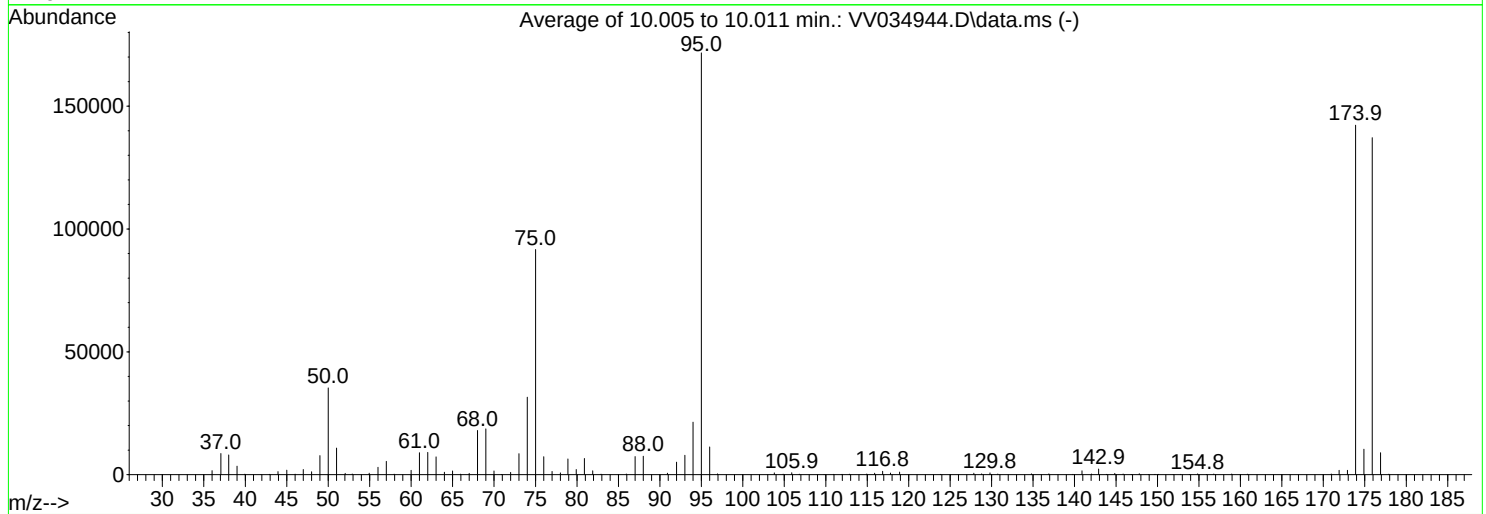


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040324\
Data File : VV034944.D
Acq On : 03 Apr 2024 08:31
Operator : SY/MD
Sample : BFB265
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB265

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 04 02:49:59 2024

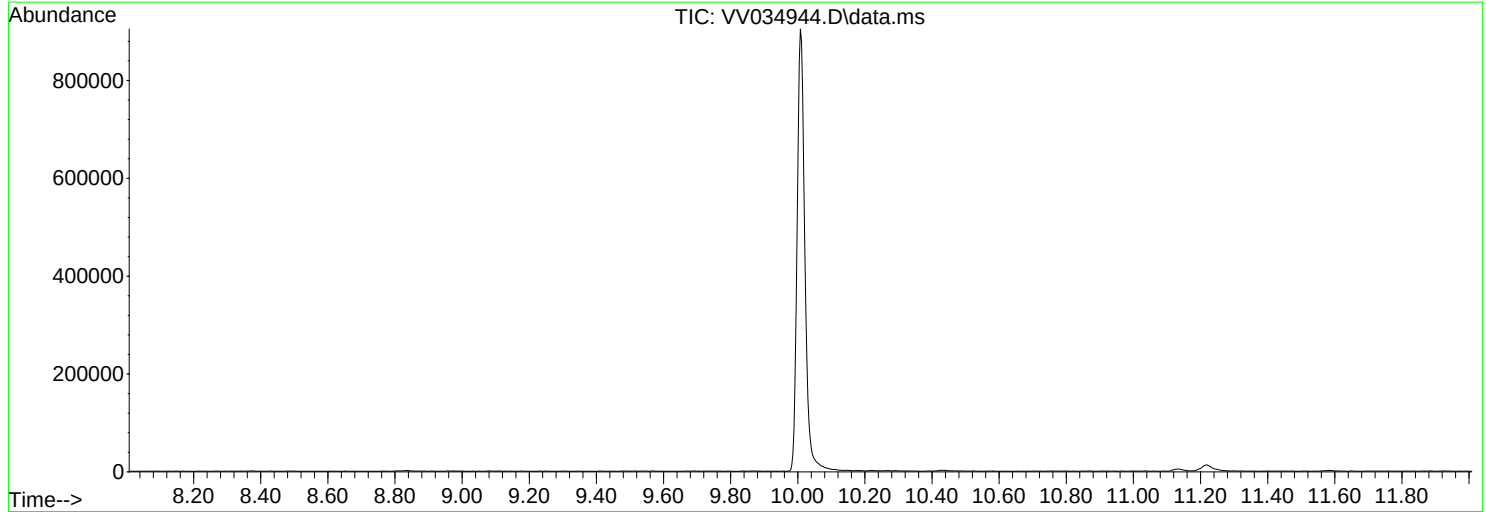

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	35333	PASS
75	95	30	80	53.4	91637	PASS
95	95	100	100	100.0	171733	PASS
96	95	5	9	6.6	11295	PASS
173	174	0.00	2	1.2	1774	PASS
174	95	50	120	82.8	142272	PASS
175	174	5	9	7.3	10358	PASS
176	174	95	105	96.5	137227	PASS
177	176	5	10	6.5	8937	PASS

m/z	Abundance
39.90	993.0
43.90	416.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	1580.0
37.10	8286.0
38.00	7723.0
39.00	3565.0
40.00	1154.0
41.90	129.0
42.90	115.0
44.00	1686.0
45.00	1805.0
47.00	1998.0
48.00	1118.0
49.00	7639.0
50.00	34176.0
51.00	10775.0
52.10	508.0
52.90	259.0
54.90	515.0
56.00	2896.0
57.00	5242.0
58.00	230.0
60.00	1735.0
61.00	8493.0
62.00	9081.0
63.00	7166.0
64.00	1184.0
65.00	1531.0
65.90	188.0
67.00	525.0
68.00	17152.0
69.00	18272.0
70.00	1530.0
70.90	131.0
72.00	915.0
73.00	8428.0
74.00	30648.0
75.00	89000.0
76.00	7212.0
77.00	1389.0
78.00	715.0
78.90	6408.0
79.90	2101.0
80.90	6426.0
81.90	1527.0
82.90	182.0
86.00	220.0
87.00	7127.0
88.00	7159.0
90.90	555.0
92.00	5032.0
93.00	7762.0
94.00	20696.0
95.00	164800.0
96.00	11175.0
96.90	330.0
103.80	687.0
104.80	194.0
105.90	767.0
106.80	179.0
110.90	148.0
111.90	150.0
112.90	187.0
115.00	265.0
115.90	636.0
116.80	1193.0
117.80	610.0
118.90	1010.0
123.90	131.0
127.80	588.0
128.80	325.0
129.80	673.0
130.80	223.0
134.80	335.0
136.90	309.0
139.90	156.0
140.90	1497.0
142.10	205.0
142.90	2136.0
143.80	160.0
144.80	567.0
145.90	247.0
146.90	136.0
147.80	415.0
149.00	114.0
149.70	138.0
150.10	130.0
151.90	123.0
152.80	175.0
154.90	265.0
156.80	265.0
158.90	214.0
160.80	204.0
171.00	269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

171.90	1684.0
172.90	1571.0
173.90	133312.0
174.90	9804.0
175.90	128480.0
176.90	8688.0
177.90	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	1674.0
37.00	8945.0
38.00	8374.0
39.00	3571.0
40.00	1216.0
41.90	116.0
42.90	129.0
44.00	1680.0
45.00	1873.0
46.00	251.0
47.00	2160.0
48.00	1214.0
49.00	7952.0
50.00	36560.0
51.00	11191.0
52.10	532.0
52.90	276.0
55.00	585.0
56.00	3126.0
57.00	5600.0
57.90	228.0
60.00	1828.0
61.00	9221.0
62.00	9337.0
63.00	7486.0
64.00	1033.0
65.00	1564.0
66.00	207.0
67.00	547.0
68.00	18520.0
69.00	19448.0
70.00	1548.0
70.90	104.0
72.00	972.0
73.00	8828.0
74.00	32712.0
75.00	95024.0
76.00	7451.0
77.00	1374.0
78.00	744.0
78.90	6646.0
79.90	2175.0
80.90	6803.0
81.90	1603.0
82.90	192.0
85.90	231.0
87.00	7559.0
88.00	7841.0
90.90	641.0
92.00	5281.0
93.00	8211.0
94.00	22160.0
95.00	177536.0
96.00	11729.0
97.00	299.0
103.80	699.0
104.80	215.0
105.90	786.0
106.80	195.0
109.80	112.0
111.00	168.0
111.90	164.0
112.90	191.0
115.00	270.0
115.90	630.0
116.90	1413.0
117.80	677.0
118.90	1105.0
123.80	147.0
127.80	610.0
128.80	364.0
129.80	733.0
130.70	262.0
134.80	334.0
136.90	326.0
139.80	155.0
140.90	1647.0
142.00	277.0
142.90	2321.0
143.80	152.0
144.80	566.0
145.80	280.0
146.80	111.0
147.80	397.0
148.90	115.0
149.70	143.0
150.10	136.0
151.90	109.0
152.80	160.0
153.90	115.0
154.80	302.0
155.90	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

156.80	306.0
158.90	259.0
160.80	230.0
170.90	288.0
171.90	1853.0
172.90	1828.0
173.90	147392.0
174.90	10624.0
175.90	142272.0
176.90	9250.0
177.90	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	1634.0
37.00	8621.0
38.00	8003.0
39.00	3166.0
40.00	1199.0
42.90	121.0
44.00	1524.0
45.00	1764.0
46.00	290.0
47.00	2040.0
48.00	1191.0
49.00	7592.0
50.00	35264.0
51.00	10594.0
52.00	514.0
52.90	284.0
55.00	580.0
56.00	2960.0
57.00	5421.0
58.00	217.0
60.00	1717.0
61.00	9072.0
62.00	8868.0
63.00	7043.0
64.00	802.0
65.00	1451.0
66.00	210.0
67.00	475.0
68.00	18240.0
69.00	18264.0
70.00	1381.0
72.00	902.0
73.00	8414.0
74.00	31320.0
75.00	90888.0
76.00	7319.0
77.00	1161.0
78.00	701.0
78.90	6186.0
79.90	1940.0
80.90	6431.0
81.90	1553.0
82.90	180.0
85.90	300.0
87.00	7481.0
88.00	7572.0
90.90	654.0
92.00	4988.0
93.00	7737.0
94.00	21240.0
95.00	172864.0
96.00	10980.0
96.90	282.0
103.80	695.0
104.90	277.0
105.90	750.0
106.80	193.0
109.80	125.0
111.00	162.0
112.00	156.0
112.80	168.0
114.90	248.0
115.90	595.0
116.90	1455.0
117.80	629.0
118.90	1098.0
123.80	157.0
127.90	582.0
128.80	332.0
129.80	685.0
130.70	281.0
134.80	337.0
136.90	339.0
139.70	145.0
140.90	1652.0
142.00	292.0
142.90	2380.0
143.90	135.0
144.90	499.0
145.80	285.0
147.80	372.0
149.70	137.0
150.10	108.0
152.80	118.0
153.80	133.0
154.80	333.0
155.90	120.0
156.80	291.0
159.00	255.0
160.90	221.0
170.90	279.0
171.90	1765.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

172.90	1924.0
173.90	146112.0
174.90	10645.0
175.90	140928.0
176.90	8874.0
177.90	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265