

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040519\

Data File : VV010130.D

Acq On : 05 Apr 2019 14:28

Operator : SY/MD

Sample : K2148-11

Misc : 5.31G/10mL/MSVOA V/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 01:20:58 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 05 23:46:15 2019


Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :

BF5F8

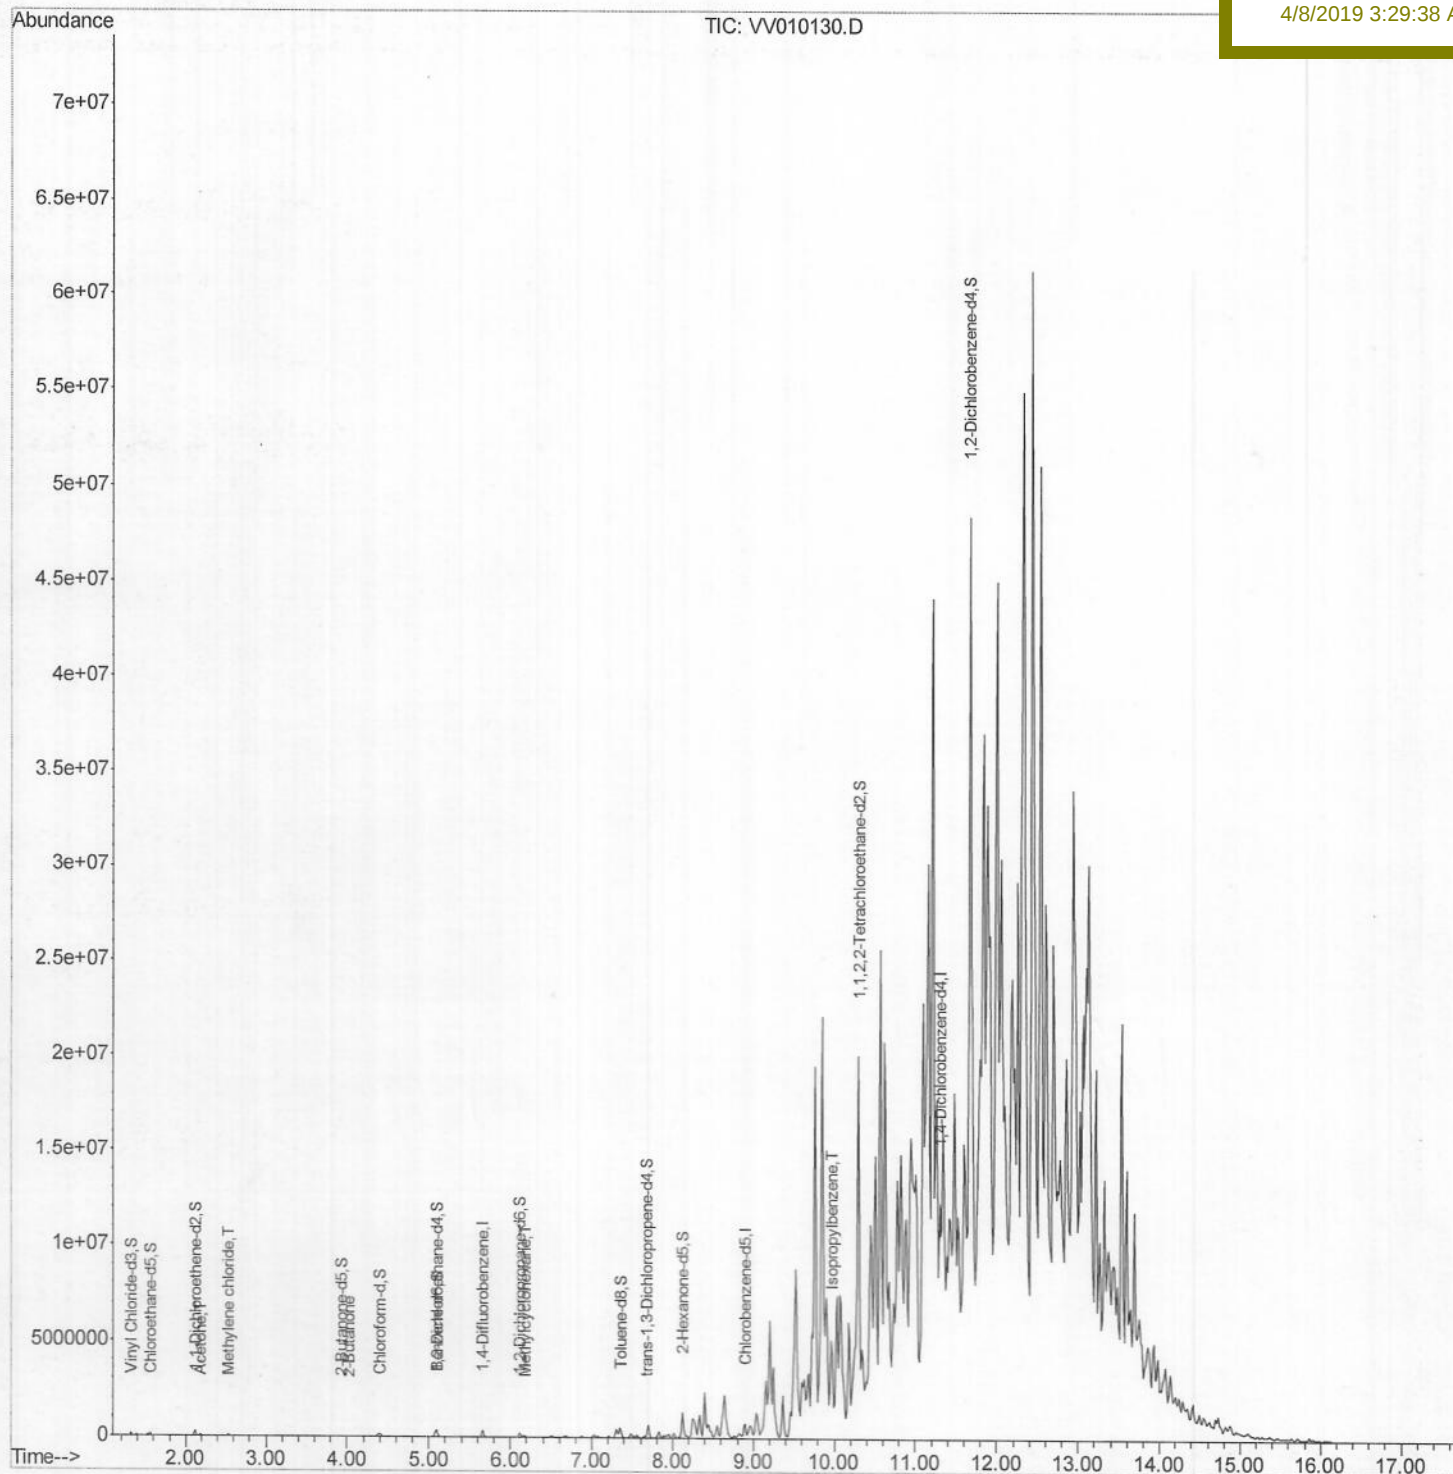Manual Integrations
APPROVEDMMDadoda
4/8/2019 3:29:38 AM


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040519\Not Reviewed Data\
Data File : VV010130.D
Acq On : 05 Apr 2019 14:28
Operator : SY/MD
Sample : K2148-11
Misc : 5.31G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 09:32:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 09 07:35:38 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
BF5F8

Manual Integrations
APPROVED

MMDadoda
4/8/2019 3:29:38 AM

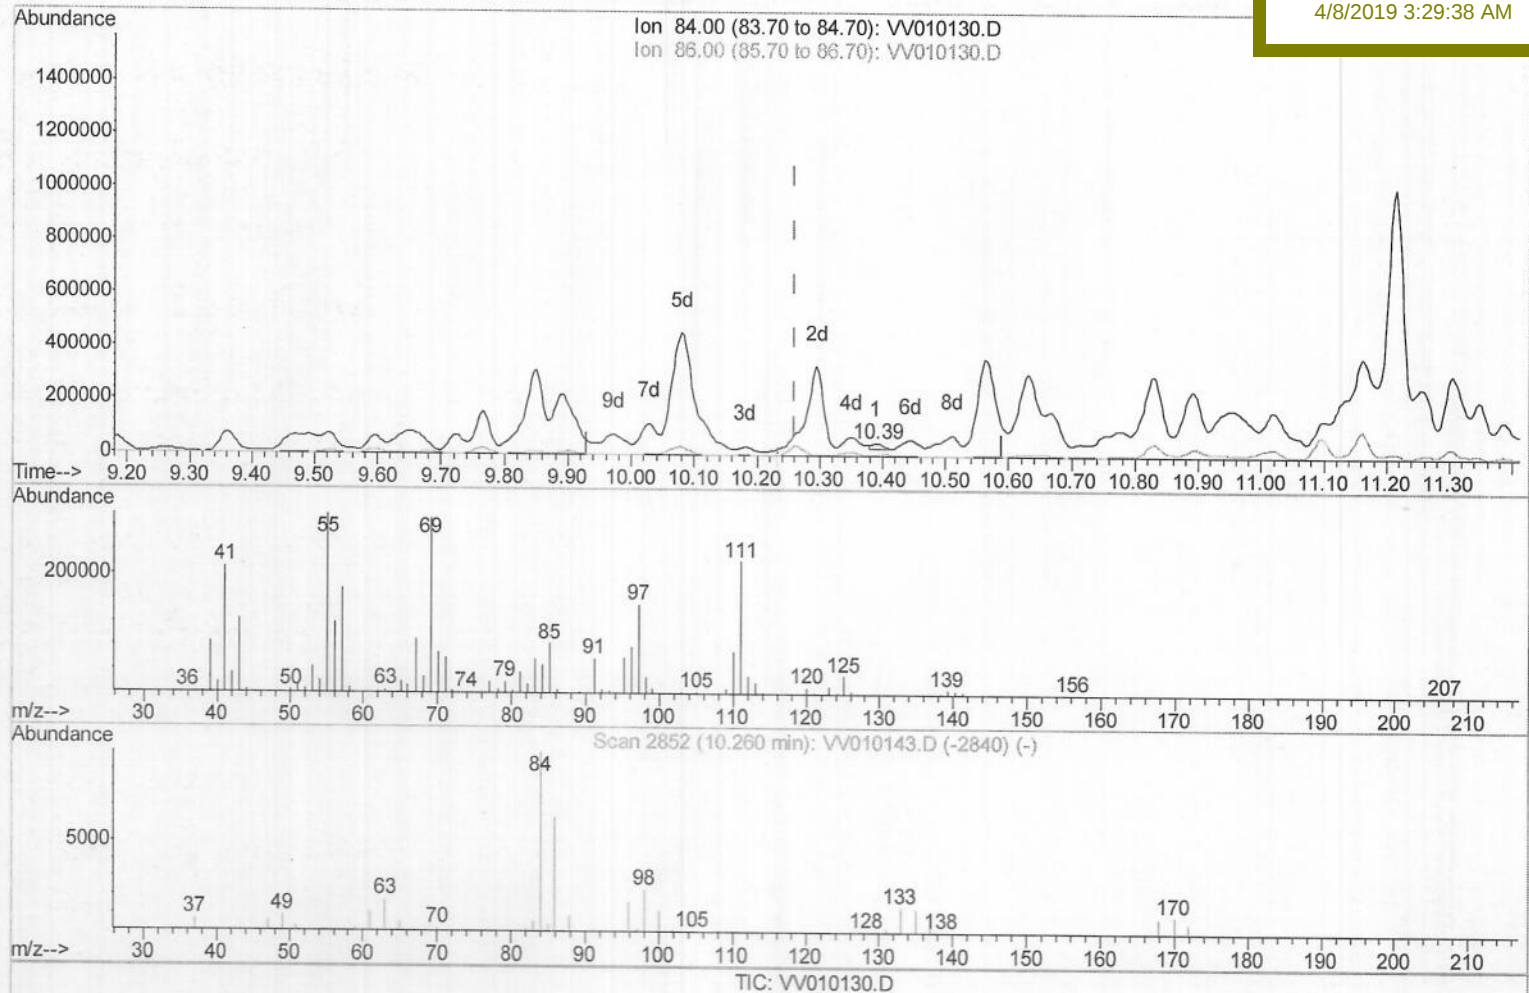

(48) 1,1,2,2-Tetrachloroethane-d2 (S)

10.389min (+0.129) 5.79ug/L

response 23006

Ion	Exp%	Act%
84.00	100	100
86.00	64.40	75.99
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040519\Not Reviewed Data\
Data File : VV010130.D
Acq On : 05 Apr 2019 14:28
Operator : SY/MD
Sample : K2148-11
Misc : 5.31G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 01:35:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 23:46:15 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
BF5F8

Manual Integrations
APPROVED

MMDadoda
4/8/2019 3:29:38 AM

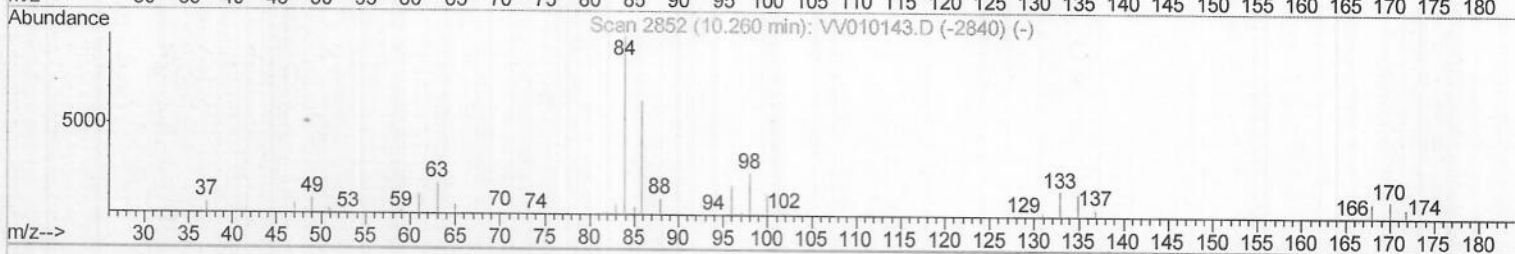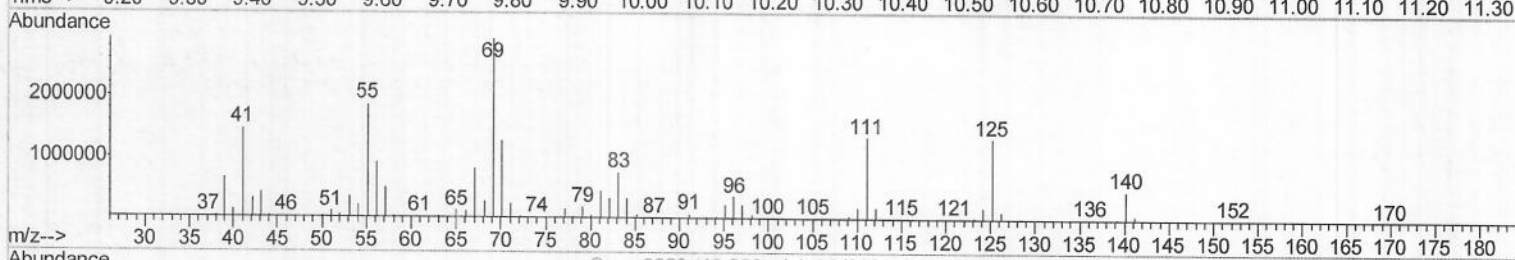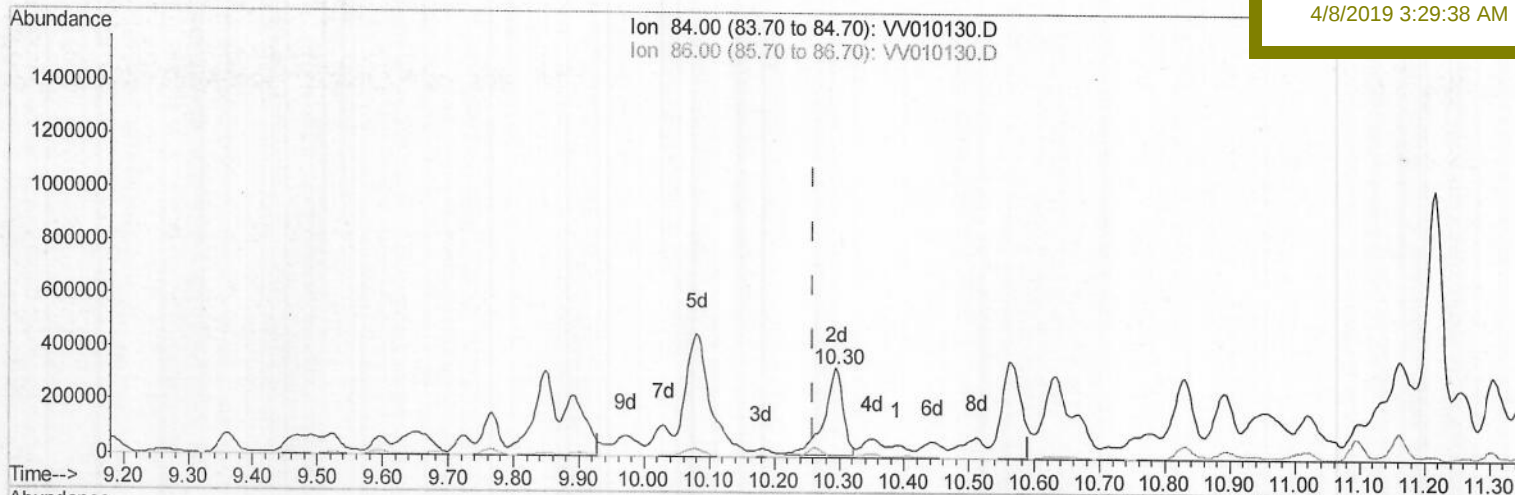

TIC: VV010130.D

(48) 1,1,2,2-Tetrachloroethane-d2 (S)

10.296min (+0.035) 163.93ug/L m

response 651526

Ion	Exp%	Act%
84.00	100	100
86.00	64.40	2.68#
0.00	0.00	0.00
0.00	0.00	0.00

M.D
4/11/19

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040519\Not Reviewed Data\
 Data File : VV010130.D
 Acq On : 05 Apr 2019 14:28
 Operator : SY/MD
 Sample : K2148-11
 Misc : 5.31G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 09:32:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 09 07:35:38 2019
 Response via : Initial Calibration

Instrument :
 MSVOA_V
 ClientSampleId :
 BF5F8

Manual Integrations
 APPROVED

MMDadoda
 4/8/2019 3:29:38 AM

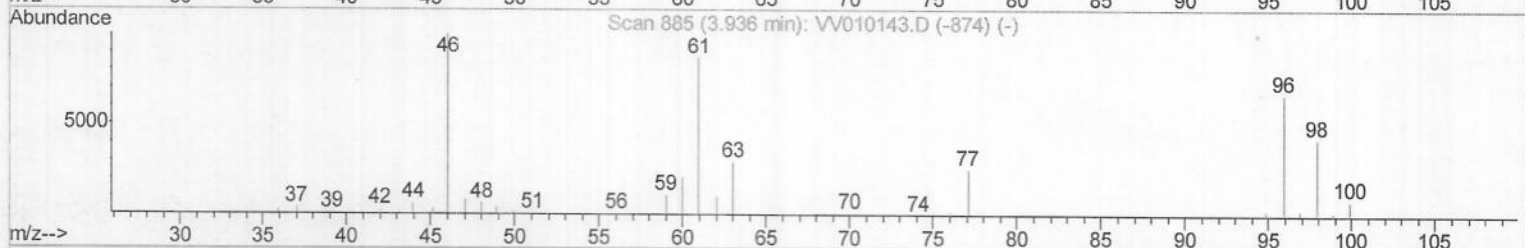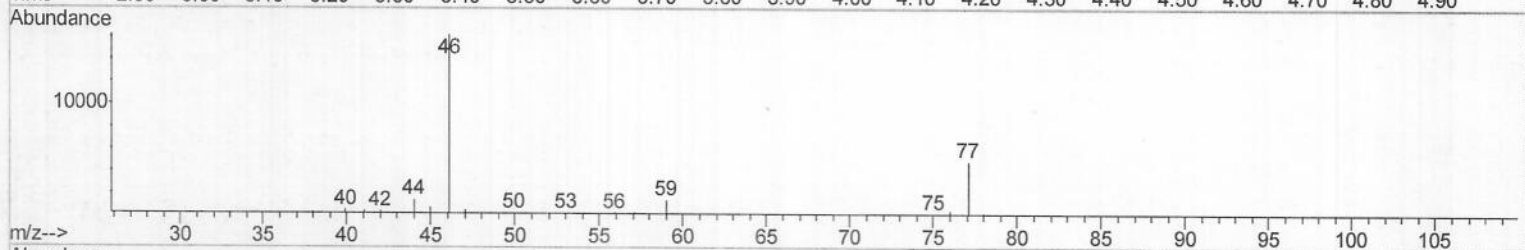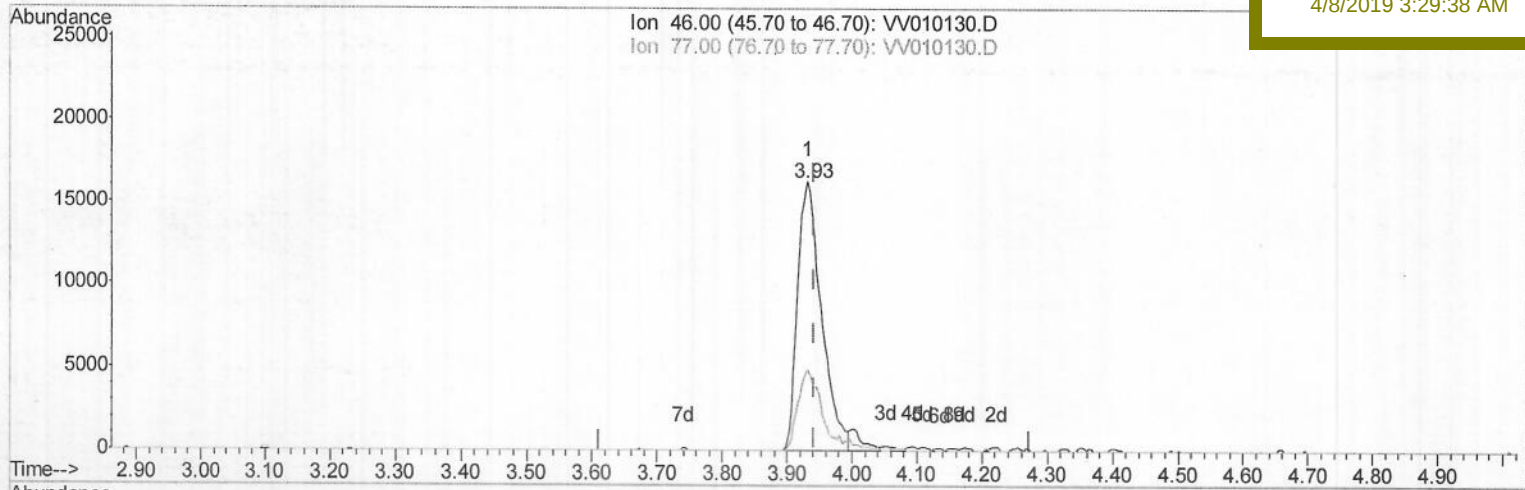

TIC: VV010130.D

(20) 2-Butanone-d5 (S)

3.933min (-0.010) 39.55ug/L

response 41238

Ion	Exp%	Act%
46.00	100	100
77.00	25.70	28.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040519\Not Reviewed Data\
 Data File : VV010130.D
 Acq On : 05 Apr 2019 14:28
 Operator : SY/MD
 Sample : K2148-11
 Misc : 5.31G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 01:35:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 23:46:15 2019
 Response via : Initial Calibration

Instrument :
 MSVOA_V
 ClientSampleId :
 BF5F8

Manual Integrations
 APPROVED

MMDadoda
 4/8/2019 3:29:38 AM

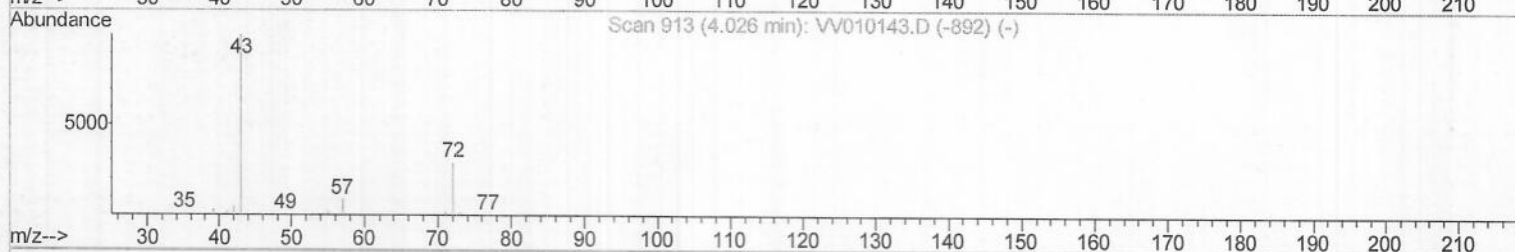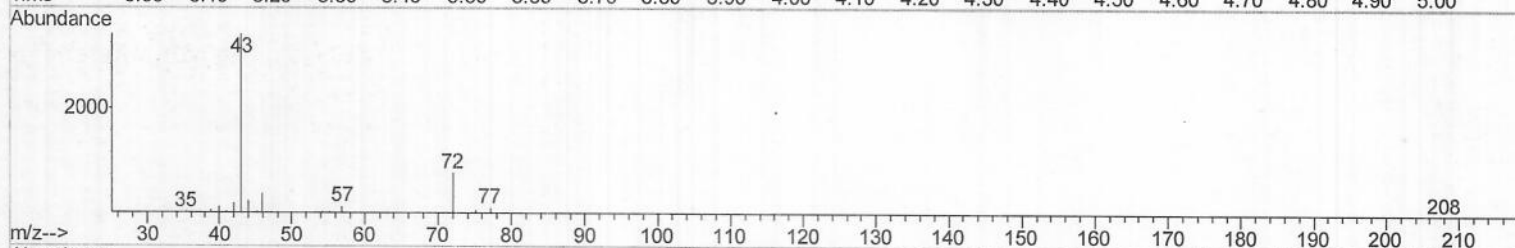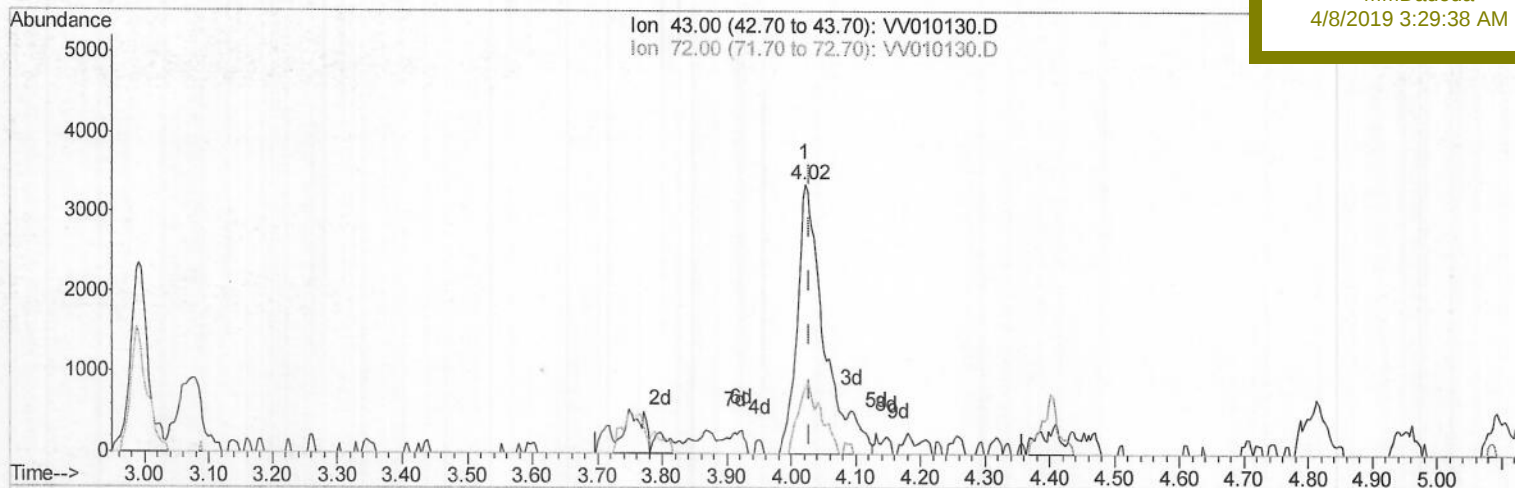

TIC: VV010130.D

(21) 2-Butanone

4.023min (-0.006) 8.65ug/L m

response 9767

Ion	Exp%	Act%
43.00	100	100
72.00	25.60	14.01
0.00	0.00	0.00
0.00	0.00	0.00

M.D
 7/11/14

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040519\

Data File : VV010130.D

Acq On : 05 Apr 2019 14:28

Operator : SY/MD

Sample : K2148-11

Misc : 5.31G/10mL/MSVOA V/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 01:20:58 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 05 23:46:15 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :

BF5F8

Manual Integrations
APPROVEDMMDadoda
4/8/2019 3:29:38 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	273669	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	263306	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.31	152	261794	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	55933	15.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.08%
7) Chloroethane-d5	1.56	69	60639	13.33	ug/L	-0.02
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.32%
10) 1,1-Dichloroethene-d2	2.12	63	117705	12.74	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.96%
20) 2-Butanone-d5	3.93	46	41238	39.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.10%
24) Chloroform-d	4.40	84	136658	19.82	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.28%
26) 1,2-Dichloroethane-d4	5.08	65	82851	21.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.92%
29) Benzene-d6	5.10	84	287620	21.06	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.24%
33) 1,2-Dichloropropane-d6	6.12	67	87309	21.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.68%
37) Toluene-d8	7.36	98	270947	20.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.36%
38) trans-1,3-Dichloropropene-	7.66	79	36916	21.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.72%
39) 2-Hexanone-d5	8.13	63	38243	47.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.64%
48) 1,1,2,2-Tetrachloroethane-	10.30	84	651526m	163.93	ug/L	0.04
Spiked Amount	25.000	Range	45 - 120	Recovery	=	655.72%#
61) 1,2-Dichlorobenzene-d4	11.68	152	520659	51.06	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	204.24%#

Target Compounds

					Ovalue	
13) Acetone	2.19	43	38751	37.595	ug/L	99
16) Methylene chloride	2.53	84	18594	3.867	ug/L	99
21) 2-Butanone	4.02	43	9767m	8.652	ug/L	
36) Methylcyclohexane	6.17	83	34778	6.264	ug/L	89
57) Isopropylbenzene	9.98	105	172945	10.975	ug/L #	85

(#)= qualifier out of range (m) = manual integration (+) = signals summed