

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040519\
 Data File : VV010126.D
 Acq On : 05 Apr 2019 12:18
 Operator : SY/MD
 Sample : K2148-15RE
 Misc : 3.54G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF5G9RE

Manual Integrations
 APPROVED

MMDadoda
 4/8/2019 3:29:35 AM

Quant Time: Apr 06 00:18:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 23:46:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	248019	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	176967	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	48246	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	61594	18.55	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.20%		
7) Chloroethane-d5	1.56	69	56885	13.79	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	55.16%		
10) 1,1-Dichloroethene-d2	2.12	63	123742	14.77	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.08%		
20) 2-Butanone-d5	3.94	46	20417m	21.61	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	43.22%		
24) Chloroform-d	4.40	84	132064	21.14	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.56%		
26) 1,2-Dichloroethane-d4	5.08	65	70595	20.19	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	80.76%		
29) Benzene-d6	5.09	84	269152	29.33	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	117.32%		
33) 1,2-Dichloropropane-d6	6.11	67	77281	28.53	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	114.12%		
37) Toluene-d8	7.36	98	223731	25.30	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	101.20%		
38) trans-1,3-Dichloropropene-	7.66	79	21406	18.49	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	73.96%		
39) 2-Hexanone-d5	8.13	63	14623	26.92	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	53.84%		
48) 1,1,2,2-Tetrachloroethane-	10.26	84	42497	15.91	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	63.64%		
61) 1,2-Dichlorobenzene-d4	11.67	152	38321	20.39	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	81.56%		
Target Compounds						
13) Acetone	2.19	43	2418	2.588	ug/L	83
16) Methylene chloride	2.53	84	39063	8.965	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040519\
Data File : VV010126.D
Acq On : 05 Apr 2019 12:18
Operator : SY/MD
Sample : K2148-15RE
Misc : 3.54G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BF5G9RE

Manual Integrations
APPROVED

MMDadoda
4/8/2019 3:29:35 AM

Quant Time: Apr 06 00:18:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 23:46:15 2019
Response via : Initial Calibration

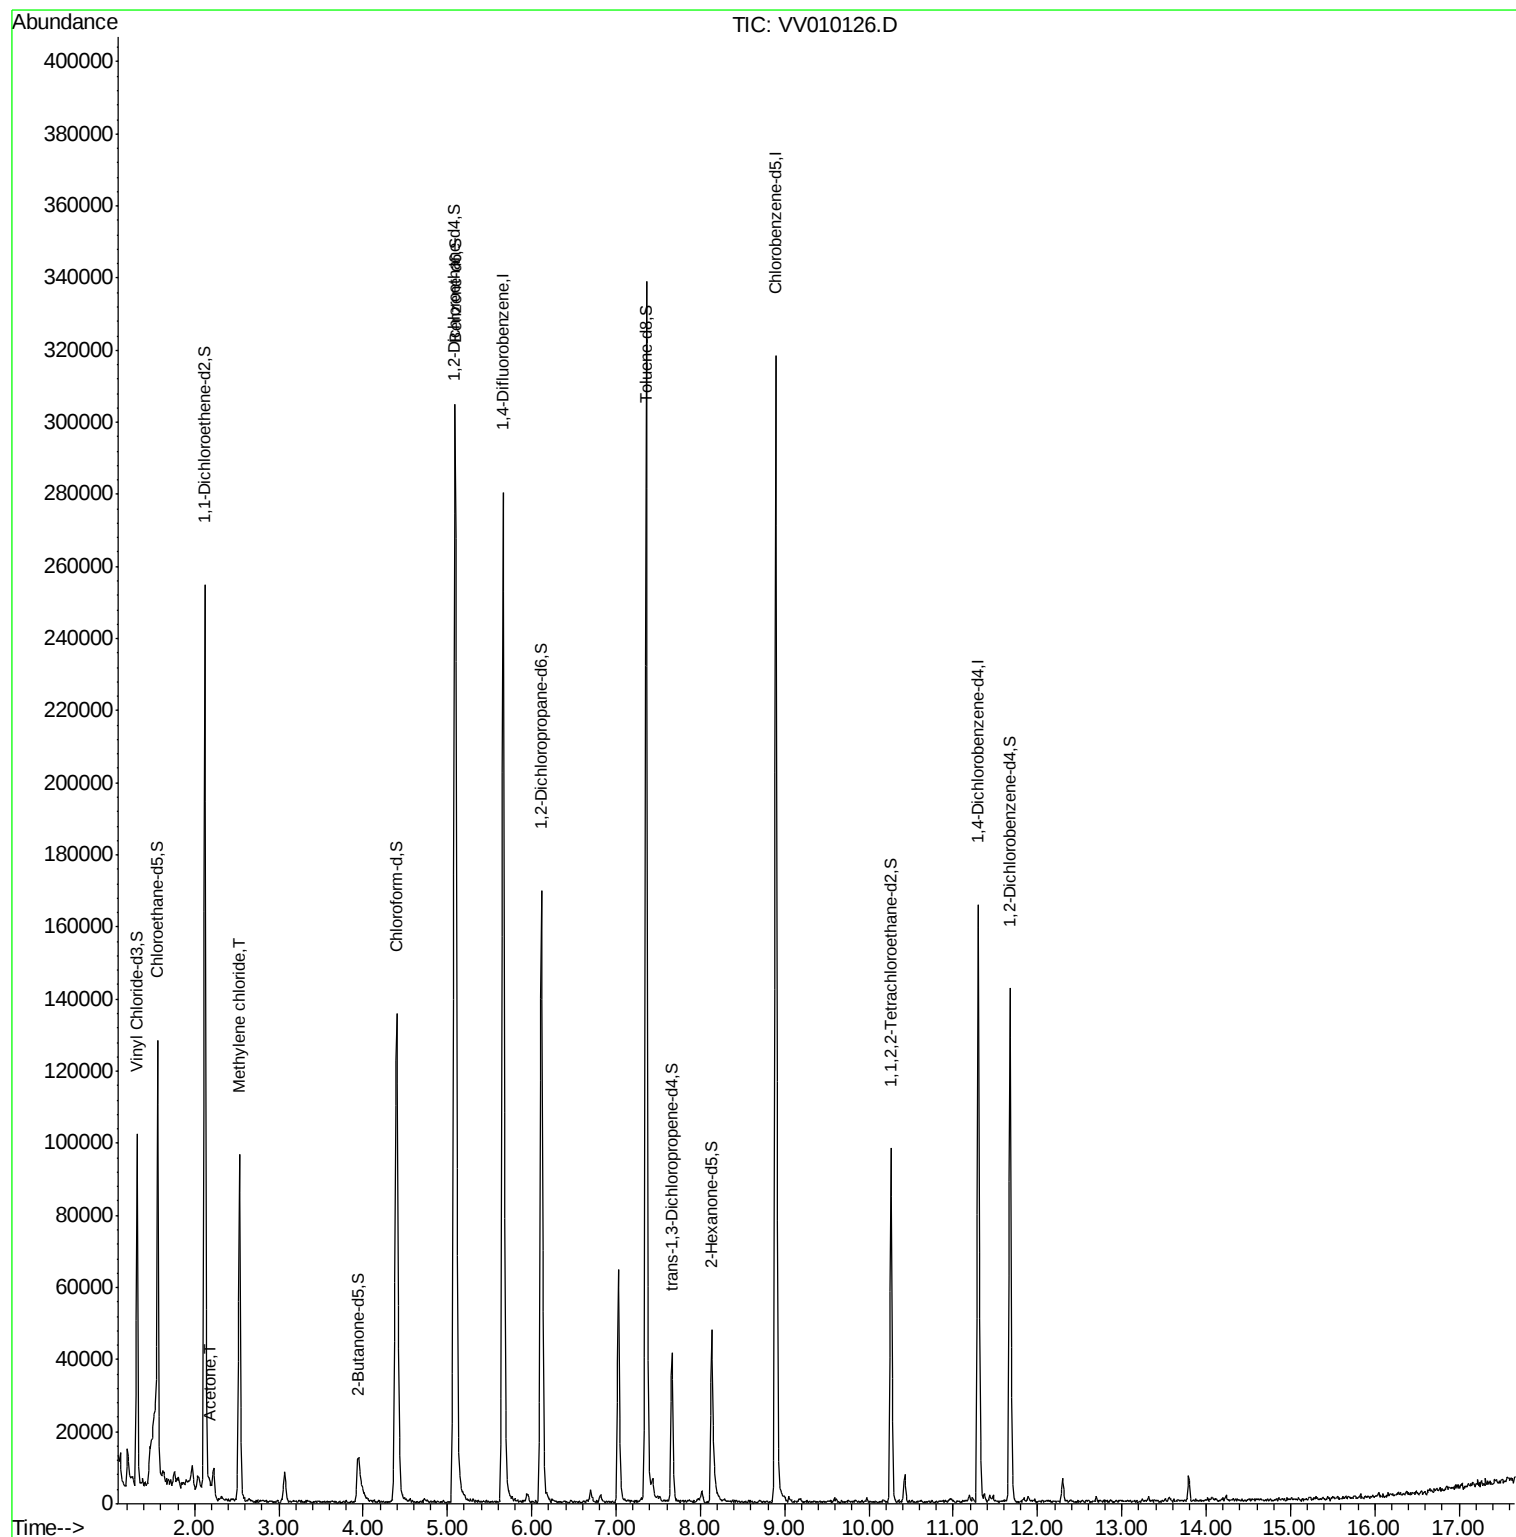

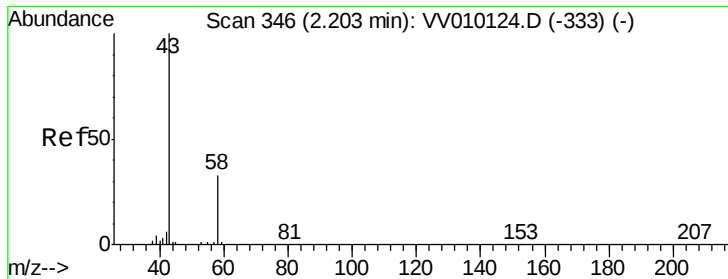

#13

Acetone

Concen: 2.588 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.01 min

Lab File: VV010126.D

Acq: 05 Apr 2019 12:18

Instrument :

MSVOA_V

ClientSampleId :

BF5G9RE

Tot Ion: 43 Resp: 2418

Ion Ratio Lower Upper

43 100


58 22.9 0.0 64.6

Manual Integrations

APPROVED

MMDadoda

4/8/2019 3:29:35 AM

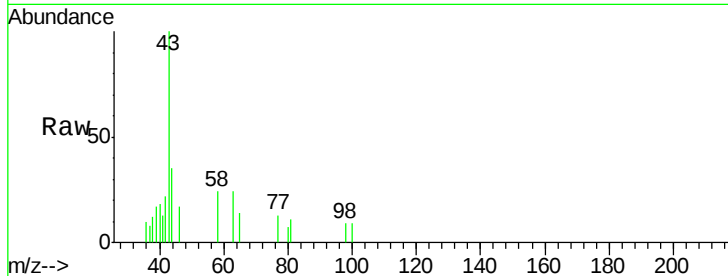

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

2.19



1500

1000

500

0

Time-->

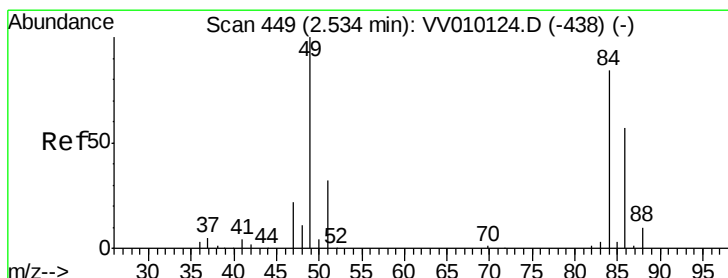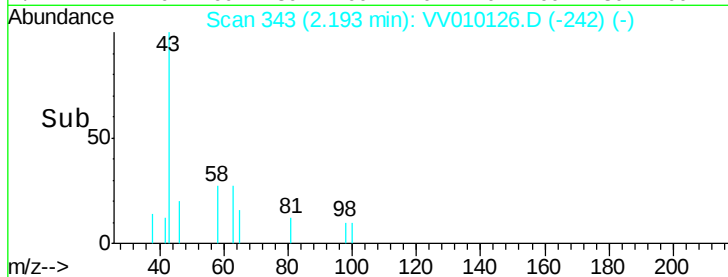

#16

Methylene chloride

Concen: 8.965 ug/L

RT: 2.53 min Scan# 449

Delta R.T. -0.00 min

Lab File: VV010126.D

Acq: 05 Apr 2019 12:18


Tgt Ion: 84 Resp: 39063

Ion Ratio Lower Upper

84 100

49 121.8 84.3 156.5

86 65.7 45.4 84.2

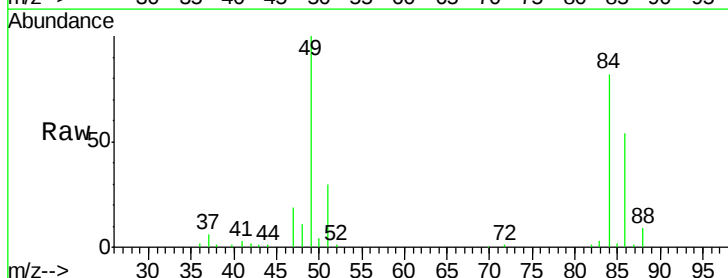

Abundance Ion 84.00 (83.70 to 84.70): VV0

Ion 49.00 (48.70 to 49.70): VV0

Ion 86.00 (85.70 to 86.70): VV0

40000

30000

20000

10000

0

Time-->

