

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020910.D
 Acq On : 05 Apr 2021 13:19
 Operator : SY/MD
 Sample : VV0415WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK90

Quant Time: Apr 06 06:22:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 06 06:22:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	615891	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	587630	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.256	152	303940	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	172412	39.43	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.86%		
7) Chloroethane-d5	1.571	69	139744	42.27	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.54%		
11) 1,1-Dichloroethene-d2	2.108	63	271817	32.95	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.90%		
21) 2-Butanone-d5	3.902	46	250446	88.04	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	88.04%		
24) Chloroform-d	4.352	84	415464	47.80	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.60%		
26) 1,2-Dichloroethane-d4	5.034	65	285202	49.82	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.64%		
32) Benzene-d6	5.053	84	766478	48.94	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.88%		
36) 1,2-Dichloropropane-d6	6.072	67	225263	46.84	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.68%		
41) Toluene-d8	7.320	98	735703	50.46	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.92%		
43) trans-1,3-Dichloroprop...	7.625	79	124216	48.55	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.10%		
47) 2-Hexanone-d5	8.092	63	176507	87.55	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.55%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	304912	43.53	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.06%		
64) 1,2-Dichlorobenzene-d4	11.632	152	318357	53.97	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	107.94%		
Target Compounds						Qvalue
59) 1,2,3-Trichloropropane	11.252	75	25858	4.66	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020910.D
Acq On : 05 Apr 2021 13:19
Operator : SY/MD
Sample : VV0415WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK90


Quant Time: Apr 06 06:22:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 06 06:22:01 2021
Response via : Initial Calibration

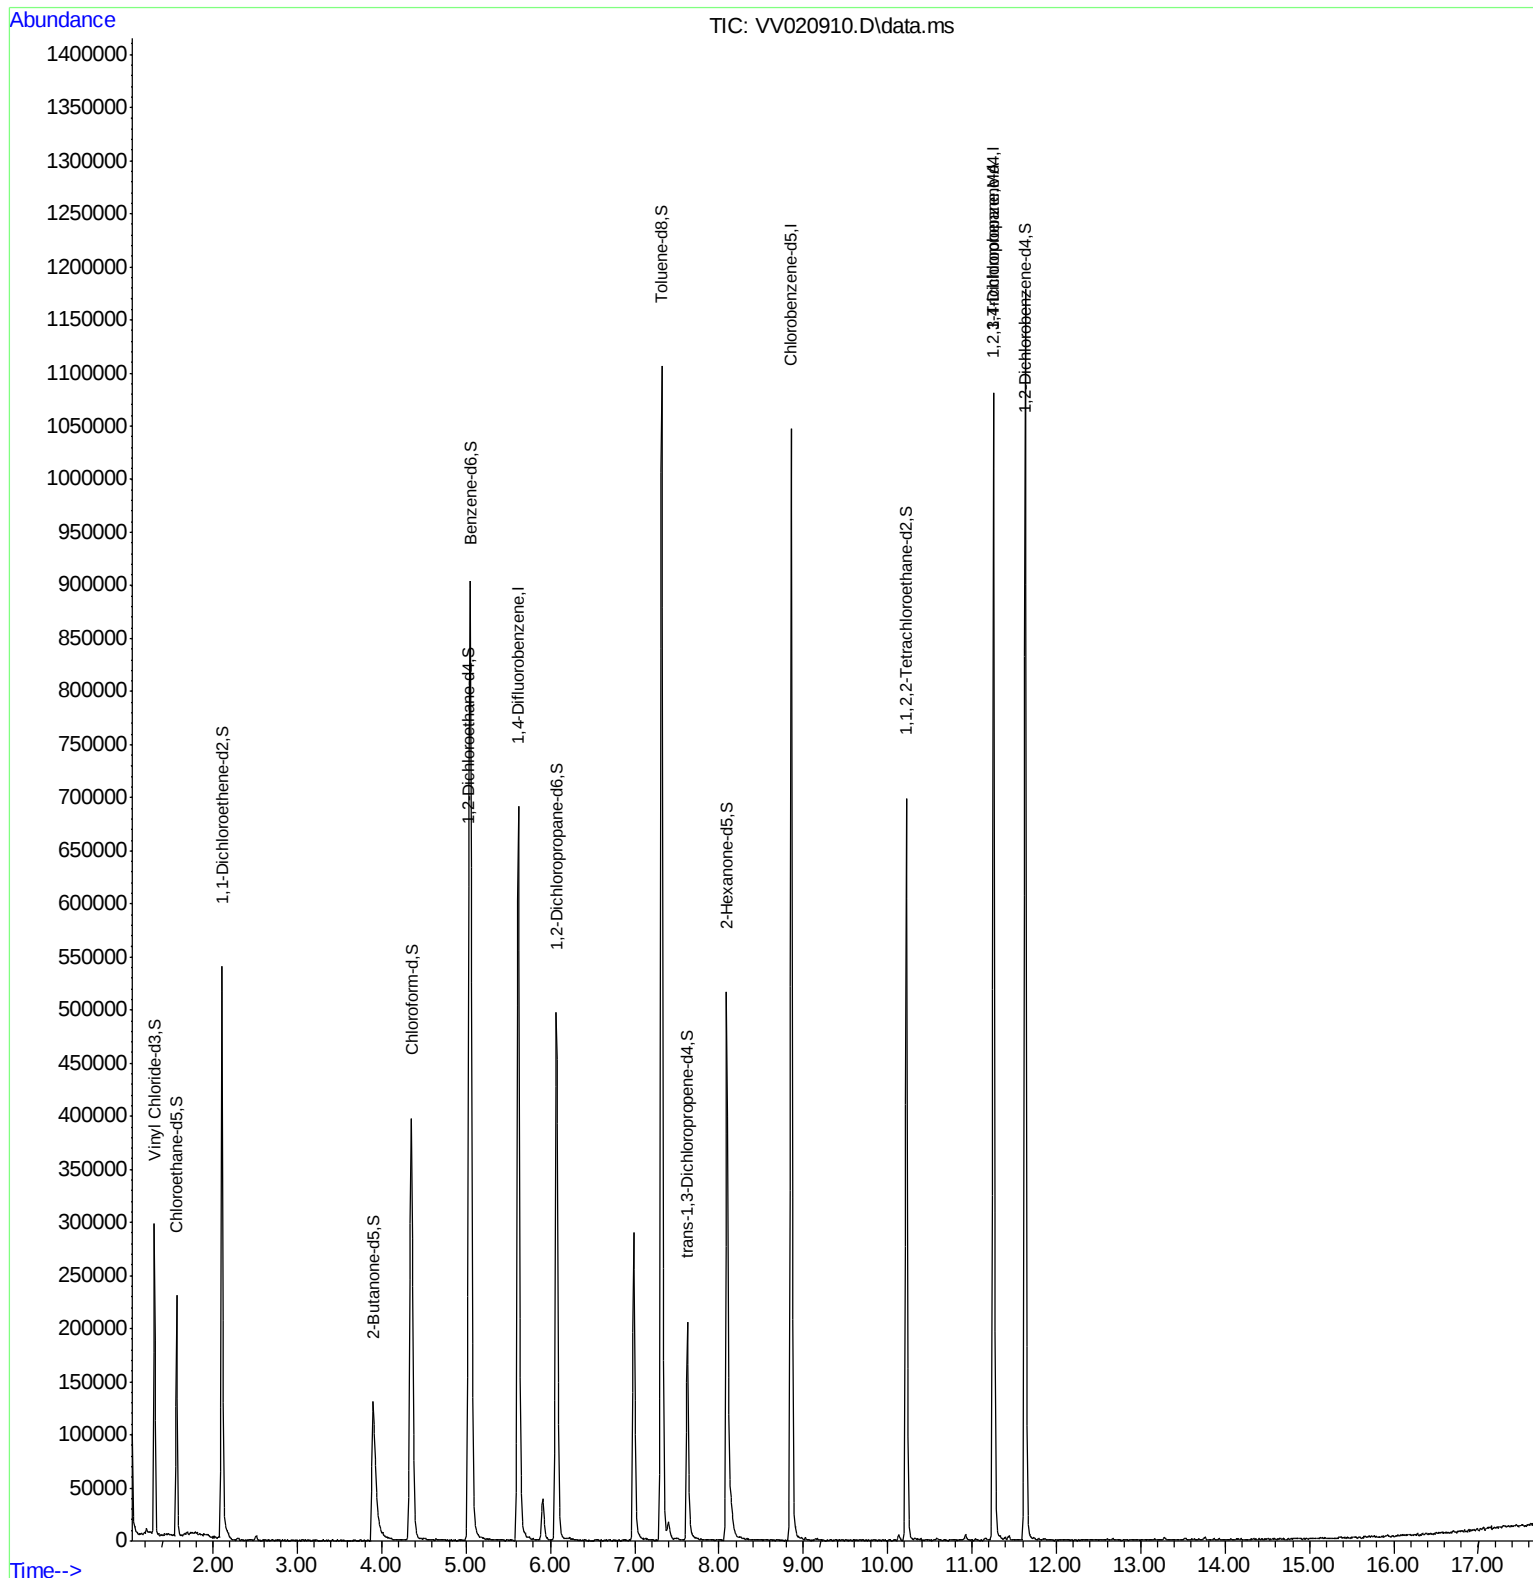

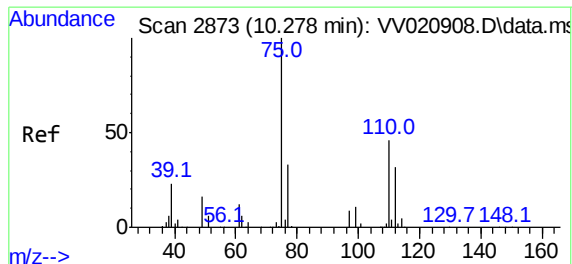

#59
 1,2,3-Trichloropropane
 Concen: 4.66 ug/L
 RT: 11.252 min Scan# 3176
 Delta R.T. 0.974 min
 Lab File: VV020910.D
 Acq: 05 Apr 2021 13:19

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK90

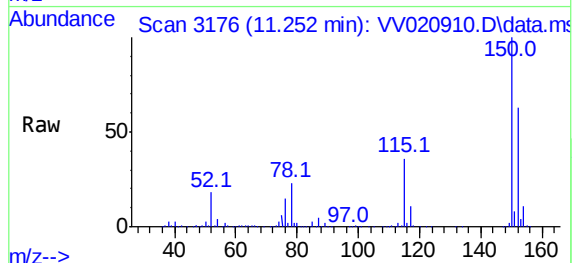

Tgt Ion: 75 Resp: 25858
 Ion Ratio Lower Upper
 75 100
 77 37.2 25.3 37.9

