

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020923.D
 Acq On : 05 Apr 2021 18:31
 Operator : SY/MD
 Sample : M1845-19DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	101	rVB2	338734	363575	16.61%	1.794%
2	1.571	158	165	183	rVB	218026	251092	11.47%	1.239%
3	2.108	322	332	344	rBV	502791	720919	32.93%	3.557%
4	2.423	425	430	432	rBV5	1080	931	0.04%	0.005%
5	2.510	450	457	470	rVB5	5759	9180	0.42%	0.045%
6	2.590	480	482	487	rVB2	616	543	0.02%	0.003%
7	2.626	489	493	496	rBV2	1047	568	0.03%	0.003%
8	2.648	496	500	502	rBV3	691	465	0.02%	0.002%
9	2.722	521	523	527	rVB2	662	395	0.02%	0.002%
10	2.764	527	536	542	rBV6	2540	4136	0.19%	0.020%
11	2.905	577	580	582	rVB	406	208	0.01%	0.001%
12	3.076	631	633	636	rBV	370	237	0.01%	0.001%
13	3.101	640	641	643	rVV2	382	203	0.01%	0.001%
14	3.127	647	649	651	rVV2	491	218	0.01%	0.001%
15	3.153	655	657	660	rBV2	464	273	0.01%	0.001%
16	3.285	696	698	699	rBV	438	204	0.01%	0.001%
17	3.330	708	712	713	rBV	369	211	0.01%	0.001%
18	3.339	713	715	718	rVB2	571	318	0.01%	0.002%
19	3.622	800	803	809	rVB2	580	466	0.02%	0.002%
20	3.661	813	815	818	rVV2	490	216	0.01%	0.001%
21	3.690	820	824	826	rBV2	341	252	0.01%	0.001%
22	3.915	878	894	922	rBV2	620856	1649033	75.33%	8.136%
23	4.352	1015	1030	1060	rVB2	378580	936802	42.79%	4.622%
24	4.635	1112	1118	1120	rBV5	1259	1228	0.06%	0.006%
25	4.783	1160	1164	1167	rVB3	746	496	0.02%	0.002%
26	4.950	1214	1216	1220	rBV3	381	326	0.01%	0.002%
27	5.050	1229	1247	1278	rBV2	845927	2189114	100.00%	10.801%
28	5.474	1376	1379	1382	rBV2	887	581	0.03%	0.003%
29	5.500	1382	1387	1390	rBV5	821	939	0.04%	0.005%
30	5.535	1396	1398	1399	rBV	561	196	0.01%	0.001%
31	5.619	1412	1424	1456	rBV	725312	1459163	66.66%	7.199%
32	5.825	1486	1488	1490	rBV	575	205	0.01%	0.001%
33	5.847	1493	1495	1497	rBV3	946	489	0.02%	0.002%
34	5.918	1502	1517	1544	rBV	1036066	2060425	94.12%	10.166%
35	6.072	1553	1565	1587	rVB	462533	930028	42.48%	4.589%
36	6.394	1661	1665	1671	rBV5	1010	1120	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020923.D
 Acq On : 05 Apr 2021 18:31
 Operator : SY/MD
 Sample : M1845-19DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.420	1671	1673	1674	rBV	744	273	0.01%	0.001%
38	6.471	1686	1689	1693	rVB4	812	648	0.03%	0.003%
39	6.494	1693	1696	1699	rBV3	690	570	0.03%	0.003%
40	6.587	1721	1725	1728	rBV3	835	715	0.03%	0.004%
41	6.651	1743	1745	1746	rBV3	575	205	0.01%	0.001%
42	6.780	1782	1785	1790	rVB3	844	477	0.02%	0.002%
43	6.812	1790	1795	1798	rBV4	866	788	0.04%	0.004%
44	6.860	1807	1810	1814	rBV4	555	491	0.02%	0.002%
45	6.989	1838	1850	1876	rBV	279577	504295	23.04%	2.488%
46	7.130	1892	1894	1900	rVB6	1224	811	0.04%	0.004%
47	7.178	1907	1909	1912	rBV2	1007	509	0.02%	0.003%
48	7.320	1940	1953	1971	rBV	1045603	1786804	81.62%	8.816%
49	7.625	2038	2048	2071	rBV	192554	333756	15.25%	1.647%
50	8.031	2172	2174	2177	rVV4	688	398	0.02%	0.002%
51	8.095	2184	2194	2234	rBV	425660	861252	39.34%	4.249%
52	8.439	2299	2301	2305	rVB3	1152	758	0.03%	0.004%
53	8.571	2340	2342	2345	rBV	749	576	0.03%	0.003%
54	8.661	2367	2370	2376	rBV4	460	511	0.02%	0.003%
55	8.686	2376	2378	2381	rBV3	512	309	0.01%	0.002%
56	8.857	2419	2431	2451	rBV	1073467	1729610	79.01%	8.534%
57	9.108	2507	2509	2513	rVB2	565	322	0.01%	0.002%
58	9.153	2513	2523	2529	rBV9	1929	3449	0.16%	0.017%
59	9.227	2543	2546	2548	rVB3	912	479	0.02%	0.002%
60	9.304	2565	2570	2571	rBV	814	514	0.02%	0.003%
61	9.400	2598	2600	2603	rVB	667	279	0.01%	0.001%
62	9.420	2603	2606	2607	rBV2	593	326	0.01%	0.002%
63	9.612	2664	2666	2669	rBV2	542	332	0.02%	0.002%
64	9.735	2700	2704	2706	rVB3	647	440	0.02%	0.002%
65	9.747	2706	2708	2712	rBV2	302	229	0.01%	0.001%
66	9.802	2721	2725	2730	rBV3	487	509	0.02%	0.003%
67	9.850	2738	2740	2741	rBV	788	287	0.01%	0.001%
68	9.892	2750	2753	2756	rBV3	348	264	0.01%	0.001%
69	9.969	2775	2777	2780	rBV2	472	255	0.01%	0.001%
70	10.014	2789	2791	2792	rBV2	774	323	0.01%	0.002%
71	10.027	2793	2795	2799	rVB2	996	638	0.03%	0.003%
72	10.130	2819	2827	2837	rVB5	5046	7272	0.33%	0.036%
73	10.220	2844	2855	2872	rBV	663844	1036511	47.35%	5.114%
74	10.506	2941	2944	2948	rBV3	567	559	0.03%	0.003%
75	10.664	2989	2993	2998	rBV4	845	772	0.04%	0.004%
76	10.712	3005	3008	3009	rBV	325	210	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020923.D
 Acq On : 05 Apr 2021 18:31
 Operator : SY/MD
 Sample : M1845-19DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.918	3066	3072	3085	rVB9	4753	8014	0.37%	0.040%
78	10.973	3086	3089	3091	rBV2	829	491	0.02%	0.002%
79	11.011	3099	3101	3104	rBV3	529	427	0.02%	0.002%
80	11.066	3116	3118	3124	rVB2	587	444	0.02%	0.002%
81	11.095	3124	3127	3133	rVB2	710	649	0.03%	0.003%
82	11.127	3134	3137	3140	rBV2	950	703	0.03%	0.003%
83	11.149	3140	3144	3151	rVB5	1485	1835	0.08%	0.009%
84	11.255	3165	3177	3197	rBV	1082794	1683512	76.90%	8.306%
85	11.574	3274	3276	3279	rBV3	914	569	0.03%	0.003%
86	11.632	3282	3294	3317	rVV	1070474	1696930	77.52%	8.372%
87	11.989	3403	3405	3411	rVB2	746	619	0.03%	0.003%
88	12.268	3490	3492	3493	rBV	757	290	0.01%	0.001%
89	12.300	3500	3502	3506	rVB3	954	505	0.02%	0.002%
90	12.345	3513	3516	3520	rBV	561	458	0.02%	0.002%
91	12.445	3544	3547	3551	rBV3	863	605	0.03%	0.003%
92	12.657	3611	3613	3618	rBV5	635	548	0.03%	0.003%
93	12.709	3625	3629	3633	rBV2	759	722	0.03%	0.004%
94	12.747	3638	3641	3642	rBV	510	316	0.01%	0.002%
95	12.966	3702	3709	3713	rBV3	1224	1276	0.06%	0.006%
96	13.017	3722	3725	3726	rBV	740	452	0.02%	0.002%
97	13.744	3946	3951	3954	rBV2	1004	740	0.03%	0.004%
98	14.050	4045	4046	4047	rBV	697	255	0.01%	0.001%
99	14.124	4066	4069	4072	rBV3	859	795	0.04%	0.004%
100	15.599	4525	4528	4532	rBV	7691	4502	0.21%	0.022%



Sum of corrected areas: 20268138

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020923.D
Acq On : 05 Apr 2021 18:31
Operator : SY/MD
Sample : M1845-19DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

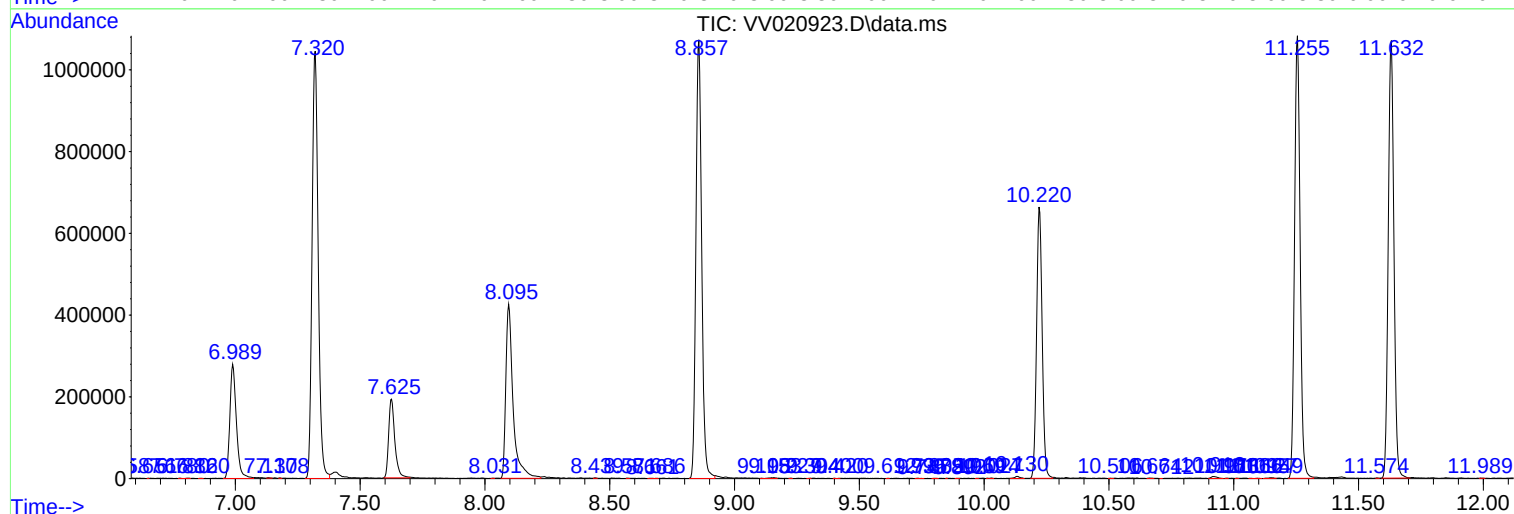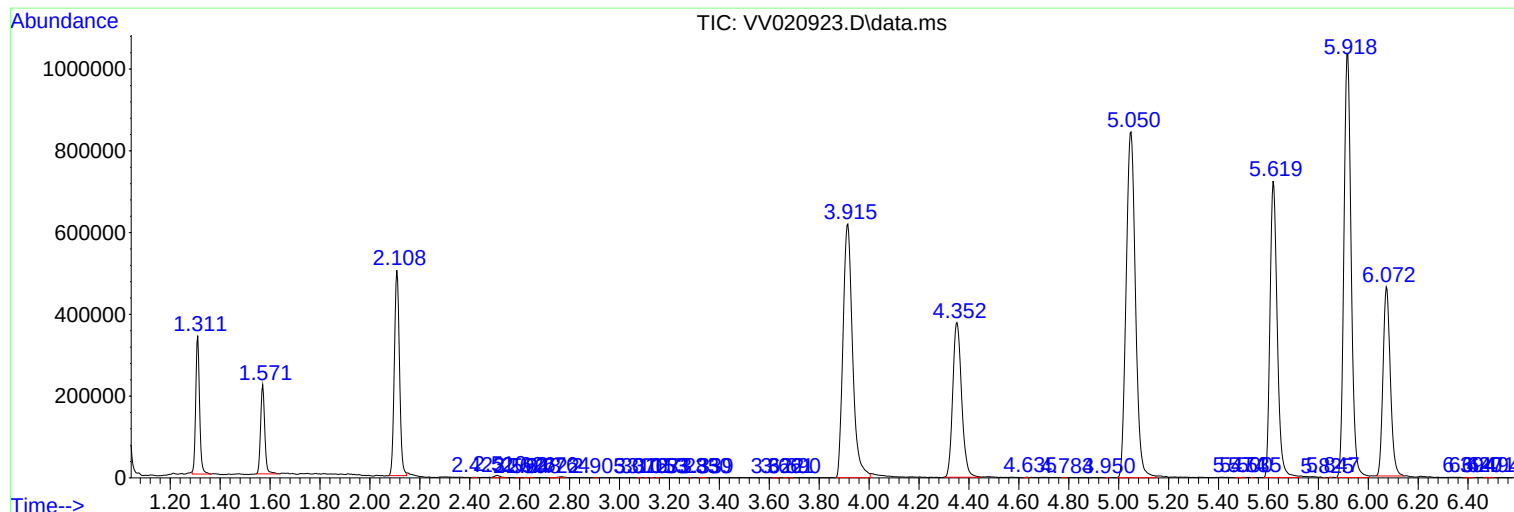

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020923.D
Acq On : 05 Apr 2021 18:31
Operator : SY/MD
Sample : M1845-19DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020923.D
Acq On : 05 Apr 2021 18:31
Operator : SY/MD
Sample : M1845-19DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
