

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020924.D
 Acq On : 05 Apr 2021 18:55
 Operator : SY/MD
 Sample : M1845-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	102	rVB2	1257036	1314210	58.75%	6.713%
2	1.571	158	165	176	rVB	193415	215238	9.62%	1.099%
3	2.108	322	332	355	rBV2	463515	697220	31.17%	3.561%
4	2.372	412	414	419	rVB2	778	415	0.02%	0.002%
5	2.548	468	469	471	rBV2	546	245	0.01%	0.001%
6	2.693	511	514	515	rBV2	406	232	0.01%	0.001%
7	2.764	529	536	544	rBV3	6414	10235	0.46%	0.052%
8	2.960	590	597	600	rBV5	1615	2062	0.09%	0.011%
9	3.005	608	611	613	rBV	583	449	0.02%	0.002%
10	3.050	622	625	626	rBV	255	176	0.01%	0.001%
11	3.098	633	640	645	rVB	406	539	0.02%	0.003%
12	3.130	645	650	656	rBV3	943	1033	0.05%	0.005%
13	3.169	660	662	666	rBV4	608	506	0.02%	0.003%
14	3.272	692	694	696	rBV	558	281	0.01%	0.001%
15	3.323	707	710	712	rVV	317	197	0.01%	0.001%
16	3.352	717	719	721	rVV2	651	284	0.01%	0.001%
17	3.449	743	749	750	rBV2	645	567	0.03%	0.003%
18	3.580	788	790	792	rBV2	568	247	0.01%	0.001%
19	3.671	815	818	821	rBV	425	323	0.01%	0.002%
20	3.735	836	838	840	rVB2	597	196	0.01%	0.001%
21	3.751	840	843	845	rBV4	720	553	0.02%	0.003%
22	3.780	849	852	854	rVB2	685	341	0.02%	0.002%
23	3.812	858	862	864	rBV2	705	448	0.02%	0.002%
24	3.831	865	868	876	rVB5	1351	1588	0.07%	0.008%
25	3.912	876	893	938	rBV2	848533	2237010	100.00%	11.426%
26	4.352	1015	1030	1058	rVB2	360346	890589	39.81%	4.549%
27	4.600	1104	1107	1110	rBV	1054	818	0.04%	0.004%
28	4.658	1121	1125	1129	rBV5	841	785	0.04%	0.004%
29	4.831	1176	1179	1182	rBV3	857	453	0.02%	0.002%
30	4.905	1200	1202	1205	rBV	287	226	0.01%	0.001%
31	5.047	1229	1246	1280	rBV2	804129	2076447	92.82%	10.606%
32	5.494	1380	1385	1388	rBV2	640	608	0.03%	0.003%
33	5.532	1394	1397	1400	rBV	872	625	0.03%	0.003%
34	5.619	1412	1424	1460	rBV	688764	1375356	61.48%	7.025%
35	5.918	1503	1517	1533	rBV4	129452	285178	12.75%	1.457%
36	6.072	1552	1565	1592	rBV2	437150	898570	40.17%	4.590%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020924.D
 Acq On : 05 Apr 2021 18:55
 Operator : SY/MD
 Sample : M1845-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.394	1664	1665	1668	rBV	700	360	0.02%	0.002%
38	6.474	1688	1690	1692	rBV2	489	225	0.01%	0.001%
39	6.686	1751	1756	1758	rBV3	988	945	0.04%	0.005%
40	6.789	1785	1788	1790	rVB2	832	374	0.02%	0.002%
41	6.805	1790	1793	1796	rBV2	802	535	0.02%	0.003%
42	6.834	1798	1802	1804	rVB	466	294	0.01%	0.002%
43	6.857	1804	1809	1813	rBV5	736	852	0.04%	0.004%
44	6.876	1813	1815	1817	rBV2	432	174	0.01%	0.001%
45	6.989	1839	1850	1875	rBV	265235	481828	21.54%	2.461%
46	7.320	1941	1953	1970	rBV	980739	1677031	74.97%	8.566%
47	7.625	2038	2048	2067	rBV	185192	328704	14.69%	1.679%
48	7.776	2091	2095	2101	rBV6	844	1061	0.05%	0.005%
49	8.027	2170	2173	2177	rBV2	555	516	0.02%	0.003%
50	8.053	2179	2181	2184	rVB2	644	330	0.01%	0.002%
51	8.095	2184	2194	2235	rBV	472934	966618	43.21%	4.937%
52	8.545	2332	2334	2335	rBV	800	397	0.02%	0.002%
53	8.571	2341	2342	2346	rVB2	777	344	0.02%	0.002%
54	8.590	2346	2348	2353	rVB3	621	345	0.02%	0.002%
55	8.770	2402	2404	2405	rBV2	567	244	0.01%	0.001%
56	8.857	2418	2431	2457	rBV	1038001	1677634	74.99%	8.569%
57	9.117	2511	2512	2514	rBV2	689	315	0.01%	0.002%
58	9.207	2538	2540	2542	rBV2	503	291	0.01%	0.001%
59	9.297	2565	2568	2570	rBV	697	501	0.02%	0.003%
60	9.313	2571	2573	2575	rVB2	765	325	0.01%	0.002%
61	9.342	2580	2582	2584	rVB2	585	256	0.01%	0.001%
62	9.558	2645	2649	2650	rBV2	530	454	0.02%	0.002%
63	9.609	2662	2665	2666	rBV2	558	328	0.01%	0.002%
64	9.638	2672	2674	2676	rVB	385	171	0.01%	0.001%
65	9.657	2676	2680	2683	rBV2	601	507	0.02%	0.003%
66	9.693	2688	2691	2696	rVB4	770	611	0.03%	0.003%
67	9.738	2703	2705	2708	rBV4	829	571	0.03%	0.003%
68	9.773	2713	2716	2717	rBV	430	230	0.01%	0.001%
69	9.825	2729	2732	2736	rBV4	938	669	0.03%	0.003%
70	9.911	2753	2759	2761	rBV4	759	754	0.03%	0.004%
71	9.995	2783	2785	2789	rBV3	505	309	0.01%	0.002%
72	10.050	2799	2802	2803	rBV	375	244	0.01%	0.001%
73	10.101	2814	2818	2819	rBV3	905	614	0.03%	0.003%
74	10.175	2839	2841	2843	rBV	425	219	0.01%	0.001%
75	10.223	2843	2856	2874	rVV	682700	1075804	48.09%	5.495%
76	10.509	2943	2945	2946	rVB2	731	234	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020924.D
 Acq On : 05 Apr 2021 18:55
 Operator : SY/MD
 Sample : M1845-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.519	2946	2948	2950	rBV2	725	445	0.02%	0.002%
78	10.554	2957	2959	2962	rBV3	699	410	0.02%	0.002%
79	10.648	2986	2988	2994	rBV2	600	523	0.02%	0.003%
80	10.693	2997	3002	3004	rBV3	930	855	0.04%	0.004%
81	10.780	3025	3029	3030	rBV3	797	586	0.03%	0.003%
82	10.995	3093	3096	3101	rVB2	819	647	0.03%	0.003%
83	11.114	3130	3133	3134	rBV2	638	287	0.01%	0.001%
84	11.255	3165	3177	3197	rBV	1060549	1632217	72.96%	8.337%
85	11.538	3258	3265	3279	rBV4	21650	39044	1.75%	0.199%
86	11.632	3282	3294	3319	rVB	1049296	1659855	74.20%	8.478%
87	11.760	3332	3334	3335	rBV2	1169	514	0.02%	0.003%
88	11.927	3384	3386	3388	rBV2	936	453	0.02%	0.002%
89	12.034	3416	3419	3421	rBV3	826	431	0.02%	0.002%
90	12.323	3507	3509	3510	rBV3	784	240	0.01%	0.001%
91	12.355	3516	3519	3524	rBV4	1431	959	0.04%	0.005%
92	12.561	3581	3583	3585	rBV2	727	290	0.01%	0.001%
93	12.802	3656	3658	3660	rBV2	713	420	0.02%	0.002%
94	12.873	3678	3680	3685	rBV4	1047	958	0.04%	0.005%
95	12.902	3686	3689	3691	rBV4	1007	645	0.03%	0.003%
96	12.976	3710	3712	3714	rBV2	623	299	0.01%	0.002%
97	13.030	3728	3729	3731	rBV2	496	237	0.01%	0.001%
98	13.387	3837	3840	3842	rBV3	1038	801	0.04%	0.004%
99	13.638	3916	3918	3920	rBV2	1101	581	0.03%	0.003%
100	13.741	3948	3950	3952	rBV	660	321	0.01%	0.002%




Sum of corrected areas: 19578486

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020924.D
Acq On : 05 Apr 2021 18:55
Operator : SY/MD
Sample : M1845-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

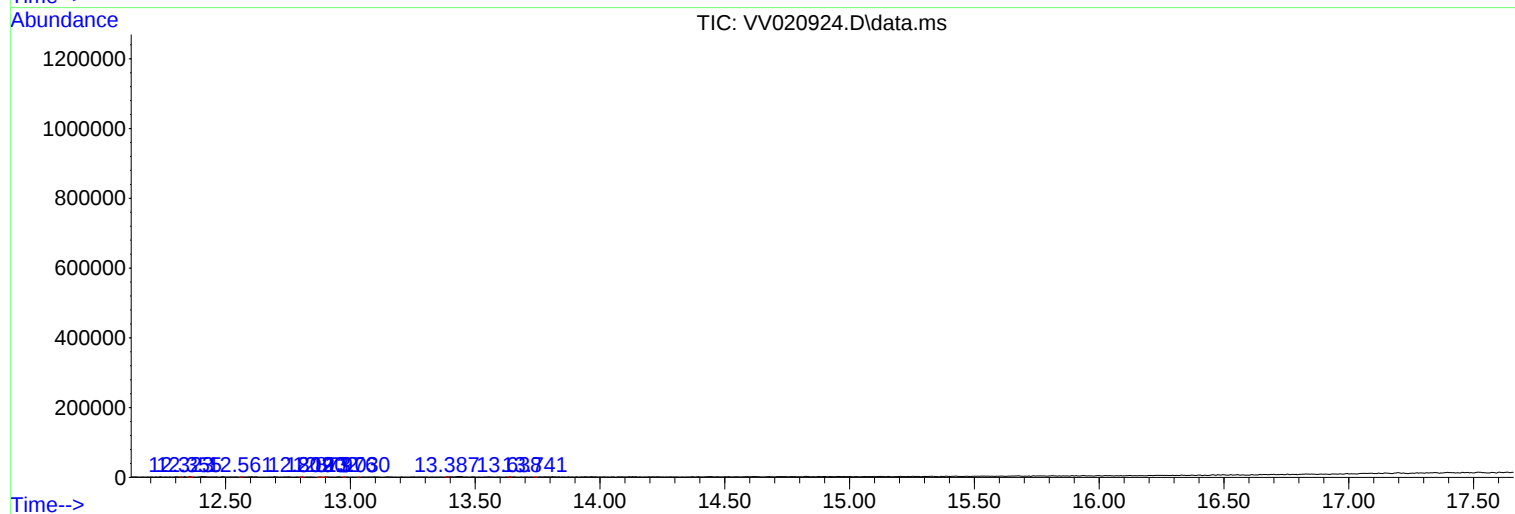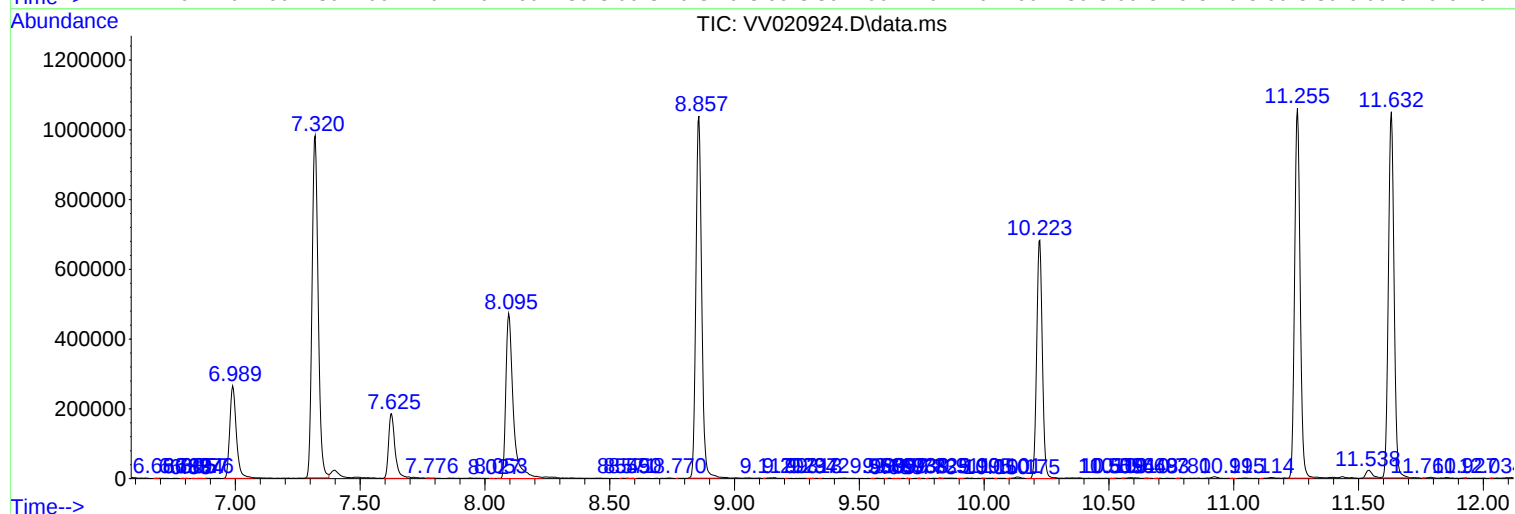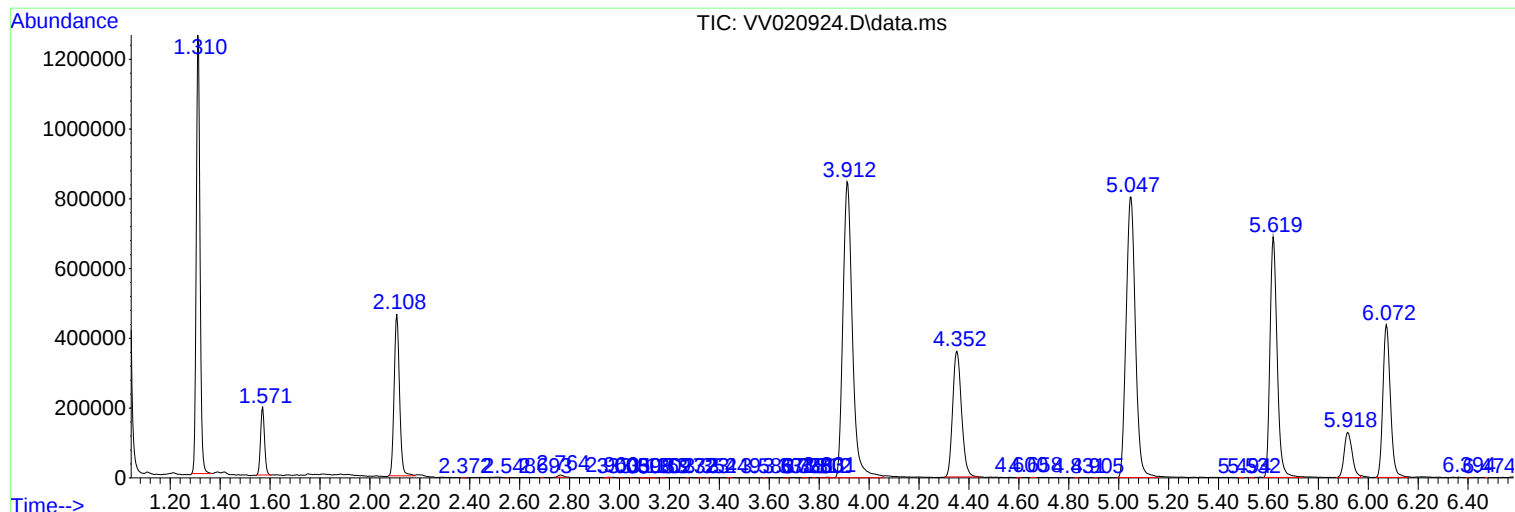

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020924.D
Acq On : 05 Apr 2021 18:55
Operator : SY/MD
Sample : M1845-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020924.D
Acq On : 05 Apr 2021 18:55
Operator : SY/MD
Sample : M1845-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
