

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020928.D
 Acq On : 05 Apr 2021 20:31
 Operator : SY/MD
 Sample : M1880-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	97	rVB	256872	261818	12.23%	1.584%
2	1.571	158	165	178	rVB	213304	235581	11.00%	1.425%
3	2.108	323	332	361	rVB	486734	722043	33.73%	4.368%
4	2.738	524	528	531	rVV3	593	459	0.02%	0.003%
5	2.754	531	533	535	rVV	693	332	0.02%	0.002%
6	2.767	535	537	542	rVB2	931	494	0.02%	0.003%
7	2.851	561	563	564	rBV	283	111	0.01%	0.001%
8	2.995	606	608	609	rBV	325	137	0.01%	0.001%
9	3.092	636	638	641	rBV	341	206	0.01%	0.001%
10	3.143	652	654	658	rVV2	527	305	0.01%	0.002%
11	3.178	662	665	668	rBV2	531	369	0.02%	0.002%
12	3.400	730	734	735	rBV	560	396	0.02%	0.002%
13	3.471	754	756	758	rBV	392	251	0.01%	0.002%
14	3.548	775	780	784	rBV2	536	552	0.03%	0.003%
15	3.590	791	793	795	rBV	315	131	0.01%	0.001%
16	3.619	800	802	807	rBV2	342	221	0.01%	0.001%
17	3.693	824	825	826	rBV2	107	26	0.00%	0.000%
18	3.699	826	827	828	rBV2	410	137	0.01%	0.001%
19	3.748	834	842	844	rBV3	1015	984	0.05%	0.006%
20	3.764	844	847	852	rVB2	756	463	0.02%	0.003%
21	3.818	862	864	867	rVB	642	282	0.01%	0.002%
22	3.841	869	871	874	rBV	431	283	0.01%	0.002%
23	3.899	879	889	919	rBV	106100	356485	16.65%	2.156%
24	4.352	1013	1030	1055	rBV	375982	944507	44.12%	5.713%
25	4.715	1141	1143	1145	rBV2	495	148	0.01%	0.001%
26	4.815	1171	1174	1177	rBV2	692	436	0.02%	0.003%
27	4.886	1191	1196	1199	rBV5	870	710	0.03%	0.004%
28	4.905	1199	1202	1208	rVB2	496	410	0.02%	0.002%
29	4.953	1211	1217	1218	rBV2	562	538	0.03%	0.003%
30	5.050	1230	1247	1276	rBV2	832680	2140972	100.00%	12.950%
31	5.227	1300	1302	1305	rBV3	871	480	0.02%	0.003%
32	5.461	1372	1375	1378	rBV	839	659	0.03%	0.004%
33	5.490	1382	1384	1385	rBV	353	142	0.01%	0.001%
34	5.619	1412	1424	1453	rBV	688617	1375134	64.23%	8.318%
35	5.915	1504	1516	1530	rBV2	27917	59361	2.77%	0.359%
36	6.072	1553	1565	1594	rBV	455072	927147	43.30%	5.608%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020928.D
 Acq On : 05 Apr 2021 20:31
 Operator : SY/MD
 Sample : M1880-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.310	1637	1639	1641	rBV3	688	363	0.02%	0.002%
38	6.503	1697	1699	1701	rBV	704	318	0.01%	0.002%
39	6.648	1740	1744	1746	rBV2	751	589	0.03%	0.004%
40	6.683	1750	1755	1762	rVB4	962	1205	0.06%	0.007%
41	6.712	1762	1764	1765	rBV	661	300	0.01%	0.002%
42	6.809	1790	1794	1796	rVB2	397	270	0.01%	0.002%
43	6.821	1796	1798	1799	rBV2	330	118	0.01%	0.001%
44	6.989	1839	1850	1876	rBV	267748	496424	23.19%	3.003%
45	7.320	1941	1953	1971	rBV	1013543	1776509	82.98%	10.746%
46	7.625	2038	2048	2066	rBV	189791	329669	15.40%	1.994%
47	8.014	2167	2169	2171	rBV2	502	237	0.01%	0.001%
48	8.095	2184	2194	2234	rBV	429531	851463	39.77%	5.150%
49	8.574	2338	2343	2346	rBV2	672	550	0.03%	0.003%
50	8.673	2372	2374	2377	rBV	469	337	0.02%	0.002%
51	8.857	2416	2431	2450	rBV	1008893	1661997	77.63%	10.053%
52	9.017	2478	2481	2486	rBV3	885	905	0.04%	0.005%
53	9.149	2520	2522	2526	rVB3	1212	698	0.03%	0.004%
54	9.268	2553	2559	2564	rBV2	713	945	0.04%	0.006%
55	9.442	2609	2613	2616	rBV3	967	753	0.04%	0.005%
56	9.497	2627	2630	2632	rBV	599	342	0.02%	0.002%
57	9.509	2632	2634	2636	rBV	351	188	0.01%	0.001%
58	9.561	2647	2650	2651	rBV	827	450	0.02%	0.003%
59	9.702	2692	2694	2695	rBV	482	132	0.01%	0.001%
60	9.815	2726	2729	2731	rBV2	899	538	0.03%	0.003%
61	9.873	2745	2747	2751	rVB2	557	334	0.02%	0.002%
62	9.976	2777	2779	2780	rBV	433	210	0.01%	0.001%
63	10.136	2819	2829	2837	rVB3	4080	6804	0.32%	0.041%
64	10.220	2844	2855	2877	rBV	656562	1031701	48.19%	6.241%
65	10.635	2981	2984	2988	rBV2	747	425	0.02%	0.003%
66	10.657	2990	2991	2993	rBV	482	162	0.01%	0.001%
67	10.738	3012	3016	3018	rBV3	755	496	0.02%	0.003%
68	10.924	3069	3074	3082	rVB7	3582	5256	0.25%	0.032%
69	11.255	3165	3177	3201	rBV	1054729	1601863	74.82%	9.689%
70	11.551	3259	3269	3276	rBV9	2593	5239	0.24%	0.032%
71	11.632	3281	3294	3316	rBV	1082915	1718349	80.26%	10.394%
72	12.046	3420	3423	3425	rBV2	585	348	0.02%	0.002%
73	12.201	3469	3471	3473	rBV	509	294	0.01%	0.002%
74	12.554	3579	3581	3585	rBV3	710	503	0.02%	0.003%
75	12.680	3617	3620	3623	rBV3	778	621	0.03%	0.004%
76	12.722	3630	3633	3636	rBV3	616	390	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020928.D
Acq On : 05 Apr 2021 20:31
Operator : SY/MD
Sample : M1880-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Title : VOC Analysis

77	12.908	3689	3691	3692	rBV3	424	167	0.01%	0.001%
78	13.011	3721	3723	3724	rBV	836	356	0.02%	0.002%
79	13.484	3867	3870	3871	rBV2	733	455	0.02%	0.003%




Sum of corrected areas: 16531983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020928.D
Acq On : 05 Apr 2021 20:31
Operator : SY/MD
Sample : M1880-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

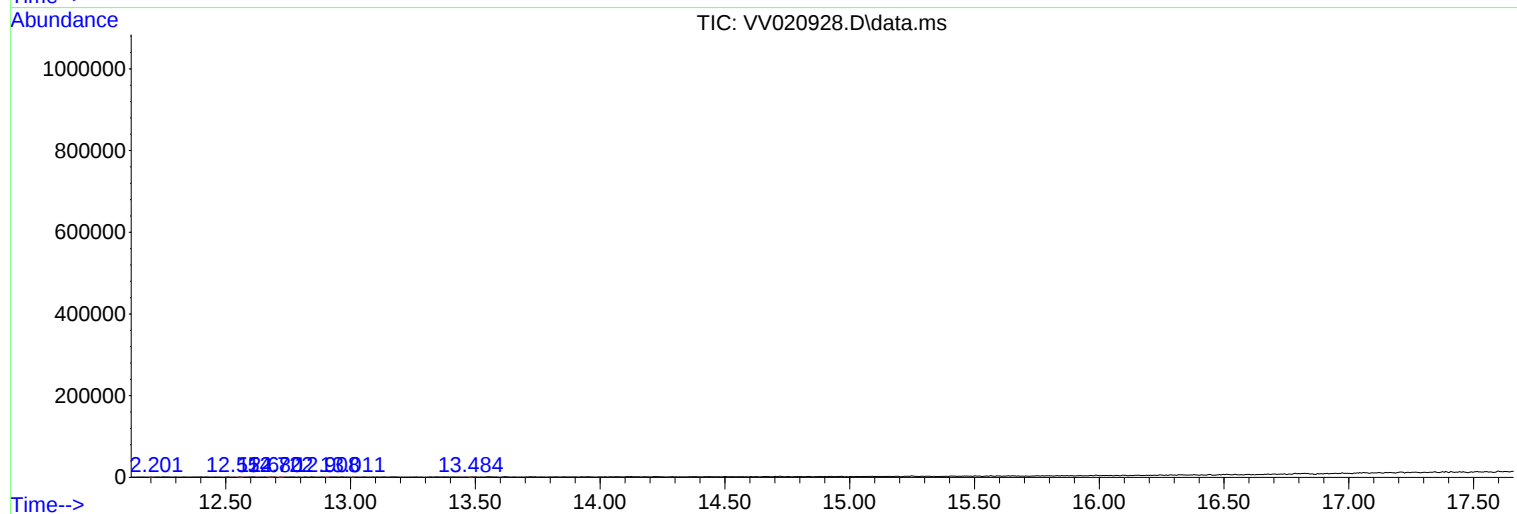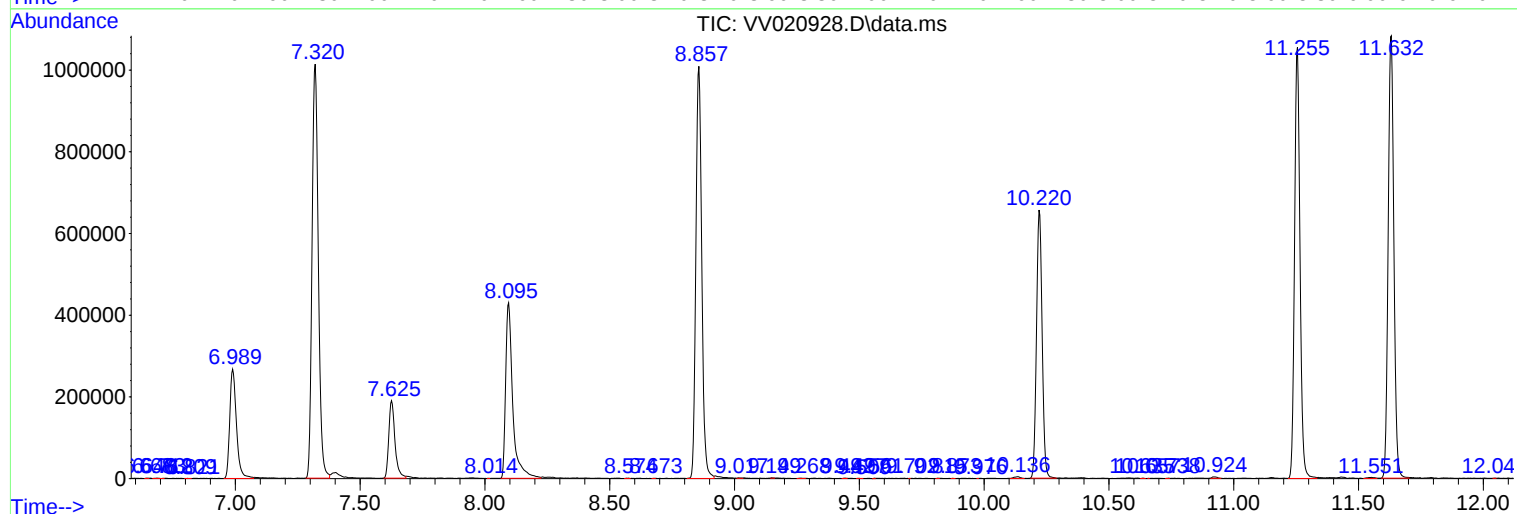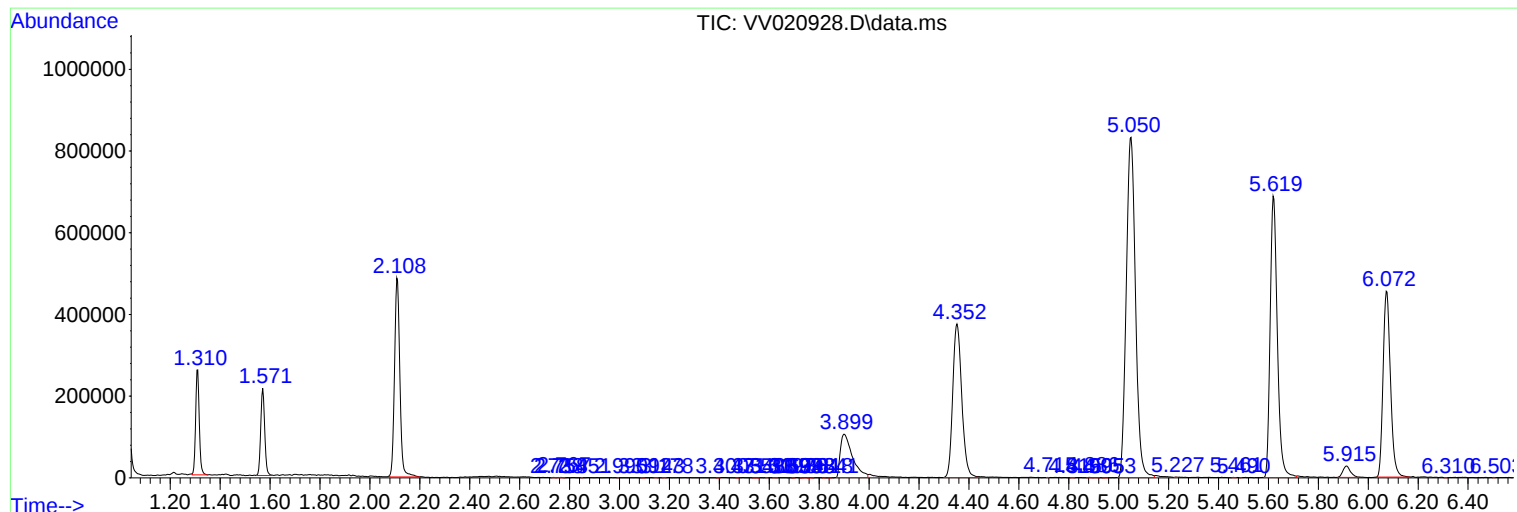

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020928.D
Acq On : 05 Apr 2021 20:31
Operator : SY/MD
Sample : M1880-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020928.D
Acq On : 05 Apr 2021 20:31
Operator : SY/MD
Sample : M1880-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
