

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020933.D
 Acq On : 05 Apr 2021 22:30
 Operator : SY/MD
 Sample : M1880-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	96	rVB2	271072	280015	12.56%	1.742%
2	1.571	158	165	177	rVB	203236	226266	10.15%	1.408%
3	2.108	322	332	370	rVB	469938	701104	31.45%	4.363%
4	2.362	409	411	413	rBV2	536	228	0.01%	0.001%
5	2.407	422	425	429	rVB3	602	371	0.02%	0.002%
6	2.426	429	431	432	rBV	580	207	0.01%	0.001%
7	2.465	440	443	448	rBV4	852	875	0.04%	0.005%
8	2.535	463	465	470	rVB3	1159	838	0.04%	0.005%
9	2.571	470	476	480	rBV2	963	897	0.04%	0.006%
10	2.683	508	511	512	rBV	571	302	0.01%	0.002%
11	2.744	527	530	531	rBV2	664	295	0.01%	0.002%
12	2.754	531	533	535	rBV2	491	253	0.01%	0.002%
13	2.850	561	563	566	rVB2	547	283	0.01%	0.002%
14	2.886	572	574	576	rBV2	433	177	0.01%	0.001%
15	3.124	646	648	649	rBV	484	124	0.01%	0.001%
16	3.198	658	671	685	rBV2	14716	31165	1.40%	0.194%
17	3.262	689	691	693	rVV	339	202	0.01%	0.001%
18	3.272	693	694	696	rVB2	808	250	0.01%	0.002%
19	3.320	704	709	711	rVB2	668	429	0.02%	0.003%
20	3.339	711	715	717	rBV2	428	358	0.02%	0.002%
21	3.381	726	728	735	rVB2	402	346	0.02%	0.002%
22	3.423	738	741	744	rVB2	437	230	0.01%	0.001%
23	3.439	744	746	748	rBV	301	110	0.00%	0.001%
24	3.455	749	751	754	rBV2	538	277	0.01%	0.002%
25	3.629	802	805	810	rBV3	726	620	0.03%	0.004%
26	3.696	825	826	827	rBV3	128	44	0.00%	0.000%
27	3.712	827	831	833	rBV	623	387	0.02%	0.002%
28	3.815	859	863	864	rBV	434	292	0.01%	0.002%
29	3.905	879	891	928	rBV2	100951	359684	16.14%	2.238%
30	4.352	1013	1030	1056	rBV2	362049	889546	39.91%	5.535%
31	4.847	1182	1184	1187	rBV3	507	337	0.02%	0.002%
32	4.934	1205	1211	1214	rBV	544	719	0.03%	0.004%
33	4.956	1216	1218	1220	rVB	366	145	0.01%	0.001%
34	4.976	1221	1224	1228	rVB3	727	342	0.02%	0.002%
35	5.050	1230	1247	1285	rBV2	799180	2228976	100.00%	13.870%
36	5.291	1318	1322	1324	rBV4	1064	768	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020933.D
 Acq On : 05 Apr 2021 22:30
 Operator : SY/MD
 Sample : M1880-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.471	1373	1378	1382	rBV4	1037	1200	0.05%	0.007%
38	5.551	1397	1403	1408	rBV5	1111	1243	0.06%	0.008%
39	5.571	1408	1409	1411	rBV2	480	195	0.01%	0.001%
40	5.619	1412	1424	1461	rBV	660679	1325324	59.46%	8.247%
41	5.911	1506	1515	1530	rBV3	20216	39632	1.78%	0.247%
42	5.995	1538	1541	1544	rBV4	826	782	0.04%	0.005%
43	6.072	1551	1565	1591	rBV	429494	897405	40.26%	5.584%
44	6.288	1630	1632	1638	rBV3	715	449	0.02%	0.003%
45	6.374	1657	1659	1665	rBV2	717	558	0.03%	0.003%
46	6.400	1665	1667	1672	rVB2	496	325	0.01%	0.002%
47	6.429	1672	1676	1680	rBV4	811	736	0.03%	0.005%
48	6.490	1691	1695	1697	rBV2	618	484	0.02%	0.003%
49	6.574	1719	1721	1729	rVB4	706	722	0.03%	0.004%
50	6.651	1741	1745	1751	rBV3	989	1054	0.05%	0.007%
51	6.709	1760	1763	1764	rBV	364	173	0.01%	0.001%
52	6.989	1838	1850	1876	rBV	256476	471648	21.16%	2.935%
53	7.162	1902	1904	1907	rBV2	623	299	0.01%	0.002%
54	7.320	1938	1953	1972	rBV	974607	1686455	75.66%	10.494%
55	7.625	2038	2048	2067	rBV	176786	310483	13.93%	1.932%
56	7.931	2141	2143	2146	rBV3	815	576	0.03%	0.004%
57	8.095	2183	2194	2224	rBV	409612	797375	35.77%	4.962%
58	8.480	2312	2314	2318	rVB2	876	525	0.02%	0.003%
59	8.551	2332	2336	2337	rBV2	695	447	0.02%	0.003%
60	8.577	2343	2344	2349	rVB2	325	238	0.01%	0.001%
61	8.609	2351	2354	2356	rVV2	633	309	0.01%	0.002%
62	8.657	2367	2369	2370	rBV	356	112	0.01%	0.001%
63	8.731	2390	2392	2394	rBV	412	220	0.01%	0.001%
64	8.857	2417	2431	2462	rBV	983647	1605045	72.01%	9.988%
65	9.210	2537	2541	2547	rBV3	893	937	0.04%	0.006%
66	9.278	2560	2562	2564	rBV2	741	352	0.02%	0.002%
67	9.406	2599	2602	2606	rBV2	599	516	0.02%	0.003%
68	9.554	2644	2648	2651	rBV2	750	547	0.02%	0.003%
69	9.599	2660	2662	2665	rVB2	661	294	0.01%	0.002%
70	9.619	2665	2668	2670	rBV2	733	450	0.02%	0.003%
71	9.734	2702	2704	2707	rBV	473	290	0.01%	0.002%
72	9.879	2747	2749	2751	rBV2	429	236	0.01%	0.001%
73	9.937	2765	2767	2769	rBV	353	175	0.01%	0.001%
74	10.001	2784	2787	2791	rVB2	595	483	0.02%	0.003%
75	10.053	2800	2803	2806	rBV2	329	188	0.01%	0.001%
76	10.220	2843	2855	2878	rBV	645500	1009119	45.27%	6.279%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020933.D
 Acq On : 05 Apr 2021 22:30
 Operator : SY/MD
 Sample : M1880-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.448	2924	2926	2930	rBV3	627	506	0.02%	0.003%
78	10.574	2962	2965	2967	rBV3	1137	779	0.03%	0.005%
79	10.857	3049	3053	3061	rVB7	2111	1968	0.09%	0.012%
80	10.921	3067	3073	3084	rVB8	3226	5490	0.25%	0.034%
81	10.985	3091	3093	3094	rBV	216	62	0.00%	0.000%
82	11.001	3094	3098	3100	rBV3	781	547	0.02%	0.003%
83	11.255	3165	3177	3199	rBV	989117	1537423	68.97%	9.567%
84	11.545	3260	3267	3277	rBV8	3890	6637	0.30%	0.041%
85	11.631	3281	3294	3313	rBV	1033385	1628560	73.06%	10.134%
86	11.959	3394	3396	3403	rVB3	1081	846	0.04%	0.005%
87	12.461	3550	3552	3555	rVB2	581	266	0.01%	0.002%
88	12.599	3591	3595	3596	rBV2	1114	809	0.04%	0.005%
89	13.059	3736	3738	3739	rBV	602	266	0.01%	0.002%
90	13.178	3773	3775	3777	rBV	481	204	0.01%	0.001%
91	14.110	4063	4065	4070	rBV3	1318	932	0.04%	0.006%




Sum of corrected areas: 16070358

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020933.D
Acq On : 05 Apr 2021 22:30
Operator : SY/MD
Sample : M1880-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
EW1D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

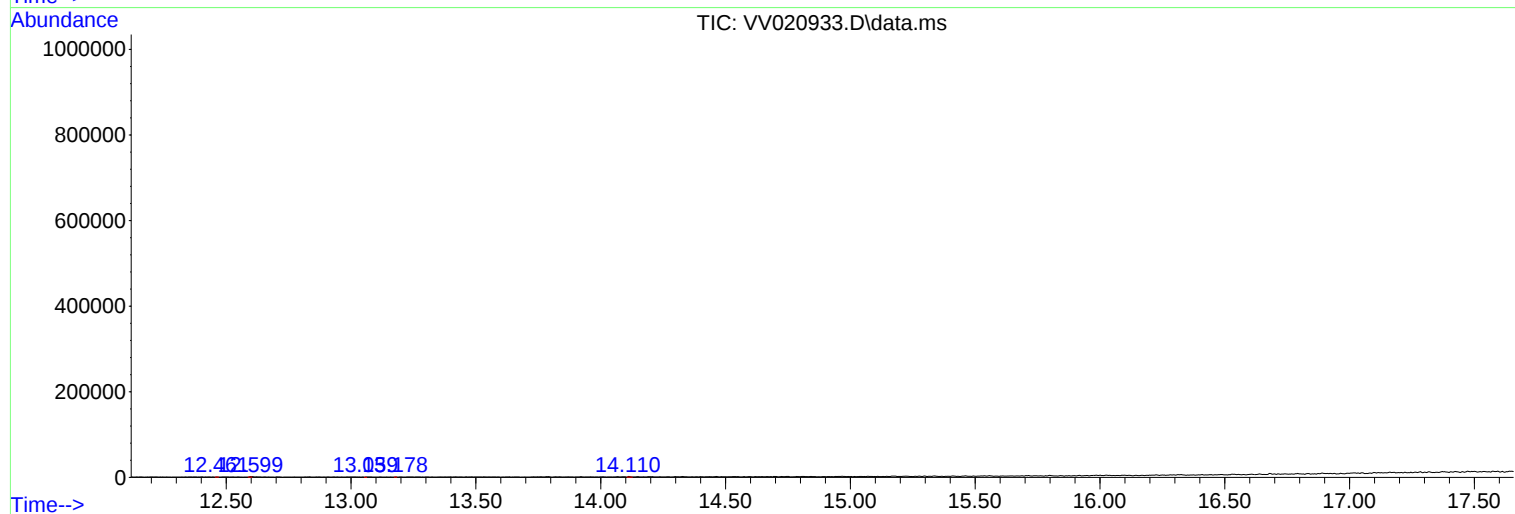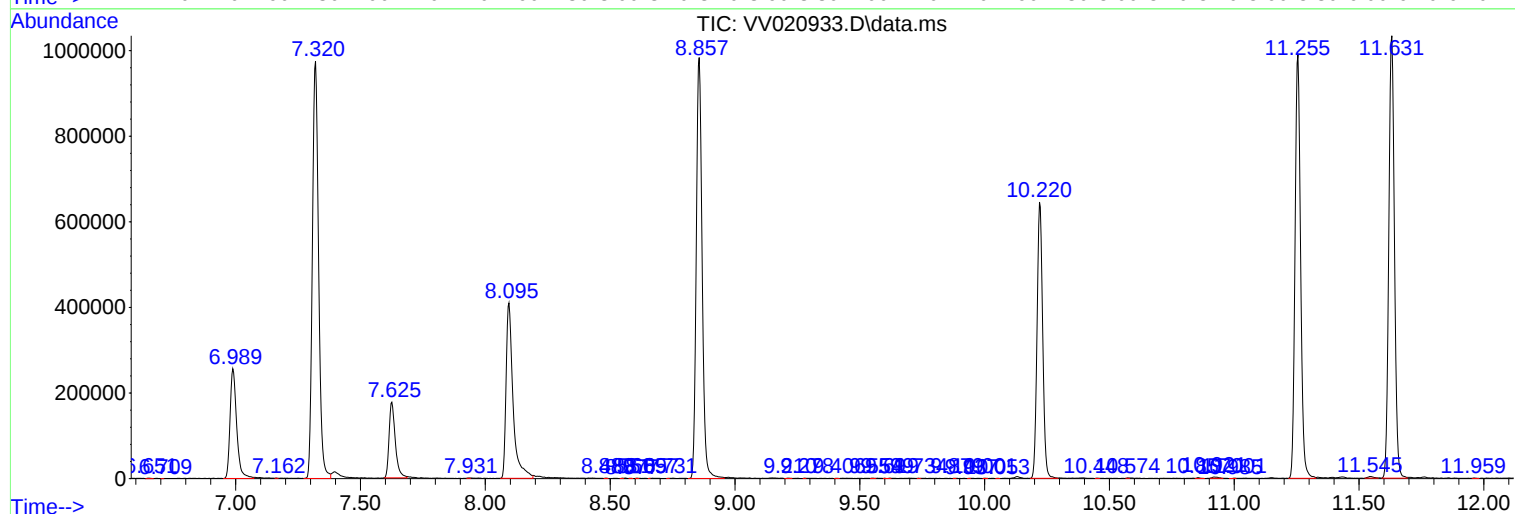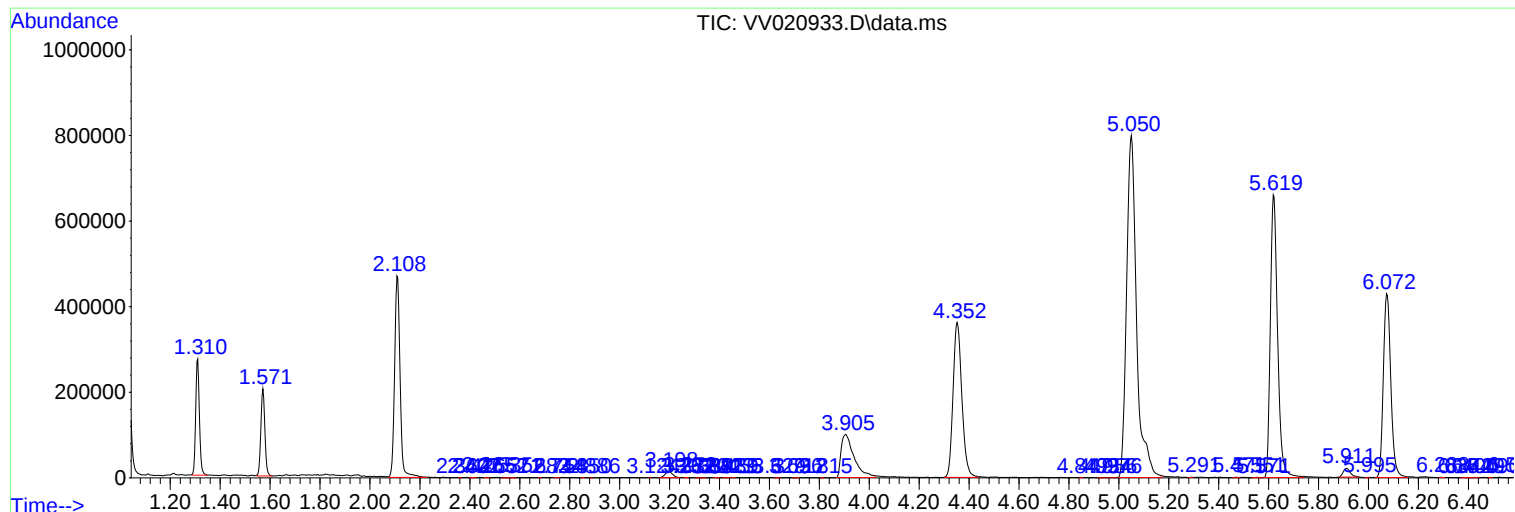

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020933.D
Acq On : 05 Apr 2021 22:30
Operator : SY/MD
Sample : M1880-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
Data File : VV020933.D
Acq On : 05 Apr 2021 22:30
Operator : SY/MD
Sample : M1880-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
