
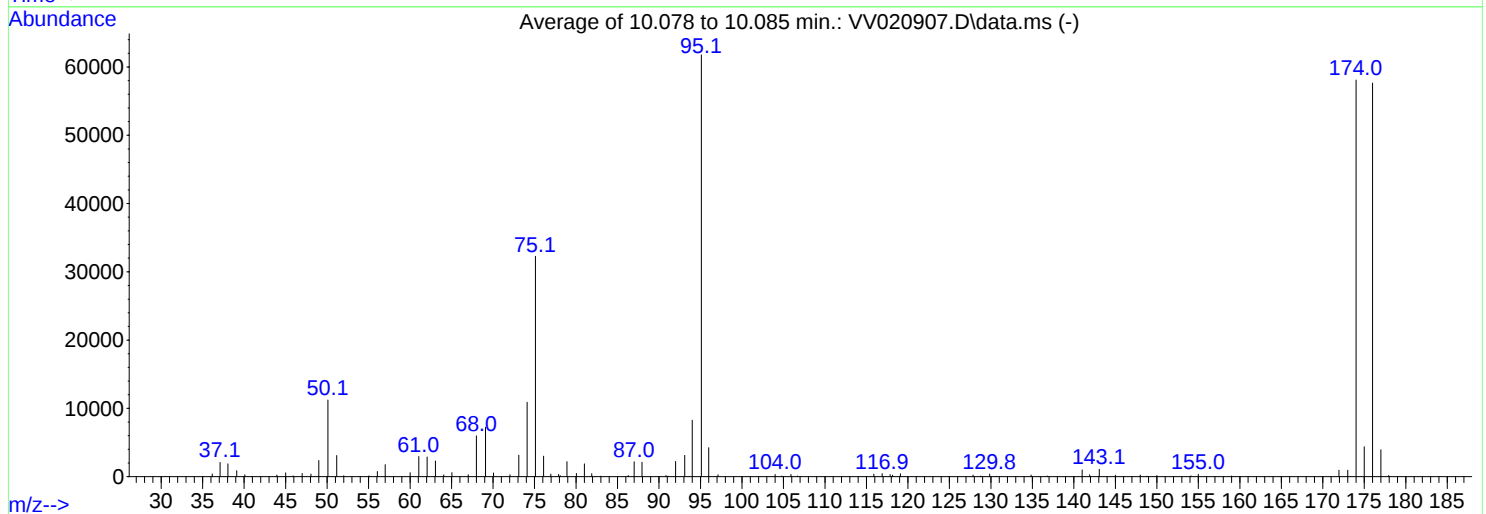


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040521\
 Data File : VV020907.D
 Acq On : 05 Apr 2021 11:51
 Operator : SY/MD
 Sample : BFB72
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB72

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis
 Last Update : Wed Apr 07 02:10:23 2021

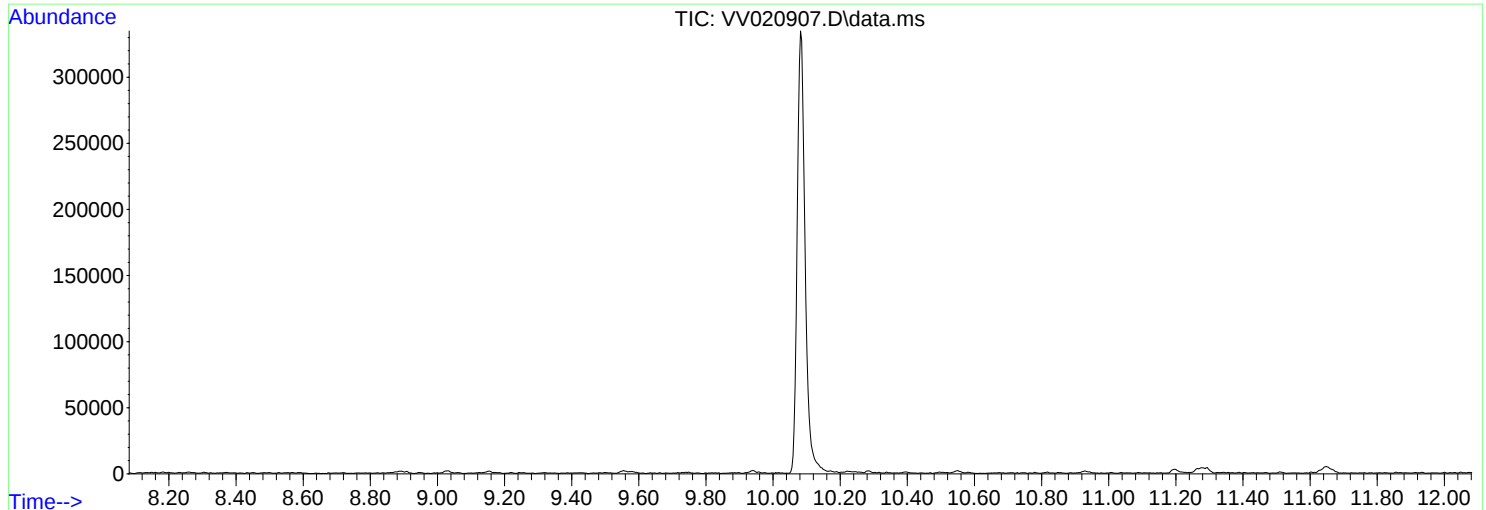

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	11233	PASS
75	95	30	80	52.2	32267	PASS
95	95	100	100	100.0	61776	PASS
96	95	5	9	6.9	4252	PASS
173	174	0.00	2	1.6	932	PASS
174	95	50	120	94.0	58088	PASS
175	174	5	9	7.5	4376	PASS
176	174	95	101	99.2	57645	PASS
177	176	5	9	6.8	3938	PASS

m/z	Abundance
39.80	190.0
43.90	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.10	457.0
37.10	2204.0
38.00	1807.0
39.10	797.0
40.10	280.0
44.10	571.0
45.00	659.0
45.90	180.0
47.10	425.0
48.10	411.0
49.00	2239.0
50.10	10518.0
51.20	3179.0
51.90	173.0
55.10	108.0
56.10	685.0
57.00	1789.0
60.00	570.0
61.10	2841.0
62.00	2807.0
63.00	2350.0
64.00	245.0
65.10	586.0
67.00	335.0
68.00	5630.0
69.10	7136.0
70.00	649.0
72.00	247.0
73.10	2857.0
74.10	10879.0
75.10	31256.0
76.10	3006.0
76.90	360.0
77.90	238.0
78.90	2150.0
80.00	458.0
81.00	1732.0
81.90	374.0
86.30	112.0
87.00	2006.0
88.00	2030.0
91.10	232.0
92.00	2208.0
93.10	3098.0
94.00	8023.0
95.10	59448.0
96.00	4072.0
97.10	318.0
104.00	435.0
105.90	315.0
106.70	147.0
115.90	271.0
116.90	439.0
117.80	241.0
118.20	329.0
119.10	523.0
127.90	275.0
129.90	437.0
134.90	278.0
136.80	167.0
141.00	888.0
141.90	286.0
143.00	943.0
145.00	194.0
147.00	125.0
148.00	135.0
150.00	175.0
154.10	112.0
155.00	271.0
159.00	153.0
172.00	924.0
172.90	909.0
174.00	54928.0
175.00	4306.0
176.00	53408.0
177.00	3774.0
177.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.10	386.0
37.10	2118.0
38.00	1860.0
39.10	867.0
40.10	279.0
40.90	106.0
44.00	460.0
45.00	595.0
45.90	166.0
47.00	420.0
48.10	378.0
49.00	2369.0
50.10	11756.0
51.20	3240.0
52.00	140.0
55.00	106.0
56.10	782.0
57.00	1860.0
60.00	611.0
61.00	2990.0
62.10	2955.0
63.00	2398.0
64.10	266.0
65.10	588.0
67.00	292.0
68.00	6169.0
69.10	7592.0
70.00	543.0
72.10	277.0
73.10	3304.0
74.10	11150.0
75.10	33496.0
76.10	3065.0
77.00	405.0
77.90	340.0
78.90	2316.0
80.10	460.0
81.00	2008.0
81.90	439.0
86.30	175.0
87.00	2242.0
87.90	2200.0
90.80	245.0
92.00	2365.0
93.10	3241.0
94.00	8684.0
95.10	63328.0
96.00	4497.0
97.10	298.0
104.00	352.0
104.80	150.0
105.90	338.0
106.70	152.0
115.90	388.0
116.90	474.0
117.80	339.0
118.10	335.0
119.10	428.0
127.80	235.0
128.80	143.0
129.80	408.0
134.90	259.0
136.80	102.0
141.00	1064.0
141.90	323.0
143.00	1089.0
145.00	227.0
148.00	249.0
150.00	203.0
154.10	136.0
155.00	392.0
159.00	123.0
172.00	981.0
173.00	945.0
174.00	59640.0
175.00	4530.0
176.00	59824.0
177.00	4050.0
178.00	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.20	378.0
37.10	1939.0
38.10	1986.0
39.10	968.0
40.10	277.0
44.00	412.0
45.00	468.0
46.90	541.0
48.00	312.0
49.00	2476.0
50.10	11424.0
51.10	2867.0
52.10	126.0
55.00	153.0
56.00	771.0
57.00	1638.0
60.00	557.0
61.00	3020.0
62.10	2913.0
63.10	2129.0
64.10	297.0
65.00	613.0
67.00	206.0
68.00	6149.0
69.10	7019.0
70.10	437.0
72.10	308.0
73.10	3282.0
74.10	10689.0
75.10	32048.0
76.10	2905.0
77.00	381.0
77.90	418.0
78.10	399.0
78.90	2140.0
80.10	466.0
81.00	1920.0
81.90	497.0
83.00	196.0
86.30	180.0
87.00	2316.0
87.90	2101.0
90.90	219.0
92.00	2112.0
93.10	3007.0
94.00	8145.0
95.10	62552.0
96.00	4187.0
97.10	256.0
104.00	224.0
104.80	160.0
105.90	328.0
115.90	462.0
116.90	452.0
117.90	365.0
119.10	348.0
127.80	225.0
128.80	120.0
129.90	248.0
130.70	123.0
134.80	202.0
141.00	1036.0
141.90	241.0
143.10	1193.0
145.00	187.0
148.00	302.0
148.80	198.0
150.00	149.0
154.10	119.0
155.00	378.0
171.90	941.0
173.10	942.0
174.00	59696.0
175.00	4291.0
176.00	59704.0
177.00	3991.0
178.00	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72