

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040523\
 Data File : VW030395.D
 Acq On : 05 Apr 2023 12:28
 Operator : SY/MD
 Sample : 02193-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11C7

Quant Time: Apr 06 05:26:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	131643	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	129954	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	64948	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	27118	3.110	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	62.200%
7) Chloroethane-d5	1.535	69	32859	3.884	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.600%
11) 1,1-Dichloroethene-d2	2.063	63	50078	2.421	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	48.400%#
20) 2-Butanone-d5	3.812	46	103330	45.852	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.700%
24) Chloroform-d	4.259	84	91304	4.327	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%
26) 1,2-Dichloroethane-d4	4.953	65	46106	4.631	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
32) Benzene-d6	4.969	84	153082	4.180	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.600%
36) 1,2-Dichloropropane-d6	5.998	67	50840	4.434	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.600%
41) Toluene-d8	7.252	98	127320	3.786	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.800%
43) trans-1,3-Dichloroprop...	7.561	79	17655	4.090	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.800%
46) 2-Hexanone-d5	8.034	63	76964	44.371	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.740%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	38755	4.289	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.800%
66) 1,2-Dichlorobenzene-d4	11.570	152	54130	4.663	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.200%
Target Compounds						
13) Acetone	2.143	43	7103	3.296	ug/L	Qvalue 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030395.D
Acq On : 05 Apr 2023 12:28
Operator : SY/MD
Sample : 02193-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11C7

Quant Time: Apr 06 05:26:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration

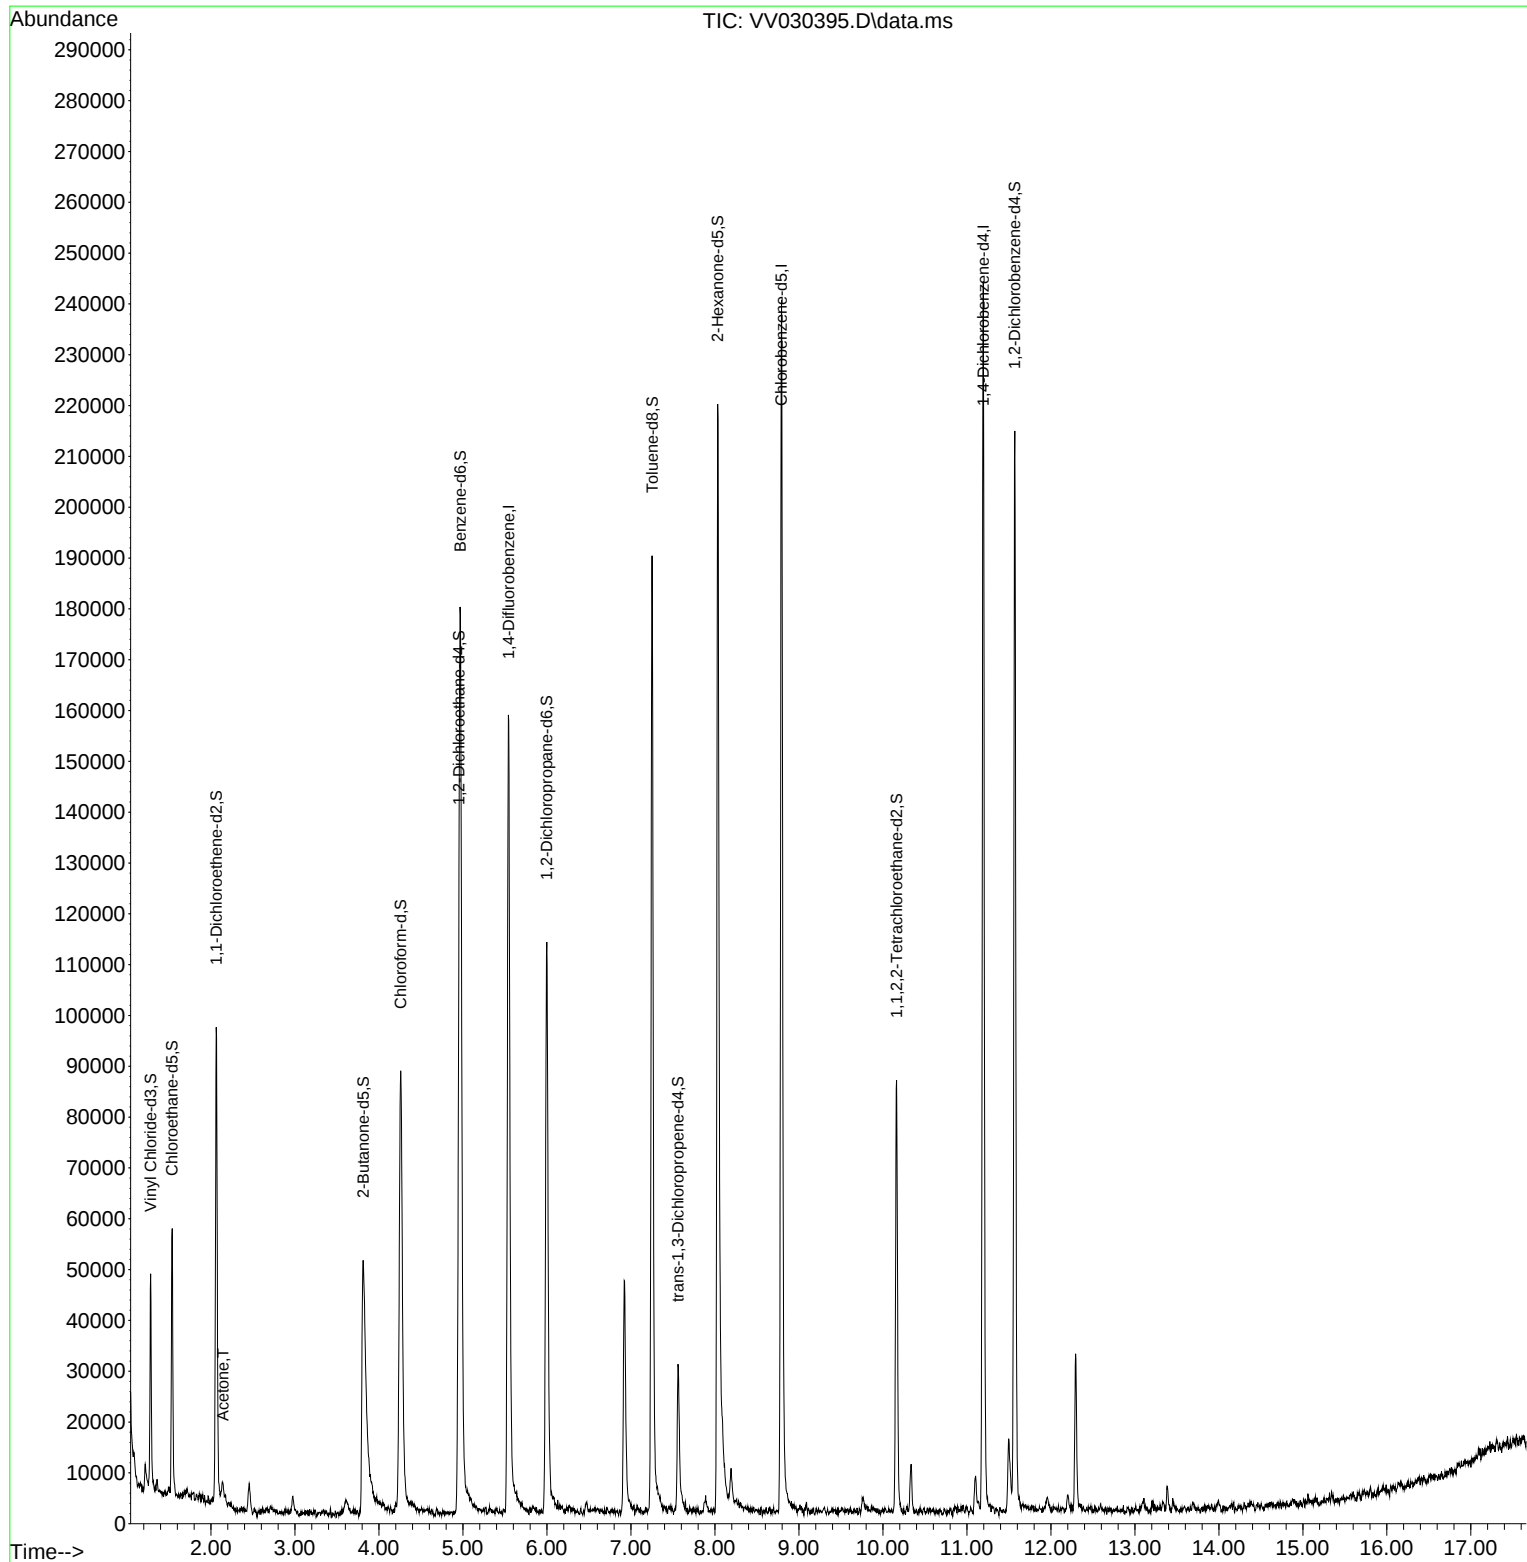

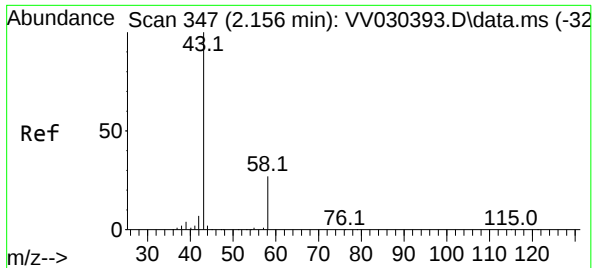

#13

Acetone

Concen: 3.296 ug/L

RT: 2.143 min Scan# 34

Delta R.T. -0.003 min

Lab File: VV030395.D

Acq: 05 Apr 2023 12:28

Instrument :

MSVOA_V

ClientSampleId :

C11C7

Tgt Ion: 43 Resp: 7103

Ion Ratio Lower Upper

43 100

58 39.9 0.0 40.8

