

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
 Data File : VV030398.D
 Acq On : 05 Apr 2023 14:06
 Operator : SY/MD
 Sample : 02194-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.372	94	103	134	rBV	64163	256480	3.99%	1.662%
2	2.076	311	322	347	rVB	728303	1119058	17.43%	7.251%
3	3.121	630	647	667	rBV	173494	370792	5.77%	2.402%
4	3.822	847	865	907	rBV2	943962	2433008	37.88%	15.764%
5	4.262	986	1002	1021	rBV3	64500	184051	2.87%	1.193%
6	4.523	1064	1083	1107	rBV	173493	432770	6.74%	2.804%
7	4.966	1203	1221	1242	rBV2	127551	345515	5.38%	2.239%
8	5.545	1389	1401	1420	rBV	106631	226899	3.53%	1.470%
9	5.841	1477	1493	1517	rBV	832332	1645931	25.63%	10.664%
10	5.998	1531	1542	1559	rVB	82190	168042	2.62%	1.089%
11	7.252	1921	1932	1952	rBV	132627	243177	3.79%	1.576%
12	7.915	2116	2138	2165	rBV	3810512	6422140	100.00%	41.611%
13	8.034	2165	2175	2208	rVB	273179	518925	8.08%	3.362%
14	8.793	2401	2411	2429	rBV	164735	281929	4.39%	1.827%
15	10.162	2825	2837	2851	rBV	84127	137393	2.14%	0.890%
16	10.336	2878	2891	2903	rVB	64208	109751	1.71%	0.711%
17	11.194	3146	3158	3175	rBV	175818	283101	4.41%	1.834%
18	11.571	3262	3275	3292	rBV	159392	254847	3.97%	1.651%




Sum of corrected areas: 15433809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030398.D
Acq On : 05 Apr 2023 14:06
Operator : SY/MD
Sample : 02194-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

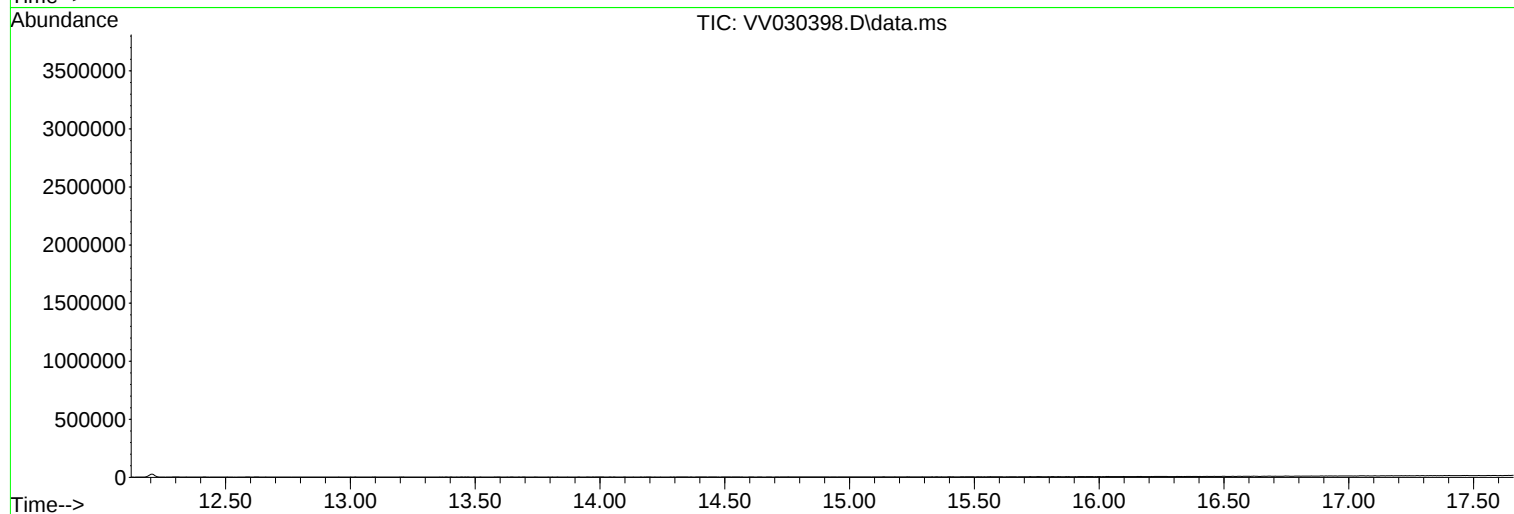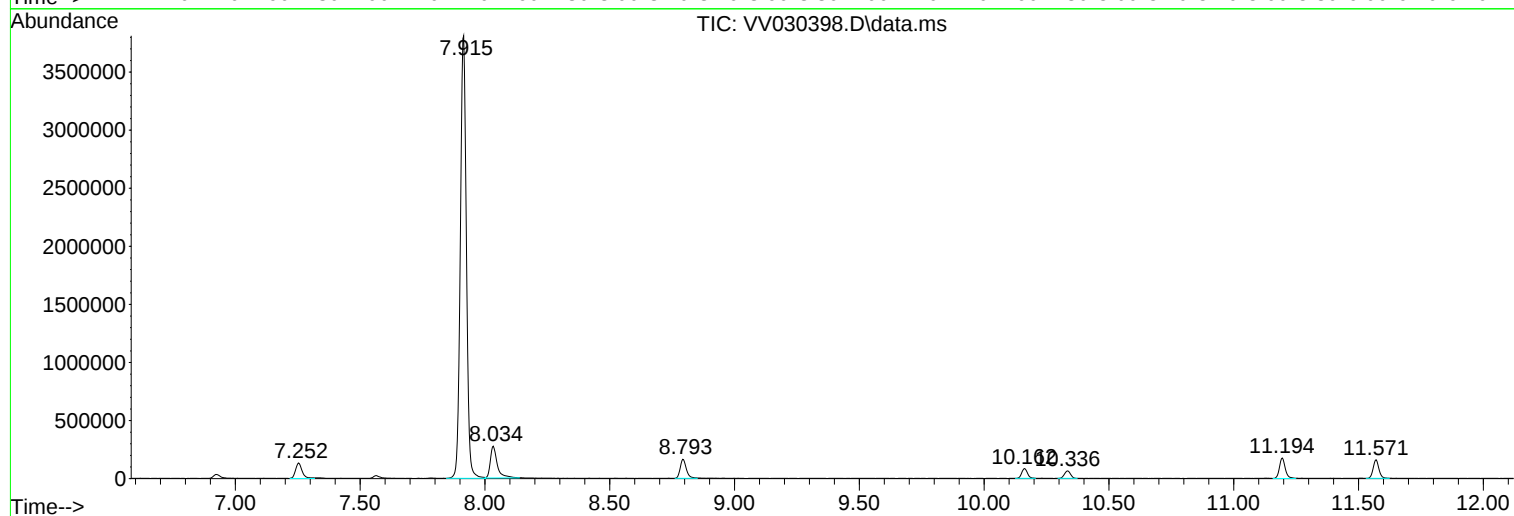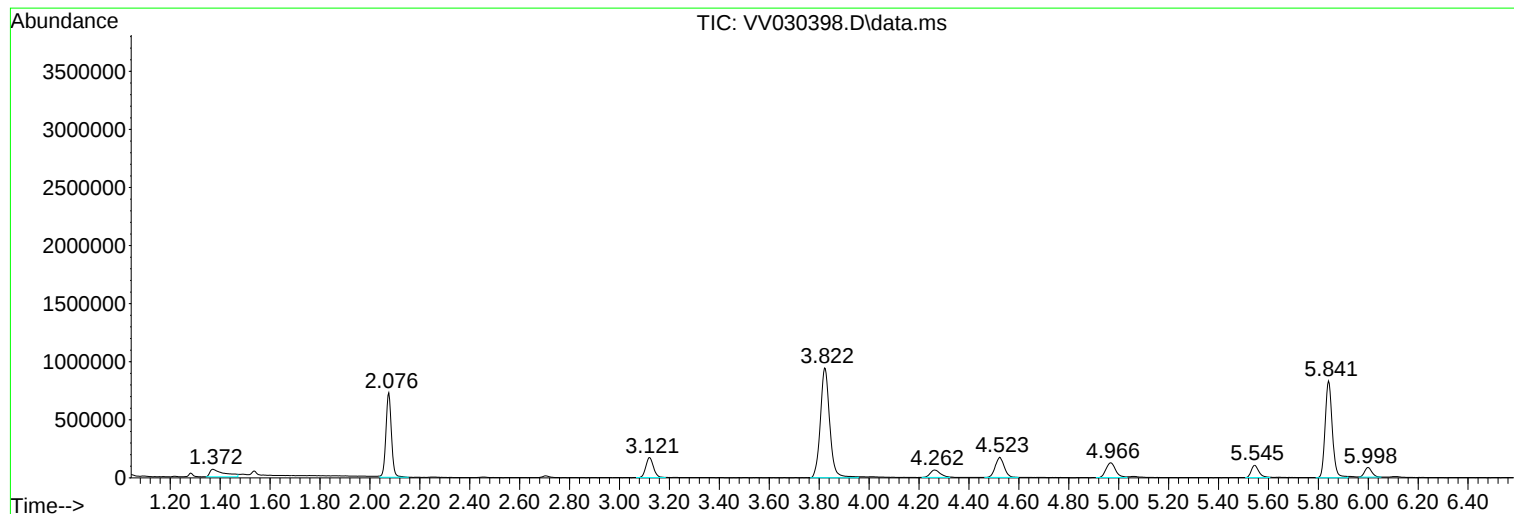

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030398.D
Acq On : 05 Apr 2023 14:06
Operator : SY/MD
Sample : 02194-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.372	5.7	ug/L	256480	1	5.545	226899	5.0