

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
 Data File : VV030399.D
 Acq On : 05 Apr 2023 14:30
 Operator : SY/MD
 Sample : 02194-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	62	rBV3	4746	5330	1.10%	0.120%
2	1.281	69	75	87	rVB	40801	43191	8.94%	0.970%
3	1.535	148	154	168	rVB	53861	66131	13.69%	1.486%
4	2.066	309	319	335	rVB	97350	152380	31.55%	3.424%
5	2.458	432	441	452	rVB	3277	7213	1.49%	0.162%
6	3.815	849	863	889	rBV	55544	194005	40.17%	4.359%
7	4.262	982	1002	1026	rBV	90583	237288	49.13%	5.332%
8	4.969	1203	1222	1242	rBV2	182292	476797	98.72%	10.713%
9	5.545	1388	1401	1424	rBV	160260	338902	70.17%	7.615%
10	5.998	1524	1542	1563	rBV	119819	257018	53.22%	5.775%
11	6.924	1818	1830	1848	rBV2	45331	90711	18.78%	2.038%
12	7.252	1919	1932	1945	rBV	191446	344451	71.32%	7.740%
13	7.326	1945	1955	1977	rVB	104501	193008	39.96%	4.337%
14	7.561	2015	2028	2043	rBV	28702	57958	12.00%	1.302%
15	7.886	2114	2129	2135	rBV	15980	31794	6.58%	0.714%
16	8.034	2166	2175	2208	rBV	238999	482959	100.00%	10.852%
17	8.792	2397	2411	2429	rBV	245929	412908	85.50%	9.278%
18	9.011	2471	2479	2488	rVB	3273	5171	1.07%	0.116%
19	9.079	2497	2500	2510	rVB9	3171	4989	1.03%	0.112%
20	9.503	2622	2632	2645	rBV9	6606	13920	2.88%	0.313%
21	10.162	2824	2837	2850	rBV	91125	150958	31.26%	3.392%
22	10.332	2877	2890	2903	rVB	44046	74373	15.40%	1.671%
23	11.194	3144	3158	3174	rBV	250532	399229	82.66%	8.970%
24	11.570	3264	3275	3294	rVB	215609	347454	71.94%	7.807%
25	12.204	3462	3472	3485	rVB2	19836	32221	6.67%	0.724%
26	12.297	3491	3501	3512	rBV10	11943	20322	4.21%	0.457%
27	12.622	3592	3602	3611	rBV7	5994	9832	2.04%	0.221%




Sum of corrected areas: 4450513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030399.D
Acq On : 05 Apr 2023 14:30
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

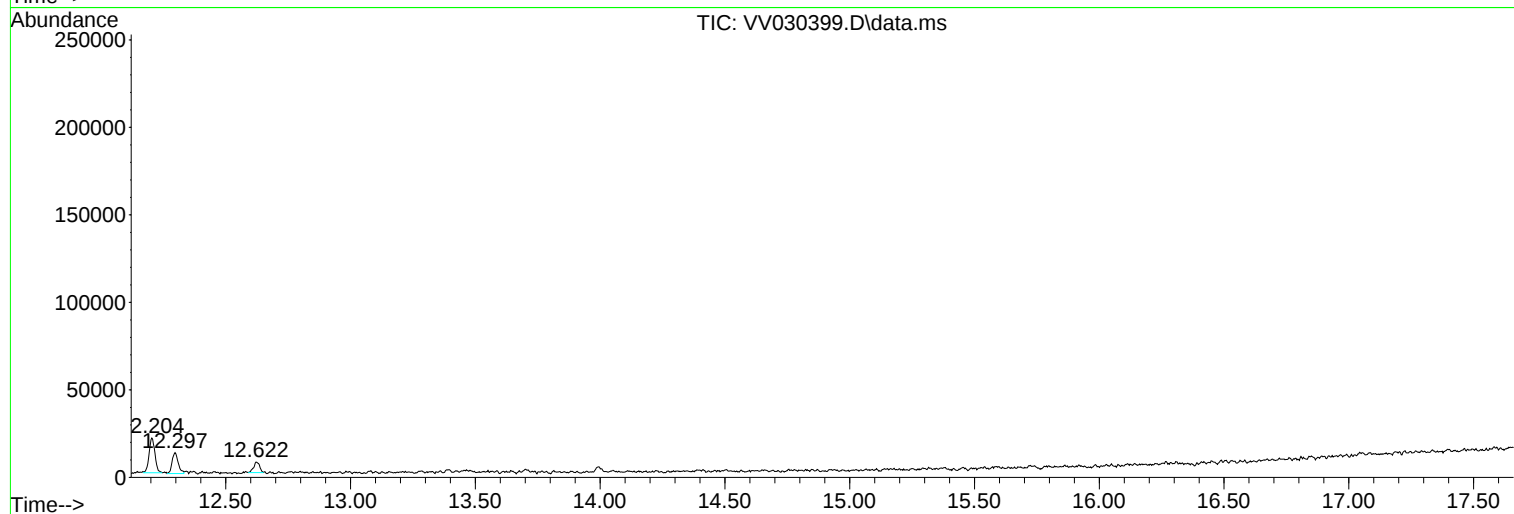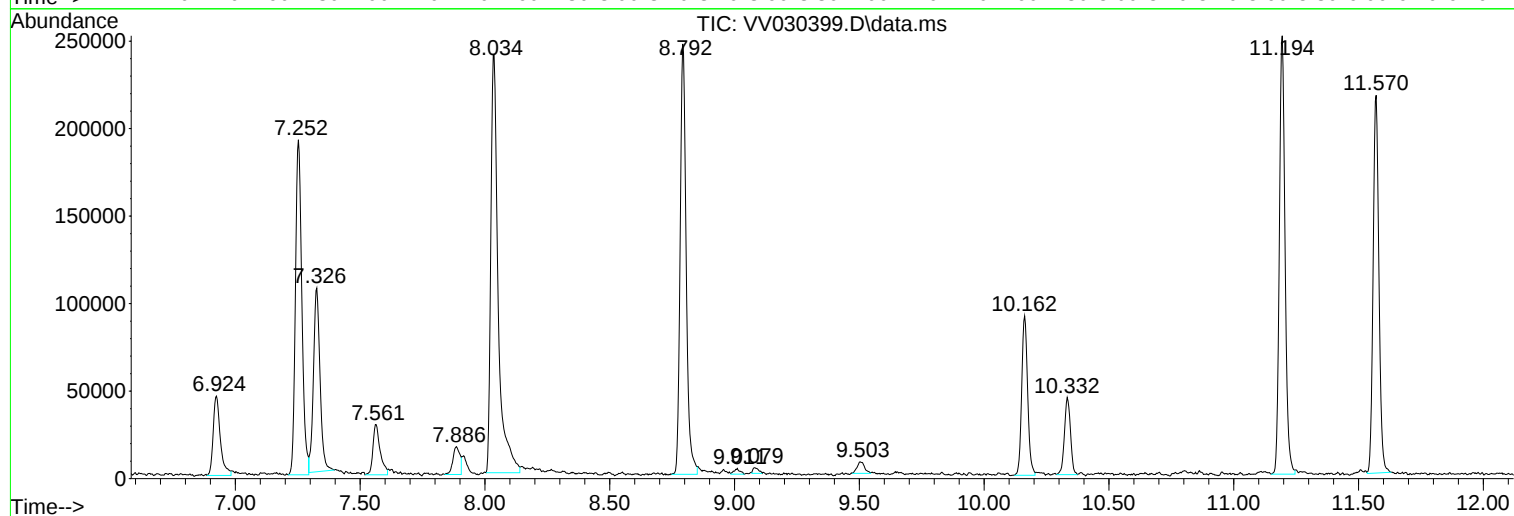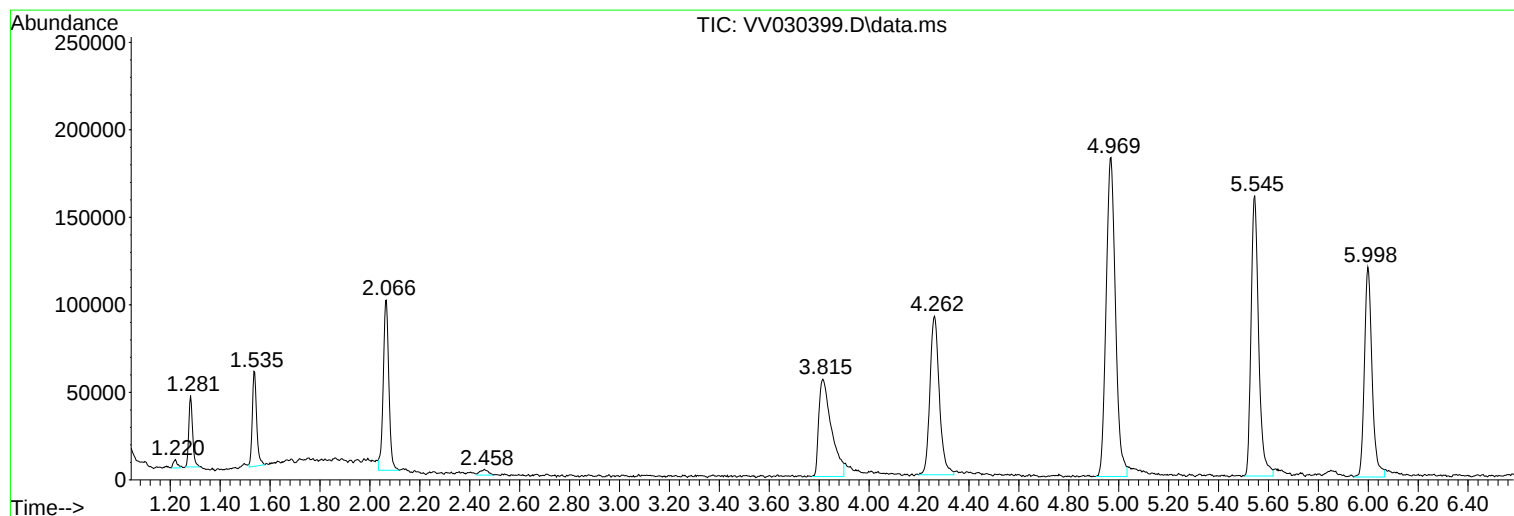

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030399.D
Acq On : 05 Apr 2023 14:30
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030399.D
Acq On : 05 Apr 2023 14:30
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------