

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
 Data File : VV030400.D
 Acq On : 05 Apr 2023 14:55
 Operator : SY/MD
 Sample : 02194-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	11	14	30	rVB3	16696	23854	5.31%	0.504%
2	1.214	50	54	62	rVB	5673	7100	1.58%	0.150%
3	1.282	68	75	85	rVB	42805	48194	10.73%	1.019%
4	1.536	148	154	167	rVB	50548	59603	13.27%	1.261%
5	2.069	309	320	340	rVB3	133773	233690	52.01%	4.942%
6	2.709	512	519	533	rVB3	7908	16665	3.71%	0.352%
7	3.121	632	647	660	rBV2	36319	82232	18.30%	1.739%
8	3.822	851	865	896	rBV2	81257	275216	61.26%	5.820%
9	4.262	983	1002	1025	rBV2	84011	223983	49.85%	4.737%
10	4.526	1071	1084	1100	rVB3	17432	43492	9.68%	0.920%
11	4.970	1202	1222	1247	rBV2	171314	449290	100.00%	9.502%
12	5.545	1388	1401	1420	rBV	151709	326364	72.64%	6.902%
13	5.844	1480	1494	1509	rBV3	37911	79095	17.60%	1.673%
14	5.998	1530	1542	1569	rBV	110201	231948	51.63%	4.905%
15	6.924	1819	1830	1844	rBV2	43496	85708	19.08%	1.813%
16	7.252	1920	1932	1954	rBV	178804	331151	73.71%	7.003%
17	7.564	2018	2029	2041	rBV	27271	50376	11.21%	1.065%
18	7.915	2117	2138	2155	rBV	207652	379968	84.57%	8.036%
19	8.034	2165	2175	2206	rBV	222477	440882	98.13%	9.324%
20	8.793	2396	2411	2435	rBV	235323	400499	89.14%	8.470%
21	10.162	2825	2837	2853	rBV	86708	140945	31.37%	2.981%
22	10.333	2876	2890	2901	rBV	25291	41383	9.21%	0.875%
23	11.088	3118	3125	3132	rBV9	3262	5377	1.20%	0.114%
24	11.194	3146	3158	3177	rBV	235170	380432	84.67%	8.045%
25	11.571	3262	3275	3295	rBV	197574	327734	72.94%	6.931%
26	12.204	3461	3472	3481	rBV2	14814	24058	5.35%	0.509%
27	13.313	3812	3817	3828	rVB10	4225	6887	1.53%	0.146%
28	13.487	3862	3871	3875	rBV10	4297	6506	1.45%	0.138%
29	14.316	4123	4129	4136	rBV10	4088	5883	1.31%	0.124%




Sum of corrected areas: 4728515

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030400.D
Acq On : 05 Apr 2023 14:55
Operator : SY/MD
Sample : 02194-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

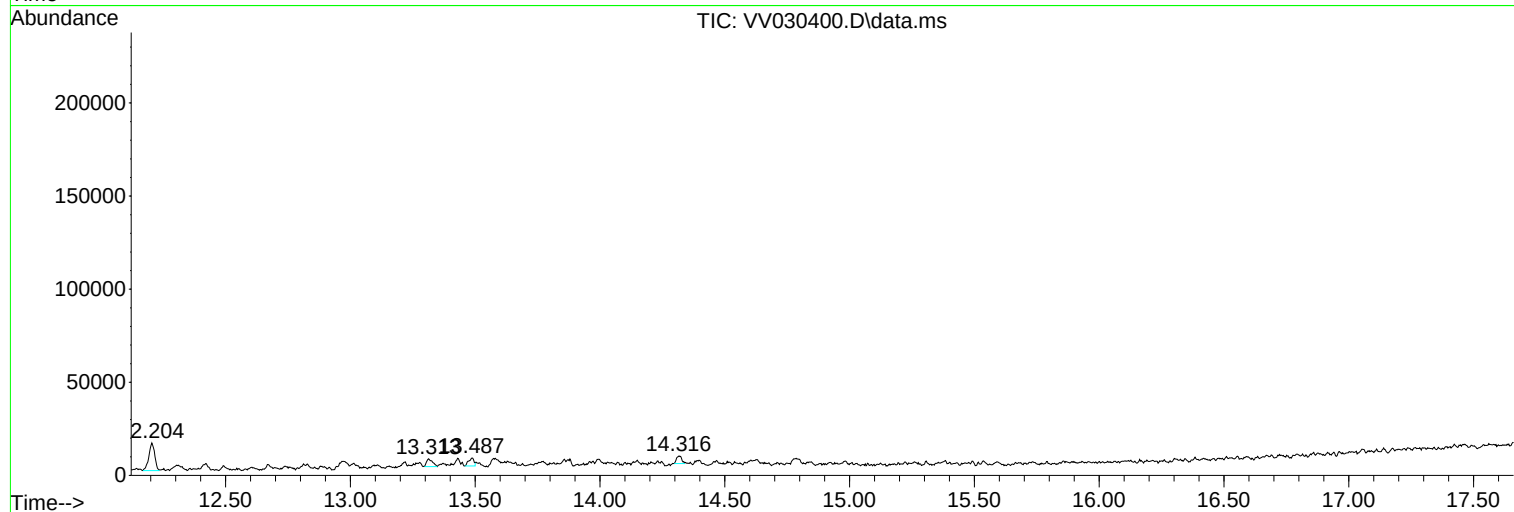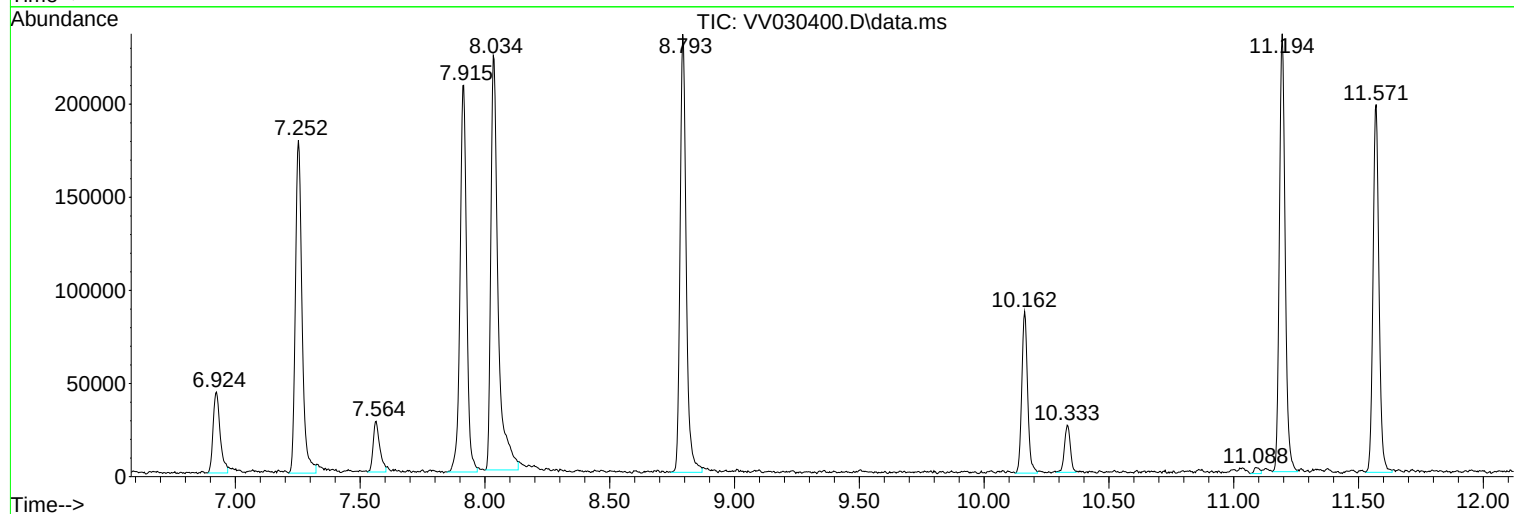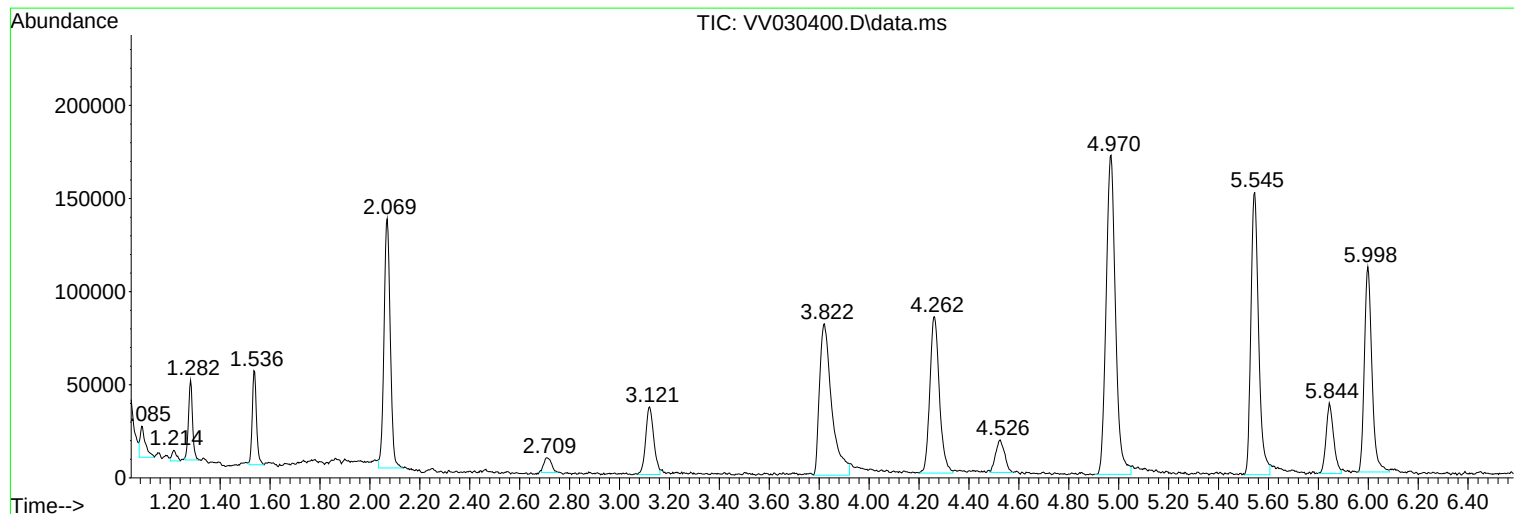

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030400.D
Acq On : 05 Apr 2023 14:55
Operator : SY/MD
Sample : 02194-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
Data File : VV030400.D
Acq On : 05 Apr 2023 14:55
Operator : SY/MD
Sample : 02194-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------