


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040523\
 Data File : VV030392.D
 Acq On : 05 Apr 2023 09:07
 Operator : SY/MD
 Sample : BFB242
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB242

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 31 05:37:21 2023

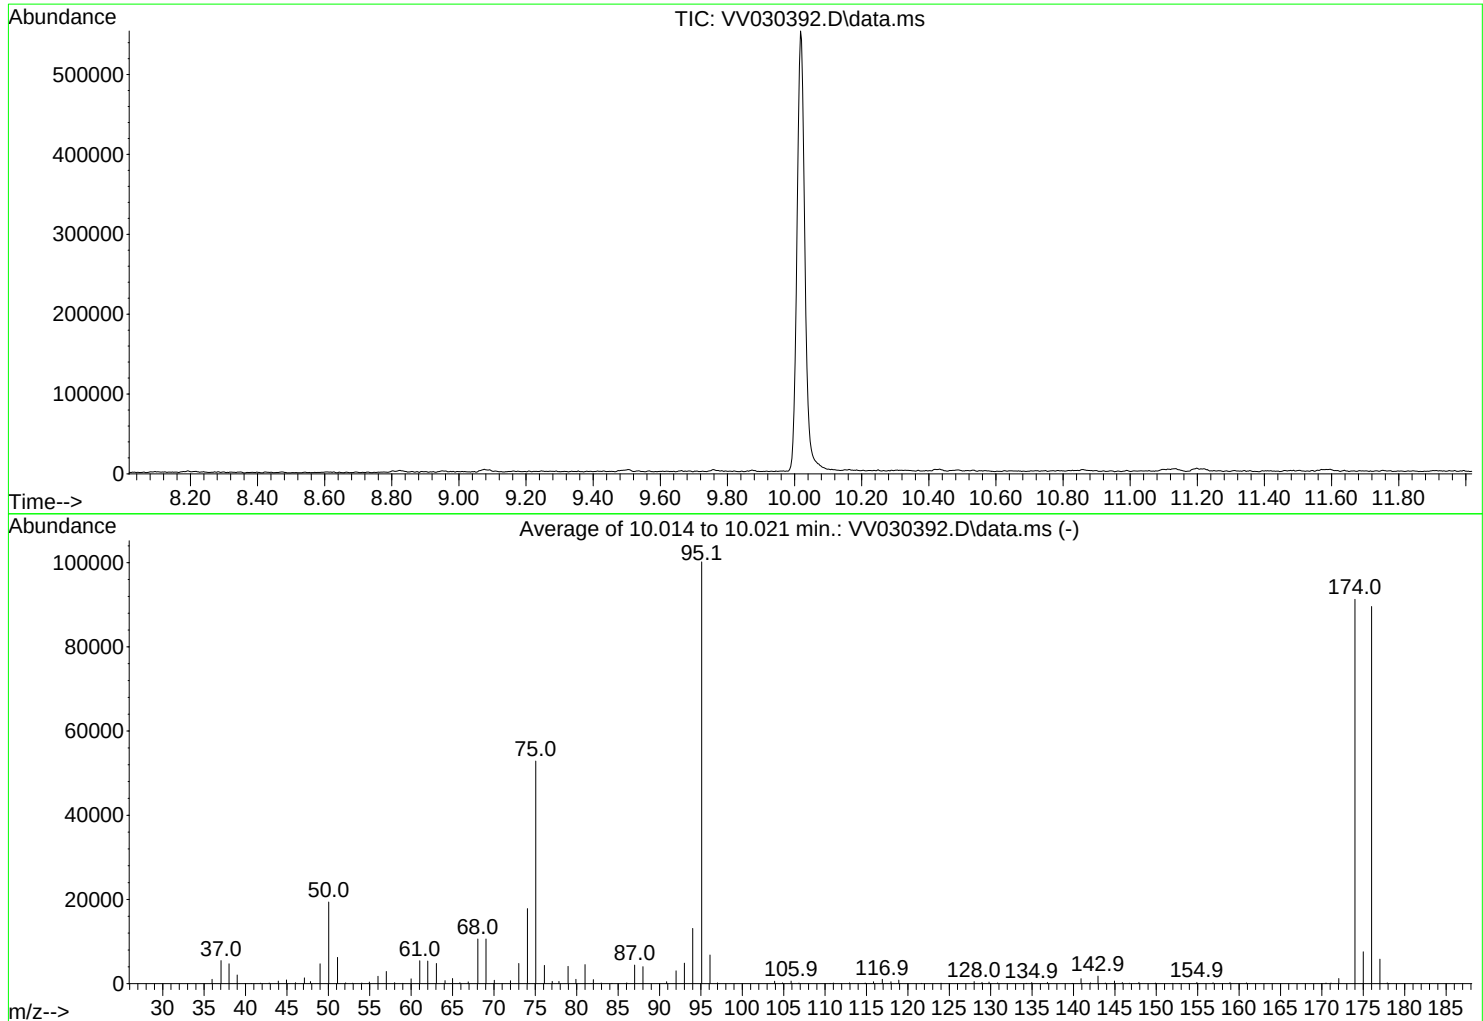

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	19400	PASS
75	95	30	80	52.8	52888	PASS
95	95	100	100	100.0	100200	PASS
96	95	5	9	6.8	6794	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.1	91301	PASS
175	174	5	9	8.3	7555	PASS
176	174	95	105	98.1	89581	PASS
177	176	5	10	6.5	5823	PASS

m/z	Abundance
35.90	959.0
36.80	143.0
37.90	421.0
39.90	241.0
41.20	143.0
42.20	103.0
43.90	230.0
44.90	108.0
45.50	105.0
47.70	137.0
49.90	109.0
52.00	110.0
52.90	127.0
53.70	123.0
57.00	138.0
76.60	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
36.00	1888.0
37.00	5311.0
38.00	5032.0
39.00	2035.0
40.00	281.0
40.70	152.0
41.90	131.0
42.80	163.0
44.00	816.0
45.00	930.0
46.10	237.0
47.10	1445.0
47.90	589.0
49.00	4512.0
50.10	18488.0
51.10	5944.0
52.10	312.0
53.00	194.0
54.10	141.0
55.00	354.0
56.00	1719.0
57.00	2771.0
58.00	208.0
60.00	1057.0
61.10	5189.0
62.00	5265.0
63.00	4749.0
64.10	694.0
65.00	1048.0
65.90	220.0
66.90	441.0
68.00	10227.0
69.00	10498.0
70.10	866.0
71.00	104.0
72.00	642.0
73.00	4508.0
74.00	17272.0
75.10	50376.0
76.10	4216.0
77.00	529.0
77.90	466.0
78.90	3967.0
79.90	1002.0
81.00	4402.0
82.00	843.0
82.90	176.0
84.20	109.0
86.10	187.0
87.00	4031.0
88.00	4007.0
90.90	469.0
92.00	3026.0
93.00	4638.0
94.00	12480.0
95.10	96280.0
96.10	6824.0
97.00	221.0
103.90	487.0
104.90	187.0
105.90	570.0
106.80	144.0
111.00	133.0
112.90	171.0
114.80	136.0
115.80	422.0
116.90	954.0
117.90	463.0
118.90	758.0
121.60	109.0
124.00	103.0
128.00	540.0
128.90	271.0
129.80	426.0
130.80	199.0
134.90	265.0
136.80	281.0
139.90	127.0
140.90	1140.0
142.10	197.0
143.00	1613.0
143.90	144.0
145.00	557.0
145.90	321.0
146.70	120.0
147.90	298.0
149.90	156.0
154.90	270.0
156.80	227.0
158.90	285.0
160.90	201.0
170.50	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

172.00	1005.0
174.00	85592.0
175.00	7377.0
176.00	84336.0
177.00	5466.0
177.90	175.0
178.10	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
36.00	2076.0
37.10	5638.0
38.00	5321.0
39.00	2109.0
40.00	289.0
41.10	151.0
41.80	122.0
42.80	150.0
44.00	867.0
45.00	1009.0
46.00	212.0
47.10	1435.0
47.90	647.0
49.00	4883.0
50.10	20032.0
51.10	6543.0
52.20	303.0
53.00	250.0
54.00	144.0
54.90	379.0
56.00	1781.0
57.00	3079.0
58.00	254.0
59.00	128.0
60.00	1148.0
61.10	5669.0
62.00	5528.0
63.10	4888.0
64.10	713.0
65.00	1253.0
65.90	228.0
66.90	423.0
68.00	10911.0
69.00	10993.0
70.10	808.0
72.00	725.0
73.00	4902.0
74.00	18392.0
75.10	54976.0
76.10	4433.0
77.10	525.0
77.90	539.0
79.00	4227.0
79.90	1052.0
81.00	4672.0
82.00	997.0
83.00	186.0
84.30	105.0
86.00	195.0
87.00	4540.0
88.00	4163.0
90.90	489.0
92.00	3144.0
93.00	5062.0
94.00	13536.0
95.10	103552.0
96.10	6994.0
97.00	196.0
103.90	607.0
104.80	219.0
105.90	633.0
106.90	168.0
111.00	149.0
112.90	189.0
114.90	170.0
115.90	463.0
116.90	1057.0
118.00	478.0
118.90	859.0
121.70	103.0
124.00	127.0
128.00	536.0
128.90	317.0
129.80	392.0
130.80	206.0
134.30	114.0
135.00	294.0
136.80	326.0
139.80	117.0
140.90	1214.0
142.00	209.0
142.90	1909.0
143.90	164.0
144.90	648.0
145.90	295.0
146.80	129.0
147.90	297.0
149.90	172.0
152.00	116.0
154.90	342.0
156.80	211.0
158.90	276.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

160.90	196.0
170.50	225.0
171.10	238.0
172.10	1288.0
174.00	94440.0
175.00	7884.0
176.00	92536.0
177.00	6074.0
177.90	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
36.00	2051.0
37.10	5475.0
38.10	5115.0
39.00	2032.0
40.00	265.0
41.10	173.0
41.70	118.0
42.40	126.0
42.90	131.0
44.00	858.0
45.00	976.0
46.10	202.0
47.10	1224.0
47.90	632.0
49.00	4779.0
50.10	20008.0
51.10	6248.0
52.20	315.0
53.00	275.0
54.00	176.0
54.90	372.0
56.00	1765.0
57.10	3182.0
58.00	274.0
59.00	146.0
60.00	1196.0
61.00	5447.0
62.00	5283.0
63.10	4678.0
64.10	731.0
65.00	1312.0
65.90	215.0
66.90	357.0
68.10	10642.0
69.10	10361.0
70.00	692.0
72.00	697.0
73.00	4934.0
74.10	17840.0
75.00	53312.0
76.10	4336.0
77.00	517.0
77.80	595.0
79.00	4168.0
79.90	1035.0
81.00	4550.0
82.00	990.0
83.00	148.0
86.00	187.0
87.00	4667.0
88.00	3982.0
90.80	465.0
92.00	3011.0
93.00	4945.0
94.00	13359.0
95.10	100768.0
96.10	6565.0
97.00	181.0
103.90	673.0
104.80	199.0
105.90	585.0
106.90	187.0
110.60	102.0
111.00	137.0
111.90	118.0
113.00	184.0
114.90	175.0
115.90	496.0
116.90	1046.0
118.00	451.0
118.90	881.0
124.00	105.0
128.00	454.0
129.00	331.0
129.80	340.0
130.90	179.0
134.30	116.0
135.00	303.0
136.90	294.0
140.90	1235.0
142.10	192.0
142.90	1879.0
143.80	166.0
144.90	654.0
145.90	226.0
146.80	123.0
147.90	287.0
149.90	166.0
151.90	120.0
152.80	113.0
153.90	118.0
154.90	343.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

156.90	210.0
158.90	195.0
160.90	155.0
170.00	118.0
171.10	257.0
172.00	1357.0
174.00	93872.0
175.00	7404.0
176.00	91872.0
177.00	5929.0
177.90	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242