

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035008.D
 Acq On : 05 Apr 2024 16:07
 Operator : SY/MD
 Sample : P2007-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 06 01:04:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 06 00:54:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	379369	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	369228	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	161056	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	108851	29.710	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	59.420%#		
7) Chloroethane-d5	1.529	69	116379	36.572	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	73.140%		
11) 1,1-Dichloroethene-d2	2.060	65	52640	32.777	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.560%		
21) 2-Butanone-d5	3.789	46	176288	81.130	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	81.130%		
24) Chloroform-d	4.249	84	243824	39.582	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.160%		
26) 1,2-Dichloroethane-d4	4.941	65	157170	40.187	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.380%		
32) Benzene-d6	4.960	84	458150	36.940	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	73.880%		
36) 1,2-Dichloropropane-d6	5.985	67	161489	41.004	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	82.000%		
41) Toluene-d8	7.243	98	381523	34.157	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	68.320%#		
43) trans-1,3-Dichloroprop...	7.555	79	64070	33.463	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.920%		
47) 2-Hexanone-d5	8.024	63	99703	66.958	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	66.960%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	221334	40.810	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.620%		
66) 1,2-Dichlorobenzene-d4	11.558	152	151101	41.786	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.580%		
Target Compounds						Qvalue
48) 2-Hexanone	8.085	43	19812	5.483	ug/L	95
61) 1,2,3-Trichloropropane	11.185	75	19761	5.662	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035008.D
Acq On : 05 Apr 2024 16:07
Operator : SY/MD
Sample : P2007-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Apr 06 01:04:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 00:54:20 2024
Response via : Initial Calibration

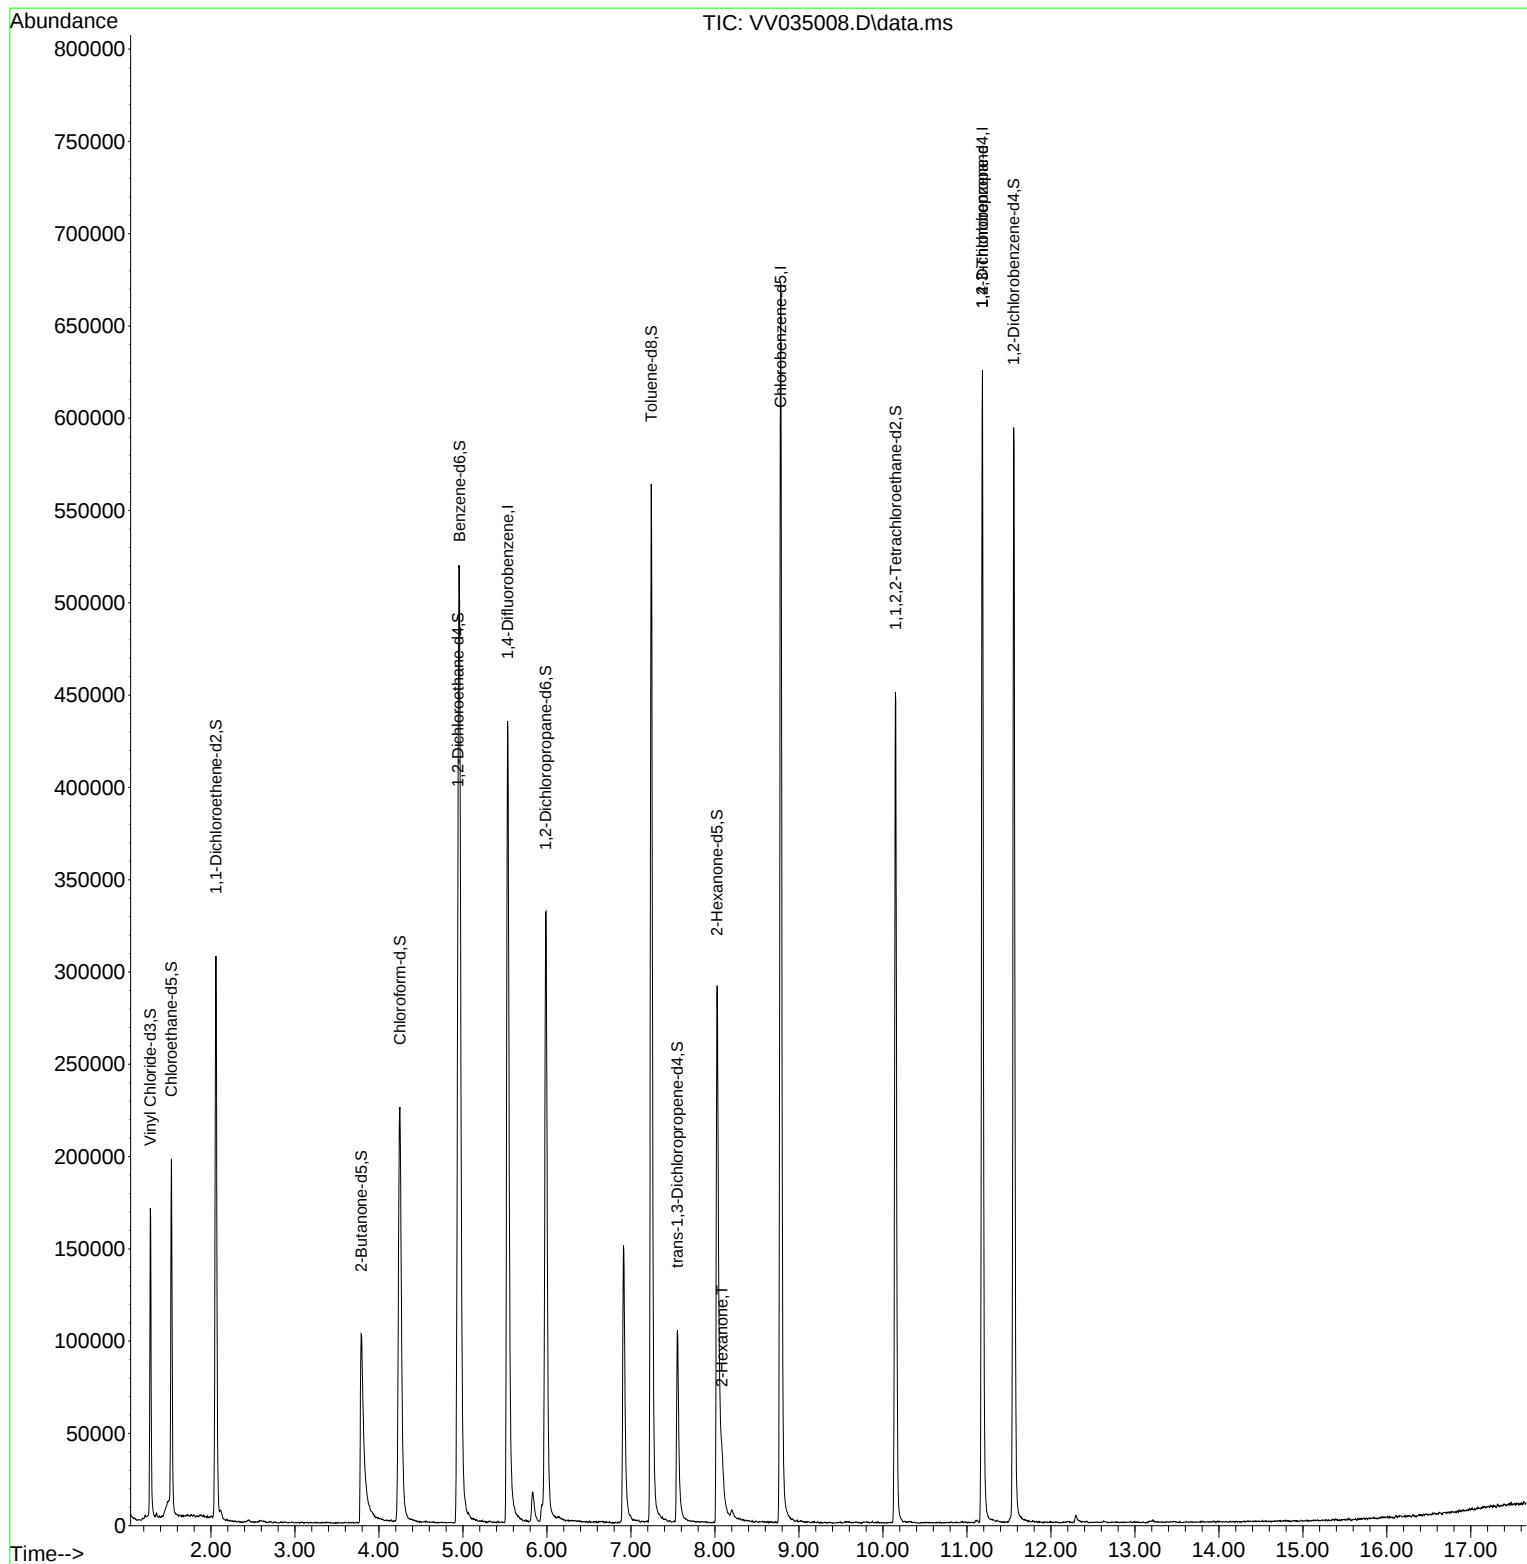

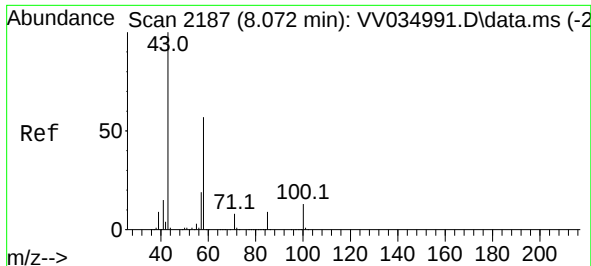




#48
2-Hexanone
Concen: 5.483 ug/L
RT: 8.085 min Scan# 2187
Delta R.T. 0.013 min
Lab File: VV035008.D
Acq: 05 Apr 2024 16:07

Instrument :
MSVOA_V
ClientSampleId :

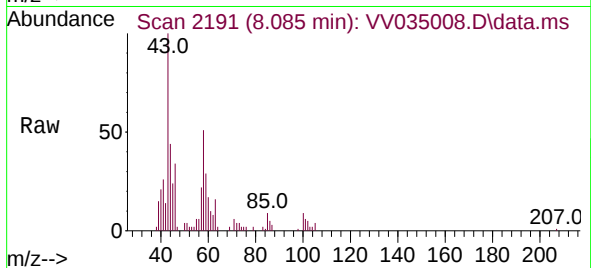

Tgt Ion: 43 Resp: 19812

Ion	Ratio	Lower	Upper
43	100		
58	51.4	45.4	68.2
57	20.0	16.2	24.4
100	10.9	10.1	15.1

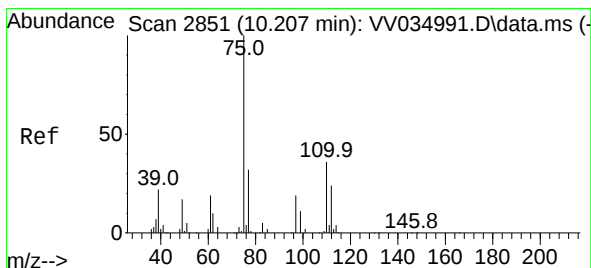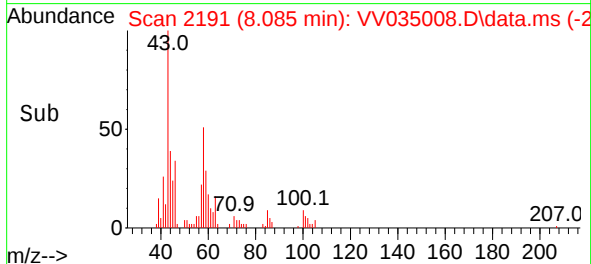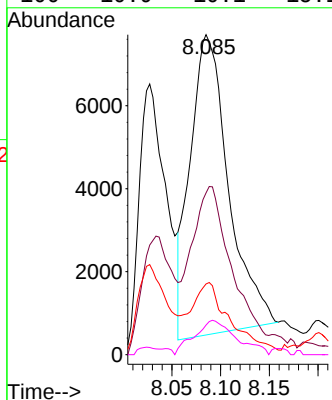

#61
1,2,3-Trichloropropane
Concen: 5.662 ug/L
RT: 11.185 min Scan# 3155
Delta R.T. 0.978 min
Lab File: VV035008.D
Acq: 05 Apr 2024 16:07

Tgt Ion: 75 Resp: 19761

Ion	Ratio	Lower	Upper
75	100		
77	34.0	26.0	39.0
110	2.6	30.5	45.7#

