

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035019.D
 Acq On : 05 Apr 2024 21:28
 Operator : SY/MD
 Sample : P2006-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 06 03:17:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 06 02:25:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	379897	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	367079	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	156115	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	169660	46.243	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.480%
7) Chloroethane-d5	1.532	69	158548	49.754	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.500%
11) 1,1-Dichloroethene-d2	2.059	65	74246	46.166	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.340%
21) 2-Butanone-d5	3.793	46	192996	88.696	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.700%
24) Chloroform-d	4.246	84	280669	45.500	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.000%
26) 1,2-Dichloroethane-d4	4.940	65	183036	46.736	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.480%
32) Benzene-d6	4.960	84	579565	47.003	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	5.985	67	189042	48.280	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.560%
41) Toluene-d8	7.243	98	494427	44.525	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.040%
43) trans-1,3-Dichloroprop...	7.551	79	73813	38.778	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.560%
47) 2-Hexanone-d5	8.024	63	107768	72.797	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	72.800%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	237120	43.977	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.960%
66) 1,2-Dichlorobenzene-d4	11.561	152	174505	49.786	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.580%
Target Compounds						
39) cis-1,3-Dichloropropene	6.911	75	4602	0.883	ug/L	Qvalue # 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035019.D
Acq On : 05 Apr 2024 21:28
Operator : SY/MD
Sample : P2006-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 06 03:17:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

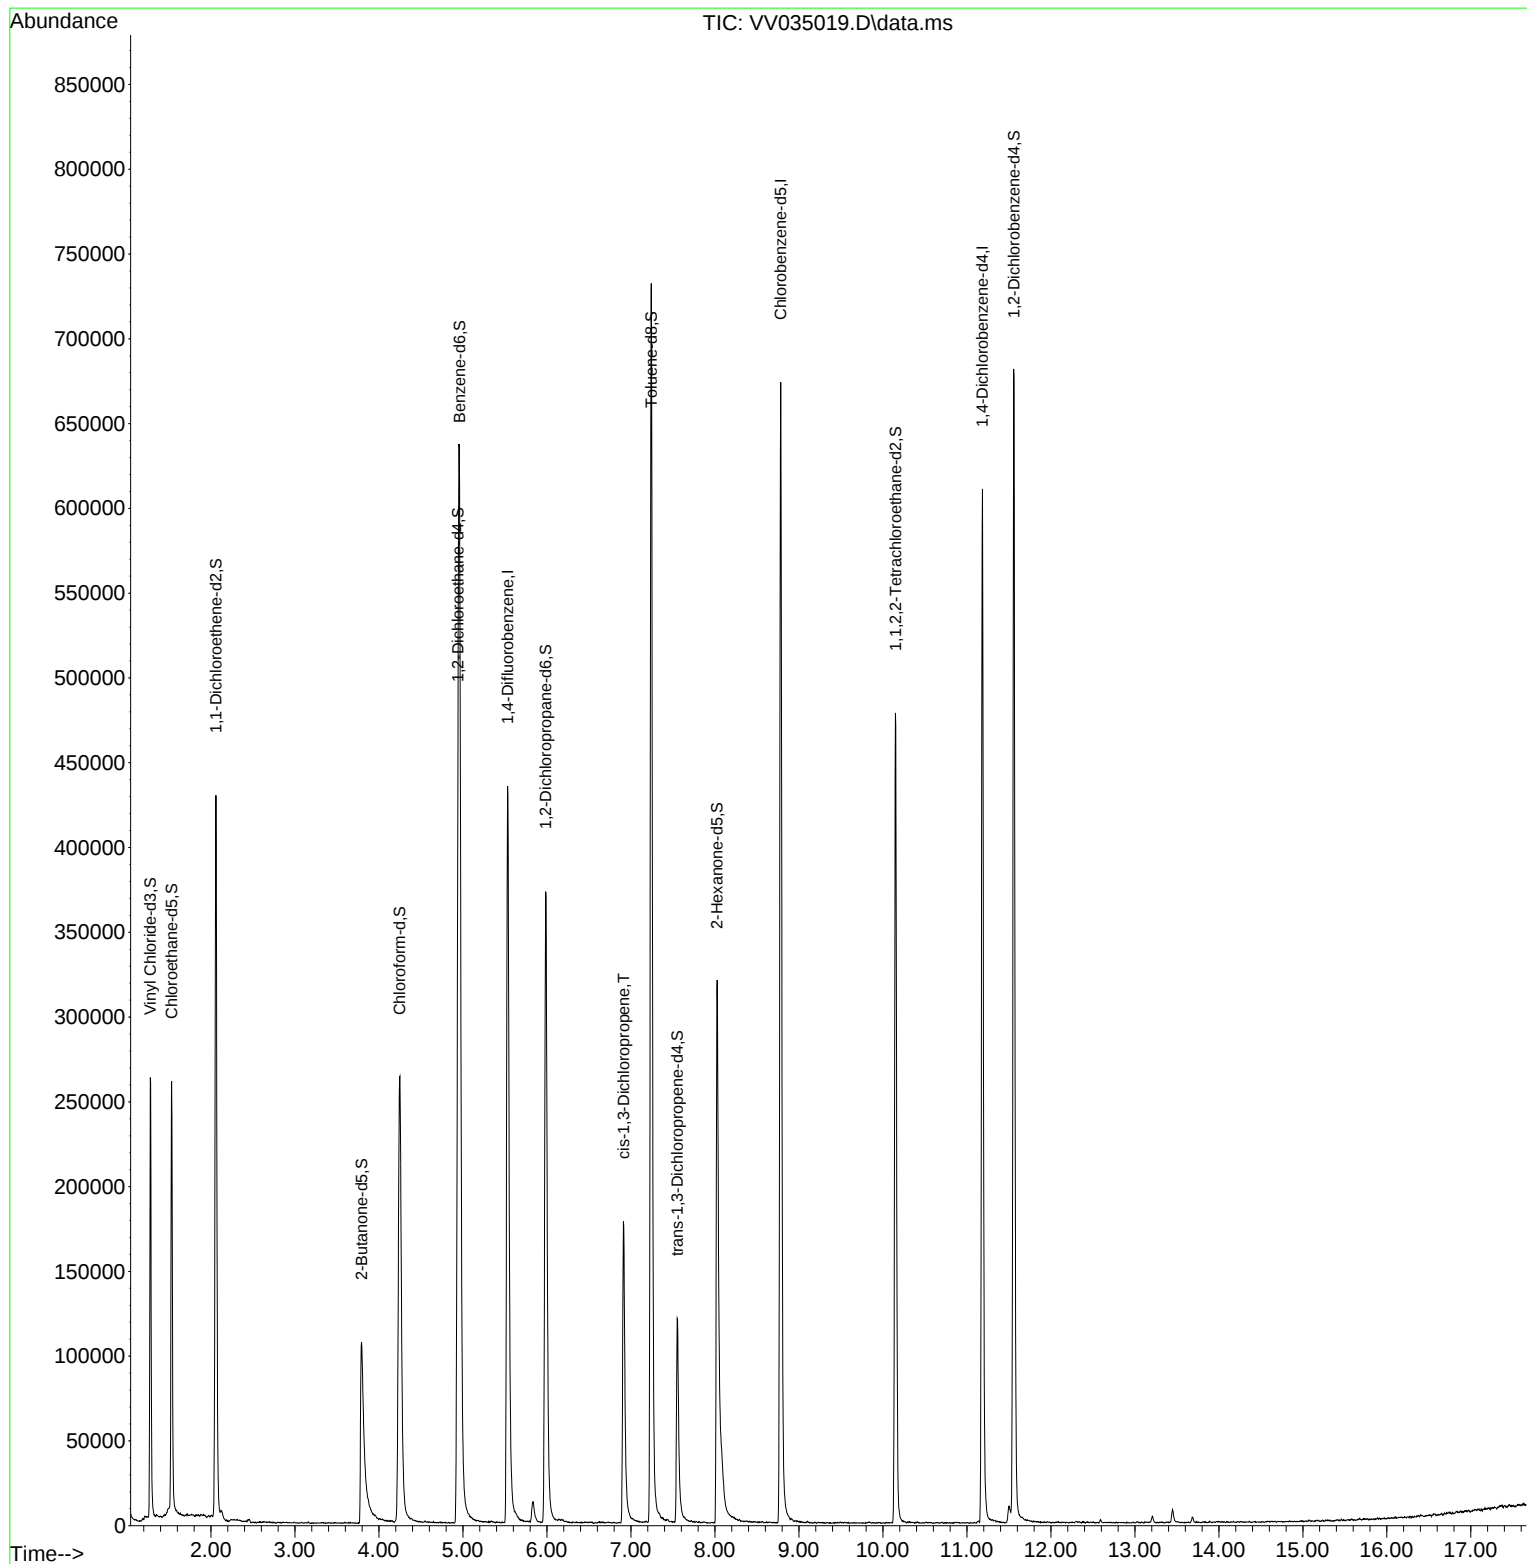

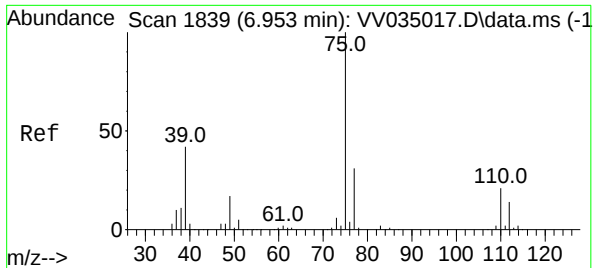

#39
 cis-1,3-Dichloropropene
 Concen: 0.883 ug/L
 RT: 6.911 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV035019.D
 Acq: 05 Apr 2024 21:28

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4602
 Ion Ratio Lower Upper
 75 100
 77 48.7 21.9 40.7#

