




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040524\  
Data File : VV035012.D  
Acq On : 05 Apr 2024 17:43  
Operator : SY/MD  
Sample : P2006-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
MC0R52

## Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024  
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 01:05:13 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Apr 06 00:54:20 2024  
Response via : Initial Calibration

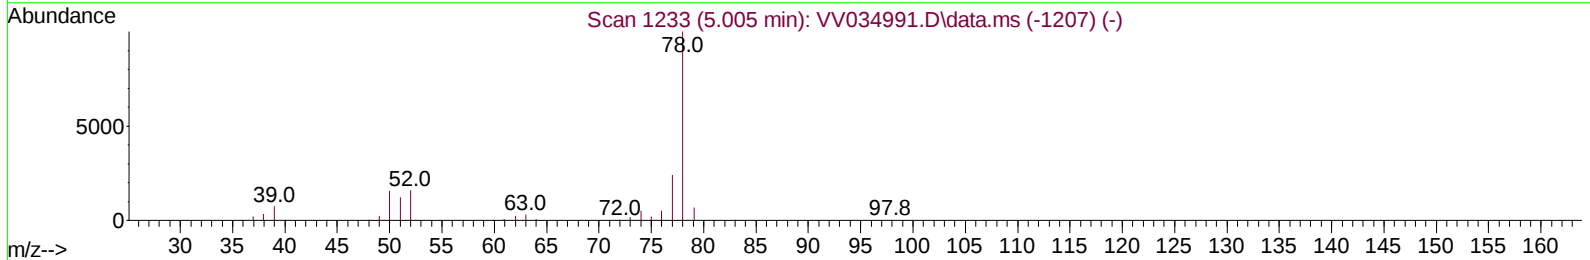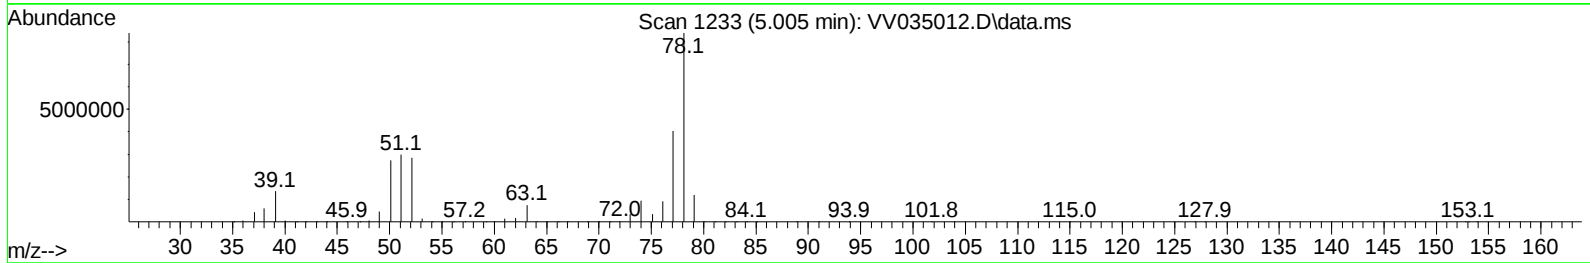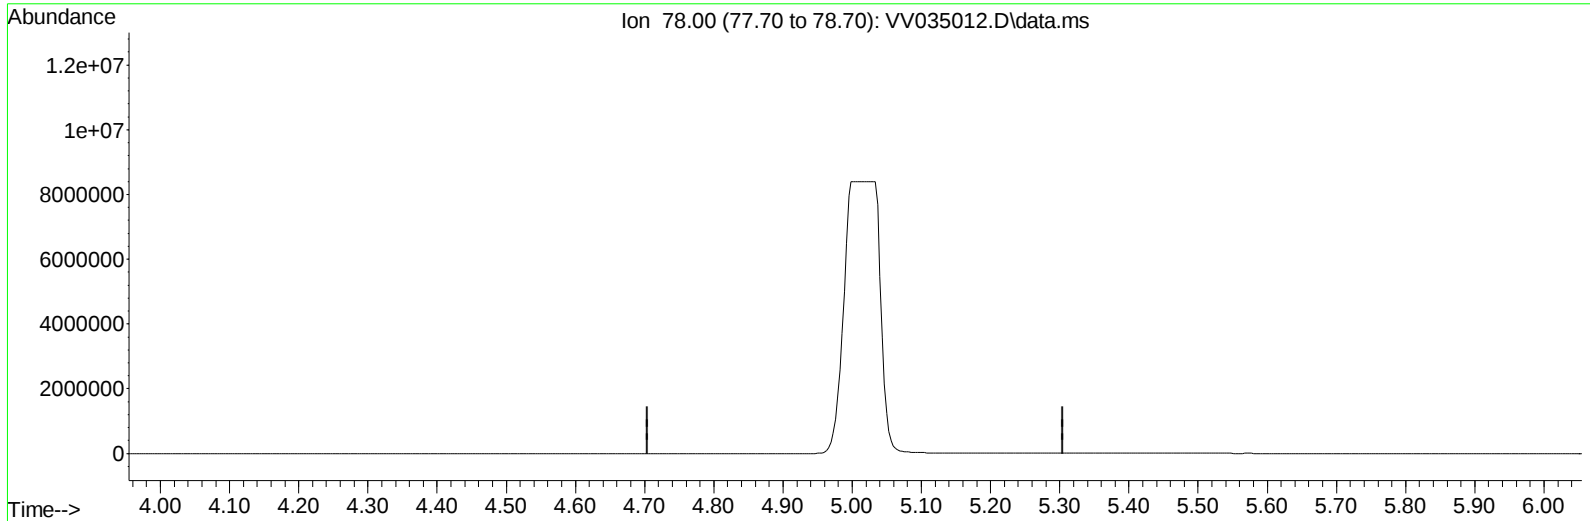

TIC: VV035012.D\data.ms

**(33) Benzene (T)**

5.005min (-5.005) 0.00 ug/L

response 0

| Ion   | Exp%   | Act% |
|-------|--------|------|
| 78.00 | 100.00 | 0.00 |
| 0.00  | 0.00   | 0.00 |
| 0.00  | 0.00   | 0.00 |
| 0.00  | 0.00   | 0.00 |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040524\  
Data File : VV035012.D  
Acq On : 05 Apr 2024 17:43  
Operator : SY/MD  
Sample : P2006-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
MC0R52

## Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024  
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 01:05:13 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Apr 06 00:54:20 2024  
Response via : Initial Calibration

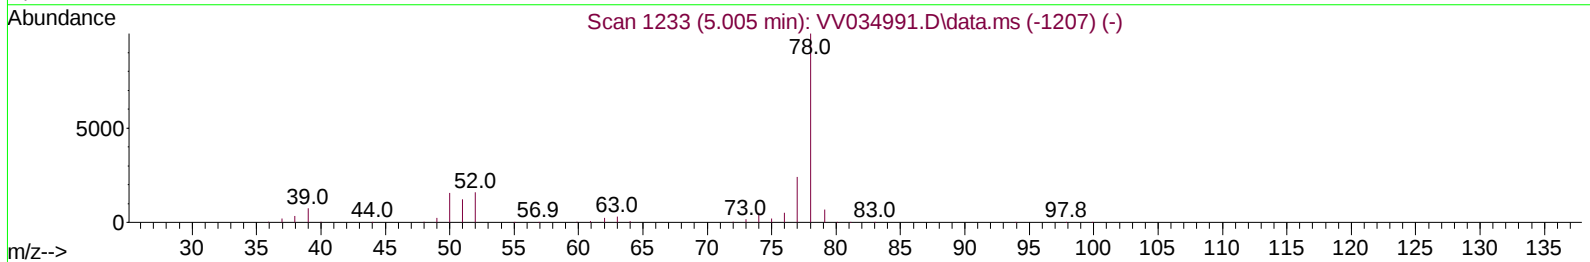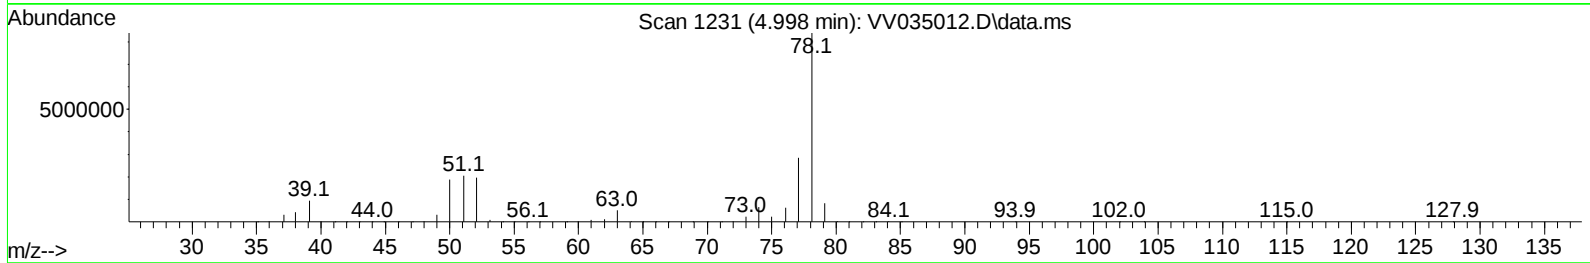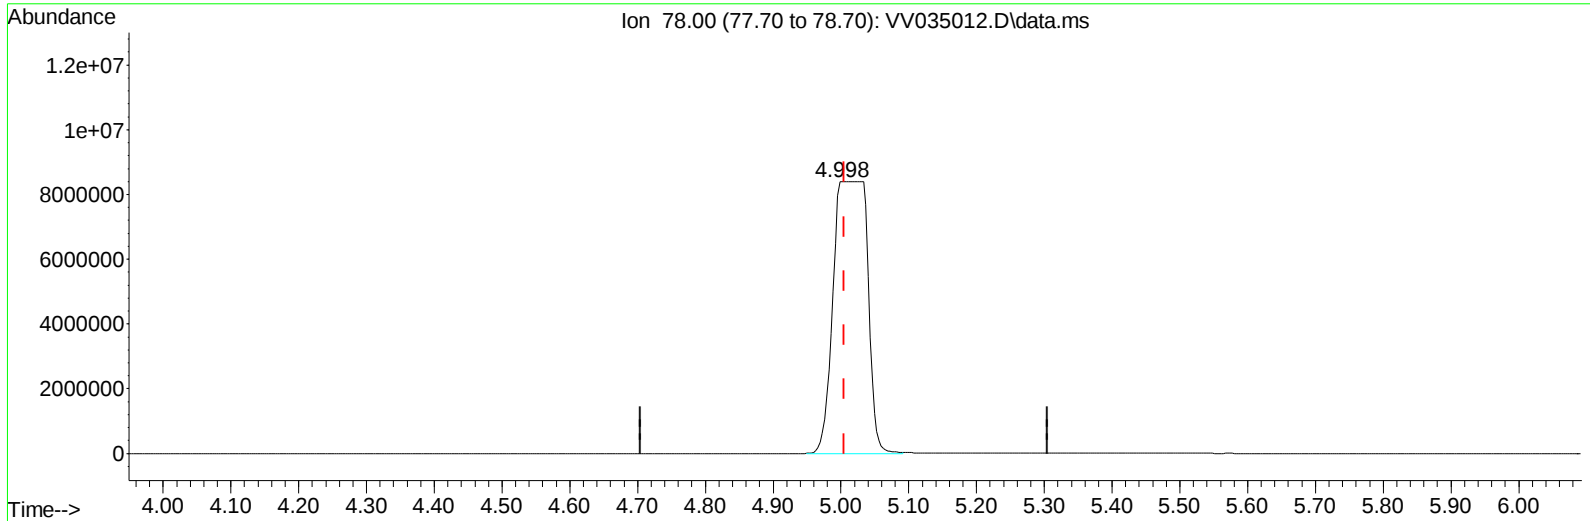

TIC: VV035012.D\data.ms

## (33) Benzene (T)

4.998min (-0.006) 2411.11 ug/L m

response 29420734

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 78.00 | 100.00 | 100.00 |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040524\  
 Data File : VV035012.D  
 Acq On : 05 Apr 2024 17:43  
 Operator : SY/MD  
 Sample : P2006-02  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 MC0R52

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:05:13 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Apr 06 00:54:20 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024  
 Supervised By :Semsettin Yesilyurt 04/08/2024

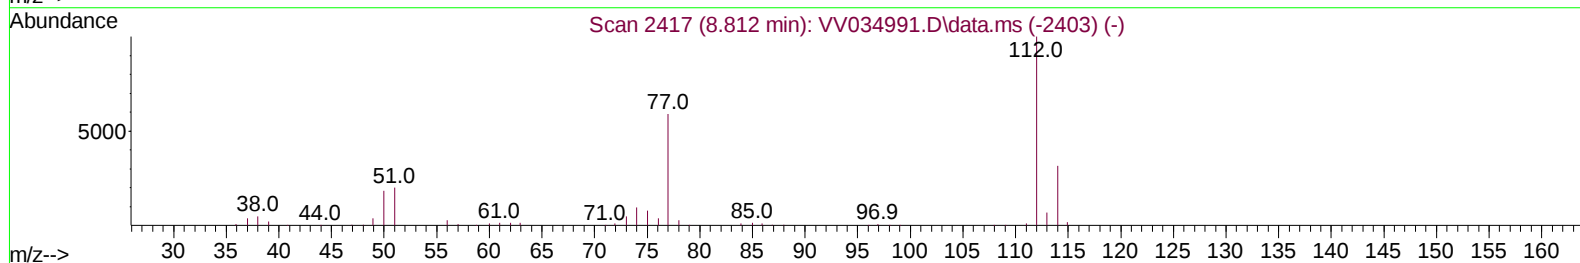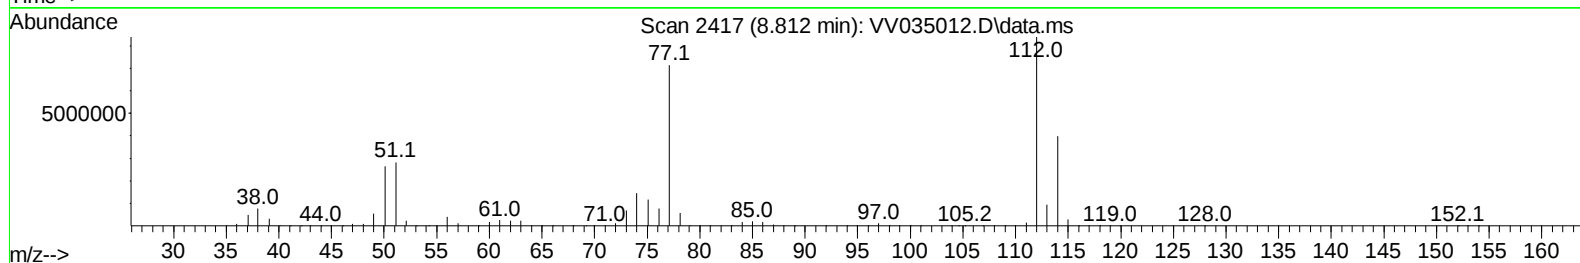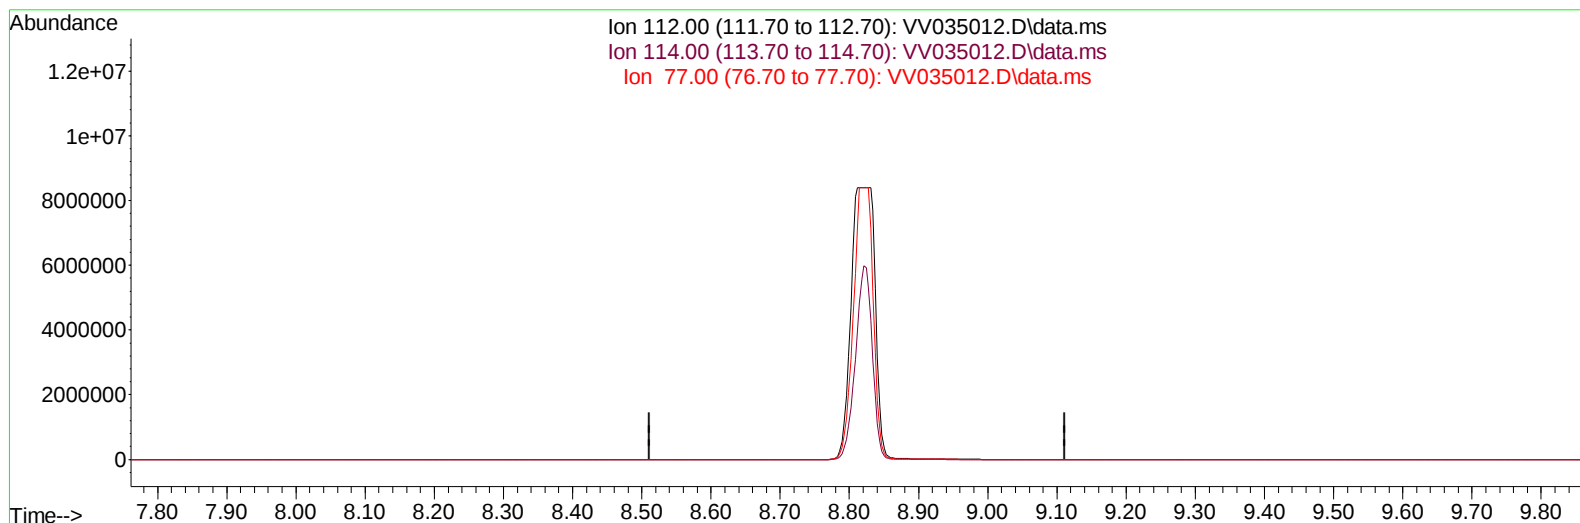

TIC: VV035012.D\data.ms

**(51) Chlorobenzene (T)**

**8.812min (-8.812) 0.00 ug/L**

**response 0**

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 112.00 | 100.00 | 0.00  |
| 114.00 | 31.50  | 0.00# |
| 77.00  | 59.30  | 0.00# |
| 0.00   | 0.00   | 0.00  |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040524\  
 Data File : VV035012.D  
 Acq On : 05 Apr 2024 17:43  
 Operator : SY/MD  
 Sample : P2006-02  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 MC0R52

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:05:13 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Apr 06 00:54:20 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024  
 Supervised By :Semsettin Yesilyurt 04/08/2024

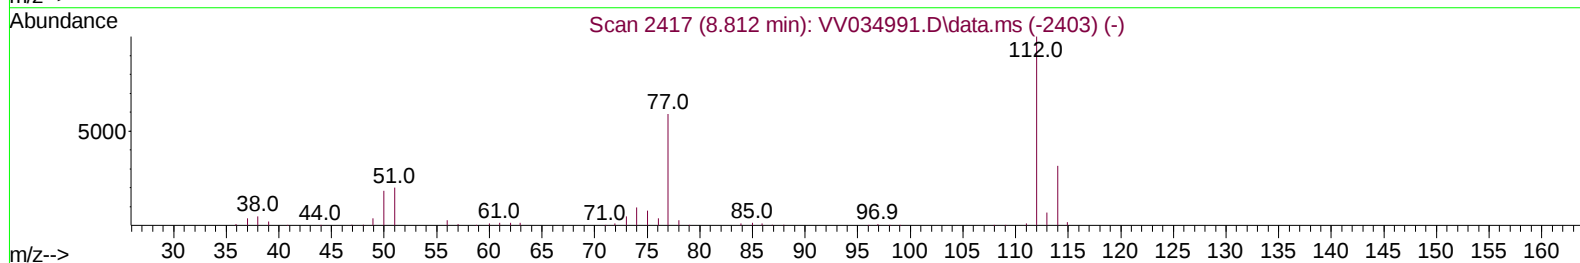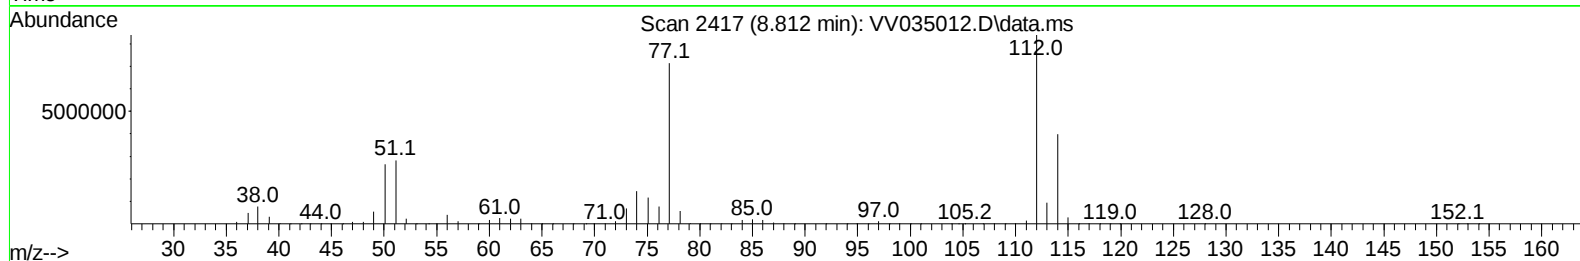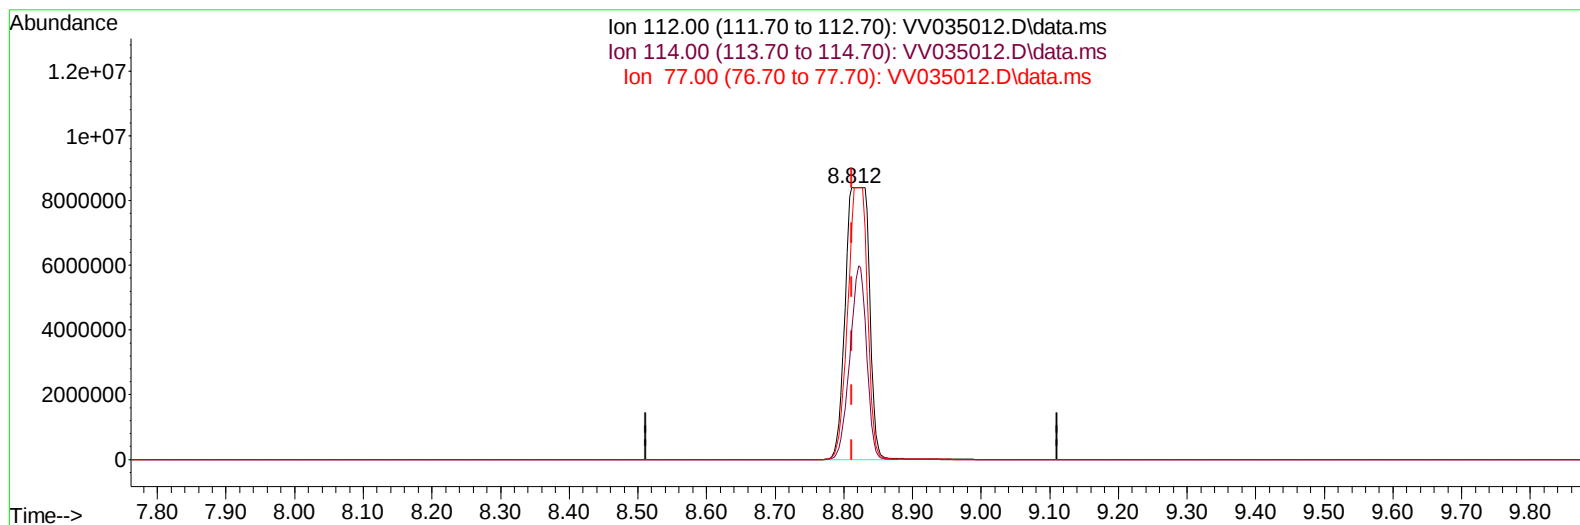

TIC: VV035012.D\data.ms

**(51) Chlorobenzene (T)**

8.812min (+ 0.000) 2435.32 ug/L m

response 20163553

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 112.00 | 100.00 | 100.00 |
| 114.00 | 31.50  | 47.38# |
| 77.00  | 59.30  | 85.25# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040524\  
 Data File : VV035012.D  
 Acq On : 05 Apr 2024 17:43  
 Operator : SY/MD  
 Sample : P2006-02  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 MC0R52

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:05:13 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Apr 06 00:54:20 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024  
 Supervised By :Semsettin Yesilyurt 04/08/2024

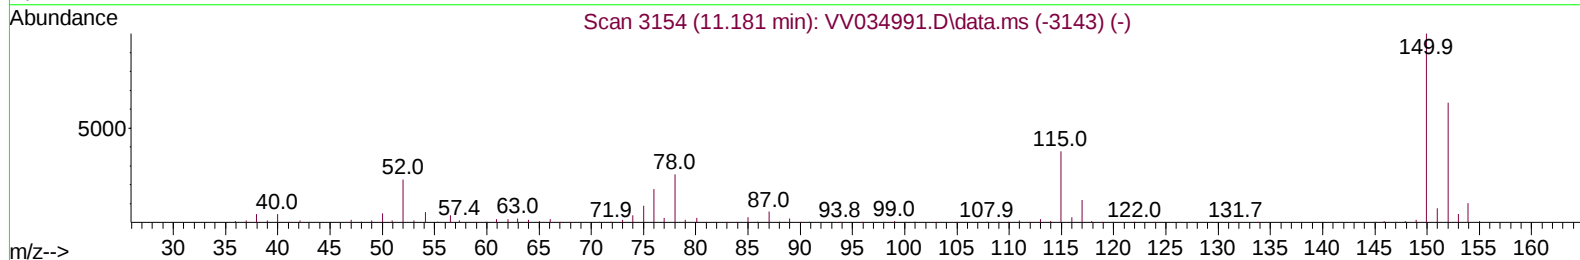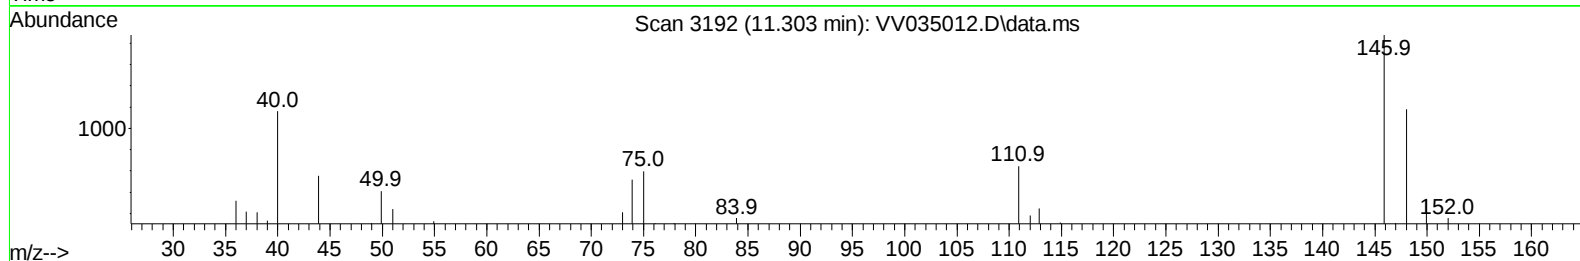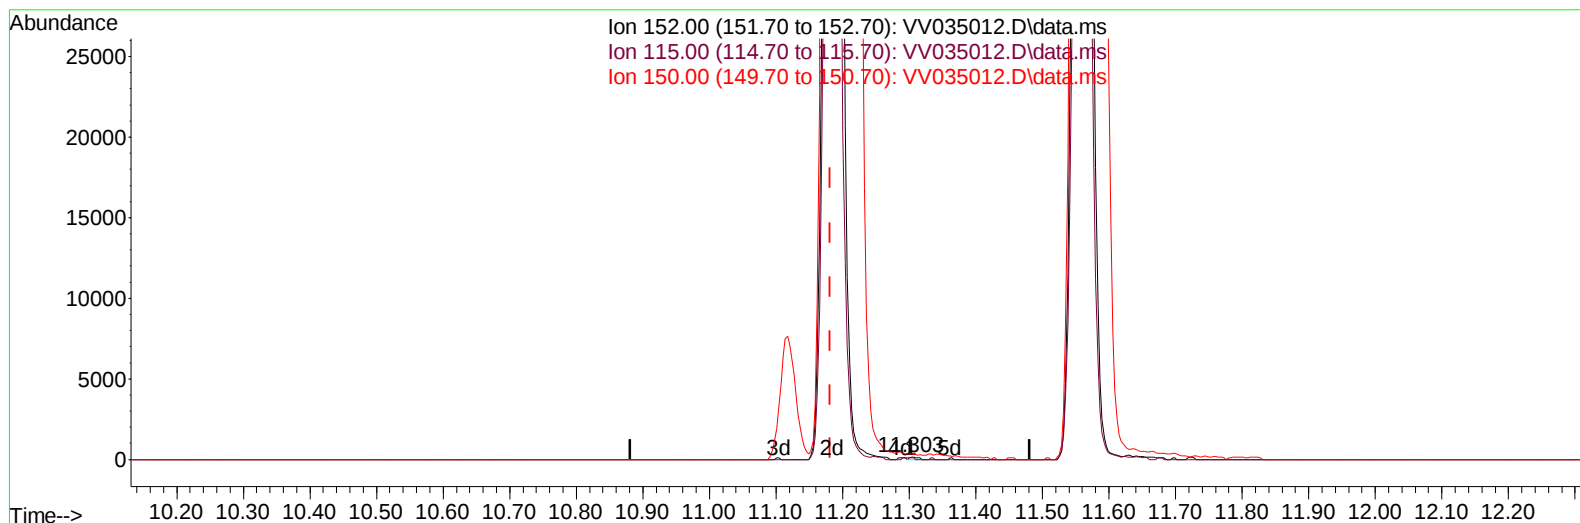

TIC: VV035012.D\data.ms

(58) 1,4-Dichlorobenzene-d4 (I)

11.303min (+ 0.122) 50.00 ug/L

response 128

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 152.00 | 100.00 | 100.00 |
| 115.00 | 60.00  | 34.38  |
| 150.00 | 177.00 | 37.50  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040524\  
Data File : VV035012.D  
Acq On : 05 Apr 2024 17:43  
Operator : SY/MD  
Sample : P2006-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
MC0R52

## Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024  
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 01:05:13 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Apr 06 00:54:20 2024  
Response via : Initial Calibration

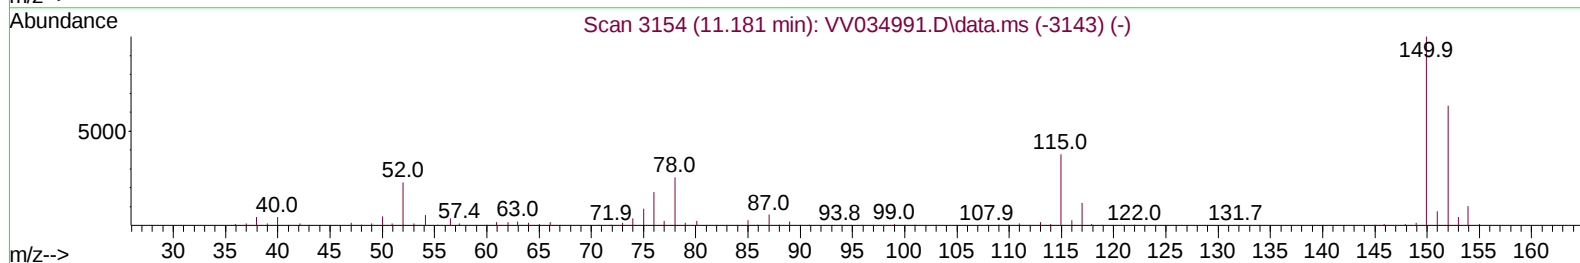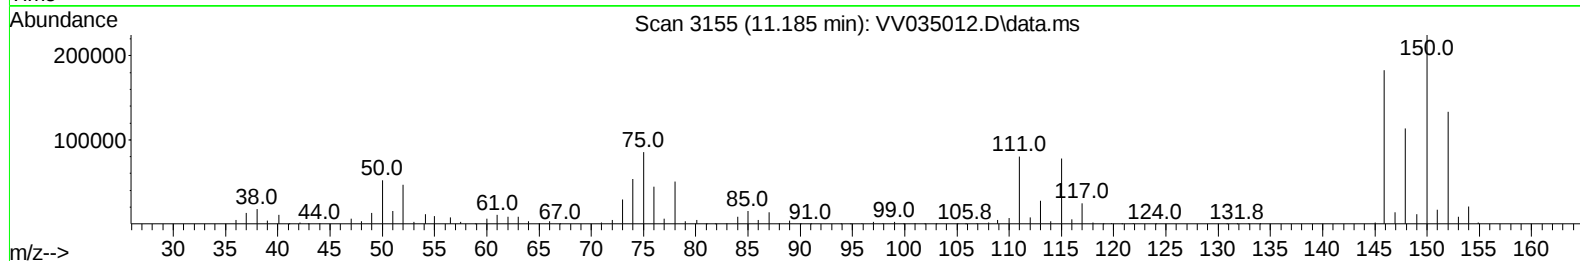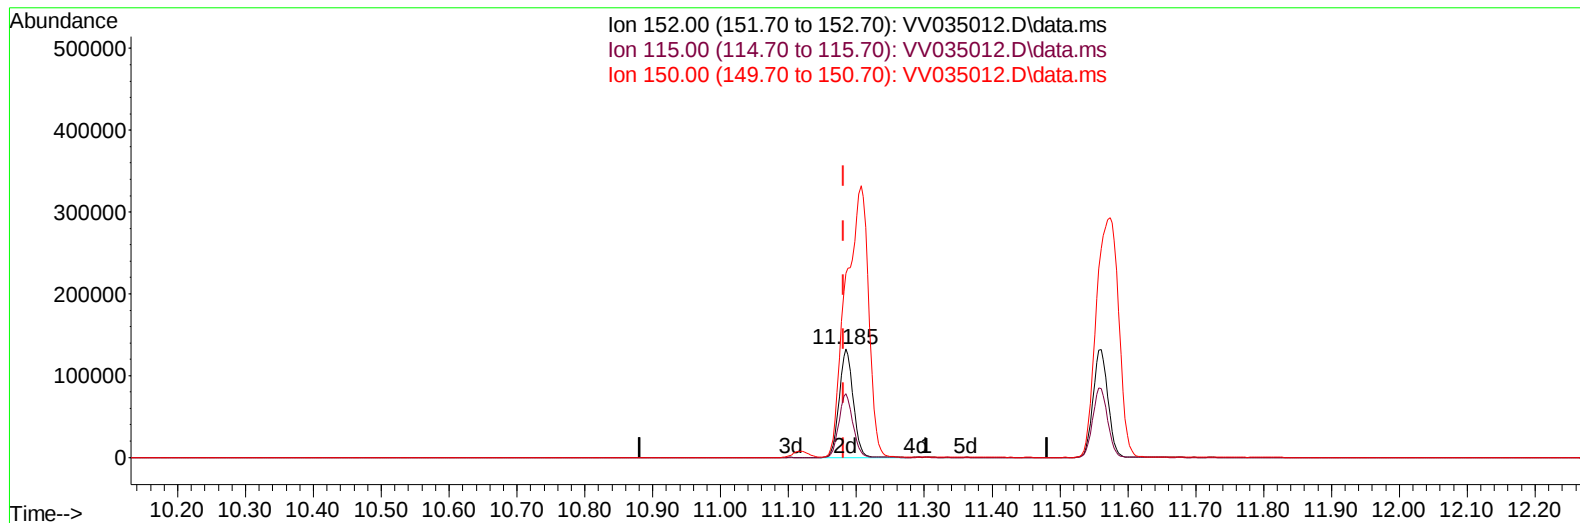

TIC: VV035012.D\data.ms

**(58) 1,4-Dichlorobenzene-d4 (I)**

11.185min (+ 0.003) 50.00 ug/L m

response 189252

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 152.00 | 100.00 | 100.00 |
| 115.00 | 60.00  | 0.02   |
| 150.00 | 177.00 | 0.03   |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040524\  
 Data File : VV035012.D  
 Acq On : 05 Apr 2024 17:43  
 Operator : SY/MD  
 Sample : P2006-02  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 MC0R52

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:05:13 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Apr 06 00:54:20 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024  
 Supervised By :Semsettin Yesilyurt 04/08/2024

| Compound                      | R.T.     | Q     | Ion       | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|----------|-------|-----------|----------|--------|----------|----------|
| -----                         |          |       |           |          |        |          |          |
| Internal Standards            |          |       |           |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.532    | 114   |           | 357908   | 50.000 | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.789    | 117   |           | 374200   | 50.000 | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.185   | 152   |           | 189252m  | 50.000 | ug/L     | 0.00     |
| System Monitoring Compounds   |          |       |           |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.278    | 65    |           | 139657   | 40.404 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 135 |           | Recovery | =      | 80.800%  |          |
| 7) Chloroethane-d5            | 1.529    | 69    |           | 139571   | 46.489 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 130 |           | Recovery | =      | 92.980%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.059    | 65    |           | 60207    | 39.736 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 |           | Recovery | =      | 79.480%  |          |
| 21) 2-Butanone-d5             | 3.789    | 46    |           | 182706   | 89.126 | ug/L     | 0.00     |
| Spiked Amount 100.000         | Range 40 | - 130 |           | Recovery | =      | 89.130%  |          |
| 24) Chloroform-d              | 4.246    | 84    |           | 270770   | 46.592 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 |           | Recovery | =      | 93.180%  |          |
| 26) 1,2-Dichloroethane-d4     | 4.944    | 65    |           | 186350   | 50.506 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 |           | Recovery | =      | 101.020% |          |
| 32) Benzene-d6                | 4.963    | 84    |           | 556287   | 44.257 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 |           | Recovery | =      | 88.520%  |          |
| 36) 1,2-Dichloropropane-d6    | 5.985    | 67    |           | 178585   | 44.742 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 120 |           | Recovery | =      | 89.480%  |          |
| 41) Toluene-d8                | 7.243    | 98    |           | 467766   | 41.322 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 |           | Recovery | =      | 82.640%  |          |
| 43) trans-1,3-Dichloroprop... | 7.551    | 79    |           | 78277    | 40.340 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 |           | Recovery | =      | 80.680%  |          |
| 47) 2-Hexanone-d5             | 8.024    | 63    |           | 115972   | 76.848 | ug/L     | 0.00     |
| Spiked Amount 100.000         | Range 45 | - 130 |           | Recovery | =      | 76.850%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.149   | 84    |           | 245701   | 44.701 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 65 | - 120 |           | Recovery | =      | 89.400%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.561   | 152   |           | 199697   | 46.997 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 |           | Recovery | =      | 94.000%  |          |
| Target Compounds              |          |       |           |          |        |          |          |
|                               |          |       |           |          |        |          | Qvalue   |
| 33) Benzene                   | 4.998    | 78    | 29420734m | 2411.114 | ug/L   |          |          |
| 51) Chlorobenzene             | 8.812    | 112   | 20163553m | 2435.324 | ug/L   |          |          |
| 64) 1,3-Dichlorobenzene       | 11.117   | 146   | 119466    | 18.737   | ug/L   |          | 99       |
| 65) 1,4-Dichlorobenzene       | 11.207   | 146   | 4542978   | 700.666  | ug/L   |          | 98       |
| 67) 1,2-Dichlorobenzene       | 11.577   | 146   | 3508351   | 552.365  | ug/L   |          | 100      |
| 70) 1,2,4-trichlorobenzene    | 13.201   | 180   | 32667     | 7.739    | ug/L   |          | 99       |
| -----                         |          |       |           |          |        |          |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040524\  
Data File : VV035012.D  
Acq On : 05 Apr 2024 17:43  
Operator : SY/MD  
Sample : P2006-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
MC0R52

## Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024  
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 01:05:13 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Apr 06 00:54:20 2024  
Response via : Initial Calibration

