




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

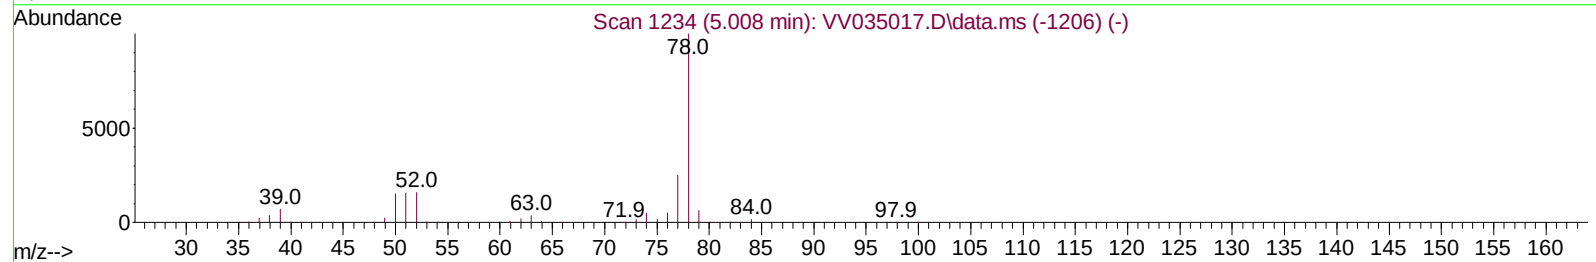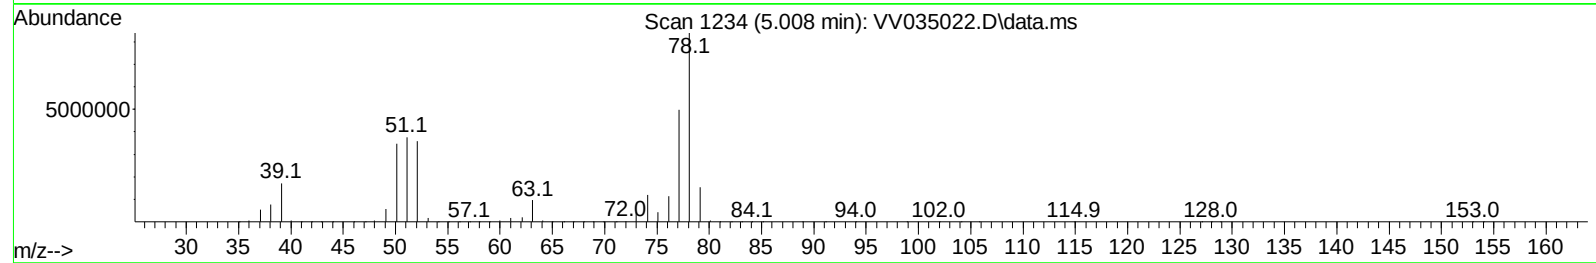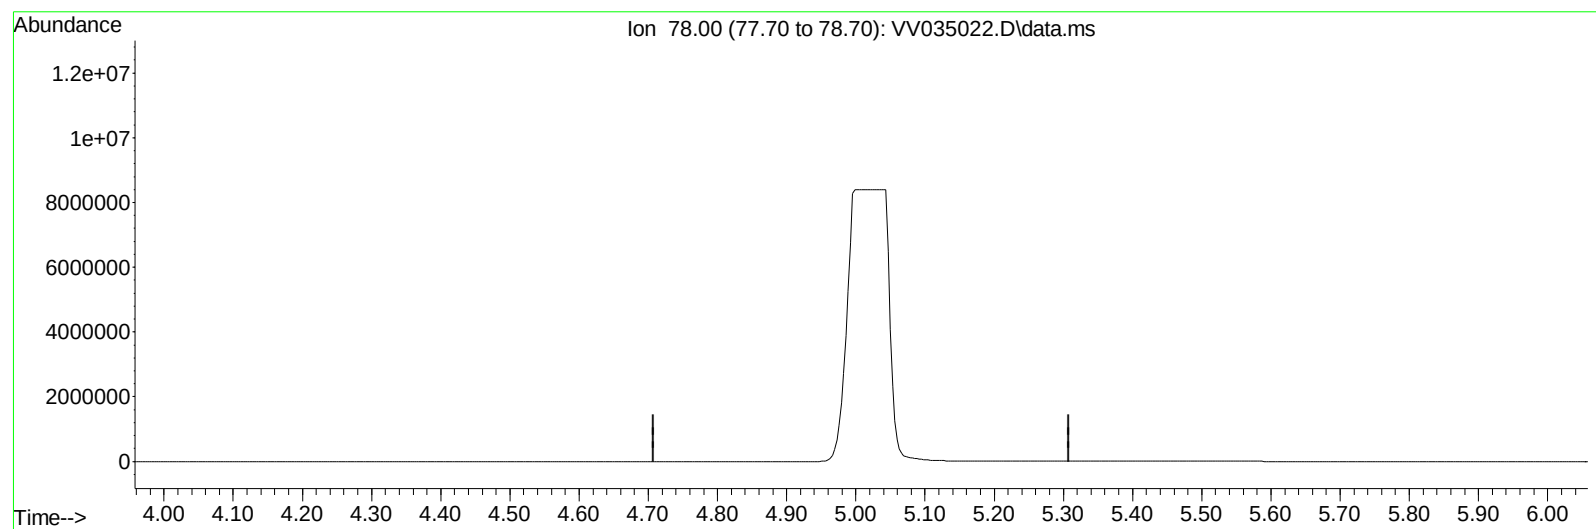

TIC: VV035022.D\data.ms

(33) Benzene (T)

5.008min (-5.008) 0.00 ug/L

response 0

Ion	Exp%	Act%
78.00	100.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

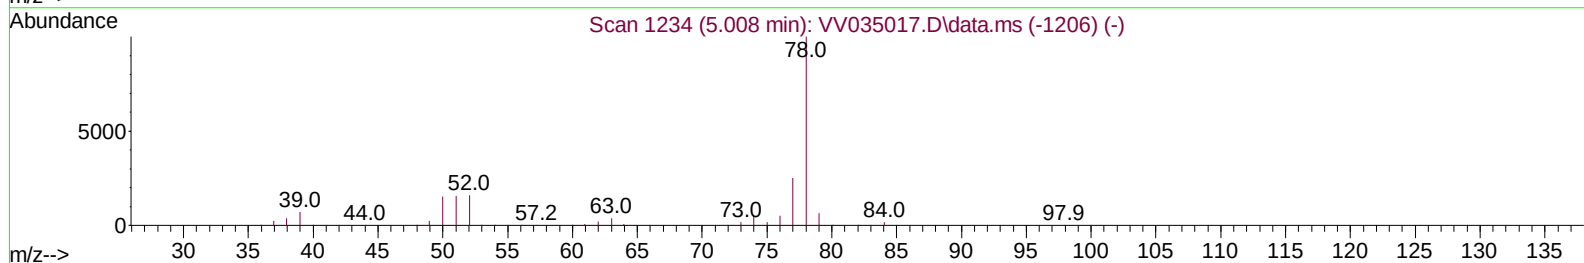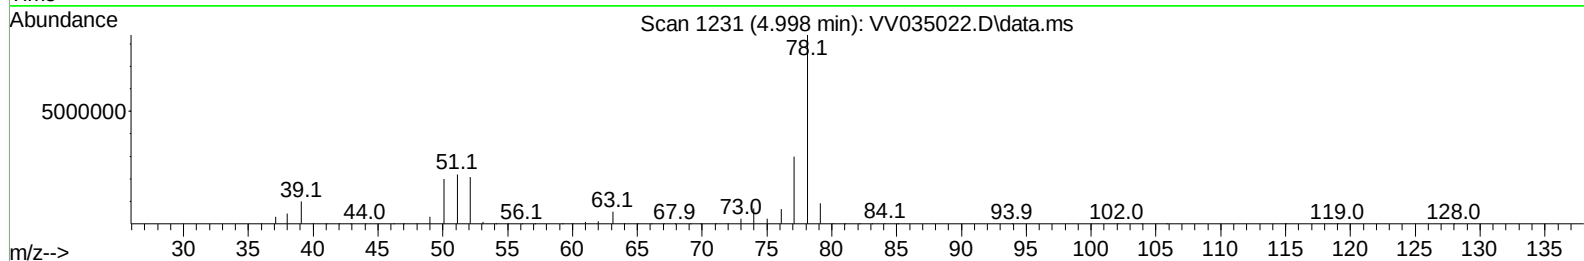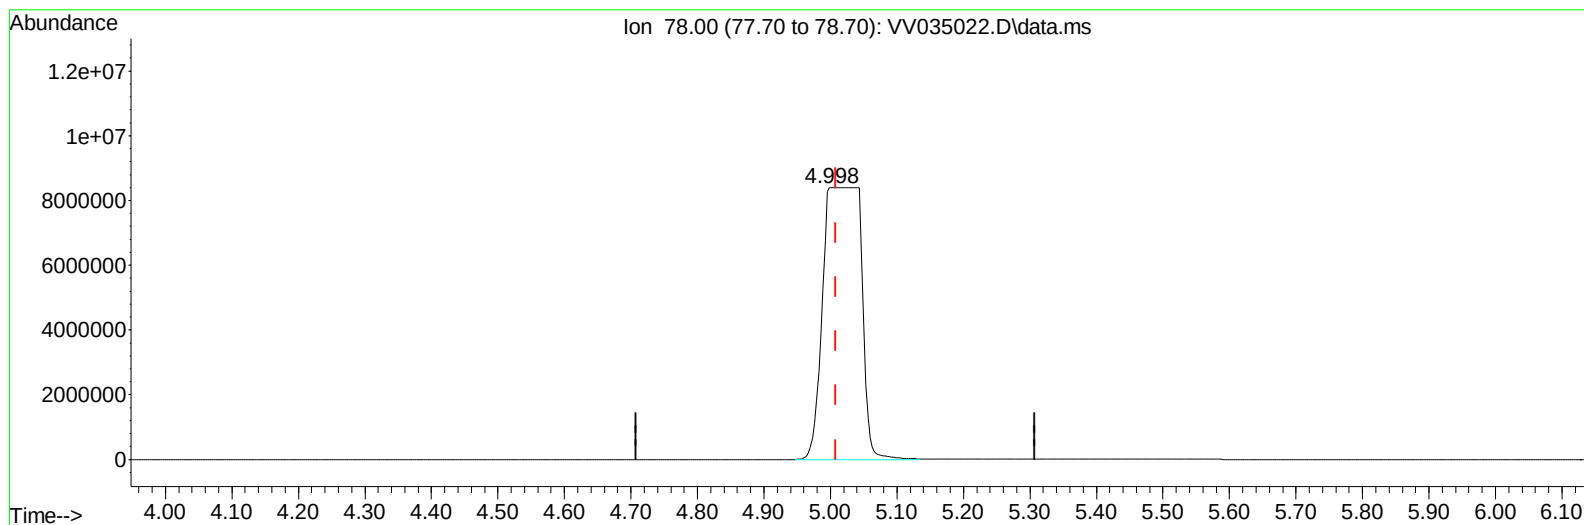

TIC: VV035022.D\data.ms

(33) Benzene (T)

4.998min (-0.010) 2526.25 ug/L m

response 33542757

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

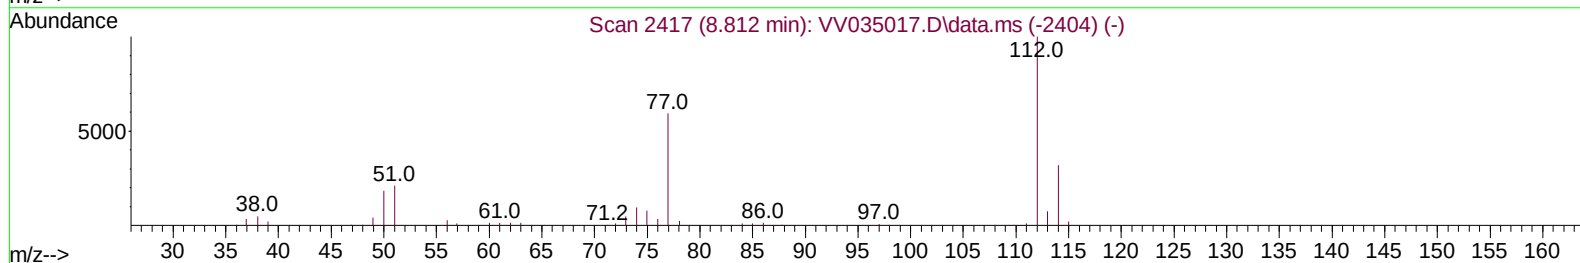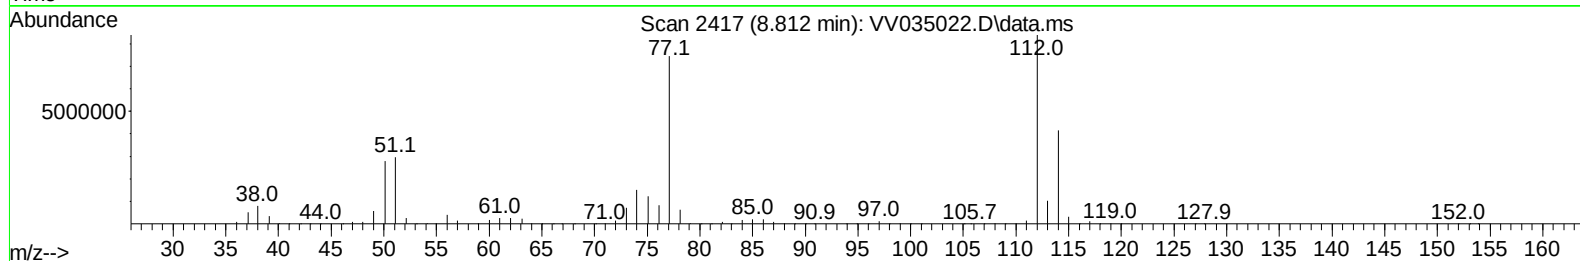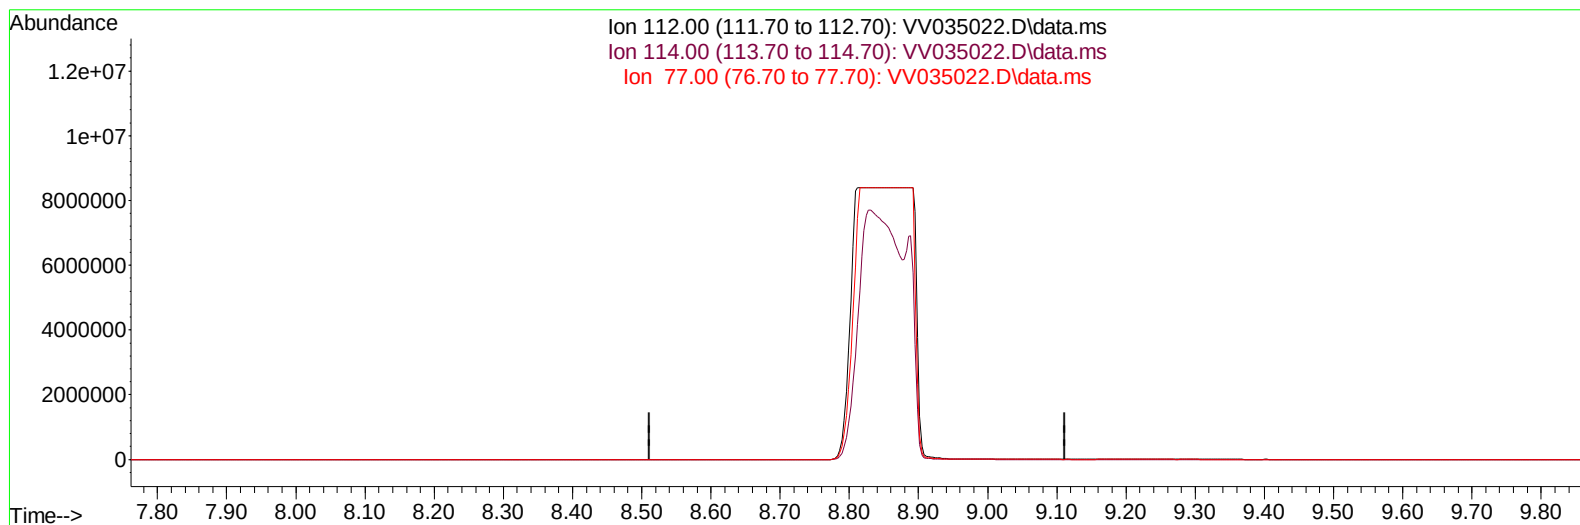

TIC: VV035022.D\data.ms

(51) Chlorobenzene (T)

8.812min (-8.812) 0.00 ug/L

response 0

Ion	Exp%	Act%
112.00	100.00	0.00
114.00	31.50	0.00#
77.00	59.30	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

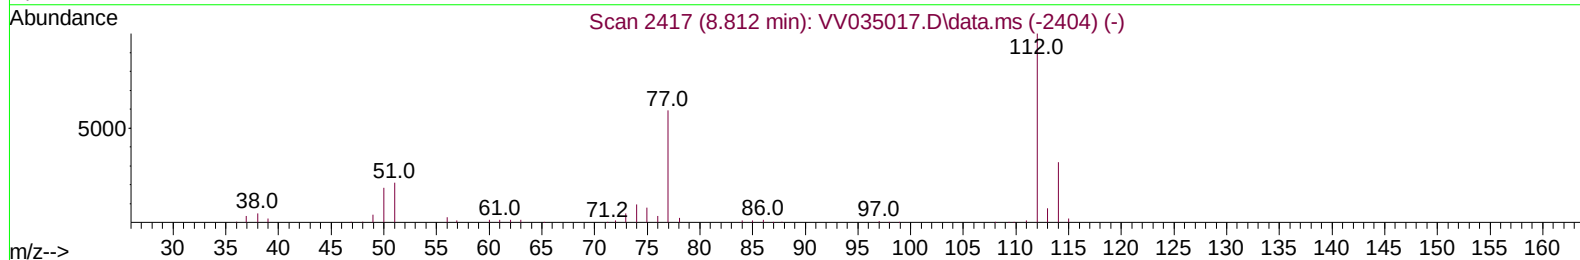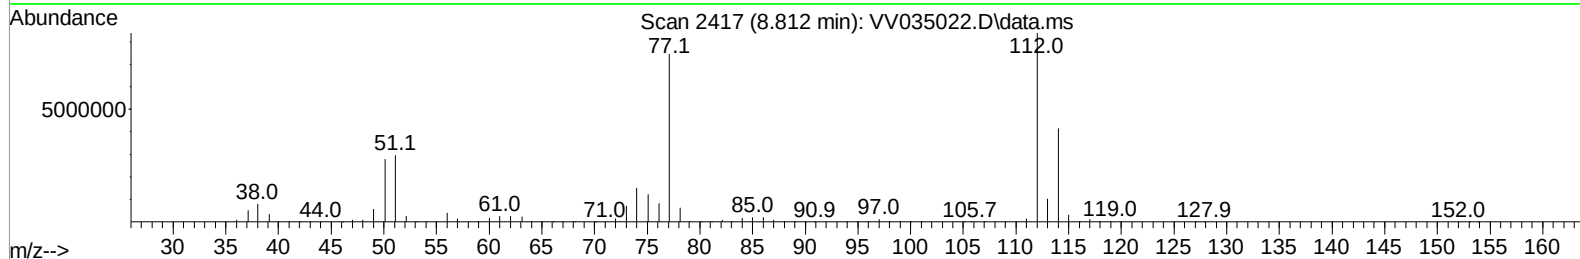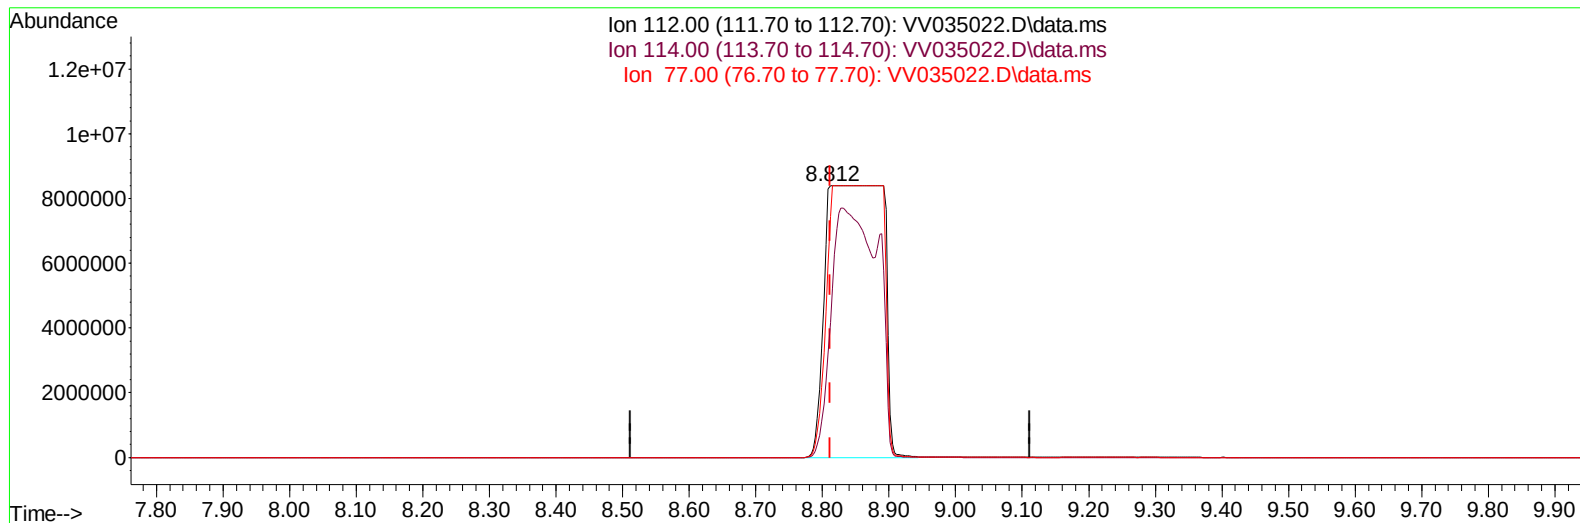

TIC: VV035022.D\data.ms

(51) Chlorobenzene (T)

8.812min (+ 0.000) 5555.81 ug/L m

response 50054706

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	31.50	49.63#
77.00	59.30	88.76#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035022.D
 Acq On : 05 Apr 2024 22:40
 Operator : SY/MD
 Sample : P2006-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 03:18:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 06 02:25:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
 Supervised By :Semsettin Yesilyurt 04/08/2024

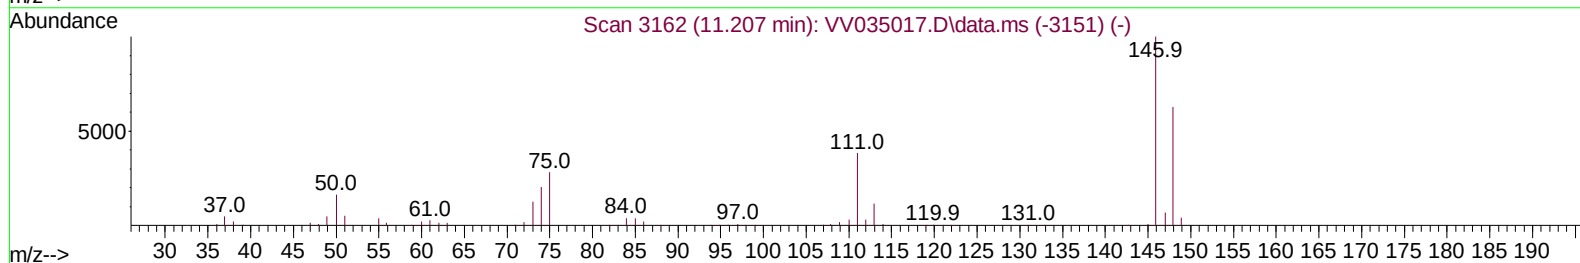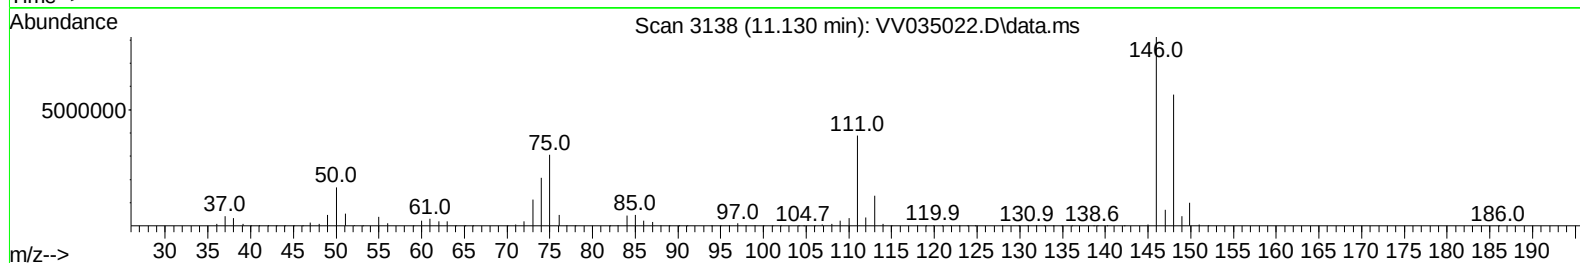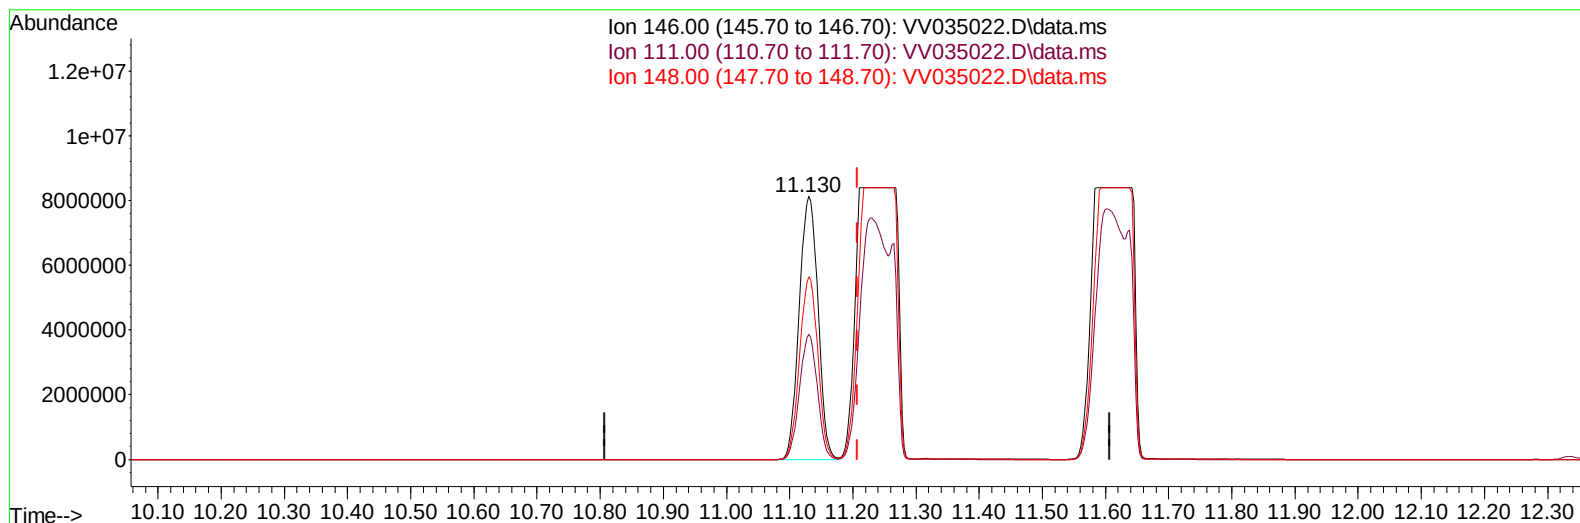

TIC: VV035022.D\data.ms

(65) 1,4-Dichlorobenzene (T)

11.130min (-0.077) 2045.60 ug/L

response 16792586

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	39.10	47.65
148.00	63.20	69.54
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

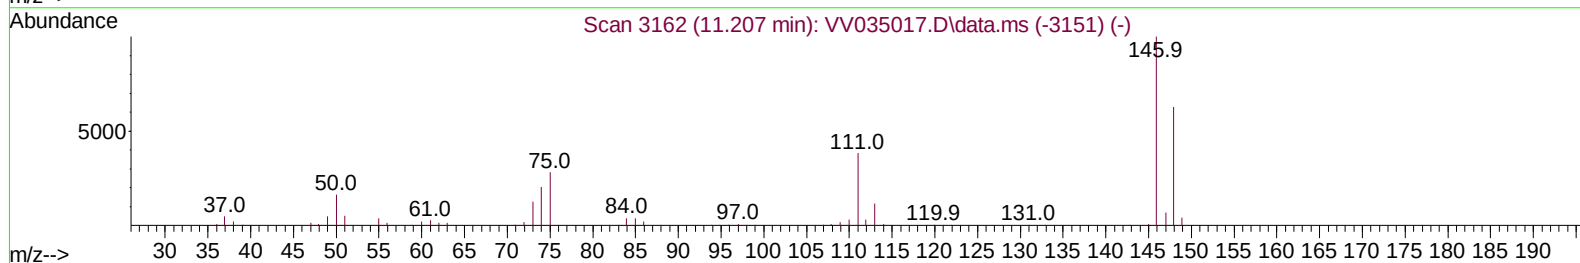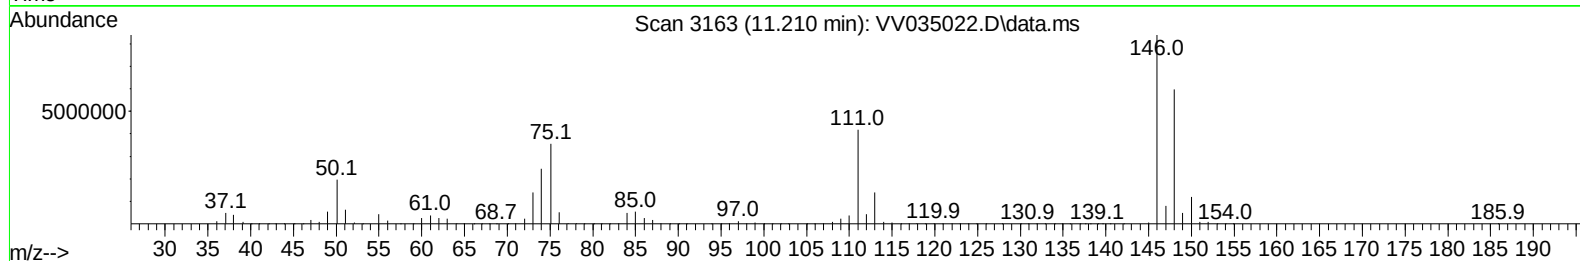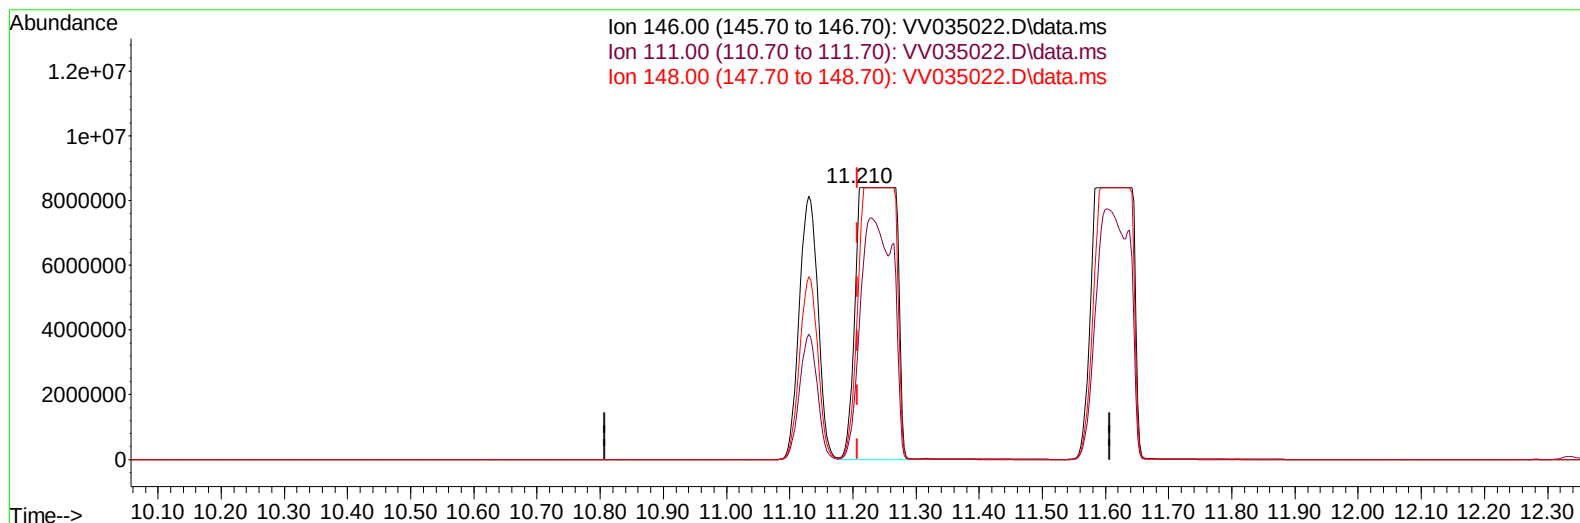

TIC: VV035022.D\data.ms

(65) 1,4-Dichlorobenzene (T)

11.210min (+ 0.003) 4535.21 ug/L m

response 37230186

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	39.10	49.73
148.00	63.20	71.07
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

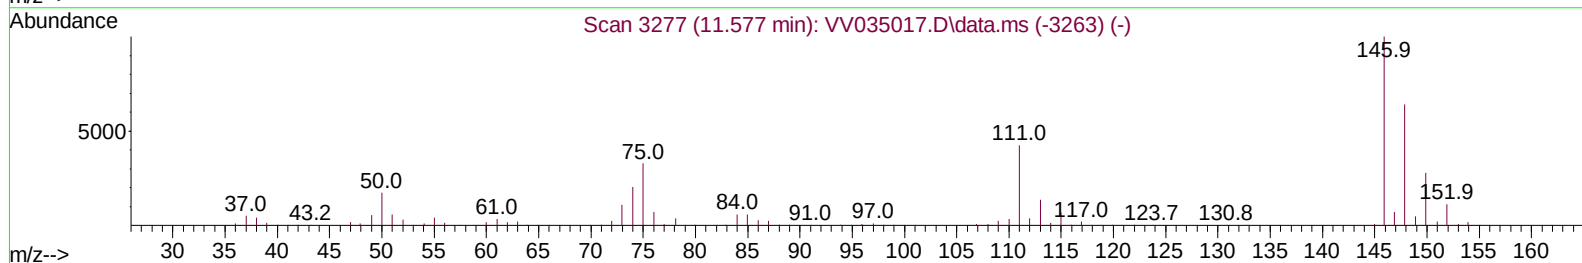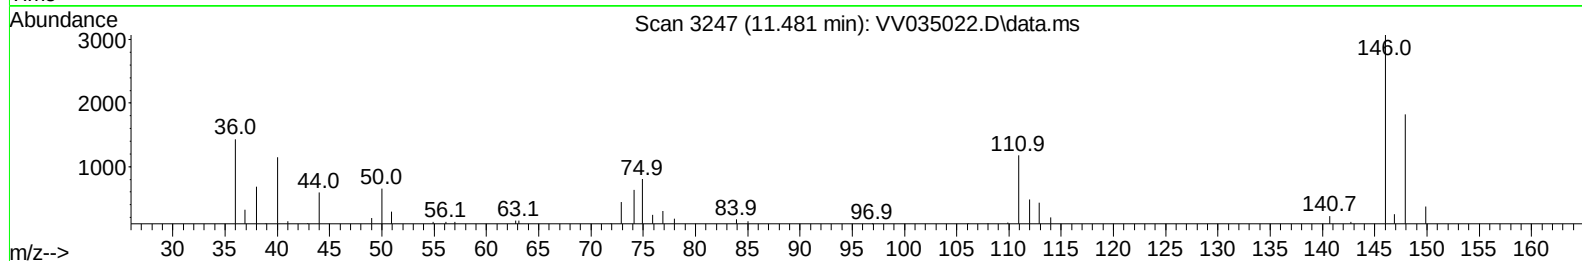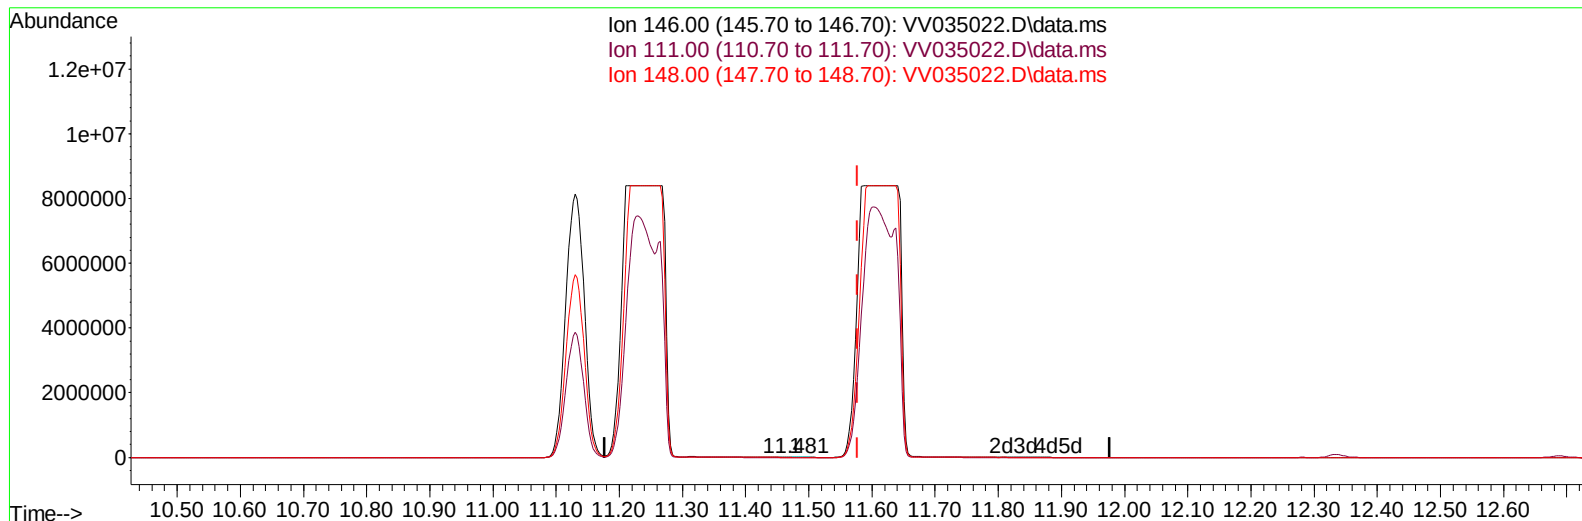

TIC: VV035022.D\data.ms

(67) 1,2-Dichlorobenzene (T)

11.481min (-0.096) 0.05 ug/L

response 402

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	43.30	38.23
148.00	64.40	59.36
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

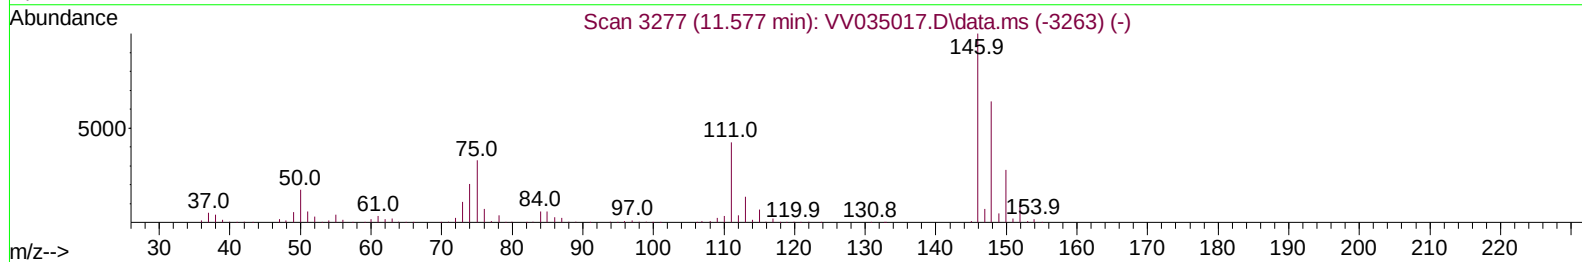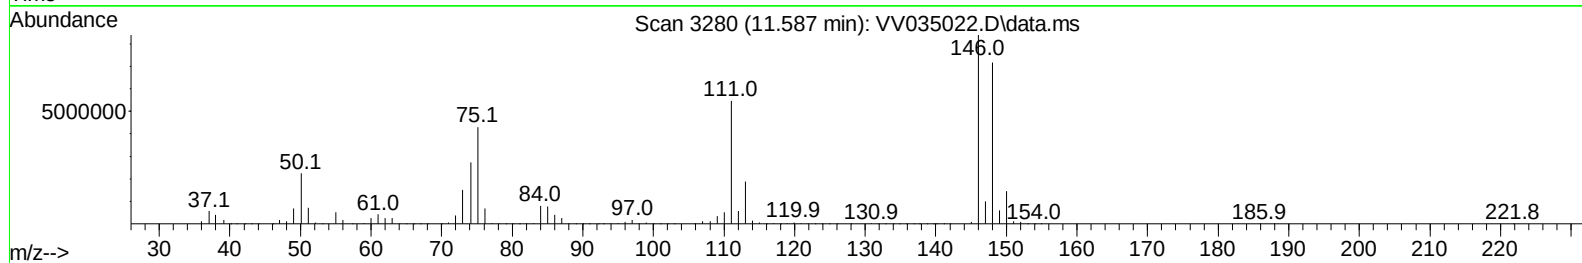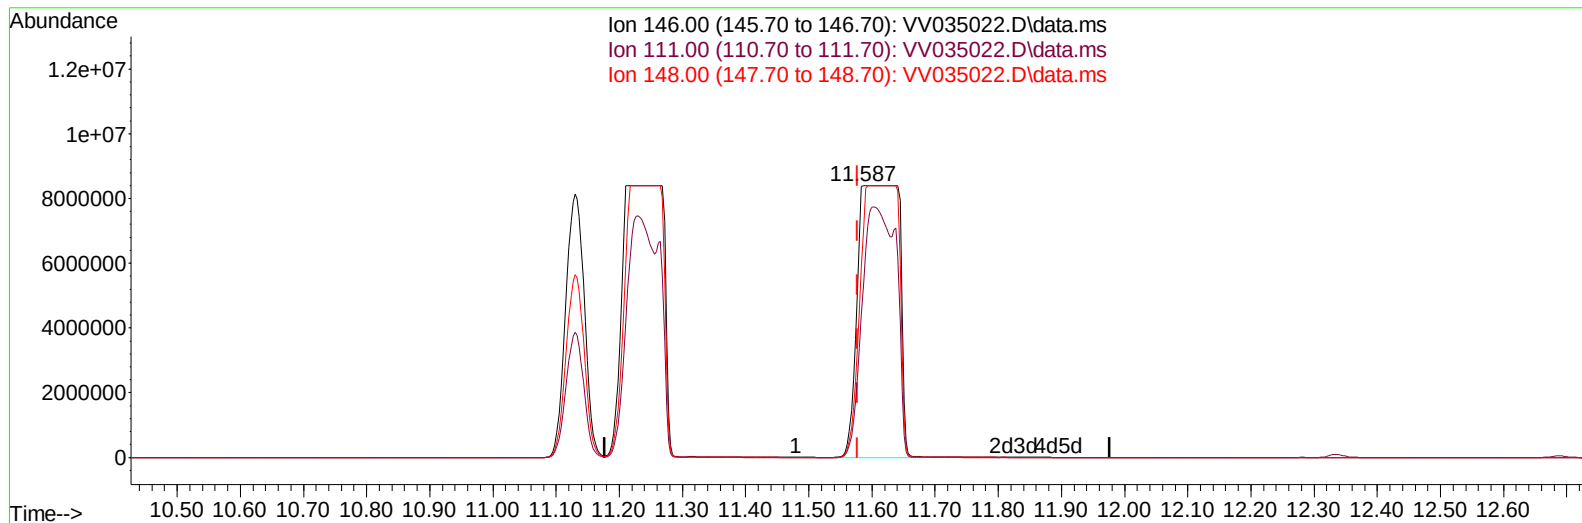

TIC: VV035022.D\data.ms

(67) 1,2-Dichlorobenzene (T)

11.587min (+ 0.010) 4682.60 ug/L m

response 37655764

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	43.30	64.95#
148.00	64.40	85.46#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

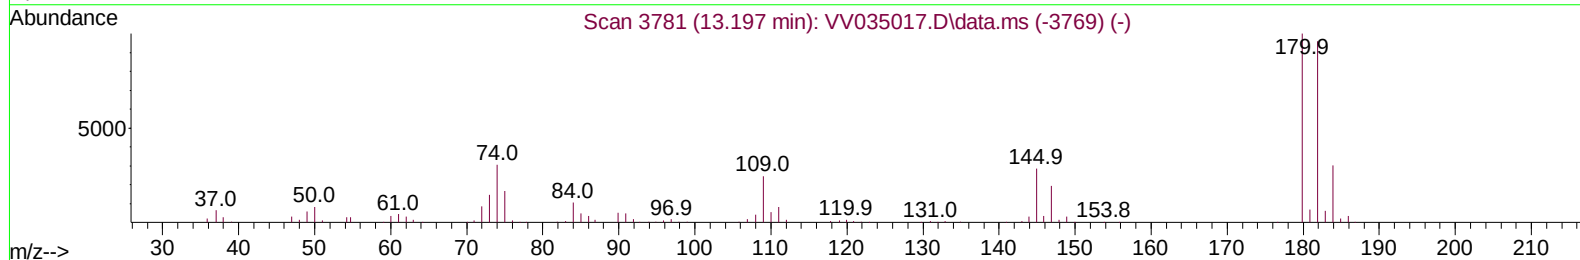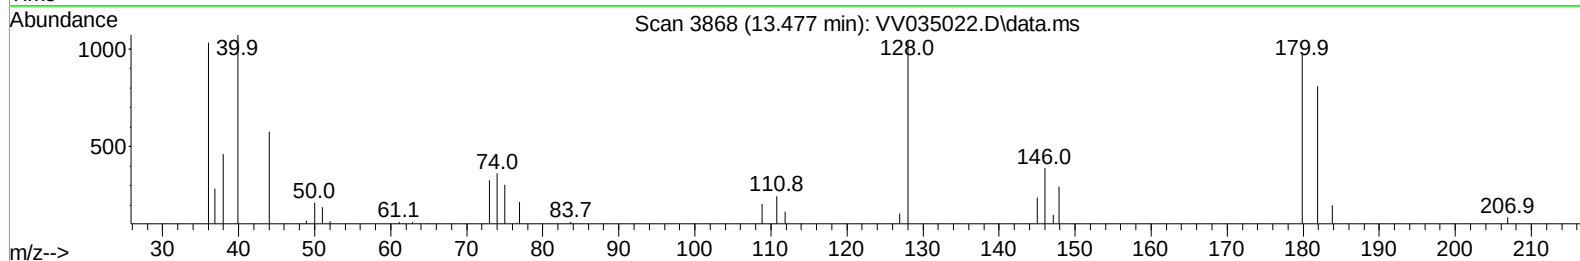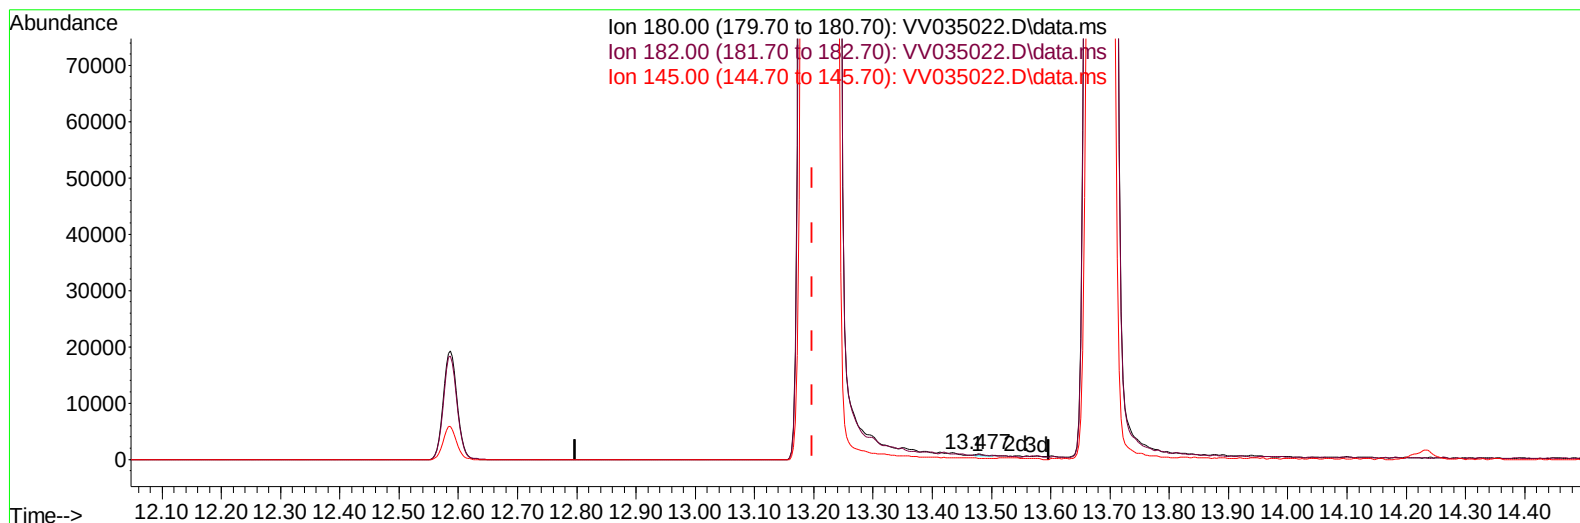

TIC: VV035022.D\data.ms

(70) 1,2,4-trichlorobenzene (T)

13.477min (+ 0.280) 0.05 ug/L

response 252

Ion	Exp%	Act%
180.00	100.00	100.00
182.00	94.50	0.00#
145.00	30.10	48.02#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

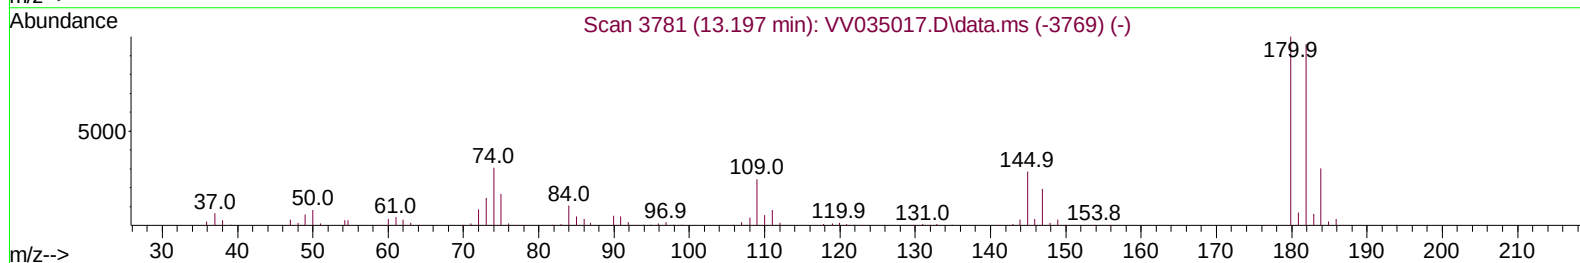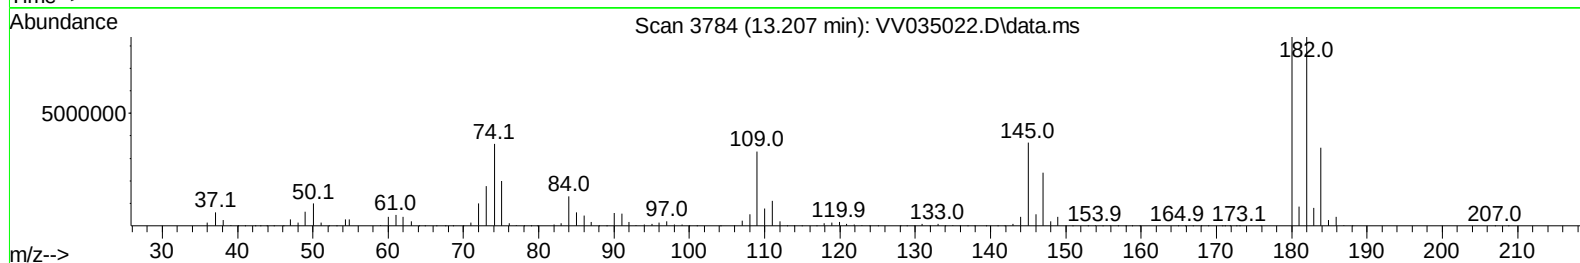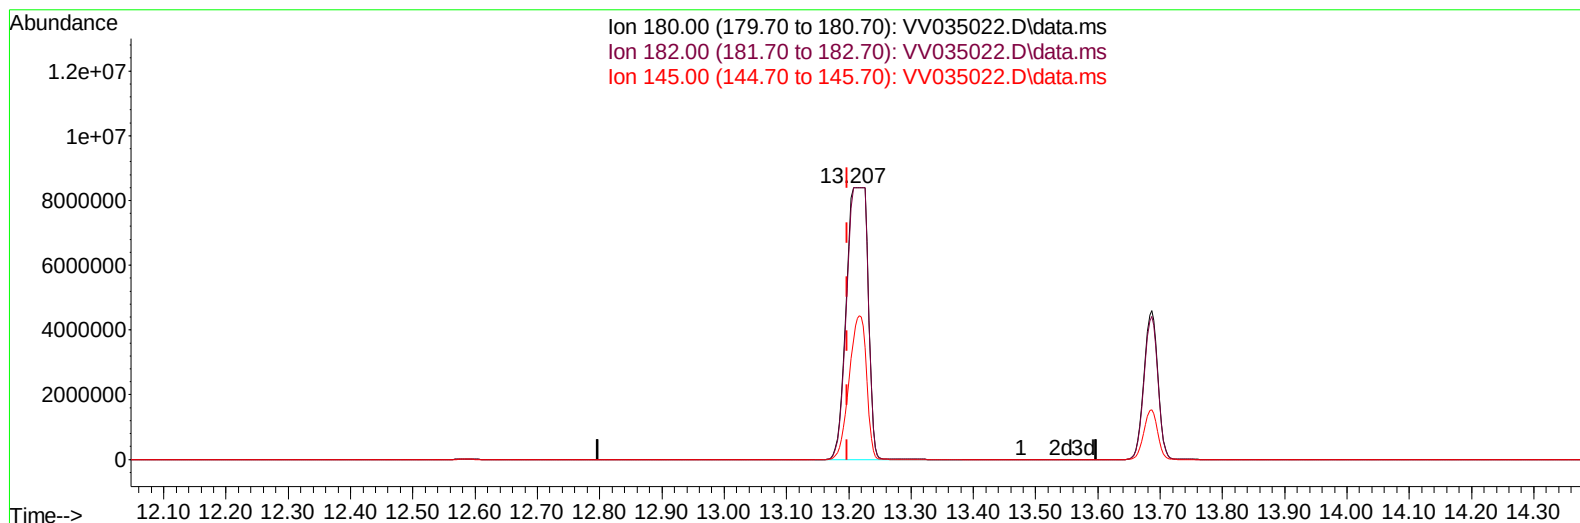

TIC: VV035022.D\data.ms

(70) 1,2,4-trichlorobenzene (T)

13.207min (+ 0.010) 3809.28 ug/L m

response 20357320

Ion	Exp%	Act%
180.00	100.00	100.00
182.00	94.50	0.00#
145.00	30.10	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035022.D
 Acq On : 05 Apr 2024 22:40
 Operator : SY/MD
 Sample : P2006-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 03:18:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 06 02:25:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
 Supervised By :Semsettin Yesilyurt 04/08/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	390104	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.818	117	407184	50.000	ug/L	0.04
58) 1,4-Dichlorobenzene-d4	11.217	152	239612	50.000	ug/L	# 0.03
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	167053	44.341	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	88.680%	
7) Chloroethane-d5	1.532	69	157079	48.003	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	2.060	65	73661	44.603	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.200%	
21) 2-Butanone-d5	3.793	46	189151	84.654	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	84.650%	
24) Chloroform-d	4.246	84	297097	46.903	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	4.947	65	184967	45.993	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.980%	
32) Benzene-d6	4.966	84	599058	43.799	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.600%	
36) 1,2-Dichloropropane-d6	5.989	67	187556	43.183	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	86.360%	
41) Toluene-d8	7.243	98	524514	42.582	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	85.160%	
43) trans-1,3-Dichloroprop...	7.555	79	85002	40.257	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	80.520%	
47) 2-Hexanone-d5	8.034	63	131448	80.048	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	80.050%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	282124	47.170	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	94.340%	
66) 1,2-Dichlorobenzene-d4	11.590	152	221421	41.158	ug/L	0.03
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.320%	
Target Compounds						
						Qvalue
13) Acetone	2.124	43	34185	16.665	ug/L	99
25) Chloroform	4.272	83	449026	78.242	ug/L	98
29) Cyclohexane	4.580	56	32589	6.390	ug/L	97
31) Carbon tetrachloride	4.735	117	355023	78.917	ug/L	100
33) Benzene	4.998	78	33542757m	2526.249	ug/L	
35) Methylcyclohexane	6.047	83	15349	2.836	ug/L #	80
38) Bromodichloromethane	6.445	83	5002	1.057	ug/L #	96
42) Toluene	7.326	91	19820	1.426	ug/L	99
46) Tetrachloroethene	7.912	164	4479	1.789	ug/L	94
51) Chlorobenzene	8.812	112	50054706m	5555.813	ug/L	
64) 1,3-Dichlorobenzene	11.130	146	16792586	2080.225	ug/L	91
65) 1,4-Dichlorobenzene	11.210	146	37230186m	4535.211	ug/L	
67) 1,2-Dichlorobenzene	11.587	146	37655764m	4682.597	ug/L	
69) 1,3,5-Trichlorobenzene	12.587	180	31023	5.332	ug/L	99
70) 1,2,4-trichlorobenzene	13.207	180	20357320m	3809.283	ug/L	
72) 1,2,3-Trichlorobenzene	13.686	180	7158429	1358.897	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)
----------	------	---	-----	----------	------	-------	-----	-------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035022.D
Acq On : 05 Apr 2024 22:40
Operator : SY/MD
Sample : P2006-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 03:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

