

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034992.D
 Acq On : 05 Apr 2024 09:44
 Operator : SY/MD
 Sample : VV0405WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rBV	206475	222376	13.73%	1.883%
2	1.532	147	153	169	rVB	220269	248159	15.32%	2.102%
3	2.060	307	317	334	rBV	376818	549934	33.95%	4.657%
4	2.568	473	475	479	rVB3	374	155	0.01%	0.001%
5	2.587	479	481	484	rBV2	747	484	0.03%	0.004%
6	2.658	500	503	506	rBV2	319	219	0.01%	0.002%
7	2.706	516	518	523	rVB4	663	419	0.03%	0.004%
8	2.783	540	542	544	rBV	331	187	0.01%	0.002%
9	2.912	580	582	586	rVV3	362	194	0.01%	0.002%
10	2.979	600	603	605	rBV2	526	407	0.03%	0.003%
11	3.011	611	613	615	rVB	519	232	0.01%	0.002%
12	3.028	616	618	621	rBV2	414	203	0.01%	0.002%
13	3.124	647	648	649	rBV	331	109	0.01%	0.001%
14	3.150	653	656	658	rBV	238	184	0.01%	0.002%
15	3.188	666	668	671	rBV2	342	193	0.01%	0.002%
16	3.304	702	704	707	rBV2	374	249	0.02%	0.002%
17	3.365	721	723	727	rVB2	485	292	0.02%	0.002%
18	3.388	727	730	732	rBV2	348	252	0.02%	0.002%
19	3.429	740	743	744	rBV	216	136	0.01%	0.001%
20	3.439	744	746	749	rVB2	384	232	0.01%	0.002%
21	3.503	761	766	768	rBV2	402	400	0.02%	0.003%
22	3.548	777	780	782	rBV	443	248	0.02%	0.002%
23	3.667	813	817	821	rVB3	384	396	0.02%	0.003%
24	3.696	821	826	829	rBV2	507	411	0.03%	0.003%
25	3.712	829	831	833	rBV2	181	109	0.01%	0.001%
26	3.722	833	834	839	rVB2	405	182	0.01%	0.002%
27	3.751	839	843	846	rBV3	333	312	0.02%	0.003%
28	3.796	848	857	904	rBV	105826	346764	21.41%	2.937%
29	4.246	983	997	1034	rBV	255086	653542	40.35%	5.535%
30	4.690	1133	1135	1138	rBV2	494	295	0.02%	0.002%
31	4.799	1165	1169	1175	rVB3	506	618	0.04%	0.005%
32	4.838	1175	1181	1187	rBV3	432	677	0.04%	0.006%
33	4.953	1202	1217	1258	rBV2	607089	1619712	100.00%	13.717%
34	5.416	1357	1361	1363	rBV4	490	394	0.02%	0.003%
35	5.532	1386	1397	1429	rBV	435468	916840	56.61%	7.764%
36	5.986	1525	1538	1572	rBV	358988	756476	46.70%	6.406%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034992.D
 Acq On : 05 Apr 2024 09:44
 Operator : SY/MD
 Sample : VV0405WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.381	1657	1661	1666	rBV3	467	516	0.03%	0.004%
38	6.439	1675	1679	1683	rBV4	492	415	0.03%	0.004%
39	6.487	1690	1694	1696	rBV	384	249	0.02%	0.002%
40	6.519	1700	1704	1706	rBV2	471	361	0.02%	0.003%
41	6.613	1731	1733	1736	rBV	292	213	0.01%	0.002%
42	6.645	1740	1743	1745	rBV2	313	160	0.01%	0.001%
43	6.677	1751	1753	1756	rBV2	464	206	0.01%	0.002%
44	6.728	1767	1769	1770	rBV2	483	212	0.01%	0.002%
45	6.757	1774	1778	1780	rBV	234	195	0.01%	0.002%
46	6.789	1785	1788	1793	rBV3	424	455	0.03%	0.004%
47	6.818	1795	1797	1798	rVB	398	131	0.01%	0.001%
48	6.831	1798	1801	1803	rBV	514	333	0.02%	0.003%
49	6.912	1816	1826	1855	rBV	176816	342994	21.18%	2.905%
50	7.243	1918	1929	1956	rBV	675739	1205385	74.42%	10.208%
51	7.551	2016	2025	2047	rBV	120508	223492	13.80%	1.893%
52	7.757	2087	2089	2092	rBV5	685	424	0.03%	0.004%
53	7.799	2099	2102	2105	rBV3	845	453	0.03%	0.004%
54	8.027	2164	2173	2213	rBV3	307048	737751	45.55%	6.248%
55	8.593	2346	2349	2351	rVB2	480	279	0.02%	0.002%
56	8.606	2351	2353	2354	rBV	506	268	0.02%	0.002%
57	8.635	2360	2362	2365	rVB	363	196	0.01%	0.002%
58	8.651	2365	2367	2369	rBV	553	278	0.02%	0.002%
59	8.703	2379	2383	2384	rBV3	571	311	0.02%	0.003%
60	8.735	2390	2393	2396	rVB2	379	226	0.01%	0.002%
61	8.783	2396	2408	2432	rBV	675129	1126339	69.54%	9.539%
62	9.153	2521	2523	2526	rBV	247	179	0.01%	0.002%
63	9.204	2536	2539	2542	rBV3	531	385	0.02%	0.003%
64	9.297	2566	2568	2569	rBV3	504	217	0.01%	0.002%
65	9.368	2587	2590	2593	rBV2	551	321	0.02%	0.003%
66	9.407	2600	2602	2606	rVB2	536	344	0.02%	0.003%
67	9.436	2609	2611	2612	rBV	356	162	0.01%	0.001%
68	9.490	2624	2628	2630	rBV	533	322	0.02%	0.003%
69	9.535	2640	2642	2644	rBV	383	215	0.01%	0.002%
70	9.600	2660	2662	2668	rVV2	802	510	0.03%	0.004%
71	9.632	2670	2672	2678	rVB3	605	421	0.03%	0.004%
72	9.674	2682	2685	2690	rBV2	352	255	0.02%	0.002%
73	9.905	2754	2757	2759	rBV2	362	233	0.01%	0.002%
74	9.953	2770	2772	2776	rBV2	281	190	0.01%	0.002%
75	10.085	2811	2813	2819	rVB2	494	255	0.02%	0.002%
76	10.149	2819	2833	2858	rBV	492981	784047	48.41%	6.640%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034992.D
 Acq On : 05 Apr 2024 09:44
 Operator : SY/MD
 Sample : VV0405WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.416	2911	2916	2918	rBV3	494	353	0.02%	0.003%
78	10.448	2923	2926	2928	rBV2	235	128	0.01%	0.001%
79	10.461	2928	2930	2933	rBV2	207	124	0.01%	0.001%
80	10.738	3014	3016	3018	rBV2	458	279	0.02%	0.002%
81	10.866	3051	3056	3059	rBV2	718	677	0.04%	0.006%
82	10.924	3069	3074	3077	rBV2	397	369	0.02%	0.003%
83	10.950	3080	3082	3085	rVB	386	155	0.01%	0.001%
84	10.998	3093	3097	3101	rBV2	391	360	0.02%	0.003%
85	11.063	3115	3117	3119	rBV2	236	171	0.01%	0.001%
86	11.072	3119	3120	3122	rVB	423	104	0.01%	0.001%
87	11.127	3130	3137	3144	rBV5	1786	2596	0.16%	0.022%
88	11.185	3144	3155	3182	rBV	606390	954096	58.91%	8.080%
89	11.558	3259	3271	3297	rBV	652789	1044651	64.50%	8.847%
90	12.117	3440	3445	3447	rBV2	594	567	0.04%	0.005%
91	12.159	3455	3458	3460	rBV	538	378	0.02%	0.003%
92	12.297	3497	3501	3504	rBV	678	510	0.03%	0.004%
93	12.423	3538	3540	3545	rBV2	445	360	0.02%	0.003%
94	12.693	3621	3624	3628	rBV	369	317	0.02%	0.003%
95	13.079	3741	3744	3747	rBV2	438	399	0.02%	0.003%
96	13.204	3777	3783	3795	rVB7	5363	8609	0.53%	0.073%
97	13.445	3846	3858	3874	rBV2	17238	31518	1.95%	0.267%
98	13.683	3926	3932	3943	rVB4	5471	8824	0.54%	0.075%
99	13.747	3951	3952	3954	rBV	478	250	0.02%	0.002%
100	14.085	4054	4057	4060	rVB	748	430	0.03%	0.004%




Sum of corrected areas: 11808115

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034992.D
Acq On : 05 Apr 2024 09:44
Operator : SY/MD
Sample : VV0405WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

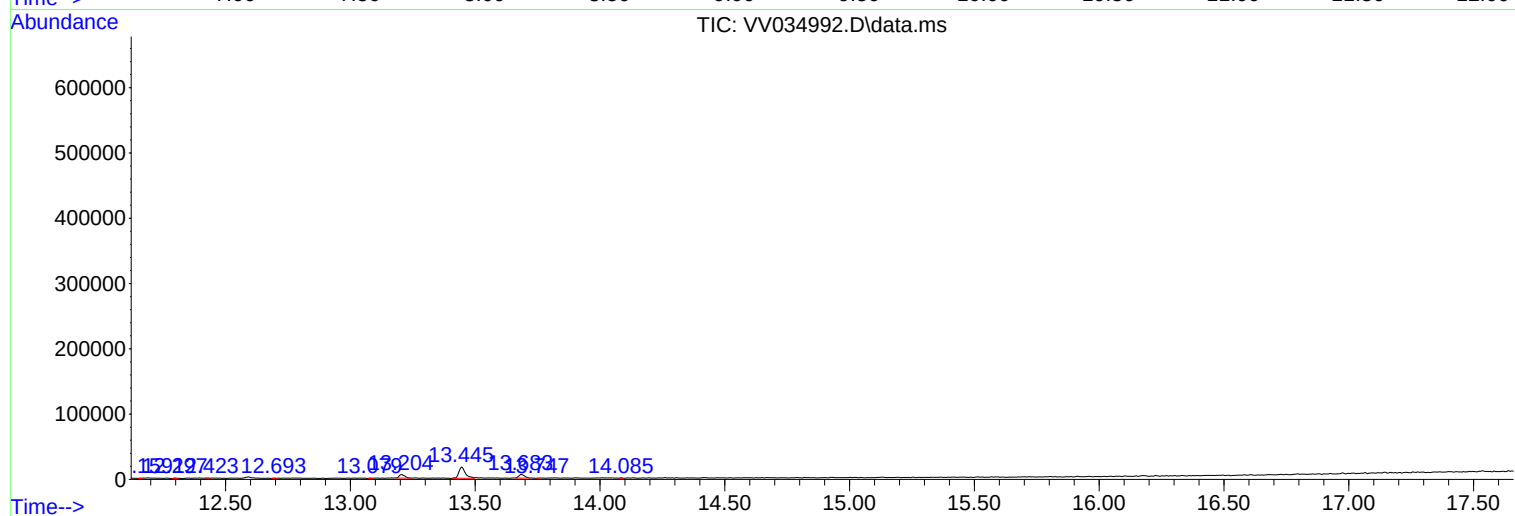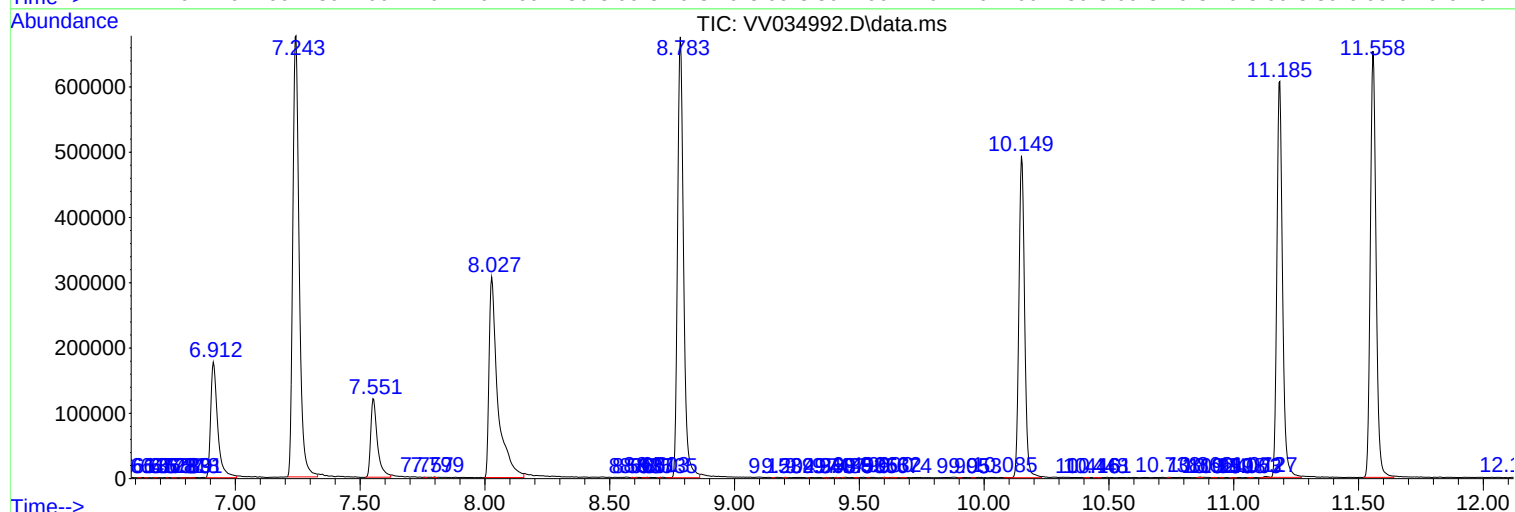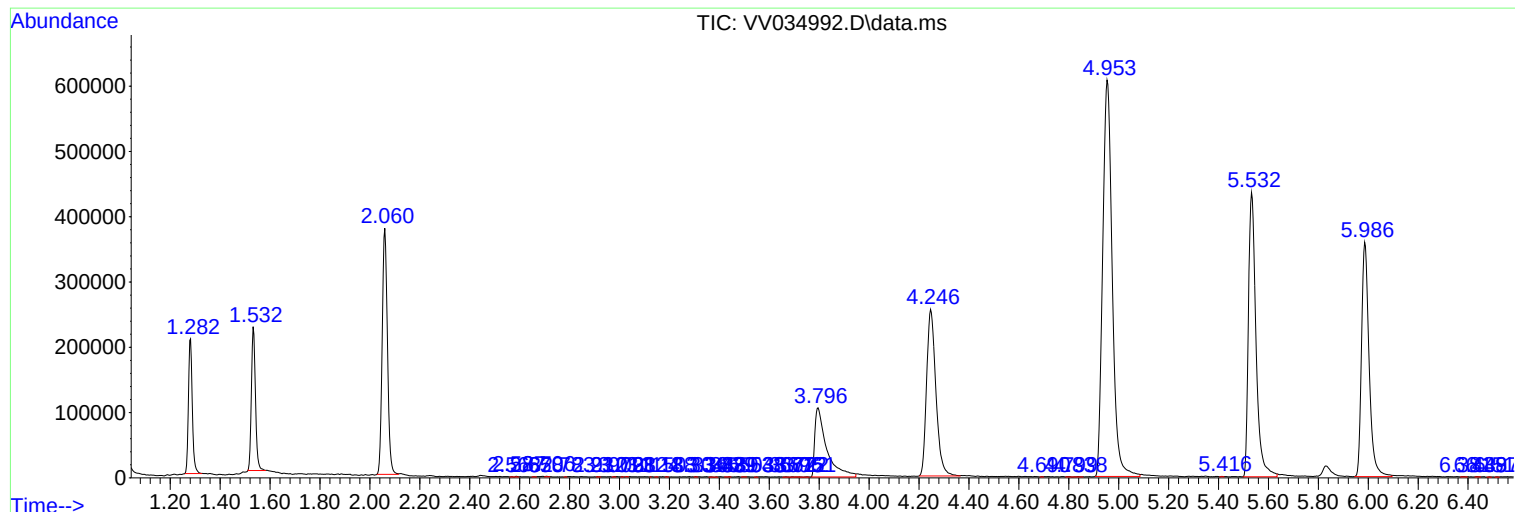

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034992.D
Acq On : 05 Apr 2024 09:44
Operator : SY/MD
Sample : VV0405WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034992.D
Acq On : 05 Apr 2024 09:44
Operator : SY/MD
Sample : VV0405WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc