

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034996.D
 Acq On : 05 Apr 2024 11:23
 Operator : SY/MD
 Sample : P1987-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	94	rVB	181578	189181	12.68%	1.746%
2	1.532	146	153	169	rVB	190859	223687	14.99%	2.065%
3	2.060	307	317	334	rBV	317868	465279	31.18%	4.295%
4	2.410	423	426	428	rBV2	413	330	0.02%	0.003%
5	2.500	451	454	458	rBV2	563	323	0.02%	0.003%
6	2.555	465	471	472	rBV	923	716	0.05%	0.007%
7	2.703	514	517	520	rBV3	645	452	0.03%	0.004%
8	2.986	601	605	608	rBV3	336	299	0.02%	0.003%
9	3.047	620	624	627	rBV	524	405	0.03%	0.004%
10	3.204	669	673	677	rBV2	705	523	0.04%	0.005%
11	3.298	697	702	704	rBV3	548	493	0.03%	0.005%
12	3.336	707	714	716	rBV3	703	790	0.05%	0.007%
13	3.410	734	737	742	rBV	335	353	0.02%	0.003%
14	3.500	759	765	767	rBV	326	313	0.02%	0.003%
15	3.513	767	769	774	rBV3	491	327	0.02%	0.003%
16	3.609	795	799	803	rBV3	381	290	0.02%	0.003%
17	3.664	814	816	822	rVB3	350	300	0.02%	0.003%
18	3.796	848	857	900	rBV	108624	350203	23.47%	3.232%
19	4.179	972	976	979	rBV3	705	550	0.04%	0.005%
20	4.249	979	998	1030	rBV	235064	608773	40.79%	5.619%
21	4.503	1074	1077	1080	rBV3	472	413	0.03%	0.004%
22	4.648	1120	1122	1130	rVB4	531	360	0.02%	0.003%
23	4.879	1191	1194	1197	rBV	434	321	0.02%	0.003%
24	4.957	1202	1218	1260	rBV2	551156	1492419	100.00%	13.775%
25	5.433	1363	1366	1370	rVB3	548	310	0.02%	0.003%
26	5.532	1384	1397	1438	rBV	384503	821574	55.05%	7.583%
27	5.834	1480	1491	1509	rBV3	12830	29105	1.95%	0.269%
28	5.986	1525	1538	1566	rBV	335025	697192	46.72%	6.435%
29	6.381	1659	1661	1663	rBV2	697	418	0.03%	0.004%
30	6.452	1680	1683	1686	rBV2	512	425	0.03%	0.004%
31	6.468	1686	1688	1692	rVB3	755	538	0.04%	0.005%
32	6.494	1692	1696	1702	rBV4	764	921	0.06%	0.009%
33	6.629	1735	1738	1741	rVV4	673	487	0.03%	0.004%
34	6.667	1745	1750	1753	rBV2	563	566	0.04%	0.005%
35	6.731	1768	1770	1773	rBV2	708	400	0.03%	0.004%
36	6.783	1783	1786	1792	rVB3	429	299	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034996.D
 Acq On : 05 Apr 2024 11:23
 Operator : SY/MD
 Sample : P1987-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.912	1812	1826	1850	rBV	162112	314473	21.07%	2.903%
38	7.159	1896	1903	1906	rBV6	661	725	0.05%	0.007%
39	7.243	1918	1929	1954	rBV	597813	1069793	71.68%	9.874%
40	7.555	2017	2026	2054	rVV	110608	209508	14.04%	1.934%
41	7.757	2085	2089	2091	rBV3	601	417	0.03%	0.004%
42	7.854	2115	2119	2122	rBV2	560	426	0.03%	0.004%
43	7.937	2141	2145	2146	rBV3	529	310	0.02%	0.003%
44	7.979	2156	2158	2161	rVB3	574	291	0.02%	0.003%
45	8.027	2164	2173	2215	rBV2	311214	745105	49.93%	6.877%
46	8.471	2308	2311	2313	rBV3	428	290	0.02%	0.003%
47	8.500	2318	2320	2324	rBV3	555	393	0.03%	0.004%
48	8.561	2337	2339	2344	rVB4	555	392	0.03%	0.004%
49	8.693	2377	2380	2382	rVB2	928	534	0.04%	0.005%
50	8.715	2382	2387	2391	rVB3	536	579	0.04%	0.005%
51	8.741	2391	2395	2397	rBV2	495	336	0.02%	0.003%
52	8.783	2397	2408	2438	rBV	608583	1010268	67.69%	9.325%
53	8.956	2460	2462	2467	rBV4	805	709	0.05%	0.007%
54	9.165	2524	2527	2529	rBV2	623	325	0.02%	0.003%
55	9.210	2537	2541	2543	rBV3	523	356	0.02%	0.003%
56	9.371	2588	2591	2594	rBV	478	322	0.02%	0.003%
57	9.493	2626	2629	2633	rVB2	399	304	0.02%	0.003%
58	9.545	2641	2645	2647	rBV2	607	326	0.02%	0.003%
59	9.574	2650	2654	2660	rVB4	337	376	0.03%	0.003%
60	9.847	2734	2739	2743	rBV2	412	389	0.03%	0.004%
61	9.902	2753	2756	2763	rVB4	598	455	0.03%	0.004%
62	10.095	2812	2816	2822	rBV	312	362	0.02%	0.003%
63	10.149	2822	2833	2854	rBV	481874	764930	51.25%	7.060%
64	10.326	2883	2888	2892	rBV5	646	719	0.05%	0.007%
65	10.368	2899	2901	2903	rBV2	657	344	0.02%	0.003%
66	10.458	2924	2929	2931	rBV3	489	401	0.03%	0.004%
67	10.519	2943	2948	2950	rBV	497	482	0.03%	0.004%
68	10.561	2959	2961	2966	rVB3	474	362	0.02%	0.003%
69	10.596	2967	2972	2975	rBV3	550	526	0.04%	0.005%
70	10.667	2991	2994	2997	rBV	363	327	0.02%	0.003%
71	10.722	3008	3011	3017	rVV3	466	500	0.03%	0.005%
72	10.751	3017	3020	3025	rVB2	494	399	0.03%	0.004%
73	10.873	3055	3058	3062	rVB2	452	318	0.02%	0.003%
74	10.992	3092	3095	3099	rBV2	439	410	0.03%	0.004%
75	11.133	3136	3139	3144	rBV4	823	659	0.04%	0.006%
76	11.185	3144	3155	3184	rBV	530298	856030	57.36%	7.901%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034996.D
 Acq On : 05 Apr 2024 11:23
 Operator : SY/MD
 Sample : P1987-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.471	3241	3244	3246	rBV3	689	392	0.03%	0.004%
78	11.558	3256	3271	3295	rBV	595495	947547	63.49%	8.746%
79	11.792	3342	3344	3346	rBV2	620	316	0.02%	0.003%
80	12.191	3464	3468	3470	rBV2	471	333	0.02%	0.003%
81	12.365	3519	3522	3525	rBV2	495	307	0.02%	0.003%
82	12.455	3543	3550	3551	rBV	601	580	0.04%	0.005%
83	12.567	3580	3585	3587	rBV	321	361	0.02%	0.003%
84	12.734	3633	3637	3641	rBV2	575	545	0.04%	0.005%
85	12.789	3652	3654	3660	rBV3	315	305	0.02%	0.003%
86	12.943	3697	3702	3706	rVB2	582	590	0.04%	0.005%
87	12.976	3709	3712	3718	rBV2	388	334	0.02%	0.003%
88	13.053	3734	3736	3742	rVB3	501	413	0.03%	0.004%
89	13.098	3745	3750	3755	rVB2	607	559	0.04%	0.005%
90	13.124	3755	3758	3764	rBV	512	532	0.04%	0.005%
91	13.210	3779	3785	3786	rBV5	1293	1326	0.09%	0.012%
92	13.307	3812	3815	3820	rBV3	496	504	0.03%	0.005%
93	13.448	3854	3859	3861	rBV3	1090	1043	0.07%	0.010%
94	13.680	3928	3931	3932	rBV2	597	325	0.02%	0.003%
95	13.734	3944	3948	3952	rBV3	660	636	0.04%	0.006%
96	13.815	3971	3973	3976	rBV2	735	481	0.03%	0.004%
97	13.902	3997	4000	4003	rBV2	519	314	0.02%	0.003%
98	14.609	4218	4220	4222	rBV2	980	586	0.04%	0.005%
99	15.278	4423	4428	4433	rBV6	1246	1722	0.12%	0.016%
100	15.615	4531	4533	4536	rBV5	824	482	0.03%	0.004%




Sum of corrected areas: 10834039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034996.D
Acq On : 05 Apr 2024 11:23
Operator : SY/MD
Sample : P1987-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

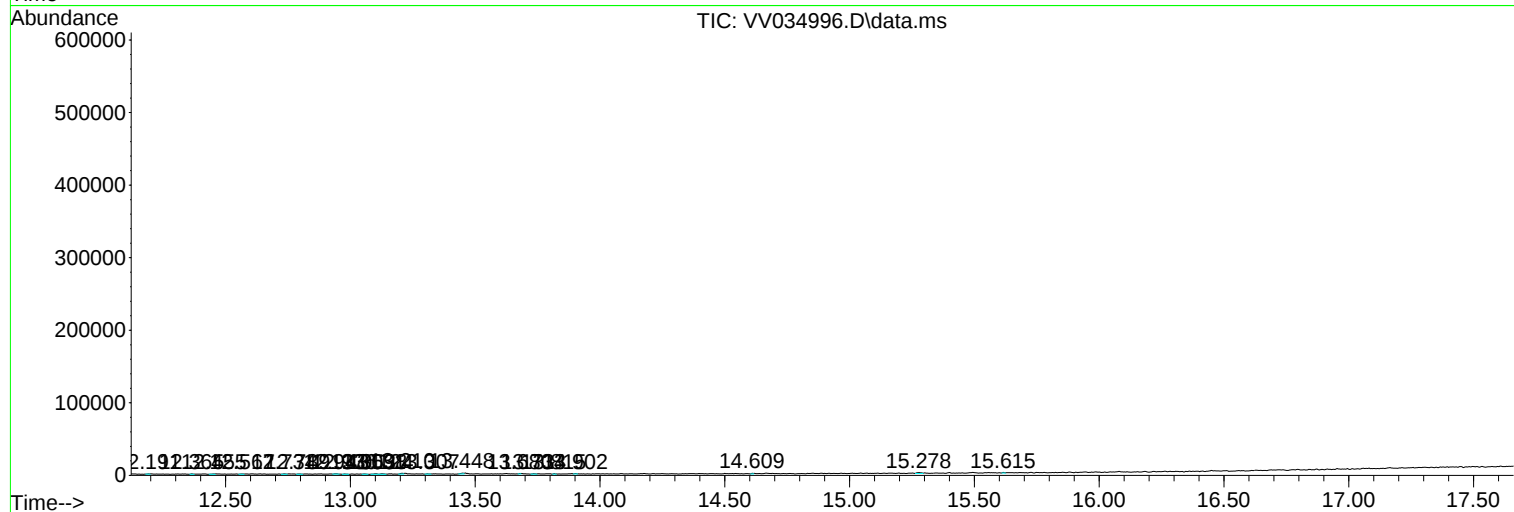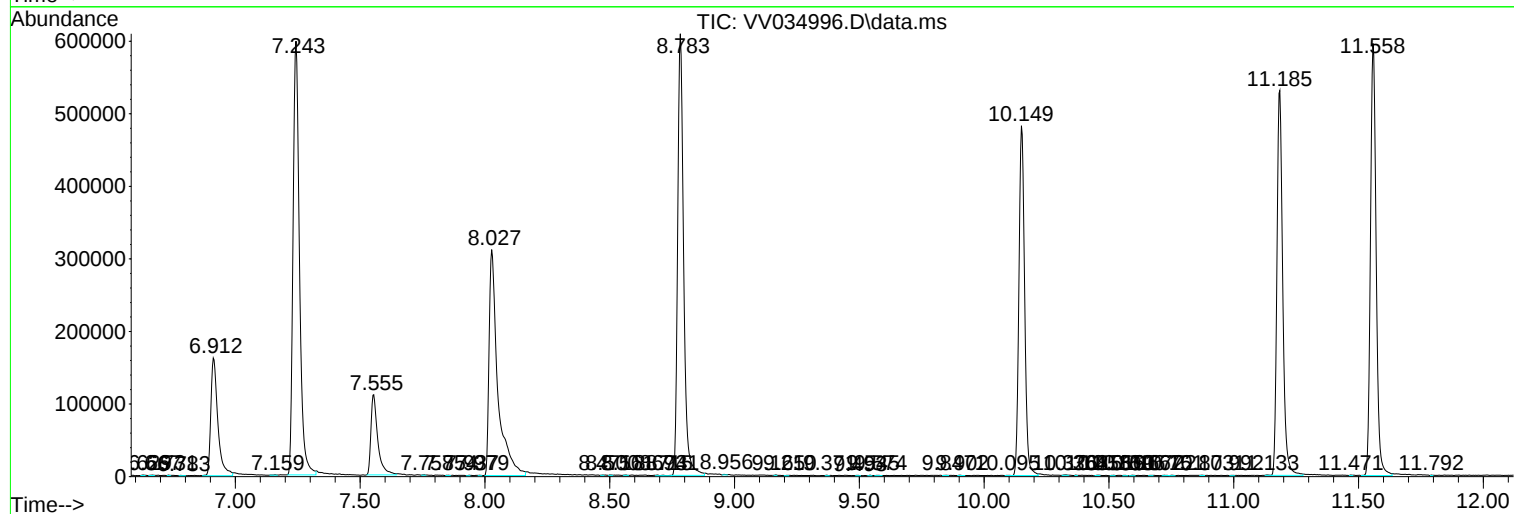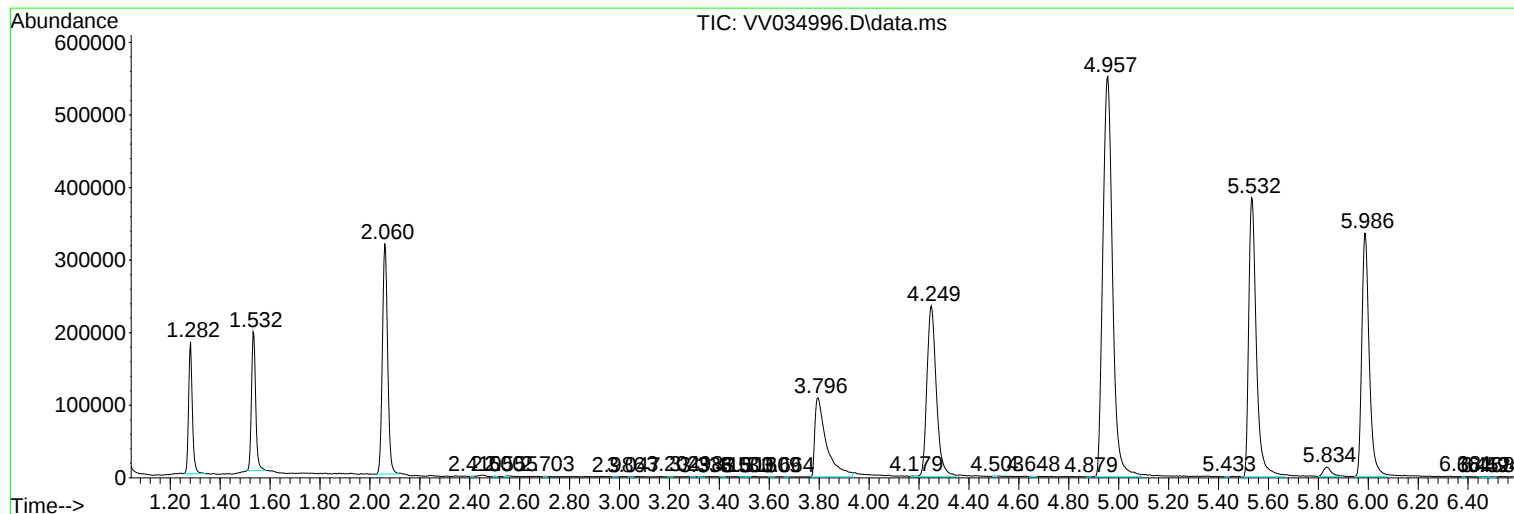

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034996.D
Acq On : 05 Apr 2024 11:23
Operator : SY/MD
Sample : P1987-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034996.D
Acq On : 05 Apr 2024 11:23
Operator : SY/MD
Sample : P1987-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------