

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034997.D
 Acq On : 05 Apr 2024 11:46
 Operator : SY/MD
 Sample : P1988-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	42	47	53	rBV	18171	18050	1.36%	0.187%
2	1.282	68	75	90	rVB	170816	186922	14.07%	1.932%
3	1.532	147	153	169	rVB	189686	221257	16.66%	2.287%
4	2.060	308	317	331	rBV	303849	440735	33.19%	4.555%
5	2.806	545	549	551	rBV2	756	443	0.03%	0.005%
6	2.863	565	567	569	rBV2	354	157	0.01%	0.002%
7	2.953	592	595	596	rBV	437	249	0.02%	0.003%
8	2.963	596	598	599	rBV	381	156	0.01%	0.002%
9	3.008	608	612	614	rBV	633	415	0.03%	0.004%
10	3.021	614	616	619	rVV3	431	217	0.02%	0.002%
11	3.111	641	644	646	rVB	409	175	0.01%	0.002%
12	3.130	646	650	652	rBV3	427	315	0.02%	0.003%
13	3.204	669	673	677	rBV3	467	488	0.04%	0.005%
14	3.275	693	695	699	rBV2	419	308	0.02%	0.003%
15	3.294	699	701	704	rVV	337	219	0.02%	0.002%
16	3.314	705	707	711	rVB2	570	335	0.03%	0.003%
17	3.339	711	715	718	rBV3	313	223	0.02%	0.002%
18	3.410	735	737	739	rBV2	503	201	0.02%	0.002%
19	3.494	759	763	765	rVV2	345	248	0.02%	0.003%
20	3.523	769	772	777	rBV3	452	388	0.03%	0.004%
21	3.590	786	793	797	rBV3	1143	1521	0.11%	0.016%
22	3.696	823	826	829	rVV2	355	298	0.02%	0.003%
23	3.716	830	832	835	rVB3	554	258	0.02%	0.003%
24	3.767	844	848	849	rBV2	368	241	0.02%	0.002%
25	3.796	849	857	899	rBV	88836	289136	21.77%	2.988%
26	4.249	983	998	1034	rBV2	220770	629693	47.41%	6.508%
27	4.699	1135	1138	1143	rVB2	444	414	0.03%	0.004%
28	4.957	1200	1218	1246	rBV2	495683	1328102	100.00%	13.725%
29	5.346	1336	1339	1341	rBV2	810	556	0.04%	0.006%
30	5.481	1378	1381	1384	rBV3	640	381	0.03%	0.004%
31	5.535	1387	1398	1436	rVV	320846	685566	51.62%	7.085%
32	5.831	1481	1490	1517	rVB3	13033	31457	2.37%	0.325%
33	5.921	1517	1518	1521	rBV2	503	185	0.01%	0.002%
34	5.989	1525	1539	1560	rBV	294469	620991	46.76%	6.418%
35	6.304	1633	1637	1642	rVB2	539	432	0.03%	0.004%
36	6.339	1642	1648	1652	rBV3	857	775	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040524\
 Data File : VV034997.D
 Acq On : 05 Apr 2024 11:46
 Operator : SY/MD
 Sample : P1988-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.442	1673	1680	1692	rVB3	6581	13034	0.98%	0.135%
38	6.555	1713	1715	1720	rBV2	337	264	0.02%	0.003%
39	6.577	1720	1722	1727	rVB2	271	157	0.01%	0.002%
40	6.600	1727	1729	1731	rBV2	331	170	0.01%	0.002%
41	6.715	1762	1765	1766	rBV2	198	133	0.01%	0.001%
42	6.744	1770	1774	1777	rVB2	383	283	0.02%	0.003%
43	6.767	1777	1781	1782	rBV3	418	291	0.02%	0.003%
44	6.873	1810	1814	1816	rBV	344	274	0.02%	0.003%
45	6.915	1816	1827	1853	rBV	141515	281352	21.18%	2.908%
46	7.243	1918	1929	1951	rBV	554051	984498	74.13%	10.174%
47	7.555	2016	2026	2054	rBV	96010	187613	14.13%	1.939%
48	7.796	2099	2101	2105	rVB2	607	362	0.03%	0.004%
49	7.844	2112	2116	2119	rVB2	543	383	0.03%	0.004%
50	7.883	2125	2128	2132	rVB4	1064	854	0.06%	0.009%
51	7.911	2134	2137	2140	rBV2	505	316	0.02%	0.003%
52	7.989	2157	2161	2163	rBV3	646	448	0.03%	0.005%
53	8.027	2164	2173	2215	rBV2	254040	618223	46.55%	6.389%
54	8.465	2307	2309	2311	rBV2	574	338	0.03%	0.003%
55	8.532	2327	2330	2335	rBV6	500	360	0.03%	0.004%
56	8.567	2336	2341	2345	rVB4	711	688	0.05%	0.007%
57	8.593	2347	2349	2351	rBV2	445	236	0.02%	0.002%
58	8.783	2397	2408	2441	rBV	514530	855305	64.40%	8.839%
59	9.095	2501	2505	2507	rBV2	834	506	0.04%	0.005%
60	9.149	2515	2522	2524	rBV2	561	518	0.04%	0.005%
61	9.284	2562	2564	2566	rBV2	304	148	0.01%	0.002%
62	9.320	2573	2575	2577	rVB	420	167	0.01%	0.002%
63	9.333	2577	2579	2581	rBV2	299	146	0.01%	0.002%
64	9.458	2616	2618	2620	rBV	330	181	0.01%	0.002%
65	9.583	2651	2657	2660	rBV6	437	556	0.04%	0.006%
66	9.625	2667	2670	2673	rVB2	267	145	0.01%	0.001%
67	9.673	2681	2685	2690	rBV2	303	317	0.02%	0.003%
68	9.709	2694	2696	2701	rVB2	552	481	0.04%	0.005%
69	9.815	2726	2729	2732	rVB2	515	304	0.02%	0.003%
70	9.841	2732	2737	2739	rBV2	416	325	0.02%	0.003%
71	9.966	2773	2776	2778	rBV	365	231	0.02%	0.002%
72	10.024	2791	2794	2796	rBV2	226	140	0.01%	0.001%
73	10.040	2797	2799	2805	rVB2	369	268	0.02%	0.003%
74	10.149	2819	2833	2854	rBV	407188	654930	49.31%	6.768%
75	10.255	2864	2866	2868	rBV	459	260	0.02%	0.003%
76	10.513	2942	2946	2948	rVB2	377	215	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034997.D
 Acq On : 05 Apr 2024 11:46
 Operator : SY/MD
 Sample : P1988-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.564	2958	2962	2964	rBV3	338	248	0.02%	0.003%
78	10.673	2992	2996	2998	rBV2	248	222	0.02%	0.002%
79	10.709	3002	3007	3017	rVV5	803	1564	0.12%	0.016%
80	10.792	3026	3033	3036	rBV4	487	619	0.05%	0.006%
81	10.950	3079	3082	3086	rBV3	539	344	0.03%	0.004%
82	10.969	3086	3088	3091	rBV	383	187	0.01%	0.002%
83	11.043	3108	3111	3115	rVB3	369	214	0.02%	0.002%
84	11.095	3119	3127	3129	rBV4	669	741	0.06%	0.008%
85	11.185	3144	3155	3178	rBV	463227	727460	54.77%	7.518%
86	11.558	3258	3271	3296	rBV	547787	872186	65.67%	9.014%
87	11.805	3345	3348	3350	rBV3	594	412	0.03%	0.004%
88	11.870	3366	3368	3370	rBV	301	154	0.01%	0.002%
89	12.024	3414	3416	3419	rBV	393	238	0.02%	0.002%
90	12.072	3429	3431	3435	rBV3	361	207	0.02%	0.002%
91	12.175	3460	3463	3464	rBV	432	216	0.02%	0.002%
92	12.246	3481	3485	3489	rVB3	481	425	0.03%	0.004%
93	12.268	3489	3492	3496	rBV3	578	475	0.04%	0.005%
94	12.705	3626	3628	3631	rVB3	373	222	0.02%	0.002%
95	12.722	3631	3633	3636	rBV	576	315	0.02%	0.003%
96	12.783	3649	3652	3654	rBV4	429	319	0.02%	0.003%
97	13.111	3752	3754	3756	rBV2	531	255	0.02%	0.003%
98	13.156	3764	3768	3769	rBV	457	315	0.02%	0.003%
99	13.207	3781	3784	3793	rVB5	1269	1404	0.11%	0.015%
100	14.300	4121	4124	4127	rBV3	869	593	0.04%	0.006%




Sum of corrected areas: 9676262

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034997.D
Acq On : 05 Apr 2024 11:46
Operator : SY/MD
Sample : P1988-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

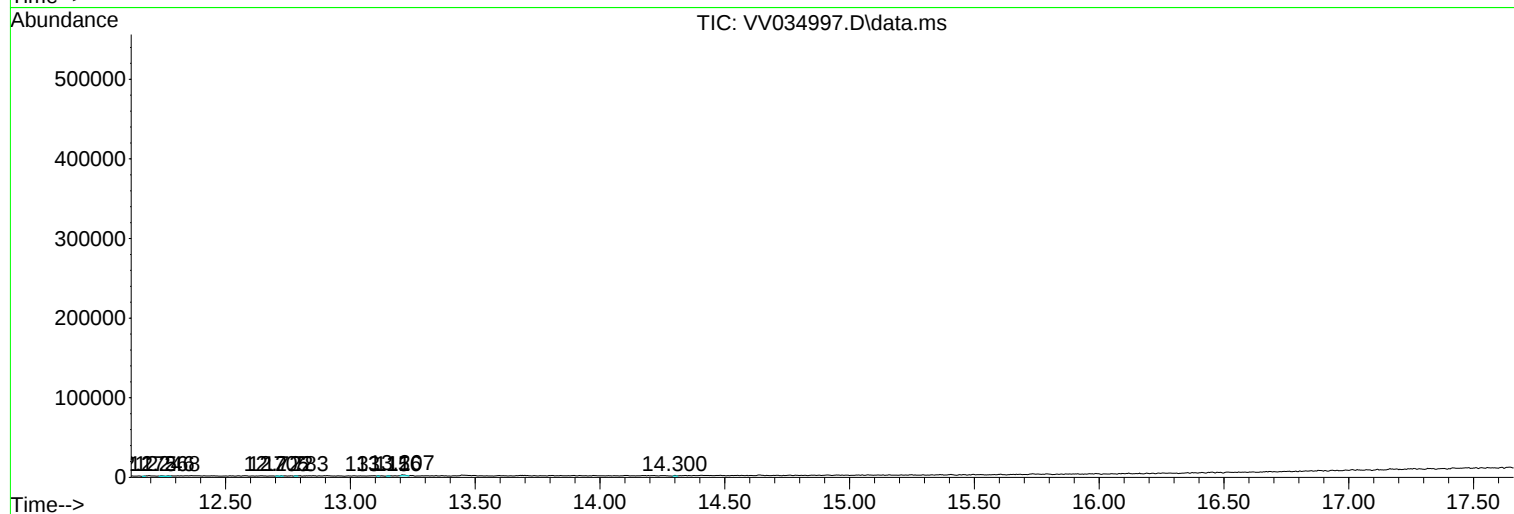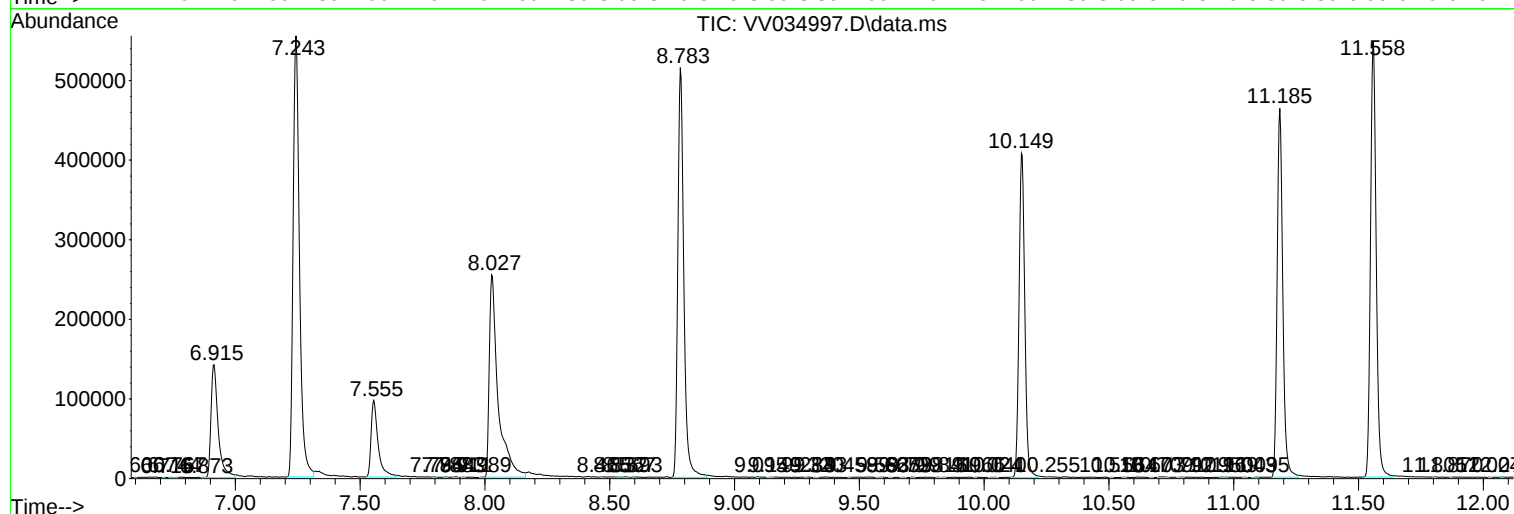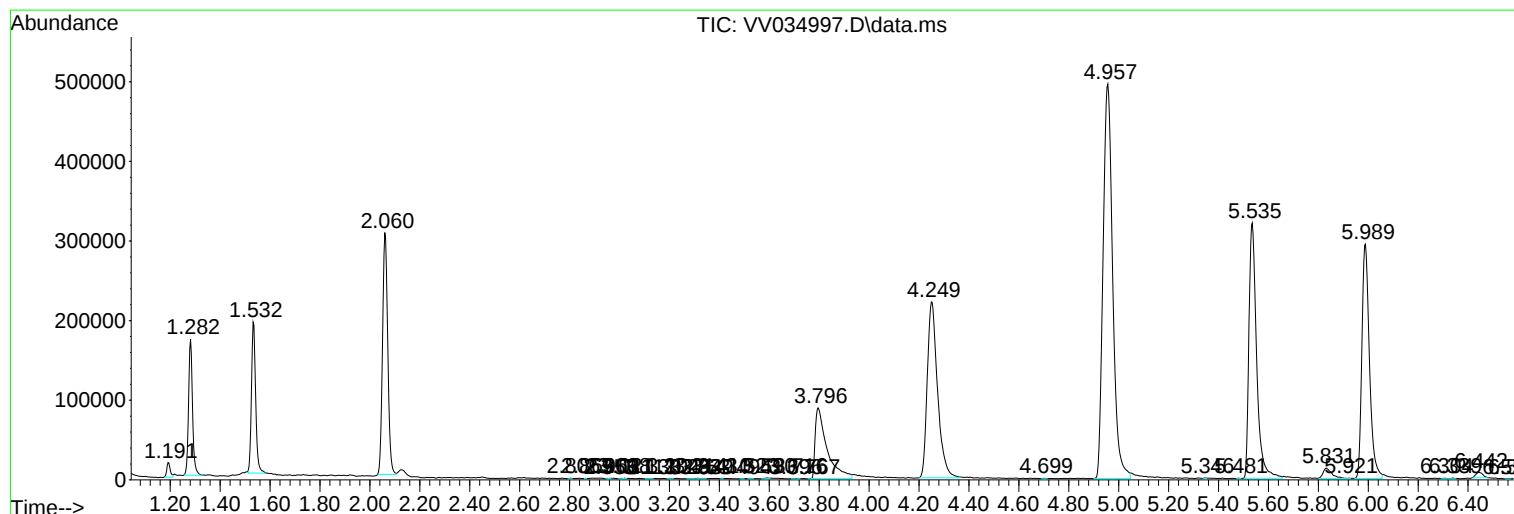

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034997.D
Acq On : 05 Apr 2024 11:46
Operator : SY/MD
Sample : P1988-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034997.D
Acq On : 05 Apr 2024 11:46
Operator : SY/MD
Sample : P1988-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc