

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034999.D
 Acq On : 05 Apr 2024 12:33
 Operator : SY/MD
 Sample : P1965-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07S0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	42	47	52	rBV	20816	18834	1.28%	0.168%
2	1.278	67	74	88	rVB	185514	198523	13.44%	1.771%
3	1.532	146	153	175	rVB	211355	257032	17.40%	2.293%
4	2.060	307	317	330	rBV	339489	493652	33.42%	4.404%
5	2.735	525	527	529	rBV2	550	283	0.02%	0.003%
6	2.790	542	544	547	rBV2	477	357	0.02%	0.003%
7	2.892	570	576	578	rBV5	896	1000	0.07%	0.009%
8	2.982	601	604	609	rBV3	390	384	0.03%	0.003%
9	3.047	621	624	626	rBV	373	234	0.02%	0.002%
10	3.085	634	636	637	rBV	260	99	0.01%	0.001%
11	3.146	653	655	658	rBV	357	281	0.02%	0.003%
12	3.214	673	676	677	rBV	234	118	0.01%	0.001%
13	3.265	686	692	694	rVB3	450	394	0.03%	0.004%
14	3.278	694	696	700	rVB2	200	128	0.01%	0.001%
15	3.301	700	703	705	rBV2	348	244	0.02%	0.002%
16	3.413	737	738	740	rBV2	258	66	0.00%	0.001%
17	3.436	744	745	747	rBV2	347	132	0.01%	0.001%
18	3.465	752	754	756	rBV2	230	114	0.01%	0.001%
19	3.478	756	758	760	rBV	356	179	0.01%	0.002%
20	3.564	782	785	790	rVB2	649	421	0.03%	0.004%
21	3.590	790	793	794	rBV	662	357	0.02%	0.003%
22	3.709	828	830	832	rBV	189	60	0.00%	0.001%
23	3.722	832	834	837	rBV	198	139	0.01%	0.001%
24	3.793	847	856	890	rBV	102521	313487	21.22%	2.797%
25	4.249	982	998	1036	rBV	242220	690637	46.76%	6.162%
26	4.690	1133	1135	1136	rBV2	199	77	0.01%	0.001%
27	4.699	1136	1138	1141	rVB3	555	308	0.02%	0.003%
28	4.957	1202	1218	1259	rBV2	550839	1477049	100.00%	13.178%
29	5.532	1386	1397	1426	rBV	437580	910734	61.66%	8.125%
30	5.831	1481	1490	1509	rBV4	12470	29687	2.01%	0.265%
31	5.937	1519	1523	1524	rBV	476	269	0.02%	0.002%
32	5.986	1524	1538	1570	rVV	325206	691526	46.82%	6.170%
33	6.352	1650	1652	1655	rBV2	537	296	0.02%	0.003%
34	6.445	1673	1681	1694	rVB2	7198	13610	0.92%	0.121%
35	6.542	1708	1711	1715	rBV2	535	429	0.03%	0.004%
36	6.558	1715	1716	1719	rBV	293	167	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034999.D
 Acq On : 05 Apr 2024 12:33
 Operator : SY/MD
 Sample : P1965-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07S0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.616	1733	1734	1735	rBV	307	73	0.00%	0.001%
38	6.625	1735	1737	1739	rVV3	413	177	0.01%	0.002%
39	6.641	1739	1742	1749	rVB3	626	550	0.04%	0.005%
40	6.670	1749	1751	1753	rBV3	451	223	0.02%	0.002%
41	6.690	1756	1757	1760	rBV2	506	236	0.02%	0.002%
42	6.748	1770	1775	1782	rVB4	745	724	0.05%	0.006%
43	6.777	1782	1784	1787	rVB2	316	142	0.01%	0.001%
44	6.818	1795	1797	1798	rBV	320	110	0.01%	0.001%
45	6.828	1798	1800	1805	rVB3	228	172	0.01%	0.002%
46	6.912	1815	1826	1860	rBV	160407	316011	21.39%	2.819%
47	7.243	1918	1929	1952	rBV	615742	1099544	74.44%	9.810%
48	7.551	2017	2025	2058	rBV	105328	203462	13.77%	1.815%
49	7.844	2114	2116	2119	rBV2	653	380	0.03%	0.003%
50	7.863	2119	2122	2124	rBV2	422	323	0.02%	0.003%
51	7.915	2134	2138	2140	rBV	459	336	0.02%	0.003%
52	7.950	2147	2149	2150	rBV	256	100	0.01%	0.001%
53	8.027	2163	2173	2215	rBV3	296398	693945	46.98%	6.191%
54	8.638	2362	2363	2364	rBV	483	168	0.01%	0.001%
55	8.783	2397	2408	2431	rBV	673125	1113847	75.41%	9.937%
56	9.063	2493	2495	2499	rBV3	625	460	0.03%	0.004%
57	9.172	2525	2529	2533	rBV4	526	519	0.04%	0.005%
58	9.239	2547	2550	2555	rVB3	867	648	0.04%	0.006%
59	9.307	2568	2571	2573	rBV3	593	313	0.02%	0.003%
60	9.384	2594	2595	2597	rBV	200	59	0.00%	0.001%
61	9.400	2597	2600	2605	rBV4	765	684	0.05%	0.006%
62	9.455	2615	2617	2623	rVB2	526	320	0.02%	0.003%
63	9.497	2626	2630	2637	rBV3	537	724	0.05%	0.006%
64	9.555	2646	2648	2649	rBV	317	120	0.01%	0.001%
65	9.641	2673	2675	2677	rBV	367	164	0.01%	0.001%
66	9.690	2687	2690	2692	rBV2	341	142	0.01%	0.001%
67	9.786	2719	2720	2721	rBV2	282	91	0.01%	0.001%
68	9.841	2736	2737	2740	rBV	125	61	0.00%	0.001%
69	9.879	2746	2749	2752	rBV2	403	262	0.02%	0.002%
70	9.960	2773	2774	2776	rVB	237	71	0.00%	0.001%
71	9.976	2776	2779	2781	rBV2	272	132	0.01%	0.001%
72	10.001	2785	2787	2788	rBV2	305	131	0.01%	0.001%
73	10.072	2807	2809	2813	rBV	242	140	0.01%	0.001%
74	10.149	2822	2833	2863	rBV	463137	728560	49.33%	6.500%
75	10.452	2923	2927	2931	rBV3	473	439	0.03%	0.004%
76	10.481	2934	2936	2937	rBV2	239	78	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV034999.D
 Acq On : 05 Apr 2024 12:33
 Operator : SY/MD
 Sample : P1965-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07S0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.712	3002	3008	3009	rBV3	1180	1164	0.08%	0.010%
78	10.757	3020	3022	3024	rBV	338	209	0.01%	0.002%
79	10.802	3033	3036	3038	rBV	529	324	0.02%	0.003%
80	10.908	3066	3069	3071	rBV2	212	111	0.01%	0.001%
81	10.969	3084	3088	3090	rBV3	590	370	0.03%	0.003%
82	11.069	3117	3119	3122	rVB	340	165	0.01%	0.001%
83	11.130	3134	3138	3143	rBV4	916	916	0.06%	0.008%
84	11.185	3144	3155	3188	rVV	611535	964853	65.32%	8.608%
85	11.558	3260	3271	3297	rBV	600285	969750	65.65%	8.652%
86	11.796	3344	3345	3347	rBV	469	196	0.01%	0.002%
87	12.046	3419	3423	3426	rVB2	440	364	0.02%	0.003%
88	12.066	3426	3429	3431	rBV	513	376	0.03%	0.003%
89	12.088	3434	3436	3439	rBV	358	206	0.01%	0.002%
90	12.162	3456	3459	3465	rBV5	557	614	0.04%	0.005%
91	12.271	3489	3493	3497	rBV2	500	454	0.03%	0.004%
92	12.333	3510	3512	3515	rBV2	446	280	0.02%	0.002%
93	12.390	3527	3530	3532	rBV2	550	281	0.02%	0.003%
94	12.448	3546	3548	3552	rVB2	621	356	0.02%	0.003%
95	12.898	3686	3688	3695	rVB4	598	534	0.04%	0.005%
96	13.445	3856	3858	3860	rBV	588	361	0.02%	0.003%
97	13.567	3893	3896	3899	rBV2	654	542	0.04%	0.005%
98	14.532	4194	4196	4198	rBV2	616	302	0.02%	0.003%




Sum of corrected areas: 11208676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034999.D
Acq On : 05 Apr 2024 12:33
Operator : SY/MD
Sample : P1965-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

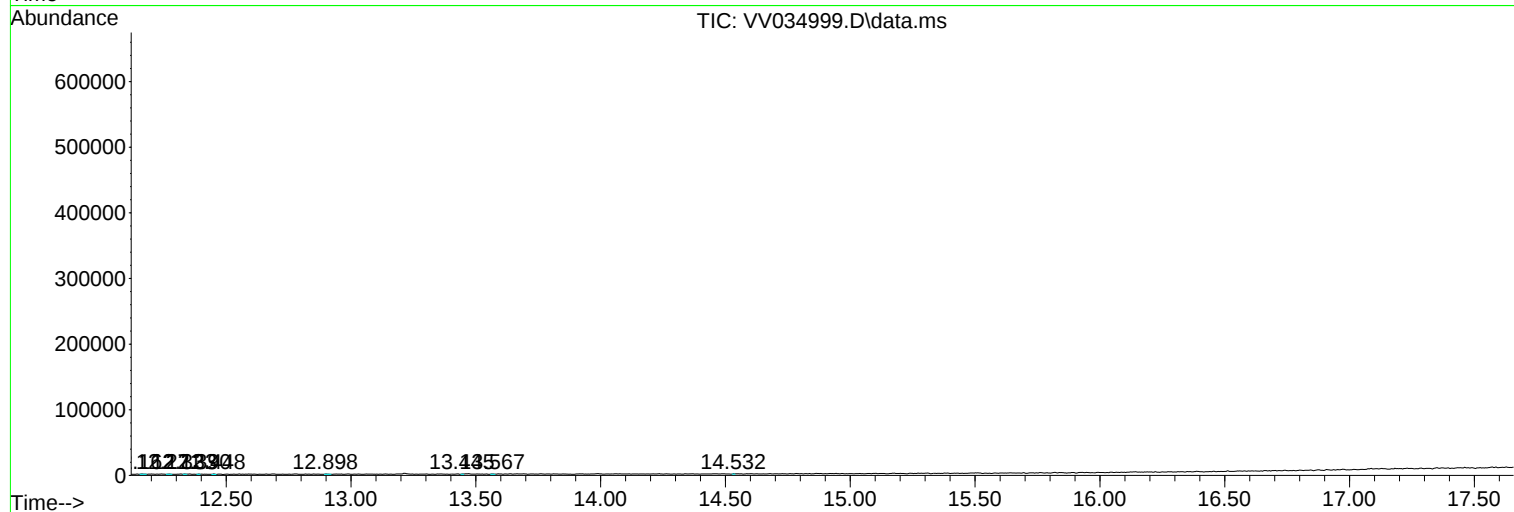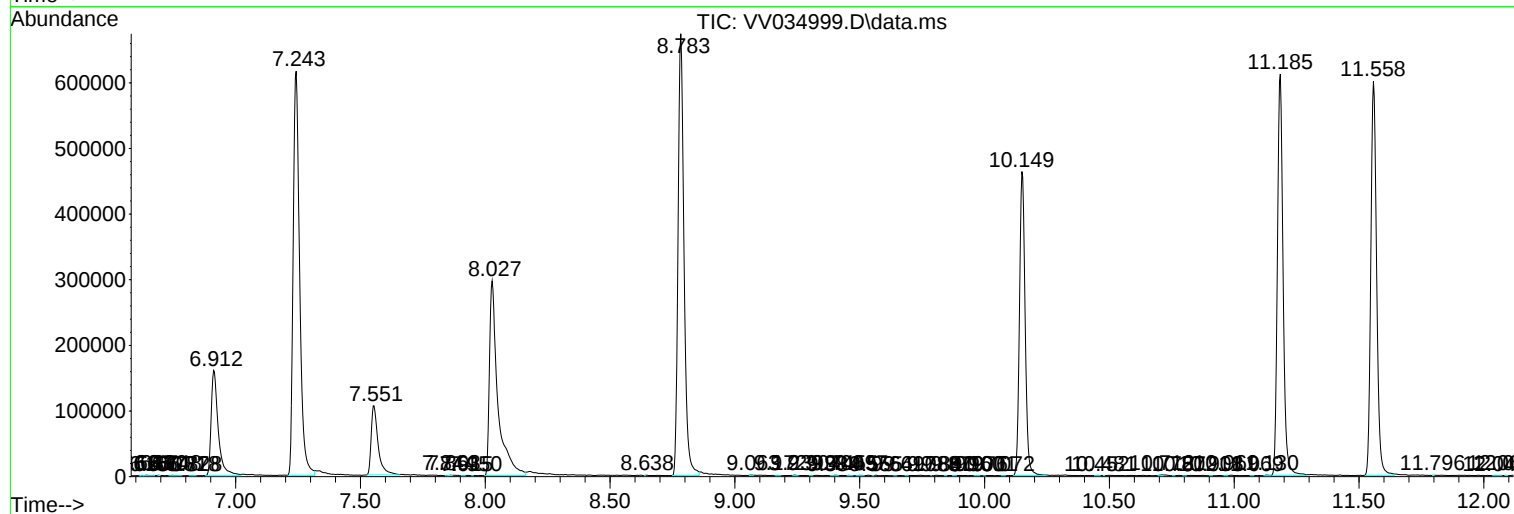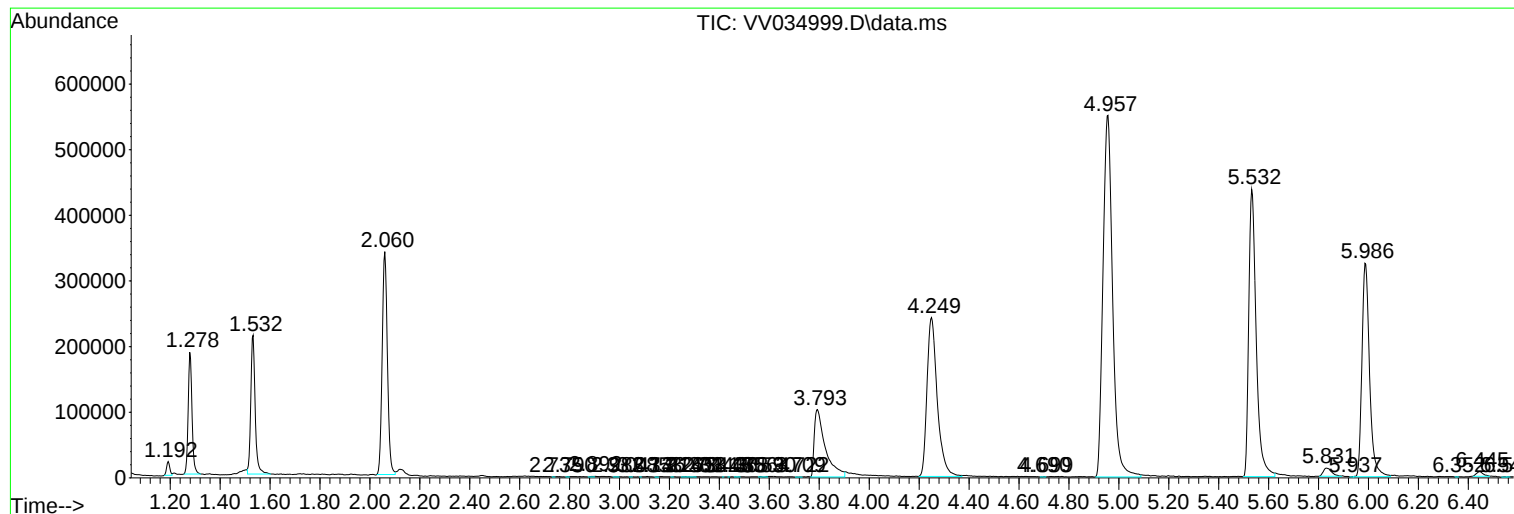

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034999.D
Acq On : 05 Apr 2024 12:33
Operator : SY/MD
Sample : P1965-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034999.D
Acq On : 05 Apr 2024 12:33
Operator : SY/MD
Sample : P1965-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc