

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035000.D
 Acq On : 05 Apr 2024 12:57
 Operator : SY/MD
 Sample : VIBLK276
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	301586	321951	16.77%	2.406%
2	1.529	146	152	172	rVB	300926	356474	18.56%	2.664%
3	2.060	307	317	344	rVB	488415	723294	37.67%	5.406%
4	2.449	429	438	452	rVB5	6026	12325	0.64%	0.092%
5	2.507	452	456	458	rBV	489	352	0.02%	0.003%
6	2.626	489	493	499	rBV4	665	753	0.04%	0.006%
7	2.677	505	509	512	rBV2	542	393	0.02%	0.003%
8	2.696	514	515	519	rVV2	432	316	0.02%	0.002%
9	2.773	536	539	540	rBV2	339	179	0.01%	0.001%
10	2.806	547	549	551	rBV	205	133	0.01%	0.001%
11	2.896	575	577	579	rBV	444	203	0.01%	0.002%
12	2.908	579	581	585	rVB2	423	265	0.01%	0.002%
13	2.992	604	607	611	rBV3	490	407	0.02%	0.003%
14	3.066	627	630	632	rBV3	254	171	0.01%	0.001%
15	3.134	648	651	653	rVB3	453	250	0.01%	0.002%
16	3.162	655	660	662	rBV2	641	475	0.02%	0.004%
17	3.240	679	684	689	rVV4	357	467	0.02%	0.003%
18	3.281	695	697	701	rBV	321	243	0.01%	0.002%
19	3.349	711	718	720	rBV3	431	453	0.02%	0.003%
20	3.362	720	722	725	rVV2	482	278	0.01%	0.002%
21	3.391	729	731	734	rVV	444	283	0.01%	0.002%
22	3.552	779	781	785	rVB2	242	137	0.01%	0.001%
23	3.590	785	793	797	rBV2	508	537	0.03%	0.004%
24	3.613	797	800	804	rVB2	430	263	0.01%	0.002%
25	3.635	804	807	808	rBV2	265	161	0.01%	0.001%
26	3.696	823	826	828	rBV	378	256	0.01%	0.002%
27	3.738	835	839	846	rBV2	541	450	0.02%	0.003%
28	3.789	846	855	891	rBV	121707	375482	19.55%	2.806%
29	4.246	983	997	1030	rBV	291687	745015	38.80%	5.568%
30	4.600	1104	1107	1109	rBV3	361	229	0.01%	0.002%
31	4.683	1127	1133	1134	rBV5	493	456	0.02%	0.003%
32	4.748	1149	1153	1155	rBV3	464	310	0.02%	0.002%
33	4.783	1162	1164	1168	rVB3	733	458	0.02%	0.003%
34	4.805	1168	1171	1172	rBV2	274	156	0.01%	0.001%
35	4.857	1186	1187	1191	rVB3	258	161	0.01%	0.001%
36	4.876	1191	1193	1196	rBV2	364	240	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035000.D
 Acq On : 05 Apr 2024 12:57
 Operator : SY/MD
 Sample : VIBLK276
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.953	1201	1217	1252	rBV2	723566	1920182	100.00%	14.351%
38	5.336	1333	1336	1338	rBV3	960	562	0.03%	0.004%
39	5.532	1386	1397	1432	rBV	433757	909950	47.39%	6.801%
40	5.934	1518	1522	1525	rBV4	808	606	0.03%	0.005%
41	5.986	1525	1538	1566	rBV	418714	875040	45.57%	6.540%
42	6.297	1633	1635	1636	rBV	293	141	0.01%	0.001%
43	6.313	1639	1640	1642	rBV2	464	198	0.01%	0.001%
44	6.606	1729	1731	1734	rBV2	255	154	0.01%	0.001%
45	6.658	1740	1747	1753	rBV5	755	1039	0.05%	0.008%
46	6.706	1759	1762	1765	rVB	686	487	0.03%	0.004%
47	6.722	1765	1767	1770	rBV	312	154	0.01%	0.001%
48	6.748	1770	1775	1778	rVV3	794	526	0.03%	0.004%
49	6.767	1778	1781	1783	rVV2	488	337	0.02%	0.003%
50	6.783	1784	1786	1789	rVB3	646	253	0.01%	0.002%
51	6.850	1801	1807	1809	rBV	341	383	0.02%	0.003%
52	6.912	1815	1826	1858	rBV	207786	398894	20.77%	2.981%
53	7.239	1918	1928	1965	rBV	840671	1478648	77.01%	11.051%
54	7.551	2016	2025	2053	rBV	139973	262746	13.68%	1.964%
55	7.895	2129	2132	2134	rBV2	418	234	0.01%	0.002%
56	7.937	2143	2145	2149	rBV	335	244	0.01%	0.002%
57	8.024	2163	2172	2211	rBV2	355941	814977	42.44%	6.091%
58	8.715	2384	2387	2390	rBV2	651	465	0.02%	0.003%
59	8.783	2397	2408	2429	rBV	671335	1108200	57.71%	8.283%
60	9.252	2551	2554	2557	rBV	708	486	0.03%	0.004%
61	9.368	2587	2590	2591	rBV2	346	223	0.01%	0.002%
62	9.410	2600	2603	2605	rBV	212	163	0.01%	0.001%
63	9.426	2605	2608	2611	rVV2	325	267	0.01%	0.002%
64	9.458	2616	2618	2620	rBV2	488	264	0.01%	0.002%
65	9.497	2628	2630	2634	rBV	318	239	0.01%	0.002%
66	9.564	2645	2651	2654	rBV2	400	454	0.02%	0.003%
67	9.580	2654	2656	2660	rVV3	188	134	0.01%	0.001%
68	9.645	2670	2676	2679	rVB3	454	433	0.02%	0.003%
69	9.670	2679	2684	2686	rVB3	285	267	0.01%	0.002%
70	9.686	2686	2689	2690	rBV	462	219	0.01%	0.002%
71	9.780	2716	2718	2721	rVB	388	198	0.01%	0.001%
72	9.805	2721	2726	2727	rBV2	236	160	0.01%	0.001%
73	9.841	2735	2737	2740	rVB2	289	148	0.01%	0.001%
74	9.902	2754	2756	2762	rVB3	287	168	0.01%	0.001%
75	10.072	2807	2809	2810	rBV3	275	126	0.01%	0.001%
76	10.149	2821	2833	2851	rBV	549334	878188	45.73%	6.564%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035000.D
 Acq On : 05 Apr 2024 12:57
 Operator : SY/MD
 Sample : VIBLK276
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.371	2899	2902	2903	rBV	430	246	0.01%	0.002%
78	10.448	2923	2926	2928	rBV	277	199	0.01%	0.001%
79	10.564	2959	2962	2967	rBV2	286	254	0.01%	0.002%
80	10.625	2979	2981	2985	rBV2	260	141	0.01%	0.001%
81	10.709	3003	3007	3008	rBV	360	255	0.01%	0.002%
82	10.763	3019	3024	3027	rBV3	384	395	0.02%	0.003%
83	10.844	3046	3049	3056	rBV2	505	431	0.02%	0.003%
84	10.915	3069	3071	3074	rBV2	225	128	0.01%	0.001%
85	11.008	3098	3100	3103	rBV2	186	151	0.01%	0.001%
86	11.185	3144	3155	3181	rBV	602514	956974	49.84%	7.152%
87	11.558	3259	3271	3298	rBV	770987	1215436	63.30%	9.084%
88	11.937	3385	3389	3396	rVB3	556	620	0.03%	0.005%
89	11.972	3396	3400	3403	rBV2	503	379	0.02%	0.003%
90	12.001	3407	3409	3412	rBV2	400	363	0.02%	0.003%
91	12.194	3466	3469	3472	rVB	726	466	0.02%	0.003%
92	12.271	3491	3493	3496	rVB2	500	247	0.01%	0.002%
93	12.288	3496	3498	3500	rBV	376	209	0.01%	0.002%
94	12.570	3584	3586	3587	rBV	441	196	0.01%	0.001%
95	12.779	3648	3651	3655	rBV2	452	372	0.02%	0.003%
96	12.815	3658	3662	3665	rVB2	614	413	0.02%	0.003%
97	12.879	3676	3682	3685	rBV3	516	548	0.03%	0.004%
98	13.011	3721	3723	3726	rBV2	402	223	0.01%	0.002%
99	13.451	3857	3860	3861	rBV	403	207	0.01%	0.002%
100	13.892	3995	3997	4000	rBV	582	347	0.02%	0.003%




Sum of corrected areas: 13379733

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035000.D
Acq On : 05 Apr 2024 12:57
Operator : SY/MD
Sample : VIBLK276
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

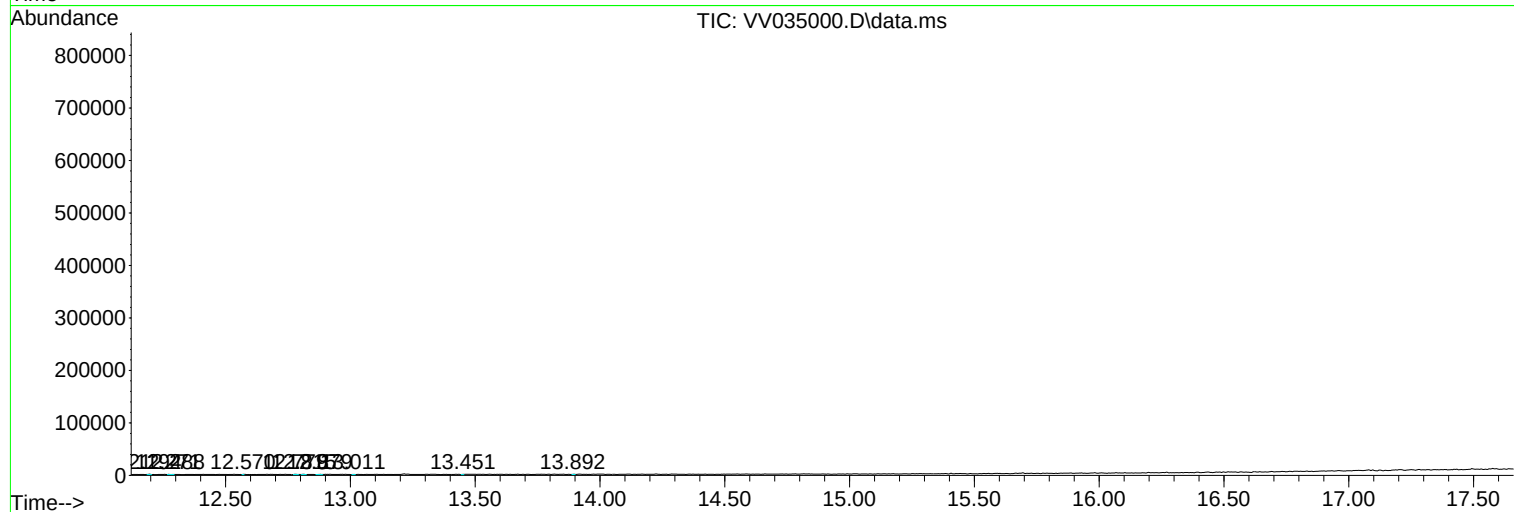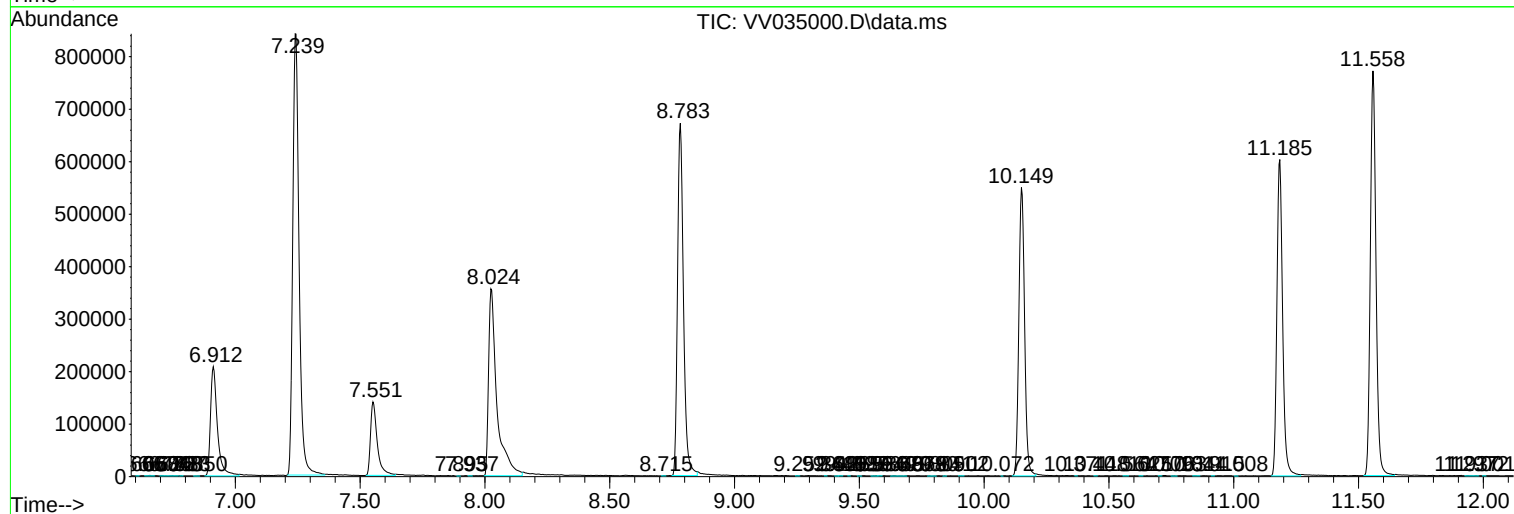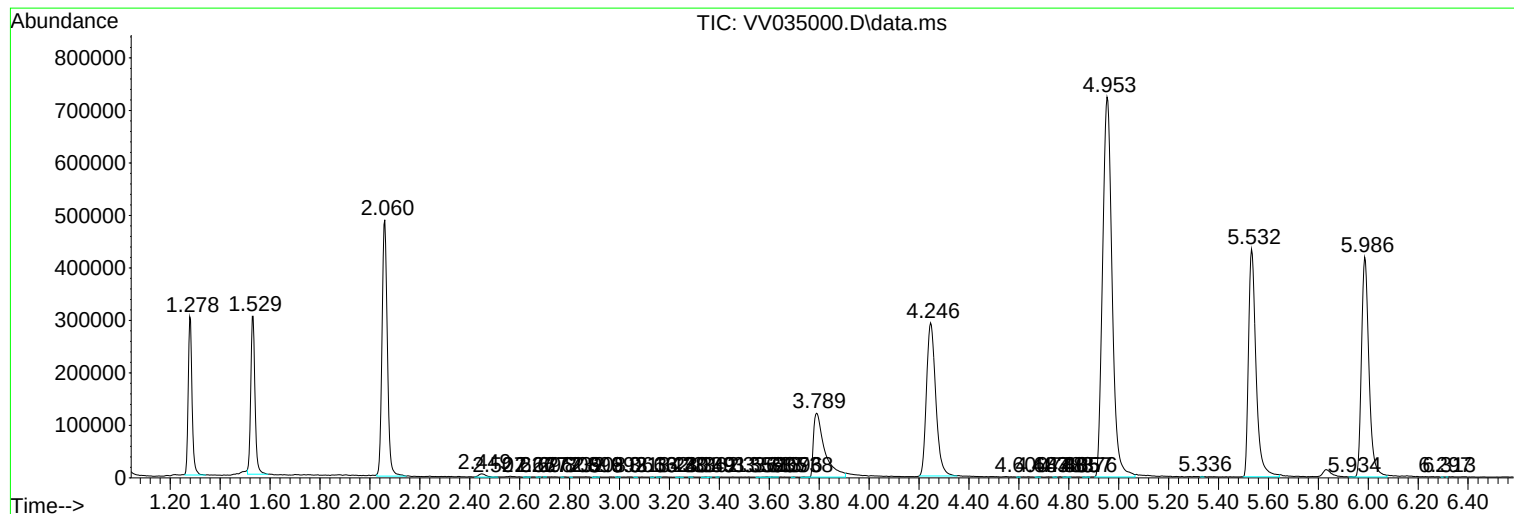

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035000.D
Acq On : 05 Apr 2024 12:57
Operator : SY/MD
Sample : VIBLK276
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035000.D
Acq On : 05 Apr 2024 12:57
Operator : SY/MD
Sample : VIBLK276
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc