

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040524\
 Data File : VV035002.D
 Acq On : 05 Apr 2024 13:45
 Operator : SY/MD
 Sample : P1993-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	159267	173292	12.13%	1.614%
2	1.529	146	152	179	rVB	191313	240291	16.82%	2.238%
3	2.056	307	316	332	rBV	293559	423766	29.67%	3.946%
4	2.445	432	437	439	rBV5	1573	1678	0.12%	0.016%
5	2.828	553	556	558	rBV2	279	175	0.01%	0.002%
6	2.886	570	574	577	rVB	458	351	0.02%	0.003%
7	2.944	591	592	594	rVB2	383	126	0.01%	0.001%
8	2.998	607	609	611	rVB2	360	133	0.01%	0.001%
9	3.018	611	615	616	rBV	434	323	0.02%	0.003%
10	3.063	625	629	632	rBV3	426	346	0.02%	0.003%
11	3.114	642	645	651	rBV4	281	274	0.02%	0.003%
12	3.182	662	666	670	rVB3	522	380	0.03%	0.004%
13	3.368	721	724	727	rBV	218	157	0.01%	0.001%
14	3.416	736	739	740	rBV2	403	256	0.02%	0.002%
15	3.532	770	775	778	rBV3	353	325	0.02%	0.003%
16	3.558	780	783	790	rVB3	476	567	0.04%	0.005%
17	3.587	790	792	795	rVB	233	110	0.01%	0.001%
18	3.619	795	802	805	rBV3	416	517	0.04%	0.005%
19	3.651	809	812	817	rVB2	421	311	0.02%	0.003%
20	3.677	817	820	824	rBV2	475	383	0.03%	0.004%
21	3.793	847	856	902	rBV2	101225	321228	22.49%	2.991%
22	4.246	982	997	1031	rBV	227349	589866	41.30%	5.493%
23	4.632	1115	1117	1120	rVB2	666	304	0.02%	0.003%
24	4.693	1133	1136	1140	rVB3	600	412	0.03%	0.004%
25	4.725	1143	1146	1148	rBV3	341	231	0.02%	0.002%
26	4.767	1156	1159	1161	rBV	599	344	0.02%	0.003%
27	4.802	1168	1170	1174	rBV3	438	299	0.02%	0.003%
28	4.879	1192	1194	1195	rBV	400	174	0.01%	0.002%
29	4.953	1202	1217	1253	rBV2	533205	1428335	100.00%	13.300%
30	5.532	1386	1397	1429	rBV	425952	890605	62.35%	8.293%
31	5.831	1482	1490	1504	rBV4	13618	26762	1.87%	0.249%
32	5.940	1515	1524	1526	rBV5	19417	30148	2.11%	0.281%
33	5.985	1529	1538	1562	rVB	338478	700649	49.05%	6.524%
34	6.599	1727	1729	1730	rBV	553	245	0.02%	0.002%
35	6.702	1757	1761	1763	rBV2	505	259	0.02%	0.002%
36	6.808	1789	1794	1795	rBV3	748	465	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035002.D
 Acq On : 05 Apr 2024 13:45
 Operator : SY/MD
 Sample : P1993-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.866	1810	1812	1816	rBV4	588	530	0.04%	0.005%
38	6.911	1816	1826	1854	rBV	157190	311517	21.81%	2.901%
39	7.243	1918	1929	1956	rBV	578563	1045167	73.17%	9.732%
40	7.554	2017	2026	2053	rBV2	106920	202869	14.20%	1.889%
41	7.780	2094	2096	2102	rVB5	860	759	0.05%	0.007%
42	7.963	2147	2153	2155	rBV4	484	549	0.04%	0.005%
43	7.992	2159	2162	2164	rBV	634	414	0.03%	0.004%
44	8.027	2164	2173	2215	rBV2	299140	694645	48.63%	6.468%
45	8.622	2354	2358	2359	rBV3	615	378	0.03%	0.004%
46	8.783	2395	2408	2439	rBV	653585	1092325	76.48%	10.172%
47	9.194	2534	2536	2540	rVB2	685	350	0.02%	0.003%
48	9.214	2540	2542	2545	rBV2	454	255	0.02%	0.002%
49	9.242	2549	2551	2554	rVB	404	167	0.01%	0.002%
50	9.262	2554	2557	2558	rBV2	330	167	0.01%	0.002%
51	9.287	2563	2565	2569	rVB	274	132	0.01%	0.001%
52	9.310	2569	2572	2575	rBV2	442	355	0.02%	0.003%
53	9.365	2586	2589	2591	rVV2	517	281	0.02%	0.003%
54	9.378	2591	2593	2595	rVB	410	159	0.01%	0.001%
55	9.506	2627	2633	2638	rBV4	619	719	0.05%	0.007%
56	9.532	2638	2641	2643	rBV3	435	267	0.02%	0.002%
57	9.609	2663	2665	2668	rBV3	297	206	0.01%	0.002%
58	9.680	2685	2687	2690	rBV3	386	277	0.02%	0.003%
59	9.722	2695	2700	2702	rBV3	730	558	0.04%	0.005%
60	9.760	2709	2712	2715	rBV	569	301	0.02%	0.003%
61	9.783	2715	2719	2722	rBV3	808	714	0.05%	0.007%
62	9.876	2746	2748	2749	rBV3	288	143	0.01%	0.001%
63	9.895	2753	2754	2758	rVV2	404	184	0.01%	0.002%
64	9.979	2774	2780	2782	rBV2	373	310	0.02%	0.003%
65	10.004	2785	2788	2789	rBV	404	191	0.01%	0.002%
66	10.050	2797	2802	2803	rBV2	415	316	0.02%	0.003%
67	10.075	2808	2810	2811	rBV	279	121	0.01%	0.001%
68	10.085	2811	2813	2814	rBV	275	102	0.01%	0.001%
69	10.149	2822	2833	2855	rBV	450211	720663	50.45%	6.711%
70	10.429	2918	2920	2925	rVB	504	229	0.02%	0.002%
71	10.541	2953	2955	2962	rVB	578	467	0.03%	0.004%
72	10.567	2962	2963	2965	rBV	388	147	0.01%	0.001%
73	10.615	2976	2978	2986	rVB3	510	532	0.04%	0.005%
74	10.670	2992	2995	2997	rVV2	252	122	0.01%	0.001%
75	10.757	3019	3022	3024	rVB2	497	252	0.02%	0.002%
76	10.783	3027	3030	3033	rBV3	408	273	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035002.D
 Acq On : 05 Apr 2024 13:45
 Operator : SY/MD
 Sample : P1993-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.805	3033	3037	3038	rBV2	402	269	0.02%	0.003%
78	10.866	3053	3056	3058	rBV3	481	324	0.02%	0.003%
79	10.924	3071	3074	3075	rBV	343	165	0.01%	0.002%
80	10.943	3078	3080	3081	rBV	363	120	0.01%	0.001%
81	10.985	3091	3093	3095	rVB	459	173	0.01%	0.002%
82	11.001	3095	3098	3102	rBV2	404	351	0.02%	0.003%
83	11.114	3125	3133	3135	rBV4	1190	1541	0.11%	0.014%
84	11.185	3144	3155	3187	rBV	571415	902498	63.19%	8.404%
85	11.403	3221	3223	3227	rBV2	677	412	0.03%	0.004%
86	11.506	3246	3255	3256	rBV6	6278	7562	0.53%	0.070%
87	11.557	3261	3271	3292	rVB	563815	903650	63.27%	8.415%
88	11.937	3388	3389	3391	rVB2	636	216	0.02%	0.002%
89	12.159	3455	3458	3459	rBV2	461	236	0.02%	0.002%
90	12.181	3461	3465	3468	rVV3	564	486	0.03%	0.005%
91	12.297	3497	3501	3514	rVB8	3075	5650	0.40%	0.053%
92	12.435	3542	3544	3548	rBV2	630	395	0.03%	0.004%
93	12.840	3660	3670	3671	rBV2	638	652	0.05%	0.006%
94	12.876	3679	3681	3683	rBV	298	143	0.01%	0.001%
95	12.937	3697	3700	3704	rVB3	649	474	0.03%	0.004%
96	13.133	3758	3761	3766	rVB4	590	407	0.03%	0.004%
97	13.155	3766	3768	3773	rBV3	474	408	0.03%	0.004%
98	13.387	3838	3840	3843	rBV2	438	249	0.02%	0.002%
99	13.416	3847	3849	3852	rVB2	449	209	0.01%	0.002%
100	14.786	4273	4275	4277	rBV2	607	202	0.01%	0.002%


Sum of corrected areas: 10738992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035002.D
Acq On : 05 Apr 2024 13:45
Operator : SY/MD
Sample : P1993-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

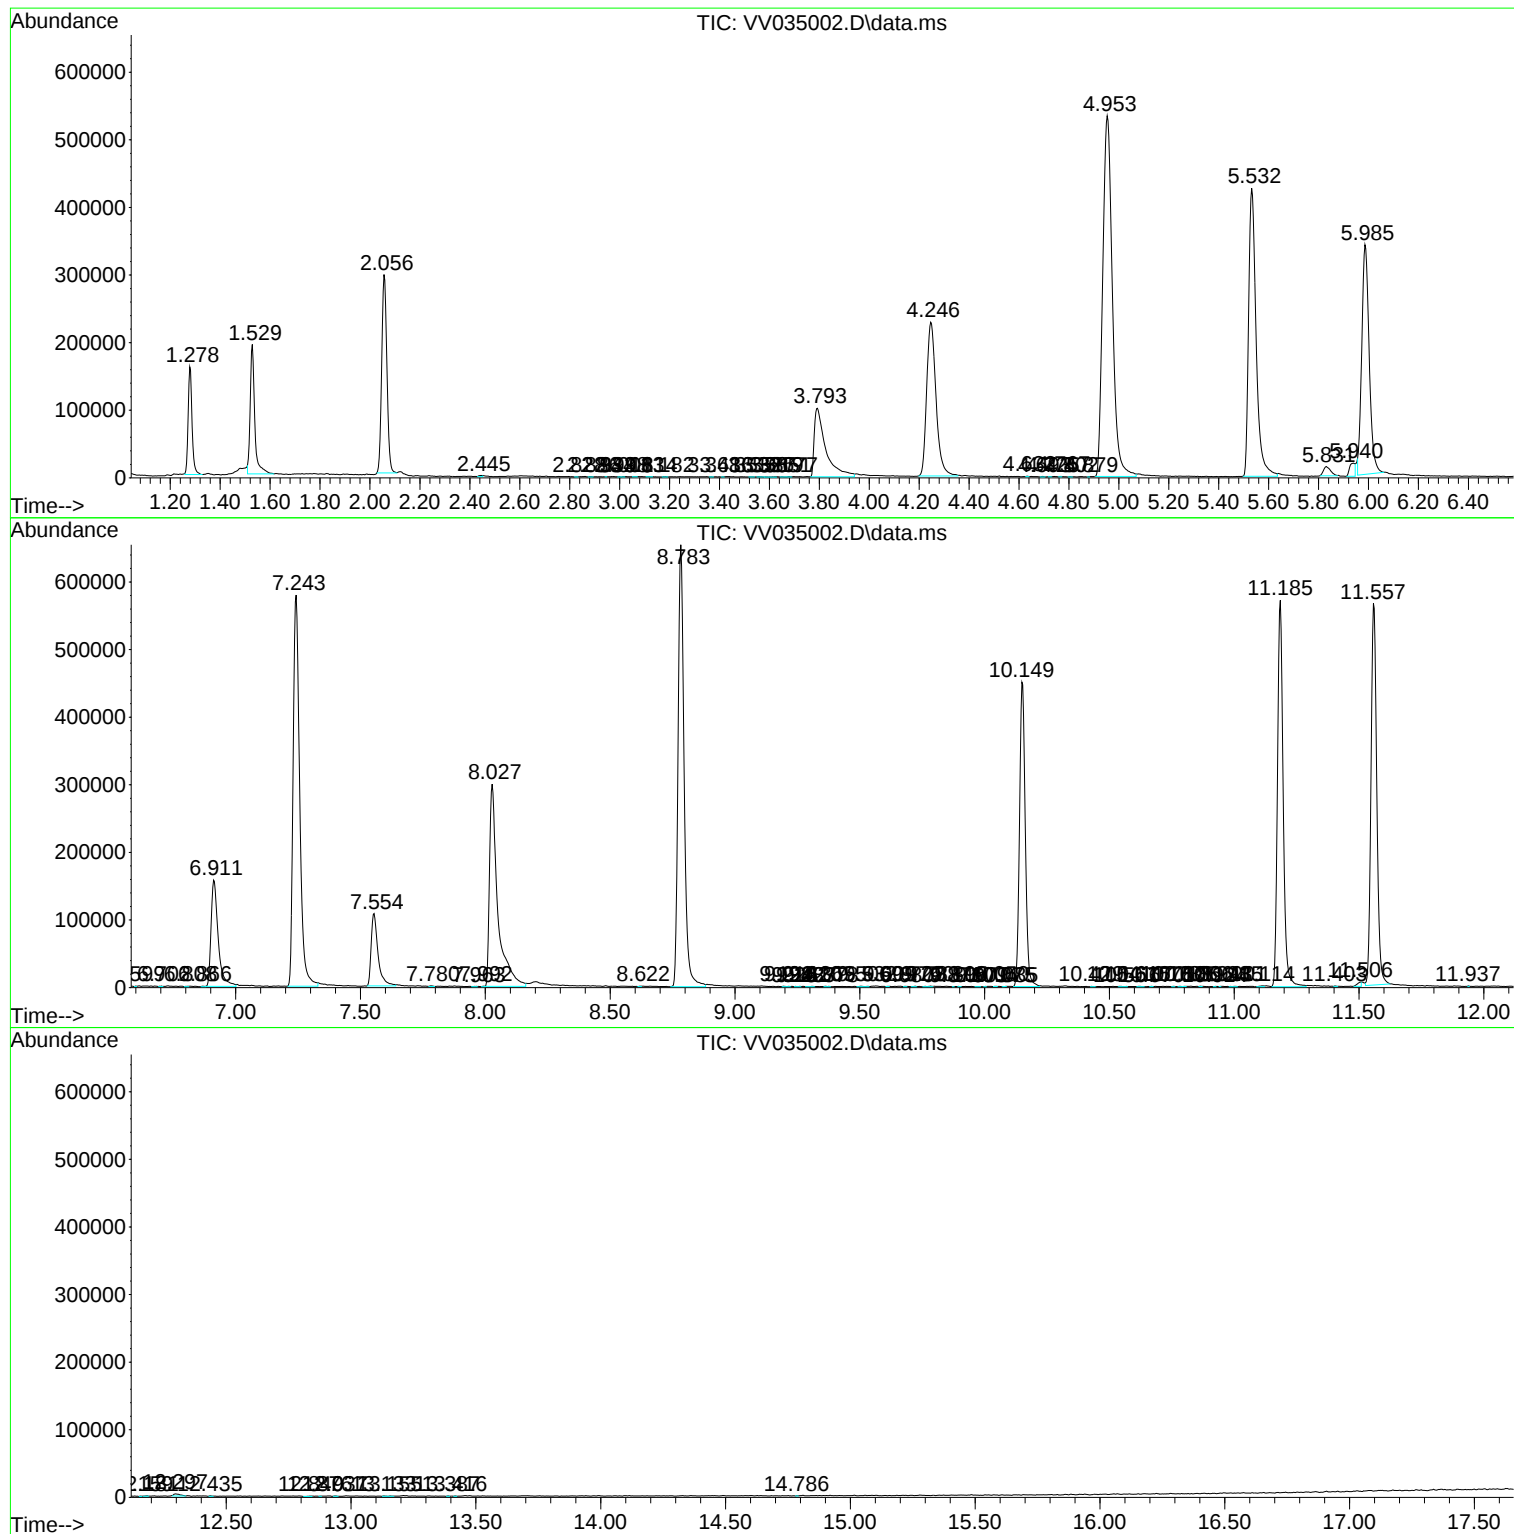

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035002.D
Acq On : 05 Apr 2024 13:45
Operator : SY/MD
Sample : P1993-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035002.D
Acq On : 05 Apr 2024 13:45
Operator : SY/MD
Sample : P1993-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------