

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035003.D
 Acq On : 05 Apr 2024 14:09
 Operator : SY/MD
 Sample : P1993-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	183974	196520	13.30%	1.755%
2	1.529	146	152	169	rVB	210041	248380	16.81%	2.218%
3	2.060	307	317	332	rBV	331499	487630	33.01%	4.354%
4	2.786	541	543	549	rVB5	519	339	0.02%	0.003%
5	2.880	569	572	576	rBV2	441	378	0.03%	0.003%
6	2.921	583	585	587	rBV2	475	252	0.02%	0.002%
7	2.957	594	596	599	rBV3	370	272	0.02%	0.002%
8	2.986	601	605	609	rVB4	685	641	0.04%	0.006%
9	3.008	609	612	614	rBV	260	208	0.01%	0.002%
10	3.021	614	616	621	rVB3	412	241	0.02%	0.002%
11	3.044	621	623	624	rBV	319	133	0.01%	0.001%
12	3.072	629	632	634	rVV	224	126	0.01%	0.001%
13	3.095	635	639	641	rVV2	230	136	0.01%	0.001%
14	3.121	643	647	649	rBV2	361	226	0.02%	0.002%
15	3.140	650	653	658	rVB3	486	403	0.03%	0.004%
16	3.163	658	660	661	rBV	340	171	0.01%	0.002%
17	3.185	665	667	672	rVB2	407	273	0.02%	0.002%
18	3.220	675	678	683	rBV2	472	381	0.03%	0.003%
19	3.262	686	691	694	rBV2	395	364	0.02%	0.003%
20	3.397	727	733	735	rBV3	307	187	0.01%	0.002%
21	3.413	735	738	742	rVB3	409	275	0.02%	0.002%
22	3.445	746	748	750	rBV2	301	153	0.01%	0.001%
23	3.487	758	761	763	rBV3	501	295	0.02%	0.003%
24	3.519	769	771	776	rVB3	443	298	0.02%	0.003%
25	3.542	776	778	779	rBV	200	105	0.01%	0.001%
26	3.597	794	795	801	rVB2	346	178	0.01%	0.002%
27	3.629	802	805	807	rBV2	234	131	0.01%	0.001%
28	3.716	828	832	835	rBV	413	409	0.03%	0.004%
29	3.744	838	841	842	rBV	398	199	0.01%	0.002%
30	3.790	847	855	905	rBV	106246	333349	22.57%	2.977%
31	4.246	982	997	1030	rBV	235160	607713	41.14%	5.427%
32	4.667	1126	1128	1131	rBV2	379	248	0.02%	0.002%
33	4.802	1165	1170	1172	rVB2	555	479	0.03%	0.004%
34	4.818	1172	1175	1179	rBV	339	323	0.02%	0.003%
35	4.870	1187	1191	1193	rBV	237	193	0.01%	0.002%
36	4.953	1202	1217	1254	rBV2	550541	1477146	100.00%	13.190%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035003.D
 Acq On : 05 Apr 2024 14:09
 Operator : SY/MD
 Sample : P1993-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.294	1321	1323	1325	rBV2	552	259	0.02%	0.002%
38	5.391	1351	1353	1355	rBV2	392	163	0.01%	0.001%
39	5.436	1365	1367	1375	rVB3	528	512	0.03%	0.005%
40	5.532	1386	1397	1433	rBV	440803	920032	62.28%	8.215%
41	5.831	1480	1490	1508	rBV2	14051	31853	2.16%	0.284%
42	5.931	1514	1521	1525	rBV3	15166	23955	1.62%	0.214%
43	5.986	1529	1538	1569	rVB	347615	716259	48.49%	6.396%
44	6.452	1680	1683	1686	rVB2	876	532	0.04%	0.005%
45	6.551	1711	1714	1718	rBV2	427	323	0.02%	0.003%
46	6.809	1791	1794	1799	rBV2	868	747	0.05%	0.007%
47	6.912	1813	1826	1859	rBV	160789	319200	21.61%	2.850%
48	7.178	1906	1909	1912	rBV3	511	374	0.03%	0.003%
49	7.243	1918	1929	1961	rBV	610312	1089224	73.74%	9.726%
50	7.555	2016	2026	2054	rBV	107993	207354	14.04%	1.852%
51	7.976	2154	2157	2159	rBV	474	316	0.02%	0.003%
52	8.027	2164	2173	2219	rBV2	316862	723809	49.00%	6.463%
53	8.584	2343	2346	2349	rBV4	657	515	0.03%	0.005%
54	8.712	2384	2386	2388	rBV3	403	191	0.01%	0.002%
55	8.783	2397	2408	2434	rBV	677840	1118586	75.73%	9.988%
56	9.140	2517	2519	2520	rBV	372	144	0.01%	0.001%
57	9.153	2520	2523	2525	rVV2	354	278	0.02%	0.002%
58	9.256	2553	2555	2558	rVV2	425	175	0.01%	0.002%
59	9.272	2558	2560	2564	rVB2	714	365	0.02%	0.003%
60	9.294	2564	2567	2569	rBV2	384	228	0.02%	0.002%
61	9.362	2584	2588	2592	rBV	356	300	0.02%	0.003%
62	9.535	2637	2642	2645	rBV4	1006	1068	0.07%	0.010%
63	9.609	2663	2665	2666	rBV	407	116	0.01%	0.001%
64	9.654	2676	2679	2681	rBV3	699	603	0.04%	0.005%
65	9.722	2698	2700	2702	rBV	378	197	0.01%	0.002%
66	9.735	2702	2704	2708	rVB2	756	409	0.03%	0.004%
67	9.767	2708	2714	2718	rBV3	627	737	0.05%	0.007%
68	9.792	2719	2722	2726	rBV3	764	549	0.04%	0.005%
69	9.883	2748	2750	2754	rVB2	423	213	0.01%	0.002%
70	9.931	2763	2765	2768	rVB2	489	218	0.01%	0.002%
71	9.982	2778	2781	2782	rBV	427	197	0.01%	0.002%
72	10.040	2797	2799	2804	rBV2	313	246	0.02%	0.002%
73	10.079	2809	2811	2813	rVB	374	142	0.01%	0.001%
74	10.098	2813	2817	2819	rBV3	703	533	0.04%	0.005%
75	10.149	2822	2833	2857	rBV	464796	738308	49.98%	6.593%
76	10.445	2923	2925	2928	rBV	357	210	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035003.D
 Acq On : 05 Apr 2024 14:09
 Operator : SY/MD
 Sample : P1993-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.519	2946	2948	2949	rBV2	242	135	0.01%	0.001%
78	10.545	2954	2956	2960	rBV2	456	320	0.02%	0.003%
79	10.606	2973	2975	2979	rBV3	340	190	0.01%	0.002%
80	10.651	2987	2989	2992	rBV2	275	196	0.01%	0.002%
81	10.757	3018	3022	3024	rBV	308	231	0.02%	0.002%
82	10.866	3052	3056	3060	rBV	704	515	0.03%	0.005%
83	10.905	3065	3068	3070	rBV	405	216	0.01%	0.002%
84	11.185	3144	3155	3182	rBV	613756	955184	64.66%	8.529%
85	11.506	3247	3255	3256	rBV5	5388	5892	0.40%	0.053%
86	11.558	3261	3271	3294	rVB	606202	963616	65.23%	8.605%
87	11.992	3403	3406	3407	rBV2	515	340	0.02%	0.003%
88	12.082	3431	3434	3437	rBV3	576	483	0.03%	0.004%
89	12.226	3477	3479	3482	rBV2	537	368	0.02%	0.003%
90	12.271	3491	3493	3494	rBV2	328	174	0.01%	0.002%
91	12.297	3494	3501	3515	rVV8	3768	7548	0.51%	0.067%
92	12.471	3554	3555	3560	rVB3	361	157	0.01%	0.001%
93	12.628	3601	3604	3612	rBV3	799	937	0.06%	0.008%
94	12.770	3642	3648	3650	rBV4	680	557	0.04%	0.005%
95	12.873	3677	3680	3685	rBV4	594	451	0.03%	0.004%
96	13.210	3780	3785	3792	rBV4	1204	1591	0.11%	0.014%
97	13.326	3817	3821	3822	rBV	271	184	0.01%	0.002%
98	13.699	3934	3937	3942	rBV3	621	556	0.04%	0.005%
99	13.886	3993	3995	3998	rBV3	496	260	0.02%	0.002%
100	13.902	3998	4000	4004	rBV	573	466	0.03%	0.004%




Sum of corrected areas: 11198762

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035003.D
Acq On : 05 Apr 2024 14:09
Operator : SY/MD
Sample : P1993-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

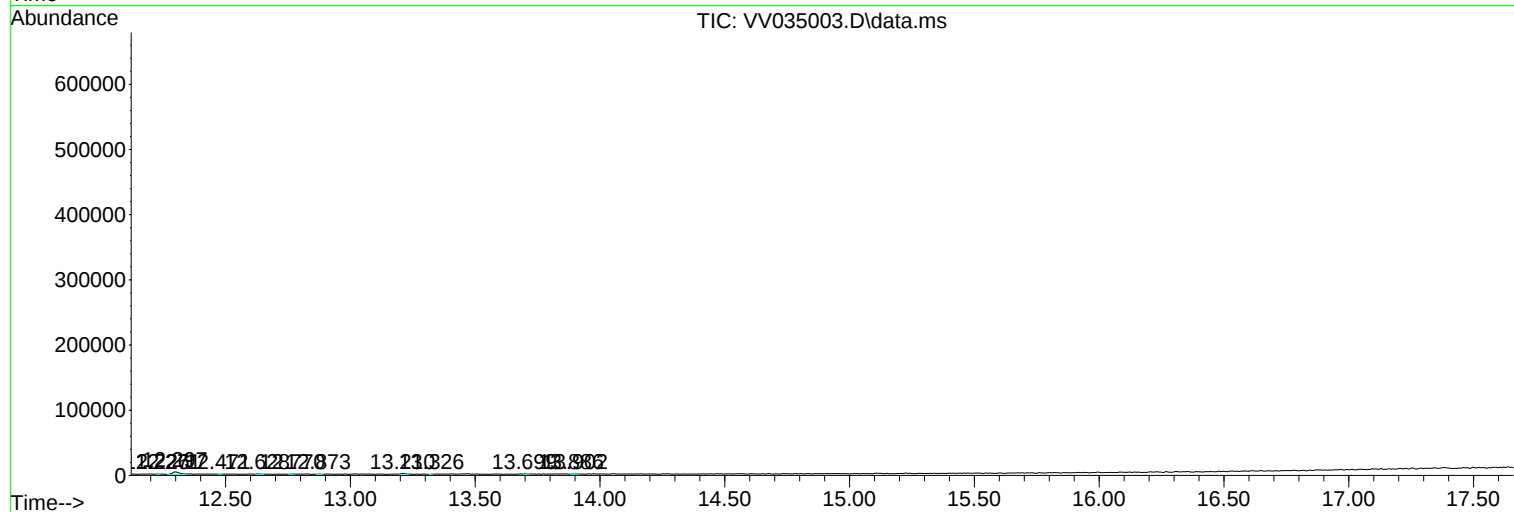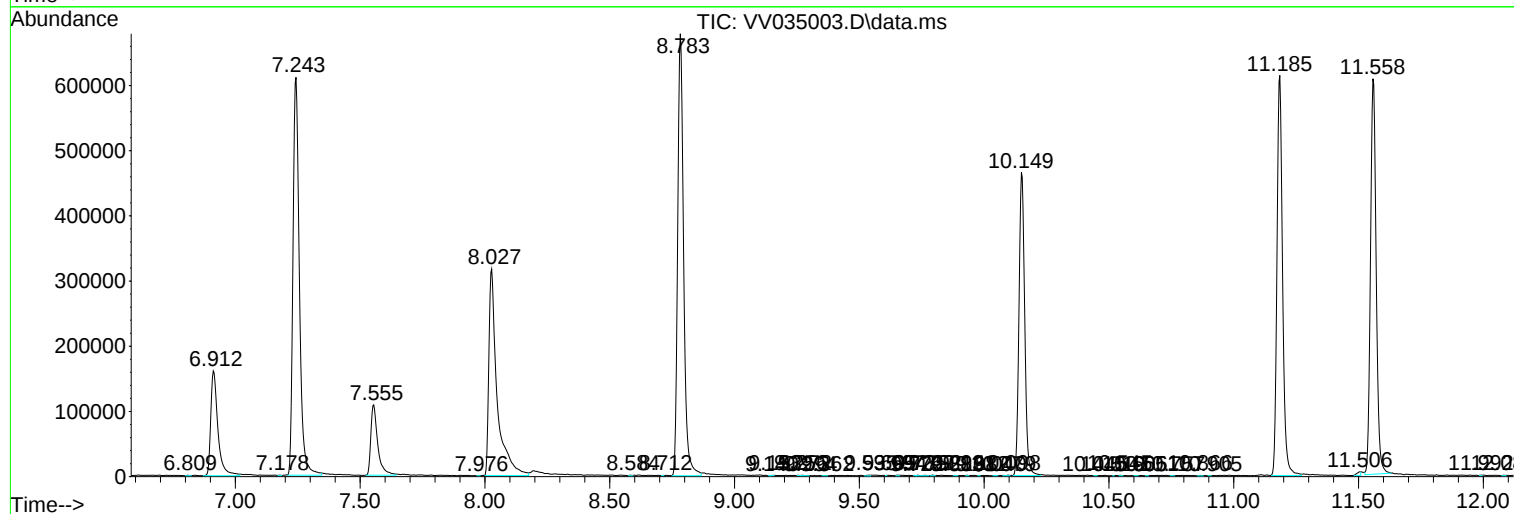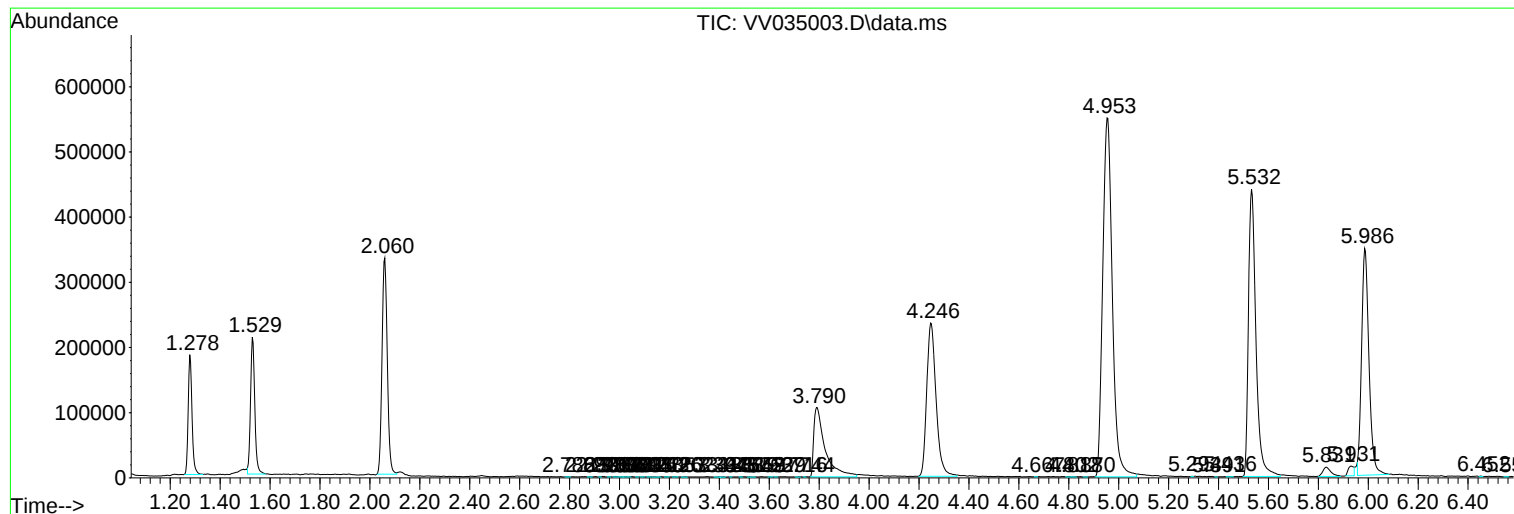

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035003.D
Acq On : 05 Apr 2024 14:09
Operator : SY/MD
Sample : P1993-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035003.D
Acq On : 05 Apr 2024 14:09
Operator : SY/MD
Sample : P1993-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------