

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035005.D
 Acq On : 05 Apr 2024 14:57
 Operator : SY/MD
 Sample : P1993-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	25	rVB	31403	31041	2.18%	0.281%
2	1.278	67	74	91	rVB	189255	210857	14.79%	1.911%
3	1.529	146	152	166	rVB	188633	222191	15.59%	2.014%
4	2.060	307	317	329	rBV	322331	468085	32.84%	4.243%
5	2.632	492	495	498	rBV2	526	368	0.03%	0.003%
6	2.658	499	503	505	rBV	661	416	0.03%	0.004%
7	2.786	541	543	546	rBV	536	339	0.02%	0.003%
8	2.873	566	570	571	rBV2	996	718	0.05%	0.007%
9	2.970	597	600	603	rBV3	845	677	0.05%	0.006%
10	3.182	664	666	669	rBV2	321	254	0.02%	0.002%
11	3.204	669	673	674	rVV	422	239	0.02%	0.002%
12	3.355	712	720	722	rBV2	352	451	0.03%	0.004%
13	3.394	729	732	735	rVB2	533	289	0.02%	0.003%
14	3.410	735	737	740	rBV2	433	233	0.02%	0.002%
15	3.494	759	763	767	rBV2	397	327	0.02%	0.003%
16	3.552	778	781	784	rVV	362	213	0.01%	0.002%
17	3.587	789	792	798	rVB	592	512	0.04%	0.005%
18	3.629	801	805	808	rBV3	332	240	0.02%	0.002%
19	3.654	808	813	815	rBV3	484	408	0.03%	0.004%
20	3.671	816	818	822	rBV2	565	347	0.02%	0.003%
21	3.728	833	836	840	rBV3	555	357	0.03%	0.003%
22	3.751	840	843	847	rBV3	514	534	0.04%	0.005%
23	3.789	847	855	897	rBV	96044	295907	20.76%	2.683%
24	4.249	982	998	1028	rBV2	243727	734378	51.53%	6.657%
25	4.513	1076	1080	1082	rBV	566	434	0.03%	0.004%
26	4.558	1092	1094	1097	rBV2	478	266	0.02%	0.002%
27	4.619	1109	1113	1115	rBV3	615	396	0.03%	0.004%
28	4.738	1147	1150	1154	rBV2	403	253	0.02%	0.002%
29	4.953	1200	1217	1253	rBV2	530197	1425282	100.00%	12.921%
30	5.487	1381	1383	1386	rVB2	453	243	0.02%	0.002%
31	5.532	1386	1397	1427	rBV	428274	894133	62.73%	8.106%
32	5.834	1482	1491	1505	rVB4	11646	25210	1.77%	0.229%
33	5.941	1521	1524	1526	rBV4	453	286	0.02%	0.003%
34	5.986	1526	1538	1567	rBV	320019	678013	47.57%	6.146%
35	6.236	1614	1616	1619	rVB3	622	284	0.02%	0.003%
36	6.323	1641	1643	1647	rBV2	700	516	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035005.D
 Acq On : 05 Apr 2024 14:57
 Operator : SY/MD
 Sample : P1993-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.416	1669	1672	1674	rBV4	745	516	0.04%	0.005%
38	6.561	1714	1717	1719	rBV	439	302	0.02%	0.003%
39	6.638	1738	1741	1743	rBV2	415	301	0.02%	0.003%
40	6.712	1762	1764	1767	rVB2	405	222	0.02%	0.002%
41	6.731	1767	1770	1772	rBV3	391	198	0.01%	0.002%
42	6.815	1793	1796	1801	rVB3	476	321	0.02%	0.003%
43	6.912	1813	1826	1857	rBV	154447	302400	21.22%	2.741%
44	7.130	1891	1894	1897	rBV3	523	355	0.02%	0.003%
45	7.153	1897	1901	1907	rBV4	521	701	0.05%	0.006%
46	7.243	1918	1929	1964	rBV	579331	1049559	73.64%	9.515%
47	7.555	2016	2026	2056	rBV	103485	202077	14.18%	1.832%
48	7.735	2078	2082	2087	rBV4	893	1036	0.07%	0.009%
49	7.911	2128	2137	2148	rBV6	3589	6184	0.43%	0.056%
50	7.973	2154	2156	2160	rVB3	545	270	0.02%	0.002%
51	8.027	2163	2173	2217	rBV3	285878	670542	47.05%	6.079%
52	8.442	2299	2302	2304	rBV2	805	531	0.04%	0.005%
53	8.487	2314	2316	2321	rVB3	540	268	0.02%	0.002%
54	8.545	2331	2334	2336	rBV3	689	415	0.03%	0.004%
55	8.651	2363	2367	2369	rBV3	540	391	0.03%	0.004%
56	8.783	2397	2408	2436	rBV	671284	1097006	76.97%	9.945%
57	9.120	2510	2513	2514	rBV	482	251	0.02%	0.002%
58	9.182	2528	2532	2535	rBV3	820	664	0.05%	0.006%
59	9.323	2570	2576	2577	rBV3	515	371	0.03%	0.003%
60	9.355	2582	2586	2587	rBV2	314	212	0.01%	0.002%
61	9.391	2594	2597	2601	rBV	254	199	0.01%	0.002%
62	9.432	2607	2610	2614	rVB2	378	278	0.02%	0.003%
63	9.458	2614	2618	2621	rBV4	534	474	0.03%	0.004%
64	9.516	2631	2636	2639	rVB3	362	276	0.02%	0.003%
65	9.535	2639	2642	2645	rBV3	354	221	0.02%	0.002%
66	9.686	2686	2689	2692	rVB2	491	309	0.02%	0.003%
67	9.712	2695	2697	2699	rVB3	463	214	0.02%	0.002%
68	9.767	2710	2714	2716	rBV	360	252	0.02%	0.002%
69	9.789	2719	2721	2722	rBV	600	271	0.02%	0.002%
70	9.873	2744	2747	2750	rVB3	579	414	0.03%	0.004%
71	9.947	2768	2770	2774	rBV	622	428	0.03%	0.004%
72	10.014	2789	2791	2794	rBV3	374	226	0.02%	0.002%
73	10.034	2794	2797	2800	rBV2	326	267	0.02%	0.002%
74	10.075	2806	2810	2812	rBV3	345	261	0.02%	0.002%
75	10.153	2820	2834	2860	rBV	455932	733229	51.44%	6.647%
76	10.506	2941	2944	2947	rBV	381	241	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035005.D
 Acq On : 05 Apr 2024 14:57
 Operator : SY/MD
 Sample : P1993-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.554	2955	2959	2960	rBV	310	210	0.01%	0.002%
78	10.587	2967	2969	2974	rVB3	832	472	0.03%	0.004%
79	10.635	2981	2984	2987	rVB2	343	199	0.01%	0.002%
80	10.712	3002	3008	3011	rBV2	551	430	0.03%	0.004%
81	10.805	3032	3037	3038	rBV2	248	208	0.01%	0.002%
82	10.972	3084	3089	3091	rBV2	306	241	0.02%	0.002%
83	10.998	3094	3097	3102	rBV2	327	269	0.02%	0.002%
84	11.021	3102	3104	3107	rBV	425	232	0.02%	0.002%
85	11.108	3123	3131	3139	rBV7	2884	4972	0.35%	0.045%
86	11.185	3144	3155	3179	rBV	616812	961728	67.48%	8.718%
87	11.490	3247	3250	3253	rBV2	631	451	0.03%	0.004%
88	11.513	3254	3257	3258	rBV2	451	222	0.02%	0.002%
89	11.558	3258	3271	3298	rBV	607074	971083	68.13%	8.803%
90	12.294	3492	3500	3515	rVV6	9093	17980	1.26%	0.163%
91	12.632	3601	3605	3610	rVV5	710	863	0.06%	0.008%
92	12.728	3632	3635	3638	rBV	391	268	0.02%	0.002%
93	12.776	3647	3650	3652	rBV3	619	390	0.03%	0.004%
94	12.863	3674	3677	3683	rBV	668	423	0.03%	0.004%
95	12.902	3683	3689	3691	rBV2	555	462	0.03%	0.004%
96	13.140	3759	3763	3766	rBV	623	441	0.03%	0.004%
97	13.207	3780	3784	3788	rBV5	875	920	0.06%	0.008%
98	13.442	3855	3857	3861	rBV2	613	352	0.02%	0.003%
99	13.480	3867	3869	3873	rBV	396	316	0.02%	0.003%
100	13.680	3925	3931	3932	rBV2	625	522	0.04%	0.005%




Sum of corrected areas: 11031004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035005.D
Acq On : 05 Apr 2024 14:57
Operator : SY/MD
Sample : P1993-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

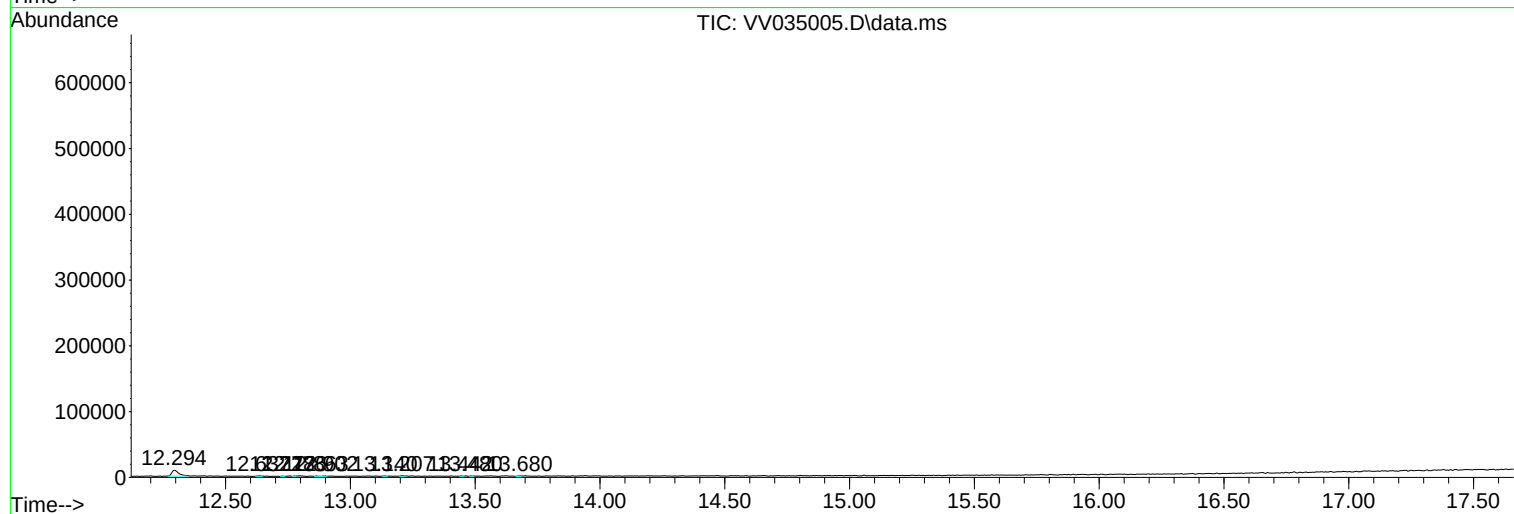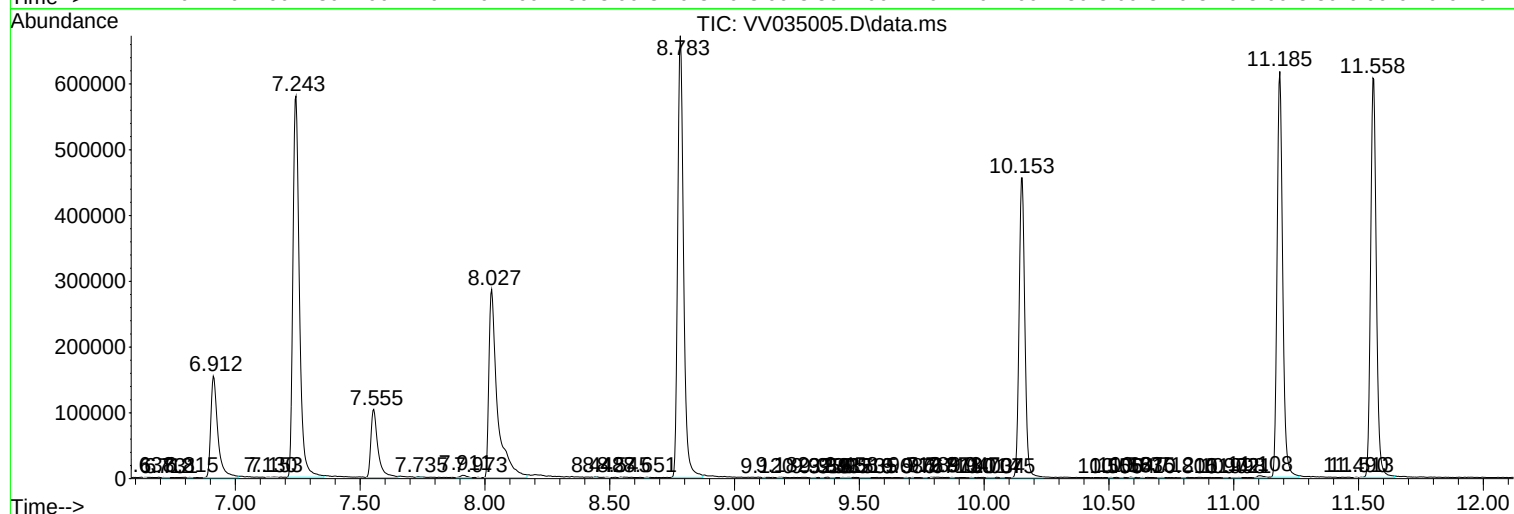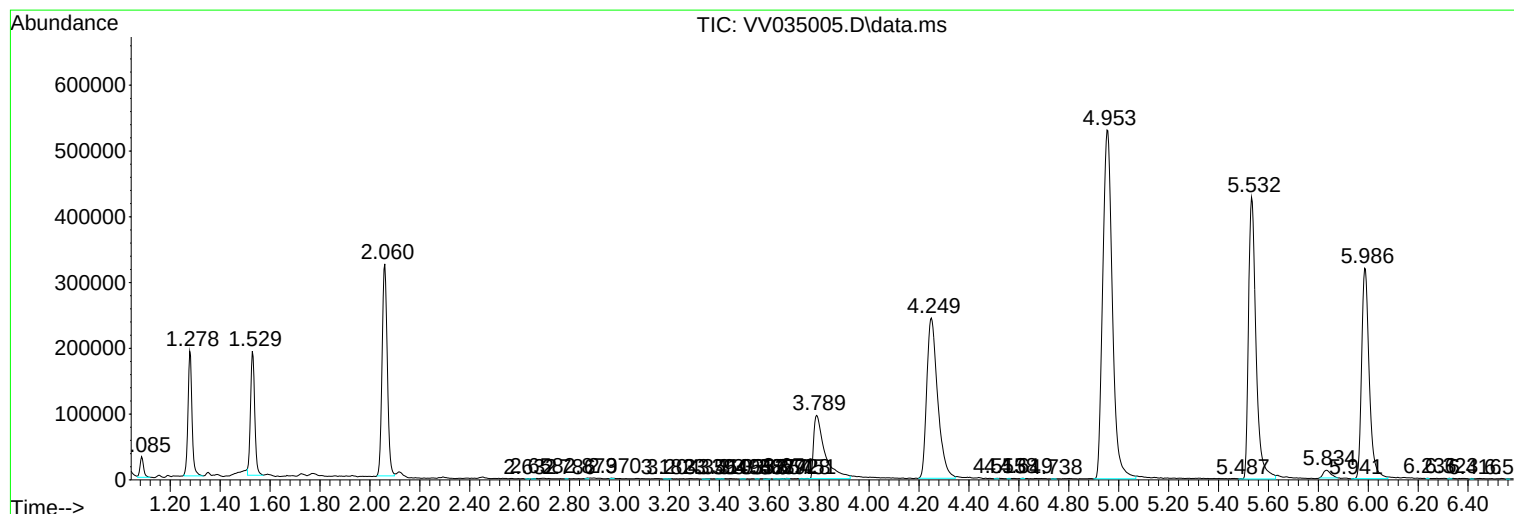

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035005.D
Acq On : 05 Apr 2024 14:57
Operator : SY/MD
Sample : P1993-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035005.D
Acq On : 05 Apr 2024 14:57
Operator : SY/MD
Sample : P1993-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
