

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035006.D
 Acq On : 05 Apr 2024 15:21
 Operator : SY/MD
 Sample : P1993-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	173912	185151	13.29%	1.722%
2	1.529	146	152	168	rVB	179468	212877	15.28%	1.980%
3	2.060	307	317	331	rBV	311444	459357	32.97%	4.273%
4	2.452	431	439	445	rBV5	1950	2710	0.19%	0.025%
5	2.703	516	517	521	rVB2	897	444	0.03%	0.004%
6	2.783	539	542	544	rBV	458	262	0.02%	0.002%
7	2.799	544	547	548	rBV	359	194	0.01%	0.002%
8	2.970	599	600	603	rBV2	392	225	0.02%	0.002%
9	3.072	630	632	636	rBV2	373	164	0.01%	0.002%
10	3.134	648	651	654	rBV3	455	349	0.03%	0.003%
11	3.195	666	670	675	rVB2	624	482	0.03%	0.004%
12	3.220	675	678	680	rBV2	424	265	0.02%	0.002%
13	3.240	680	684	686	rBV	565	394	0.03%	0.004%
14	3.320	707	709	711	rBV	411	236	0.02%	0.002%
15	3.355	718	720	725	rVB2	436	260	0.02%	0.002%
16	3.391	725	731	733	rBV2	445	366	0.03%	0.003%
17	3.452	748	750	753	rBV2	486	252	0.02%	0.002%
18	3.568	784	786	788	rVB3	305	152	0.01%	0.001%
19	3.626	801	804	807	rBV2	369	292	0.02%	0.003%
20	3.674	815	819	823	rBV2	351	245	0.02%	0.002%
21	3.696	823	826	829	rBV2	343	238	0.02%	0.002%
22	3.789	846	855	892	rBV	96342	290408	20.85%	2.701%
23	4.249	983	998	1032	rBV2	234640	678902	48.73%	6.315%
24	4.687	1132	1134	1139	rVB	485	366	0.03%	0.003%
25	4.722	1139	1145	1147	rBV2	681	682	0.05%	0.006%
26	4.793	1164	1167	1168	rBV2	334	181	0.01%	0.002%
27	4.838	1178	1181	1191	rBV4	397	510	0.04%	0.005%
28	4.953	1202	1217	1250	rBV2	517912	1393141	100.00%	12.958%
29	5.442	1366	1369	1374	rVB3	995	726	0.05%	0.007%
30	5.465	1374	1376	1379	rBV	353	263	0.02%	0.002%
31	5.532	1386	1397	1432	rBV	429346	902845	64.81%	8.398%
32	5.834	1479	1491	1507	rBV3	12230	30235	2.17%	0.281%
33	5.924	1512	1519	1524	rBV4	12830	22119	1.59%	0.206%
34	5.986	1529	1538	1563	rVB	332619	678466	48.70%	6.311%
35	6.551	1712	1714	1718	rBV3	701	427	0.03%	0.004%
36	6.613	1729	1733	1735	rBV4	1069	814	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035006.D
 Acq On : 05 Apr 2024 15:21
 Operator : SY/MD
 Sample : P1993-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.764	1778	1780	1781	rBV	461	206	0.01%	0.002%
38	6.912	1816	1826	1848	rBV	152509	292605	21.00%	2.722%
39	7.117	1888	1890	1891	rBV	509	260	0.02%	0.002%
40	7.243	1918	1929	1957	rBV	569686	1028577	73.83%	9.567%
41	7.503	2008	2010	2012	rBV	469	207	0.01%	0.002%
42	7.555	2017	2026	2047	rVV	102635	191192	13.72%	1.778%
43	7.776	2093	2095	2097	rBV	409	175	0.01%	0.002%
44	7.889	2128	2130	2133	rBV3	417	169	0.01%	0.002%
45	7.918	2134	2139	2145	rVB4	1076	1178	0.08%	0.011%
46	8.027	2163	2173	2218	rBV2	280656	655475	47.05%	6.097%
47	8.612	2352	2355	2358	rBV	601	436	0.03%	0.004%
48	8.699	2379	2382	2385	rBV3	562	402	0.03%	0.004%
49	8.738	2389	2394	2397	rBV3	722	718	0.05%	0.007%
50	8.783	2397	2408	2444	rBV	670906	1115173	80.05%	10.372%
51	9.137	2515	2518	2521	rBV2	574	393	0.03%	0.004%
52	9.326	2575	2577	2580	rBV2	283	152	0.01%	0.001%
53	9.378	2589	2593	2596	rVB3	381	328	0.02%	0.003%
54	9.448	2611	2615	2617	rVB3	280	189	0.01%	0.002%
55	9.465	2618	2620	2623	rVB3	548	292	0.02%	0.003%
56	9.490	2623	2628	2629	rBV2	558	367	0.03%	0.003%
57	9.622	2667	2669	2671	rBV	366	204	0.01%	0.002%
58	9.667	2679	2683	2684	rBV3	512	263	0.02%	0.002%
59	9.696	2690	2692	2694	rBV2	332	151	0.01%	0.001%
60	9.712	2694	2697	2700	rBV	475	216	0.02%	0.002%
61	9.735	2700	2704	2706	rBV2	513	416	0.03%	0.004%
62	9.799	2723	2724	2728	rBV2	355	238	0.02%	0.002%
63	9.886	2748	2751	2753	rBV	317	176	0.01%	0.002%
64	9.911	2758	2759	2764	rBV3	374	308	0.02%	0.003%
65	9.956	2770	2773	2776	rBV2	406	297	0.02%	0.003%
66	10.011	2786	2790	2793	rBV2	461	265	0.02%	0.002%
67	10.027	2793	2795	2800	rBV2	533	405	0.03%	0.004%
68	10.104	2816	2819	2821	rBV	435	286	0.02%	0.003%
69	10.149	2821	2833	2853	rBV	444164	709747	50.95%	6.602%
70	10.313	2880	2884	2885	rBV2	897	567	0.04%	0.005%
71	10.455	2925	2928	2933	rVB3	386	323	0.02%	0.003%
72	10.484	2934	2937	2940	rBV3	304	223	0.02%	0.002%
73	10.497	2940	2941	2949	rVB2	621	524	0.04%	0.005%
74	10.638	2984	2985	2989	rVB2	286	182	0.01%	0.002%
75	10.673	2994	2996	3000	rVB2	376	229	0.02%	0.002%
76	10.763	3021	3024	3031	rVB3	795	668	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035006.D
 Acq On : 05 Apr 2024 15:21
 Operator : SY/MD
 Sample : P1993-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.792	3031	3033	3036	rBV2	361	221	0.02%	0.002%
78	10.821	3040	3042	3044	rVV	348	166	0.01%	0.002%
79	10.841	3045	3048	3050	rVB2	447	288	0.02%	0.003%
80	10.857	3050	3053	3055	rBV	334	230	0.02%	0.002%
81	10.902	3065	3067	3073	rBV4	471	359	0.03%	0.003%
82	11.011	3099	3101	3104	rBV2	315	169	0.01%	0.002%
83	11.185	3144	3155	3175	rBV	590846	944994	67.83%	8.790%
84	11.461	3237	3241	3245	rVB3	775	683	0.05%	0.006%
85	11.487	3245	3249	3250	rBV	489	314	0.02%	0.003%
86	11.558	3261	3271	3298	rVB	592866	927261	66.56%	8.625%
87	11.931	3384	3387	3391	rBV4	476	406	0.03%	0.004%
88	11.960	3391	3396	3397	rBV2	472	408	0.03%	0.004%
89	12.159	3455	3458	3459	rBV2	491	342	0.02%	0.003%
90	12.307	3497	3504	3508	rBV6	1733	2162	0.16%	0.020%
91	12.471	3551	3555	3557	rBV3	540	493	0.04%	0.005%
92	12.525	3570	3572	3577	rBV2	325	273	0.02%	0.003%
93	12.638	3604	3607	3608	rBV	643	414	0.03%	0.004%
94	12.683	3618	3621	3624	rBV2	568	375	0.03%	0.003%
95	13.136	3758	3762	3764	rBV2	509	357	0.03%	0.003%
96	13.165	3768	3771	3775	rBV3	546	488	0.04%	0.005%
97	13.210	3780	3785	3786	rBV3	743	643	0.05%	0.006%
98	13.300	3811	3813	3817	rBV2	541	326	0.02%	0.003%
99	13.320	3817	3819	3821	rBV2	456	223	0.02%	0.002%
100	13.657	3921	3924	3928	rBV3	619	474	0.03%	0.004%




Sum of corrected areas: 10751251

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035006.D
Acq On : 05 Apr 2024 15:21
Operator : SY/MD
Sample : P1993-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

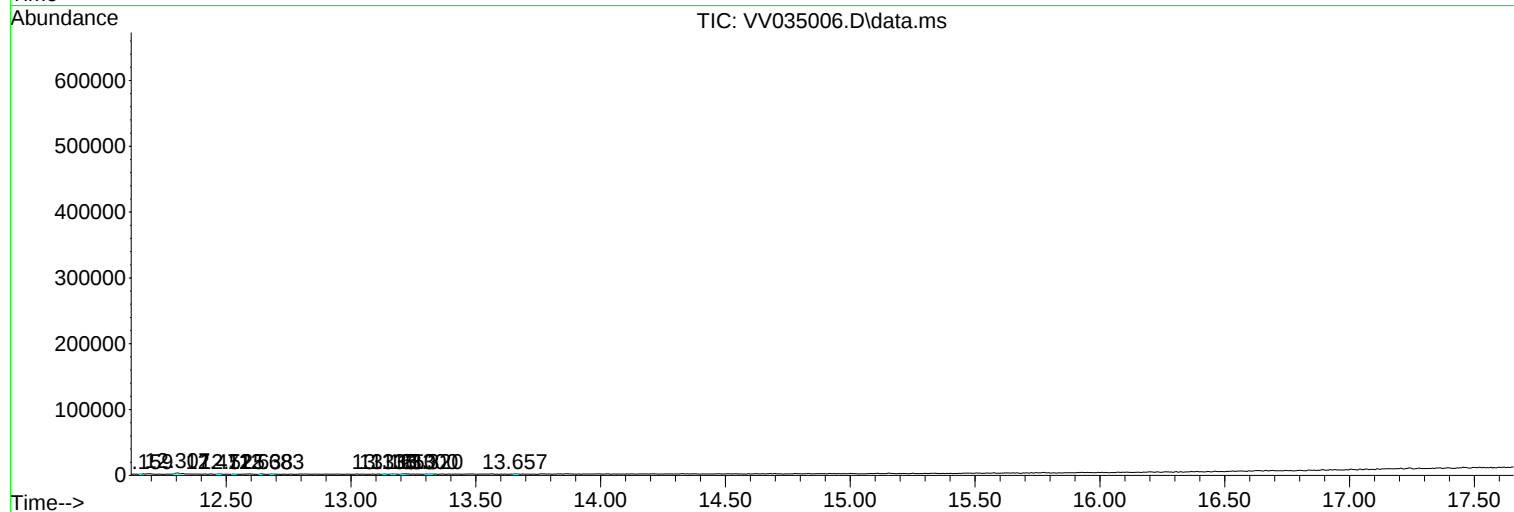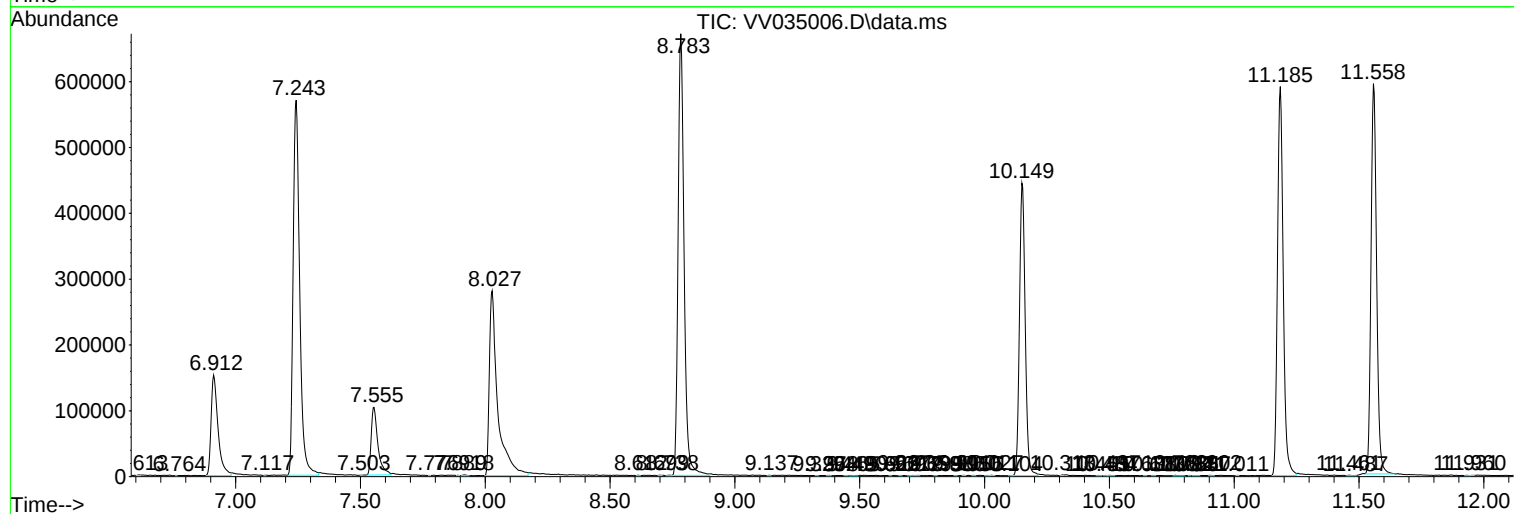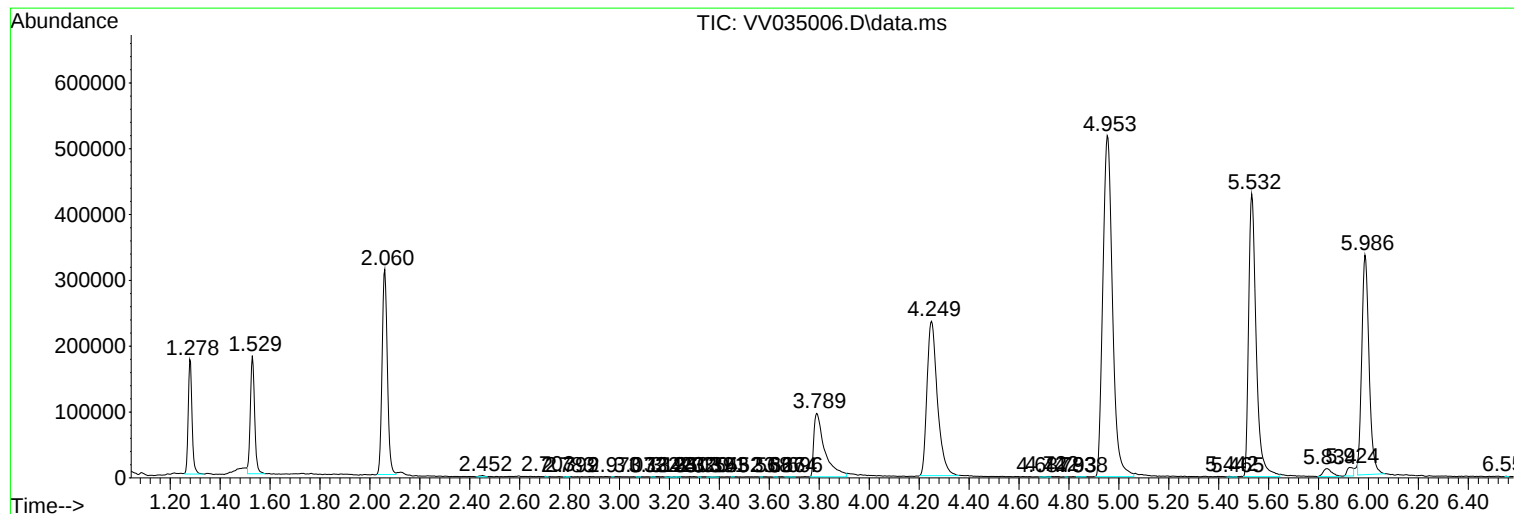

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035006.D
Acq On : 05 Apr 2024 15:21
Operator : SY/MD
Sample : P1993-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035006.D
Acq On : 05 Apr 2024 15:21
Operator : SY/MD
Sample : P1993-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
