

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035008.D
 Acq On : 05 Apr 2024 16:07
 Operator : SY/MD
 Sample : P2007-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	167138	179525	12.96%	1.668%
2	1.529	146	152	166	rVB	191822	221096	15.96%	2.055%
3	2.060	307	317	330	rBV	303134	440644	31.80%	4.095%
4	2.391	417	420	422	rBV3	538	385	0.03%	0.004%
5	2.703	513	517	519	rBV3	611	494	0.04%	0.005%
6	2.748	528	531	534	rBV2	545	438	0.03%	0.004%
7	2.863	564	567	571	rBV4	633	609	0.04%	0.006%
8	3.005	608	611	616	rBV2	397	297	0.02%	0.003%
9	3.063	627	629	632	rBV2	421	281	0.02%	0.003%
10	3.085	632	636	643	rVB2	747	827	0.06%	0.008%
11	3.121	643	647	650	rBV2	513	412	0.03%	0.004%
12	3.137	650	652	659	rVB3	581	455	0.03%	0.004%
13	3.169	659	662	664	rBV2	347	240	0.02%	0.002%
14	3.191	667	669	673	rVB3	514	330	0.02%	0.003%
15	3.220	673	678	679	rBV2	270	238	0.02%	0.002%
16	3.240	681	684	689	rBV	470	381	0.03%	0.004%
17	3.272	692	694	697	rVB	375	188	0.01%	0.002%
18	3.320	707	709	713	rVB	379	186	0.01%	0.002%
19	3.378	721	727	730	rBV2	674	550	0.04%	0.005%
20	3.458	749	752	757	rBV2	274	233	0.02%	0.002%
21	3.490	760	762	764	rVB	398	169	0.01%	0.002%
22	3.519	768	771	774	rBV2	507	305	0.02%	0.003%
23	3.597	789	795	802	rBV4	526	719	0.05%	0.007%
24	3.638	806	808	811	rVB2	521	287	0.02%	0.003%
25	3.661	811	815	819	rBV3	317	297	0.02%	0.003%
26	3.728	830	836	838	rBV2	345	354	0.03%	0.003%
27	3.789	847	855	898	rBV	102154	311753	22.50%	2.897%
28	4.249	983	998	1031	rBV	223989	579947	41.85%	5.390%
29	4.561	1092	1095	1097	rBV2	729	460	0.03%	0.004%
30	4.706	1135	1140	1144	rBV2	575	552	0.04%	0.005%
31	4.728	1144	1147	1150	rBV3	418	344	0.02%	0.003%
32	4.953	1201	1217	1249	rBV2	518962	1385715	100.00%	12.878%
33	5.400	1354	1356	1358	rBV3	451	307	0.02%	0.003%
34	5.432	1363	1366	1369	rBV3	409	325	0.02%	0.003%
35	5.532	1386	1397	1428	rBV	433993	910084	65.68%	8.458%
36	5.831	1482	1490	1513	rVB3	15893	36172	2.61%	0.336%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035008.D
 Acq On : 05 Apr 2024 16:07
 Operator : SY/MD
 Sample : P2007-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.989	1517	1539	1573	rBV	330089	715014	51.60%	6.645%
38	6.503	1697	1699	1702	rBV3	771	412	0.03%	0.004%
39	6.593	1726	1727	1731	rVB	524	200	0.01%	0.002%
40	6.690	1754	1757	1760	rBV3	633	388	0.03%	0.004%
41	6.703	1760	1761	1765	rVB3	376	211	0.02%	0.002%
42	6.748	1773	1775	1779	rVB3	833	479	0.03%	0.004%
43	6.780	1783	1785	1788	rVB3	620	371	0.03%	0.003%
44	6.799	1788	1791	1794	rBV2	457	291	0.02%	0.003%
45	6.818	1794	1797	1803	rBV3	648	573	0.04%	0.005%
46	6.847	1803	1806	1811	rBV3	789	594	0.04%	0.006%
47	6.912	1817	1826	1850	rBV2	149464	291038	21.00%	2.705%
48	7.243	1918	1929	1956	rBV	562235	1001505	72.27%	9.307%
49	7.555	2016	2026	2055	rBV	103845	197376	14.24%	1.834%
50	7.841	2111	2115	2116	rBV2	525	379	0.03%	0.004%
51	8.027	2164	2173	2220	rBV3	290715	689274	49.74%	6.406%
52	8.625	2357	2359	2363	rVB3	796	557	0.04%	0.005%
53	8.645	2363	2365	2366	rBV	694	247	0.02%	0.002%
54	8.728	2389	2391	2395	rVB3	685	355	0.03%	0.003%
55	8.783	2396	2408	2443	rBV	671378	1118214	80.70%	10.392%
56	9.095	2501	2505	2507	rBV2	545	510	0.04%	0.005%
57	9.181	2530	2532	2537	rVB2	668	385	0.03%	0.004%
58	9.223	2542	2545	2549	rBV2	623	537	0.04%	0.005%
59	9.262	2553	2557	2560	rBV3	672	424	0.03%	0.004%
60	9.407	2600	2602	2604	rBV2	327	211	0.02%	0.002%
61	9.503	2630	2632	2634	rVB	454	204	0.01%	0.002%
62	9.725	2697	2701	2703	rVB2	616	482	0.03%	0.004%
63	9.760	2707	2712	2713	rBV2	521	369	0.03%	0.003%
64	9.854	2739	2741	2744	rBV2	249	160	0.01%	0.001%
65	9.876	2744	2748	2752	rVB5	788	534	0.04%	0.005%
66	9.940	2763	2768	2774	rVB4	814	726	0.05%	0.007%
67	9.969	2774	2777	2781	rVB2	341	280	0.02%	0.003%
68	9.995	2781	2785	2788	rBV4	397	362	0.03%	0.003%
69	10.021	2791	2793	2799	rVB3	381	280	0.02%	0.003%
70	10.050	2799	2802	2803	rBV	383	185	0.01%	0.002%
71	10.149	2822	2833	2861	rVV	449975	721701	52.08%	6.707%
72	10.445	2922	2925	2928	rBV	314	218	0.02%	0.002%
73	10.464	2929	2931	2933	rVB	385	163	0.01%	0.002%
74	10.554	2956	2959	2963	rVB2	498	330	0.02%	0.003%
75	10.583	2963	2968	2971	rBV3	457	370	0.03%	0.003%
76	10.657	2988	2991	2996	rVV3	407	388	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035008.D
 Acq On : 05 Apr 2024 16:07
 Operator : SY/MD
 Sample : P2007-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.683	2996	2999	3003	rVB	685	527	0.04%	0.005%
78	10.706	3003	3006	3008	rBV	285	171	0.01%	0.002%
79	10.760	3019	3023	3028	rBV5	419	387	0.03%	0.004%
80	10.802	3032	3036	3037	rBV3	317	200	0.01%	0.002%
81	10.879	3057	3060	3062	rBV2	527	398	0.03%	0.004%
82	11.014	3099	3102	3104	rBV3	545	304	0.02%	0.003%
83	11.107	3127	3131	3133	rBV4	1211	964	0.07%	0.009%
84	11.185	3144	3155	3180	rBV	624054	966474	69.75%	8.982%
85	11.558	3250	3271	3295	rBV	593144	957673	69.11%	8.900%
86	11.915	3380	3382	3386	rBV2	683	543	0.04%	0.005%
87	11.982	3397	3403	3404	rBV	578	464	0.03%	0.004%
88	12.104	3438	3441	3445	rVB2	294	207	0.01%	0.002%
89	12.188	3464	3467	3468	rBV3	488	257	0.02%	0.002%
90	12.297	3494	3501	3508	rBV6	3803	6225	0.45%	0.058%
91	12.693	3621	3624	3625	rBV	358	233	0.02%	0.002%
92	12.789	3652	3654	3660	rVB2	423	311	0.02%	0.003%
93	12.869	3677	3679	3681	rBV	365	223	0.02%	0.002%
94	13.021	3723	3726	3729	rBV	495	349	0.03%	0.003%
95	13.140	3759	3763	3765	rBV	464	385	0.03%	0.004%
96	13.159	3766	3769	3770	rBV	414	229	0.02%	0.002%
97	13.377	3834	3837	3839	rBV2	430	332	0.02%	0.003%
98	13.535	3883	3886	3890	rBV2	797	653	0.05%	0.006%
99	13.779	3959	3962	3964	rBV2	594	229	0.02%	0.002%
100	14.207	4091	4095	4099	rBV3	574	569	0.04%	0.005%




Sum of corrected areas: 10760203

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035008.D
Acq On : 05 Apr 2024 16:07
Operator : SY/MD
Sample : P2007-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

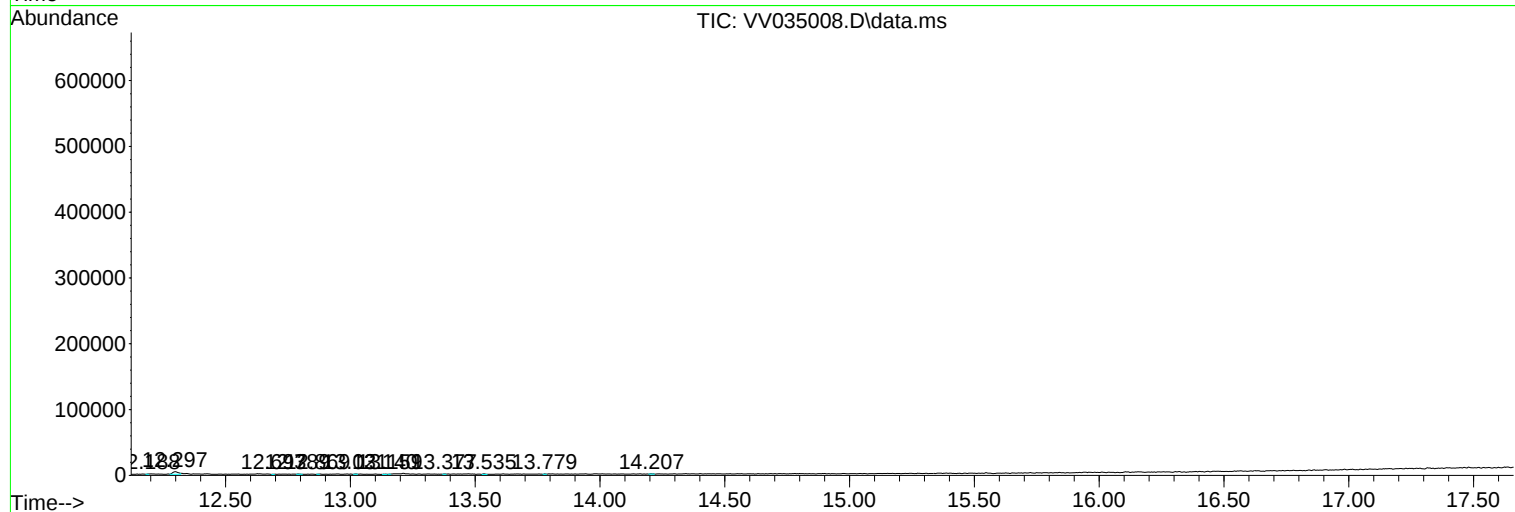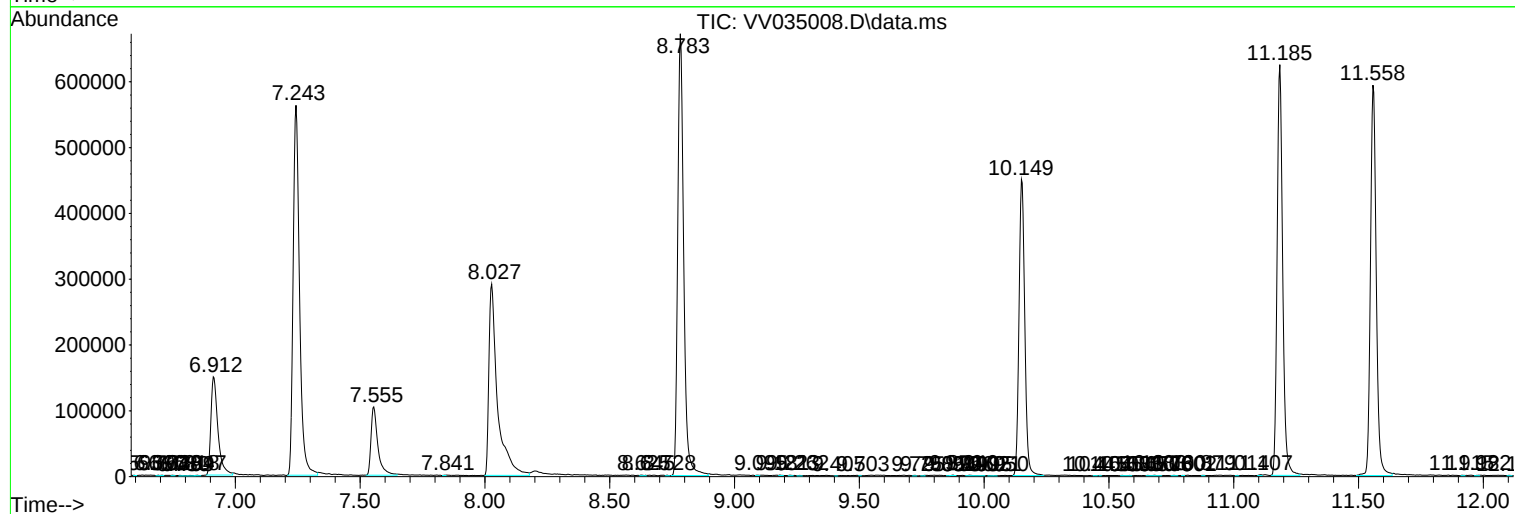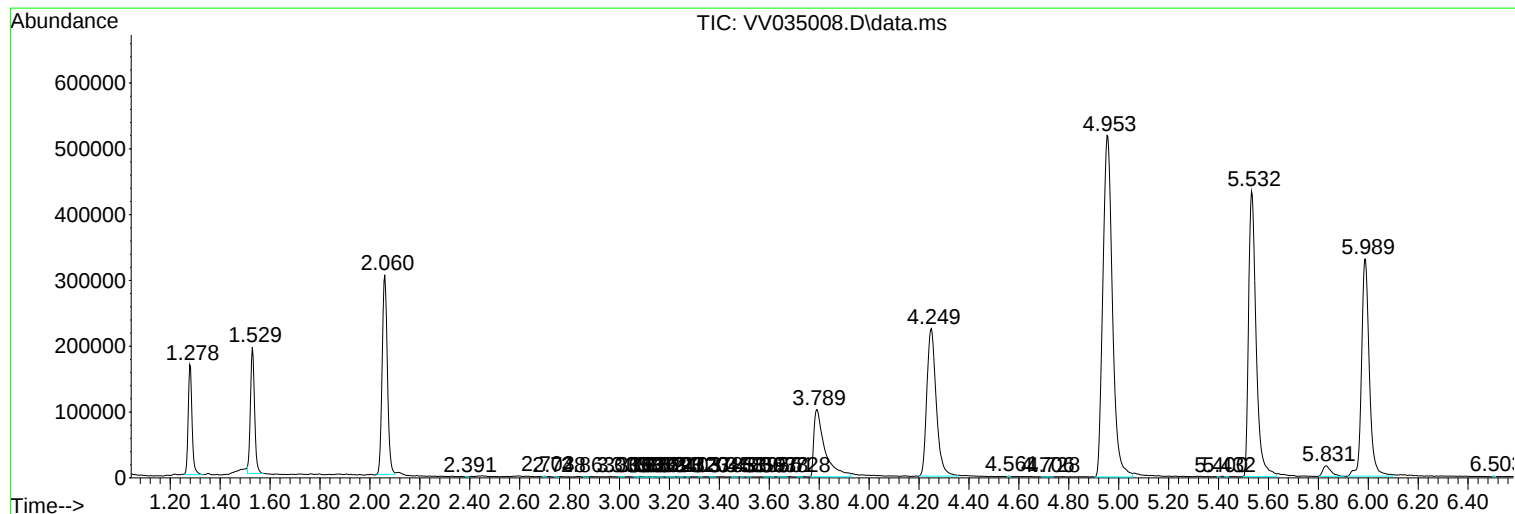

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035008.D
Acq On : 05 Apr 2024 16:07
Operator : SY/MD
Sample : P2007-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035008.D
Acq On : 05 Apr 2024 16:07
Operator : SY/MD
Sample : P2007-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------