

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035010.D
 Acq On : 05 Apr 2024 16:55
 Operator : SY/MD
 Sample : P2007-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	29	rVB2	25555	26800	1.98%	0.253%
2	1.278	68	74	88	rVB	179154	191422	14.14%	1.808%
3	1.529	146	152	166	rVB	183384	216616	16.00%	2.046%
4	2.060	308	317	331	rBV	297355	425328	31.41%	4.018%
5	2.590	475	482	485	rBV6	1173	1524	0.11%	0.014%
6	2.770	536	538	542	rBV3	610	373	0.03%	0.004%
7	2.835	553	558	561	rBV2	671	583	0.04%	0.006%
8	3.047	622	624	628	rVB2	365	229	0.02%	0.002%
9	3.079	631	634	637	rBV2	542	325	0.02%	0.003%
10	3.098	637	640	643	rVV2	556	472	0.03%	0.004%
11	3.134	647	651	655	rBV4	350	351	0.03%	0.003%
12	3.191	666	669	671	rBV	590	292	0.02%	0.003%
13	3.262	687	691	692	rBV	608	259	0.02%	0.002%
14	3.275	694	695	698	rVB	742	283	0.02%	0.003%
15	3.397	728	733	738	rVB2	393	317	0.02%	0.003%
16	3.439	744	746	748	rBV2	279	148	0.01%	0.001%
17	3.468	753	755	757	rBV	337	153	0.01%	0.001%
18	3.519	766	771	772	rBV3	415	298	0.02%	0.003%
19	3.677	817	820	824	rBV2	626	494	0.04%	0.005%
20	3.789	846	855	904	rBV	99924	310710	22.94%	2.935%
21	4.172	972	974	977	rBV3	695	427	0.03%	0.004%
22	4.249	984	998	1038	rVB	222184	605121	44.69%	5.717%
23	4.670	1127	1129	1132	rVB2	740	251	0.02%	0.002%
24	4.818	1171	1175	1178	rBV4	809	677	0.05%	0.006%
25	4.863	1185	1189	1190	rBV2	631	405	0.03%	0.004%
26	4.953	1202	1217	1257	rBV2	507205	1354170	100.00%	12.794%
27	5.352	1338	1341	1345	rVB4	829	622	0.05%	0.006%
28	5.532	1386	1397	1433	rBV	431939	903983	66.76%	8.540%
29	5.834	1481	1491	1510	rBV6	11591	25547	1.89%	0.241%
30	5.934	1514	1522	1525	rBV2	11959	17312	1.28%	0.164%
31	5.986	1528	1538	1562	rVB	320468	662451	48.92%	6.259%
32	6.584	1722	1724	1725	rBV	376	156	0.01%	0.001%
33	6.722	1765	1767	1770	rBV2	304	159	0.01%	0.002%
34	6.770	1780	1782	1784	rVB2	366	151	0.01%	0.001%
35	6.783	1784	1786	1789	rBV2	316	185	0.01%	0.002%
36	6.812	1793	1795	1798	rBV4	669	334	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035010.D
 Acq On : 05 Apr 2024 16:55
 Operator : SY/MD
 Sample : P2007-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.828	1798	1800	1806	rVB4	766	525	0.04%	0.005%
38	6.912	1815	1826	1858	rBV	147434	295055	21.79%	2.788%
39	7.243	1918	1929	1956	rBV	550470	978012	72.22%	9.240%
40	7.555	2017	2026	2054	rBV	100916	192758	14.23%	1.821%
41	7.789	2097	2099	2102	rBV2	451	254	0.02%	0.002%
42	7.841	2113	2115	2117	rBV	452	230	0.02%	0.002%
43	7.985	2157	2160	2161	rBV	508	297	0.02%	0.003%
44	8.027	2164	2173	2207	rBV3	286930	659847	48.73%	6.234%
45	8.452	2303	2305	2310	rBV3	469	330	0.02%	0.003%
46	8.474	2310	2312	2315	rBV3	612	271	0.02%	0.003%
47	8.532	2327	2330	2331	rBV2	463	241	0.02%	0.002%
48	8.596	2348	2350	2352	rBV2	406	205	0.02%	0.002%
49	8.632	2358	2361	2365	rBV3	757	692	0.05%	0.007%
50	8.690	2377	2379	2380	rBV3	382	182	0.01%	0.002%
51	8.783	2397	2408	2430	rBV	675917	1105927	81.67%	10.448%
52	9.079	2496	2500	2502	rBV4	1075	642	0.05%	0.006%
53	9.133	2515	2517	2520	rBV	568	297	0.02%	0.003%
54	9.153	2520	2523	2526	rVB4	634	392	0.03%	0.004%
55	9.329	2575	2578	2579	rBV2	510	274	0.02%	0.003%
56	9.365	2586	2589	2593	rBV5	769	518	0.04%	0.005%
57	9.400	2598	2600	2602	rBV2	306	144	0.01%	0.001%
58	9.574	2651	2654	2655	rBV2	315	143	0.01%	0.001%
59	9.606	2660	2664	2665	rBV2	283	185	0.01%	0.002%
60	9.622	2667	2669	2672	rVV4	337	184	0.01%	0.002%
61	9.677	2684	2686	2691	rVB	344	241	0.02%	0.002%
62	9.696	2691	2692	2696	rBV2	352	235	0.02%	0.002%
63	9.747	2705	2708	2714	rVB3	427	357	0.03%	0.003%
64	9.776	2714	2717	2721	rBV3	391	327	0.02%	0.003%
65	9.821	2728	2731	2733	rBV2	418	232	0.02%	0.002%
66	9.876	2746	2748	2752	rVB3	625	303	0.02%	0.003%
67	9.911	2758	2759	2762	rVB3	476	211	0.02%	0.002%
68	9.931	2762	2765	2769	rBV2	401	352	0.03%	0.003%
69	9.956	2769	2773	2777	rVB4	641	434	0.03%	0.004%
70	10.066	2804	2807	2810	rBV	350	243	0.02%	0.002%
71	10.082	2810	2812	2816	rVB	391	218	0.02%	0.002%
72	10.104	2816	2819	2821	rBV	284	229	0.02%	0.002%
73	10.149	2821	2833	2856	rBV	459422	728723	53.81%	6.885%
74	10.294	2876	2878	2882	rBV2	704	593	0.04%	0.006%
75	10.368	2898	2901	2904	rVV2	591	365	0.03%	0.003%
76	10.387	2904	2907	2910	rVB2	653	455	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035010.D
 Acq On : 05 Apr 2024 16:55
 Operator : SY/MD
 Sample : P2007-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.439	2920	2923	2926	rBV2	465	306	0.02%	0.003%
78	10.458	2926	2929	2932	rVB2	446	291	0.02%	0.003%
79	10.474	2932	2934	2936	rBV2	509	282	0.02%	0.003%
80	10.574	2962	2965	2966	rBV2	424	235	0.02%	0.002%
81	10.583	2966	2968	2970	rVV2	626	284	0.02%	0.003%
82	10.596	2970	2972	2976	rVB2	495	317	0.02%	0.003%
83	10.632	2981	2983	2985	rVB	369	162	0.01%	0.002%
84	10.654	2985	2990	2993	rBV3	493	471	0.03%	0.004%
85	10.757	3019	3022	3024	rBV2	571	341	0.03%	0.003%
86	10.892	3061	3064	3067	rBV3	305	215	0.02%	0.002%
87	10.911	3067	3070	3075	rBV3	655	480	0.04%	0.005%
88	10.940	3075	3079	3082	rBV2	414	286	0.02%	0.003%
89	10.992	3092	3095	3098	rVB2	585	334	0.02%	0.003%
90	11.108	3128	3131	3133	rBV3	325	205	0.02%	0.002%
91	11.185	3144	3155	3181	rBV	602707	947723	69.99%	8.954%
92	11.558	3261	3271	3295	rVB	577205	906303	66.93%	8.562%
93	11.927	3381	3386	3389	rBV4	709	628	0.05%	0.006%
94	12.011	3410	3412	3414	rBV	389	176	0.01%	0.002%
95	12.307	3496	3504	3513	rBV8	2539	4554	0.34%	0.043%
96	12.432	3541	3543	3546	rBV	243	143	0.01%	0.001%
97	12.500	3560	3564	3567	rBV3	414	313	0.02%	0.003%
98	13.050	3733	3735	3738	rBV2	488	259	0.02%	0.002%
99	13.545	3886	3889	3891	rBV	365	287	0.02%	0.003%
100	13.757	3953	3955	3956	rBV	406	156	0.01%	0.001%




Sum of corrected areas: 10584802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035010.D
Acq On : 05 Apr 2024 16:55
Operator : SY/MD
Sample : P2007-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

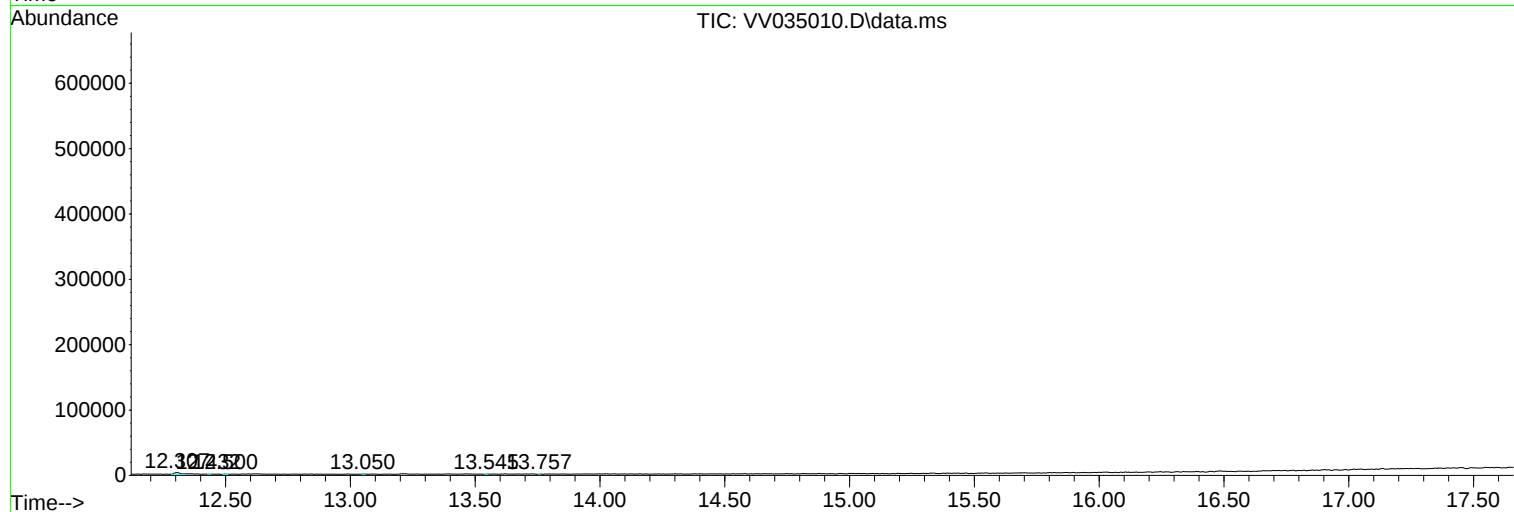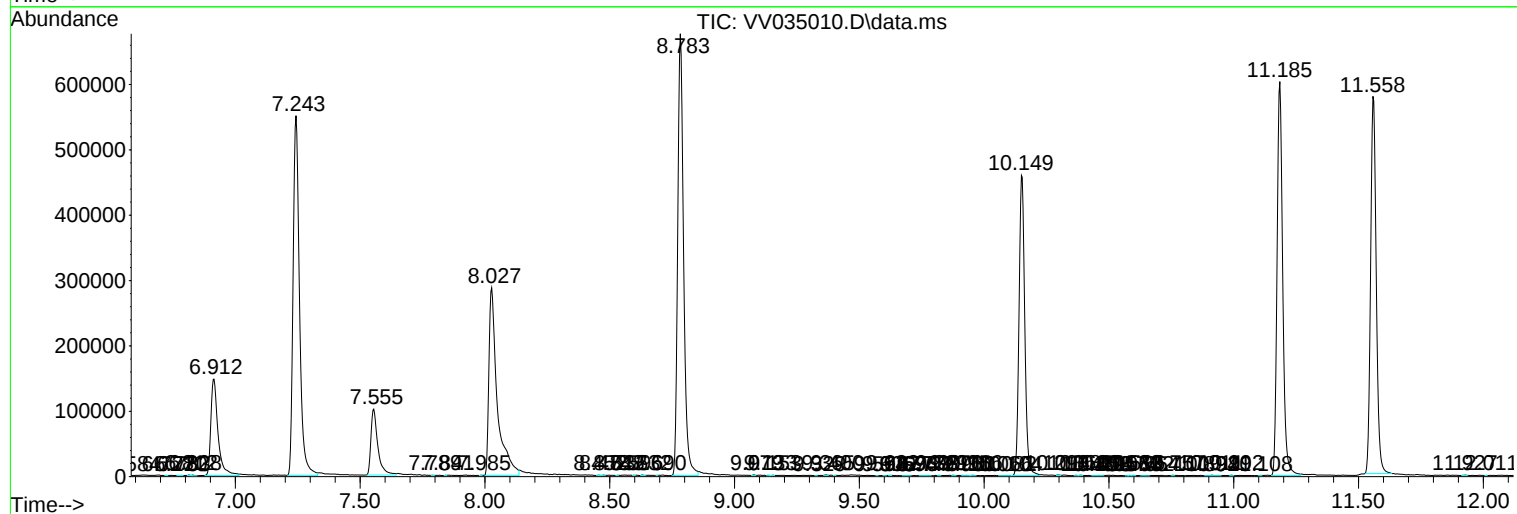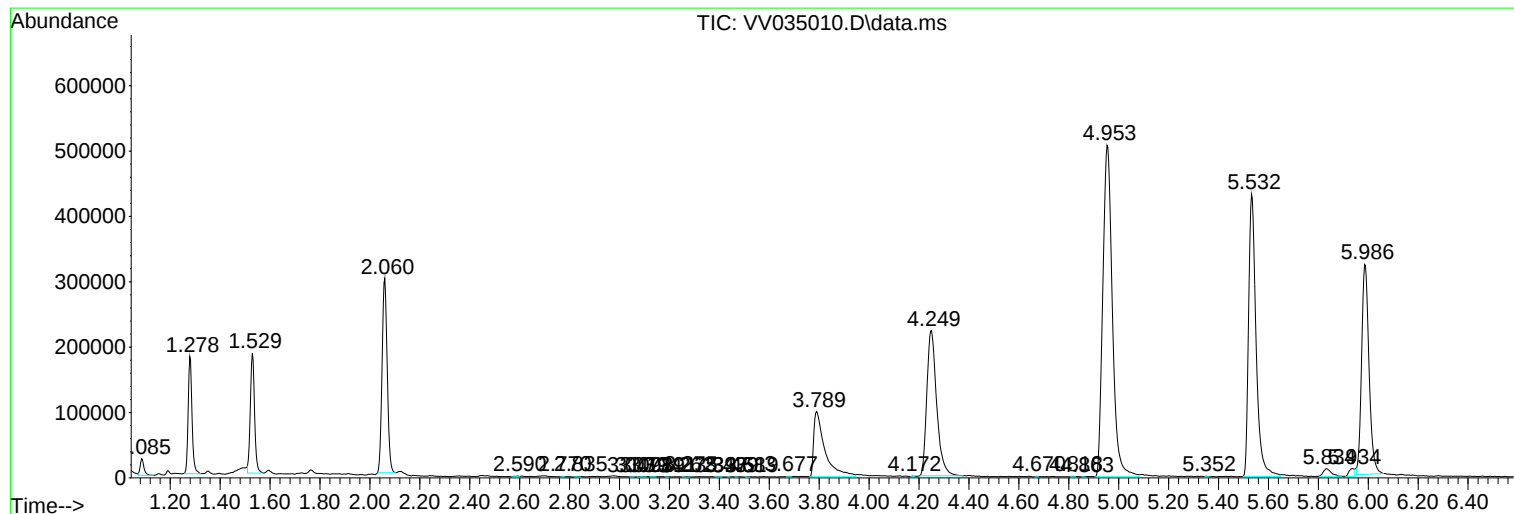

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035010.D
Acq On : 05 Apr 2024 16:55
Operator : SY/MD
Sample : P2007-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035010.D
Acq On : 05 Apr 2024 16:55
Operator : SY/MD
Sample : P2007-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc