

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035012.D
 Acq On : 05 Apr 2024 17:43
 Operator : SY/MD
 Sample : P2006-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rBV	214481	227779	0.21%	0.094%
2	1.529	145	152	170	rVB	220394	264972	0.25%	0.109%
3	2.059	307	317	331	rBV	353214	512378	0.48%	0.211%
4	2.240	366	373	374	rBV3	1817	1620	0.00%	0.001%
5	2.378	414	416	422	rVB3	617	485	0.00%	0.000%
6	2.413	425	427	429	rBV	571	314	0.00%	0.000%
7	2.449	429	438	451	rBV	9292	15525	0.01%	0.006%
8	2.516	454	459	465	rVB5	2019	2357	0.00%	0.001%
9	2.632	493	495	501	rVB2	474	413	0.00%	0.000%
10	2.703	510	517	519	rBV3	516	495	0.00%	0.000%
11	2.760	533	535	539	rVV	495	356	0.00%	0.000%
12	2.850	559	563	571	rVB3	744	770	0.00%	0.000%
13	2.889	571	575	576	rBV3	556	402	0.00%	0.000%
14	2.960	591	597	600	rBV4	628	721	0.00%	0.000%
15	2.985	601	605	608	rVB4	449	345	0.00%	0.000%
16	3.076	628	633	636	rBV3	453	371	0.00%	0.000%
17	3.111	640	644	648	rVB2	664	560	0.00%	0.000%
18	3.342	710	716	717	rBV	358	327	0.00%	0.000%
19	3.510	765	768	772	rVB2	355	307	0.00%	0.000%
20	3.622	798	803	805	rBV2	463	405	0.00%	0.000%
21	3.670	806	818	836	rVB6	5723	14939	0.01%	0.006%
22	3.789	846	855	897	rBV	112784	348111	0.33%	0.143%
23	4.149	963	967	971	rBV2	509	539	0.00%	0.000%
24	4.246	981	997	1028	rBV	248859	643619	0.60%	0.265%
25	4.510	1076	1079	1084	rVB4	618	502	0.00%	0.000%
26	4.590	1092	1104	1119	rVB9	4394	11511	0.01%	0.005%
27	4.657	1123	1125	1129	rVV3	548	415	0.00%	0.000%
28	4.715	1140	1143	1146	rBV4	472	373	0.00%	0.000%
29	5.018	1202	1237	1301	rBV2	43920319	107098018	100.00%	44.089%
30	5.532	1387	1397	1430	rVB	407804	842930	0.79%	0.347%
31	5.834	1483	1491	1511	rVB	7990	20553	0.02%	0.008%
32	5.985	1526	1538	1571	rBV	361024	745998	0.70%	0.307%
33	6.320	1636	1642	1645	rVV5	1138	998	0.00%	0.000%
34	6.339	1645	1648	1650	rVB3	636	317	0.00%	0.000%
35	6.394	1663	1665	1669	rVB3	798	502	0.00%	0.000%
36	6.445	1677	1681	1684	rBV4	447	409	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035012.D
 Acq On : 05 Apr 2024 17:43
 Operator : SY/MD
 Sample : P2006-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.526	1702	1706	1710	rVB	789	625	0.00%	0.000%
38	6.561	1714	1717	1721	rBV3	824	521	0.00%	0.000%
39	6.590	1721	1726	1729	rVB4	574	540	0.00%	0.000%
40	6.612	1729	1733	1735	rBV4	1168	852	0.00%	0.000%
41	6.664	1747	1749	1751	rBV2	605	349	0.00%	0.000%
42	6.715	1760	1765	1769	rBV5	840	827	0.00%	0.000%
43	6.738	1769	1772	1774	rVB4	762	444	0.00%	0.000%
44	6.866	1810	1812	1816	rVB3	690	377	0.00%	0.000%
45	6.911	1816	1826	1855	rBV	181747	346615	0.32%	0.143%
46	7.140	1895	1897	1902	rBV4	424	305	0.00%	0.000%
47	7.243	1918	1929	1952	rBV	693296	1223286	1.14%	0.504%
48	7.551	2016	2025	2053	rBV	125615	234105	0.22%	0.096%
49	7.911	2131	2137	2143	rBV7	2279	3149	0.00%	0.001%
50	7.963	2150	2153	2155	rBV3	454	300	0.00%	0.000%
51	8.027	2162	2173	2224	rBV2	336479	744764	0.70%	0.307%
52	8.419	2293	2295	2297	rVB2	667	321	0.00%	0.000%
53	8.509	2319	2323	2325	rBV2	500	438	0.00%	0.000%
54	8.574	2341	2343	2345	rVB3	832	367	0.00%	0.000%
55	8.603	2345	2352	2353	rBV3	505	463	0.00%	0.000%
56	8.654	2364	2368	2371	rBV3	417	387	0.00%	0.000%
57	8.821	2398	2420	2472	rBV3	52440817	93092137	86.92%	38.323%
58	9.705	2692	2695	2700	rBV6	764	621	0.00%	0.000%
59	9.760	2710	2712	2715	rVB4	652	340	0.00%	0.000%
60	9.879	2745	2749	2751	rBV4	843	670	0.00%	0.000%
61	10.072	2807	2809	2813	rBV3	702	533	0.00%	0.000%
62	10.152	2822	2834	2854	rBV	503502	800521	0.75%	0.330%
63	10.329	2885	2889	2893	rVB3	603	523	0.00%	0.000%
64	10.368	2895	2901	2911	rVB6	3511	5647	0.01%	0.002%
65	10.487	2932	2938	2940	rBV5	1192	1119	0.00%	0.000%
66	10.606	2972	2975	2977	rBV	766	332	0.00%	0.000%
67	10.686	2995	3000	3006	rBV3	455	569	0.00%	0.000%
68	10.757	3017	3022	3023	rVV	548	330	0.00%	0.000%
69	10.767	3023	3025	3029	rVV3	442	382	0.00%	0.000%
70	11.040	3107	3110	3113	rVB3	568	381	0.00%	0.000%
71	11.117	3121	3134	3145	rBV	322493	513982	0.48%	0.212%
72	11.207	3145	3162	3193	rVB	12270932	19505645	18.21%	8.030%
73	11.577	3259	3277	3303	rBV2	9633648	15482721	14.46%	6.374%
74	12.101	3438	3440	3446	rVB3	731	593	0.00%	0.000%
75	12.133	3446	3450	3455	rBV6	693	735	0.00%	0.000%
76	12.188	3465	3467	3469	rBV3	876	443	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035012.D
 Acq On : 05 Apr 2024 17:43
 Operator : SY/MD
 Sample : P2006-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.284	3493	3497	3502	rVB2	605	388	0.00%	0.000%
78	12.348	3514	3517	3523	rVV6	1050	1201	0.00%	0.000%
79	12.554	3577	3581	3586	rVB5	827	763	0.00%	0.000%
80	12.583	3586	3590	3593	rBV3	761	624	0.00%	0.000%
81	12.863	3674	3677	3684	rVB2	599	702	0.00%	0.000%
82	13.030	3724	3729	3730	rBV2	527	339	0.00%	0.000%
83	13.072	3739	3742	3745	rVB3	619	414	0.00%	0.000%
84	13.101	3745	3751	3755	rBV4	748	815	0.00%	0.000%
85	13.201	3770	3782	3800	rBV	102682	169014	0.16%	0.070%
86	13.268	3800	3803	3805	rVB4	638	365	0.00%	0.000%
87	13.319	3814	3819	3823	rBV4	592	571	0.00%	0.000%
88	13.416	3846	3849	3851	rBV2	516	396	0.00%	0.000%
89	13.455	3855	3861	3862	rVV3	690	614	0.00%	0.000%
90	13.471	3863	3866	3872	rVV6	1121	1320	0.00%	0.001%
91	13.683	3926	3932	3934	rBV4	2820	2553	0.00%	0.001%
92	13.789	3961	3965	3969	rBV3	501	528	0.00%	0.000%
93	13.811	3969	3972	3974	rVB3	651	405	0.00%	0.000%
94	13.866	3983	3989	3992	rBV3	958	812	0.00%	0.000%
95	14.226	4096	4101	4102	rBV3	572	483	0.00%	0.000%
96	14.509	4186	4189	4190	rBV2	680	356	0.00%	0.000%
97	14.564	4203	4206	4209	rVB4	574	320	0.00%	0.000%
98	15.056	4357	4359	4361	rBV2	559	318	0.00%	0.000%
99	15.184	4397	4399	4404	rBV5	584	443	0.00%	0.000%
100	15.345	4447	4449	4453	rBV3	666	498	0.00%	0.000%




Sum of corrected areas: 242912137

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035012.D
Acq On : 05 Apr 2024 17:43
Operator : SY/MD
Sample : P2006-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

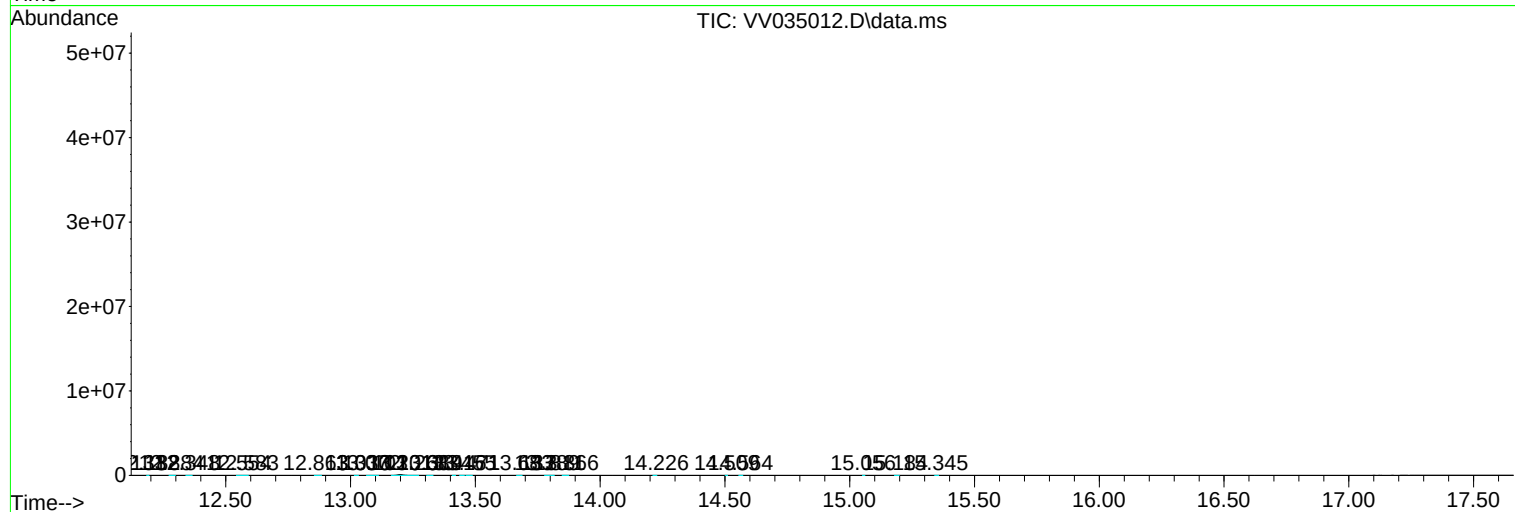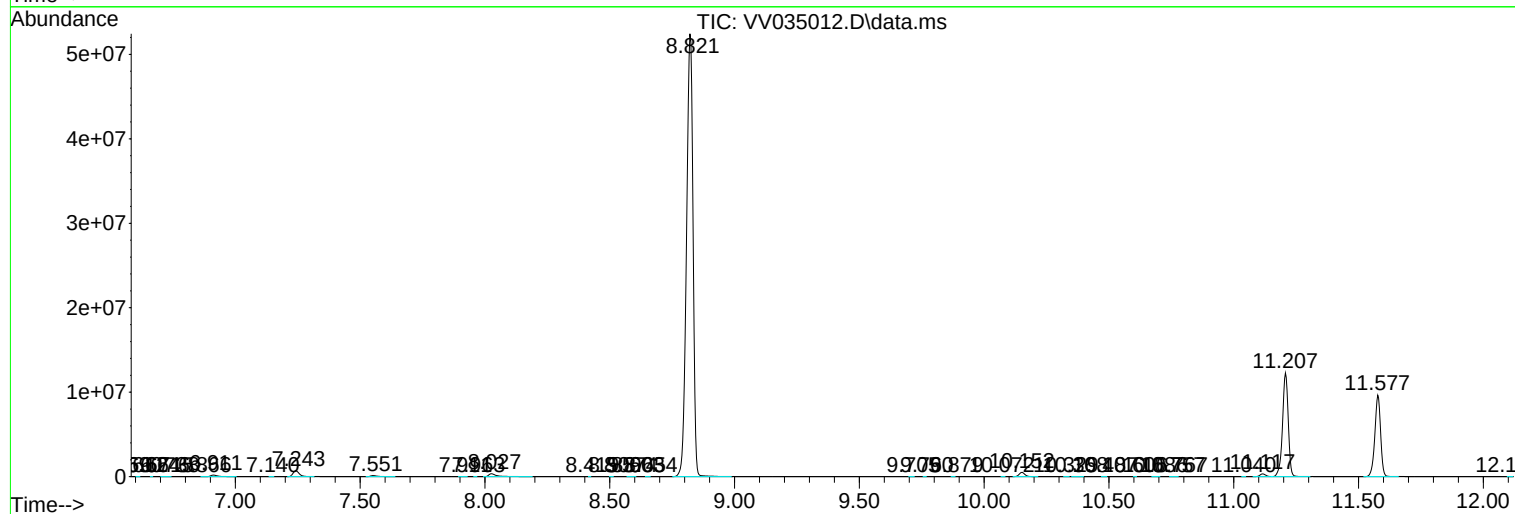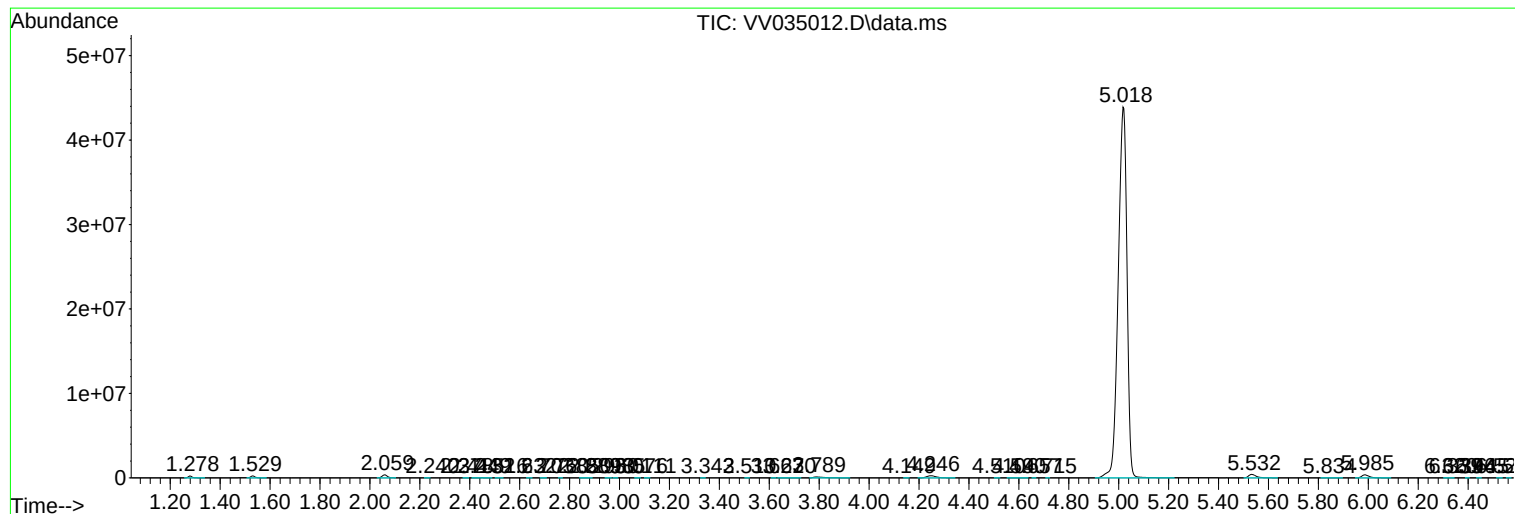

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035012.D
Acq On : 05 Apr 2024 17:43
Operator : SY/MD
Sample : P2006-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035012.D
Acq On : 05 Apr 2024 17:43
Operator : SY/MD
Sample : P2006-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------