

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040524\
 Data File : V035013.D
 Acq On : 05 Apr 2024 18:07
 Operator : SY/MD
 Sample : P2006-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: V035013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	96	rVB	270042	286023	15.83%	2.234%
2	1.529	146	152	169	rVB	275741	317734	17.58%	2.482%
3	2.060	307	317	332	rBV	430374	622944	34.47%	4.865%
4	2.552	466	470	473	rBV3	769	603	0.03%	0.005%
5	2.815	549	552	555	rVB2	461	262	0.01%	0.002%
6	2.957	594	596	599	rBV4	460	255	0.01%	0.002%
7	2.982	602	604	607	rBV2	402	262	0.01%	0.002%
8	3.043	621	623	624	rBV2	388	176	0.01%	0.001%
9	3.108	641	643	645	rBV	308	185	0.01%	0.001%
10	3.150	652	656	660	rBV2	464	504	0.03%	0.004%
11	3.220	675	678	679	rBV2	300	175	0.01%	0.001%
12	3.304	698	704	710	rBV3	609	888	0.05%	0.007%
13	3.394	729	732	734	rBV2	274	193	0.01%	0.002%
14	3.413	735	738	741	rVV	393	303	0.02%	0.002%
15	3.442	744	747	750	rBV2	386	262	0.01%	0.002%
16	3.461	750	753	755	rBV2	391	236	0.01%	0.002%
17	3.500	760	765	769	rBV3	379	437	0.02%	0.003%
18	3.535	773	776	780	rBV3	356	327	0.02%	0.003%
19	3.574	784	788	789	rBV2	599	404	0.02%	0.003%
20	3.677	816	820	822	rVB2	360	214	0.01%	0.002%
21	3.699	824	827	831	rVB2	348	281	0.02%	0.002%
22	3.725	831	835	837	rBV2	414	316	0.02%	0.002%
23	3.789	847	855	885	rBV	113309	323302	17.89%	2.525%
24	4.246	983	997	1030	rBV	257857	664340	36.76%	5.189%
25	4.622	1112	1114	1117	rBV2	426	227	0.01%	0.002%
26	4.641	1118	1120	1122	rBV3	423	255	0.01%	0.002%
27	4.715	1141	1143	1146	rBV2	482	269	0.01%	0.002%
28	4.828	1174	1178	1180	rBV2	510	432	0.02%	0.003%
29	4.953	1201	1217	1261	rBV2	646981	1807032	100.00%	14.113%
30	5.532	1386	1397	1435	rBV	430428	901555	49.89%	7.041%
31	5.838	1481	1492	1516	rVB3	9207	24976	1.38%	0.195%
32	5.985	1526	1538	1568	rBV	371457	774722	42.87%	6.051%
33	6.288	1629	1632	1634	rBV3	738	412	0.02%	0.003%
34	6.387	1661	1663	1667	rVB2	589	356	0.02%	0.003%
35	6.413	1667	1671	1673	rBV4	440	309	0.02%	0.002%
36	6.432	1674	1677	1679	rVB2	549	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035013.D
 Acq On : 05 Apr 2024 18:07
 Operator : SY/MD
 Sample : P2006-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.458	1679	1685	1691	rVB5	764	973	0.05%	0.008%
38	6.487	1691	1694	1696	rBV2	591	335	0.02%	0.003%
39	6.513	1700	1702	1707	rVB6	493	377	0.02%	0.003%
40	6.535	1707	1709	1712	rBV3	442	288	0.02%	0.002%
41	6.580	1720	1723	1726	rBV2	486	313	0.02%	0.002%
42	6.606	1728	1731	1732	rBV	473	221	0.01%	0.002%
43	6.677	1751	1753	1755	rBV3	600	254	0.01%	0.002%
44	6.757	1776	1778	1781	rBV4	402	213	0.01%	0.002%
45	6.834	1799	1802	1805	rVV2	359	257	0.01%	0.002%
46	6.911	1816	1826	1854	rBV	181237	347010	19.20%	2.710%
47	7.243	1917	1929	1953	rBV	727681	1295929	71.72%	10.122%
48	7.551	2017	2025	2058	rBV	119264	226243	12.52%	1.767%
49	7.873	2123	2125	2127	rBV2	702	399	0.02%	0.003%
50	8.027	2163	2173	2214	rBV2	323713	744095	41.18%	5.812%
51	8.600	2350	2351	2354	rBV2	566	267	0.01%	0.002%
52	8.783	2397	2408	2442	rVV2	674005	1372265	75.94%	10.718%
53	9.149	2518	2522	2526	rVB3	628	424	0.02%	0.003%
54	9.169	2526	2528	2531	rBV2	526	364	0.02%	0.003%
55	9.185	2531	2533	2537	rVB3	560	336	0.02%	0.003%
56	9.320	2570	2575	2578	rBV2	532	463	0.03%	0.004%
57	9.378	2590	2593	2597	rBV3	331	295	0.02%	0.002%
58	9.397	2597	2599	2602	rBV2	386	266	0.01%	0.002%
59	9.474	2622	2623	2626	rVB	423	171	0.01%	0.001%
60	9.500	2626	2631	2633	rBV3	504	459	0.03%	0.004%
61	9.526	2636	2639	2641	rVV3	598	333	0.02%	0.003%
62	9.542	2641	2644	2647	rVV3	543	297	0.02%	0.002%
63	9.583	2651	2657	2661	rBV4	470	489	0.03%	0.004%
64	9.648	2675	2677	2680	rBV	294	167	0.01%	0.001%
65	9.664	2680	2682	2686	rVB2	546	305	0.02%	0.002%
66	9.789	2719	2721	2723	rBV2	481	220	0.01%	0.002%
67	10.043	2796	2800	2803	rBV3	401	334	0.02%	0.003%
68	10.152	2822	2834	2863	rBV	487457	789414	43.69%	6.166%
69	10.461	2928	2930	2931	rBV	335	155	0.01%	0.001%
70	10.522	2946	2949	2953	rBV3	531	414	0.02%	0.003%
71	10.542	2953	2955	2957	rBV2	665	320	0.02%	0.002%
72	10.593	2969	2971	2974	rBV4	285	164	0.01%	0.001%
73	10.680	2993	2998	3001	rBV2	441	392	0.02%	0.003%
74	10.715	3004	3009	3011	rVB2	381	323	0.02%	0.003%
75	10.731	3011	3014	3016	rBV	375	231	0.01%	0.002%
76	10.805	3033	3037	3038	rBV	337	269	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035013.D
 Acq On : 05 Apr 2024 18:07
 Operator : SY/MD
 Sample : P2006-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.898	3064	3066	3069	rBV	487	281	0.02%	0.002%
78	10.979	3088	3091	3096	rBV3	452	364	0.02%	0.003%
79	11.011	3098	3101	3104	rBV3	465	412	0.02%	0.003%
80	11.059	3113	3116	3117	rBV2	451	249	0.01%	0.002%
81	11.124	3131	3136	3139	rBV5	2702	2706	0.15%	0.021%
82	11.185	3145	3155	3187	rVB2	609454	1079749	59.75%	8.433%
83	11.506	3249	3255	3256	rBV3	692	510	0.03%	0.004%
84	11.558	3259	3271	3301	rVV	689987	1191341	65.93%	9.305%
85	11.924	3382	3385	3388	rBV2	482	258	0.01%	0.002%
86	12.242	3482	3484	3487	rBV2	509	281	0.02%	0.002%
87	12.429	3539	3542	3543	rBV2	511	288	0.02%	0.002%
88	12.490	3559	3561	3566	rBV3	329	333	0.02%	0.003%
89	12.516	3566	3569	3570	rBV3	554	338	0.02%	0.003%
90	12.599	3592	3595	3596	rBV2	384	214	0.01%	0.002%
91	12.648	3608	3610	3613	rVB2	575	239	0.01%	0.002%
92	12.741	3636	3639	3642	rBV2	490	375	0.02%	0.003%
93	12.886	3681	3684	3685	rBV2	340	186	0.01%	0.001%
94	12.966	3706	3709	3713	rBV4	530	485	0.03%	0.004%
95	13.207	3778	3784	3793	rBV7	4291	5948	0.33%	0.046%
96	13.596	3902	3905	3906	rBV2	587	303	0.02%	0.002%
97	13.744	3949	3951	3954	rBV3	426	234	0.01%	0.002%
98	14.069	4049	4052	4054	rBV2	487	353	0.02%	0.003%
99	14.201	4091	4093	4098	rBV3	845	418	0.02%	0.003%
100	14.255	4108	4110	4114	rBV2	544	331	0.02%	0.003%




Sum of corrected areas: 12803638

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035013.D
Acq On : 05 Apr 2024 18:07
Operator : SY/MD
Sample : P2006-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

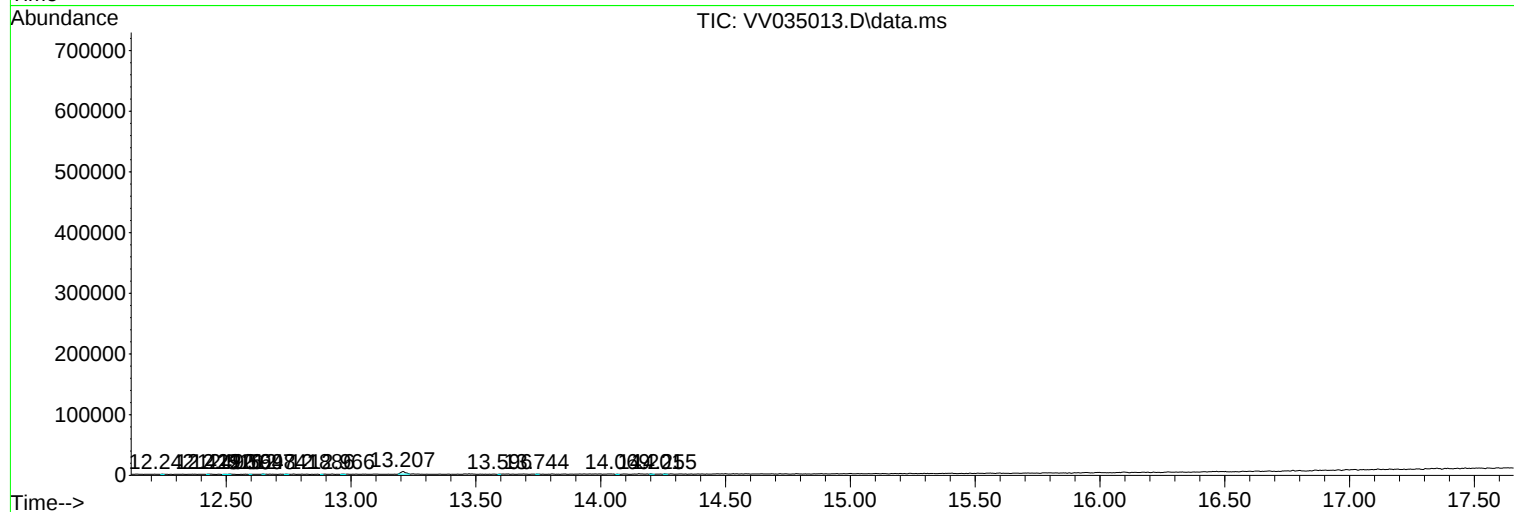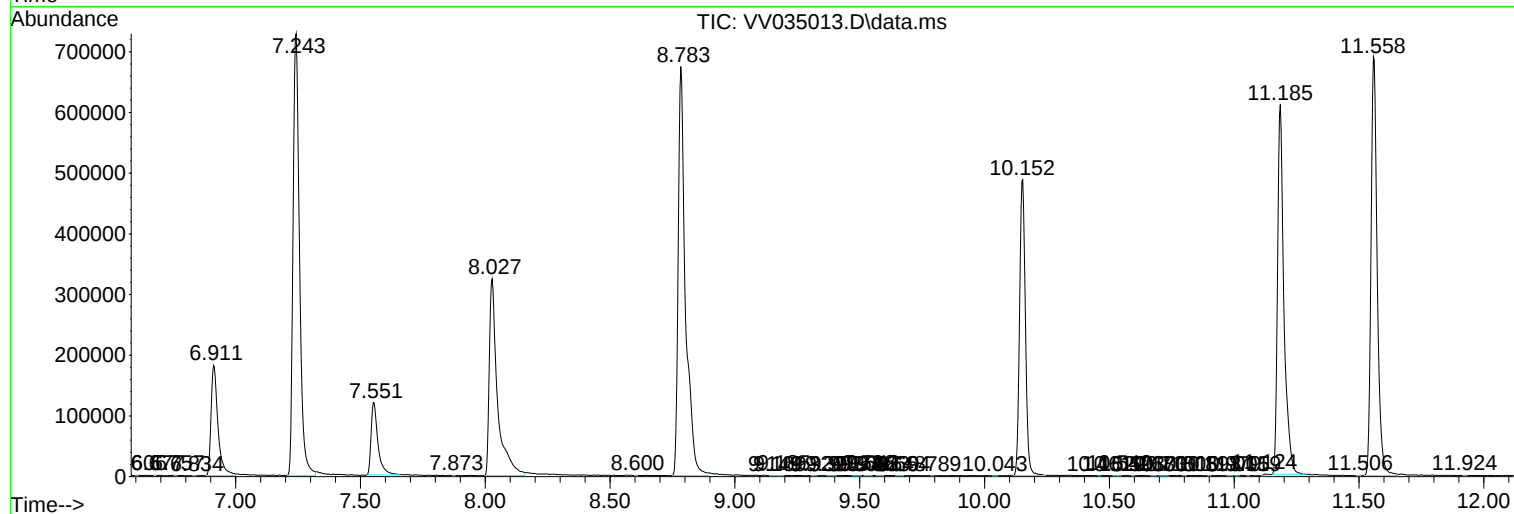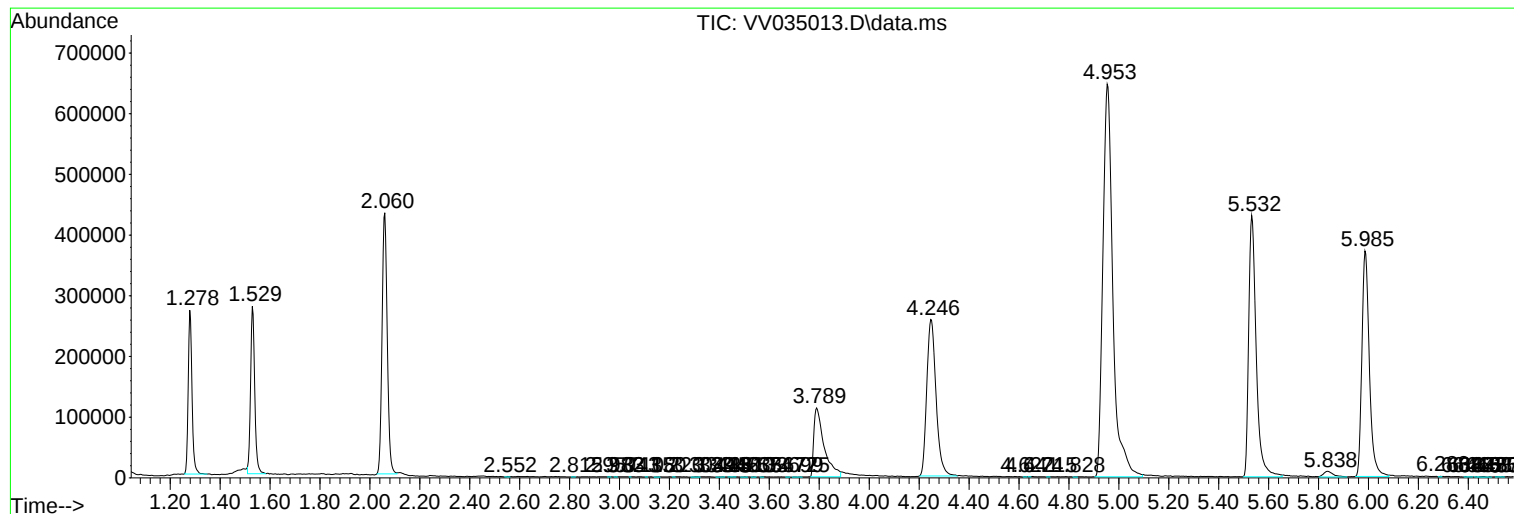

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035013.D
Acq On : 05 Apr 2024 18:07
Operator : SY/MD
Sample : P2006-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035013.D
Acq On : 05 Apr 2024 18:07
Operator : SY/MD
Sample : P2006-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
