

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035016.D
 Acq On : 05 Apr 2024 19:19
 Operator : SY/MD
 Sample : P2006-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	260391	275084	16.33%	2.290%
2	1.532	146	153	176	rVB	263140	314935	18.70%	2.621%
3	2.060	308	317	334	rVB	424038	618688	36.73%	5.150%
4	2.844	556	561	564	rBV4	554	592	0.04%	0.005%
5	2.896	575	577	579	rBV2	379	228	0.01%	0.002%
6	3.092	633	638	641	rBV3	417	456	0.03%	0.004%
7	3.117	644	646	649	rBV2	299	187	0.01%	0.002%
8	3.159	656	659	660	rBV	283	175	0.01%	0.001%
9	3.224	675	679	681	rBV2	390	252	0.01%	0.002%
10	3.269	689	693	696	rBV	325	321	0.02%	0.003%
11	3.343	714	716	718	rBV	298	149	0.01%	0.001%
12	3.391	727	731	732	rBV2	297	186	0.01%	0.002%
13	3.400	732	734	735	rBV	163	57	0.00%	0.000%
14	3.452	745	750	752	rBV2	502	419	0.02%	0.003%
15	3.510	764	768	773	rVB2	353	323	0.02%	0.003%
16	3.535	773	776	778	rBV2	344	203	0.01%	0.002%
17	3.580	788	790	793	rBV2	491	323	0.02%	0.003%
18	3.597	793	795	798	rVV2	304	176	0.01%	0.001%
19	3.645	806	810	811	rBV2	423	188	0.01%	0.002%
20	3.690	820	824	828	rVB2	464	334	0.02%	0.003%
21	3.719	828	833	836	rBV3	241	254	0.02%	0.002%
22	3.741	837	840	841	rBV2	208	99	0.01%	0.001%
23	3.793	847	856	898	rBV	103845	324244	19.25%	2.699%
24	4.246	983	997	1032	rBV	255976	654576	38.86%	5.449%
25	4.661	1124	1126	1127	rBV2	361	145	0.01%	0.001%
26	4.793	1164	1167	1169	rVB	587	319	0.02%	0.003%
27	4.844	1180	1183	1185	rBV2	394	234	0.01%	0.002%
28	4.953	1201	1217	1259	rBV2	632351	1684289	100.00%	14.020%
29	5.532	1384	1397	1427	rBV	425883	885135	52.55%	7.368%
30	5.834	1484	1491	1510	rVB8	6903	16731	0.99%	0.139%
31	5.985	1525	1538	1571	rBV	366662	767309	45.56%	6.387%
32	6.297	1629	1635	1637	rBV5	735	701	0.04%	0.006%
33	6.452	1681	1683	1686	rBV2	573	330	0.02%	0.003%
34	6.474	1688	1690	1693	rVV2	466	269	0.02%	0.002%
35	6.571	1718	1720	1726	rVB2	433	241	0.01%	0.002%
36	6.603	1727	1730	1732	rBV3	729	439	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035016.D
 Acq On : 05 Apr 2024 19:19
 Operator : SY/MD
 Sample : P2006-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.735	1766	1771	1775	rBV5	899	914	0.05%	0.008%
38	6.760	1775	1779	1782	rBV3	589	502	0.03%	0.004%
39	6.796	1787	1790	1791	rBV	338	231	0.01%	0.002%
40	6.818	1795	1797	1801	rBV2	315	195	0.01%	0.002%
41	6.854	1802	1808	1812	rBV3	376	396	0.02%	0.003%
42	6.911	1816	1826	1853	rBV	173818	338349	20.09%	2.816%
43	7.243	1917	1929	1967	rBV	722898	1291201	76.66%	10.748%
44	7.551	2016	2025	2059	rBV	116082	222092	13.19%	1.849%
45	7.789	2097	2099	2101	rBV2	651	316	0.02%	0.003%
46	7.921	2138	2140	2142	rBV2	736	310	0.02%	0.003%
47	8.027	2164	2173	2215	rBV2	315769	713693	42.37%	5.941%
48	8.664	2367	2371	2373	rBV2	876	520	0.03%	0.004%
49	8.744	2395	2396	2397	rBV2	272	89	0.01%	0.001%
50	8.783	2397	2408	2434	rBV	661249	1099798	65.30%	9.155%
51	9.239	2548	2550	2552	rBV2	288	123	0.01%	0.001%
52	9.262	2555	2557	2559	rVB	491	156	0.01%	0.001%
53	9.313	2571	2573	2576	rVB	657	413	0.02%	0.003%
54	9.333	2576	2579	2586	rBV4	417	509	0.03%	0.004%
55	9.362	2586	2588	2590	rBV	403	210	0.01%	0.002%
56	9.374	2590	2592	2595	rBV2	310	220	0.01%	0.002%
57	9.506	2631	2633	2637	rVB2	427	300	0.02%	0.002%
58	9.554	2640	2648	2652	rBV3	599	678	0.04%	0.006%
59	9.574	2652	2654	2655	rBV3	192	65	0.00%	0.001%
60	9.722	2697	2700	2702	rVB2	320	165	0.01%	0.001%
61	9.738	2702	2705	2706	rBV2	469	221	0.01%	0.002%
62	9.770	2712	2715	2717	rBV3	356	249	0.01%	0.002%
63	9.818	2727	2730	2731	rBV2	271	161	0.01%	0.001%
64	9.905	2755	2757	2761	rBV2	296	186	0.01%	0.002%
65	9.944	2767	2769	2770	rVB2	204	49	0.00%	0.000%
66	9.969	2774	2777	2779	rVB3	378	176	0.01%	0.001%
67	9.998	2782	2786	2788	rBV2	397	295	0.02%	0.002%
68	10.027	2793	2795	2797	rVB	350	127	0.01%	0.001%
69	10.095	2814	2816	2817	rBV	208	85	0.01%	0.001%
70	10.153	2822	2834	2860	rBV	490869	778824	46.24%	6.483%
71	10.445	2922	2925	2926	rBV2	411	277	0.02%	0.002%
72	10.551	2955	2958	2959	rBV	341	230	0.01%	0.002%
73	10.593	2968	2971	2974	rVB2	619	408	0.02%	0.003%
74	10.609	2974	2976	2981	rVB2	418	257	0.02%	0.002%
75	10.638	2982	2985	2990	rBV2	529	382	0.02%	0.003%
76	10.699	3001	3004	3011	rBB3	620	419	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035016.D
 Acq On : 05 Apr 2024 19:19
 Operator : SY/MD
 Sample : P2006-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.818	3037	3041	3045	rVB2	433	376	0.02%	0.003%
78	10.844	3045	3049	3051	rBV2	437	344	0.02%	0.003%
79	10.898	3064	3066	3071	rVB3	430	320	0.02%	0.003%
80	11.098	3123	3128	3130	rBV2	485	443	0.03%	0.004%
81	11.185	3144	3155	3183	rBV	587568	938113	55.70%	7.809%
82	11.410	3223	3225	3229	rVB2	600	337	0.02%	0.003%
83	11.500	3250	3253	3256	rBV2	484	362	0.02%	0.003%
84	11.558	3260	3271	3300	rBV	668466	1065240	63.25%	8.867%
85	11.934	3386	3388	3391	rBV	565	313	0.02%	0.003%
86	12.181	3463	3465	3467	rVB2	578	225	0.01%	0.002%
87	12.294	3498	3500	3503	rVB2	329	108	0.01%	0.001%
88	12.336	3503	3513	3515	rBV3	700	909	0.05%	0.008%
89	12.439	3541	3545	3548	rBV2	423	390	0.02%	0.003%
90	12.535	3572	3575	3579	rVB3	816	620	0.04%	0.005%
91	12.558	3580	3582	3587	rVV2	403	288	0.02%	0.002%
92	12.638	3604	3607	3610	rBV2	435	258	0.02%	0.002%
93	12.738	3635	3638	3641	rVB	359	197	0.01%	0.002%
94	12.754	3641	3643	3645	rBV2	429	293	0.02%	0.002%
95	12.873	3678	3680	3683	rVB2	478	260	0.02%	0.002%
96	13.037	3728	3731	3733	rBV2	578	324	0.02%	0.003%
97	13.275	3802	3805	3807	rVB2	483	231	0.01%	0.002%
98	13.294	3807	3811	3813	rBV3	589	454	0.03%	0.004%
99	13.532	3883	3885	3889	rBV3	375	261	0.02%	0.002%
100	13.644	3916	3920	3924	rBV2	594	593	0.04%	0.005%




Sum of corrected areas: 12013641

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035016.D
Acq On : 05 Apr 2024 19:19
Operator : SY/MD
Sample : P2006-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

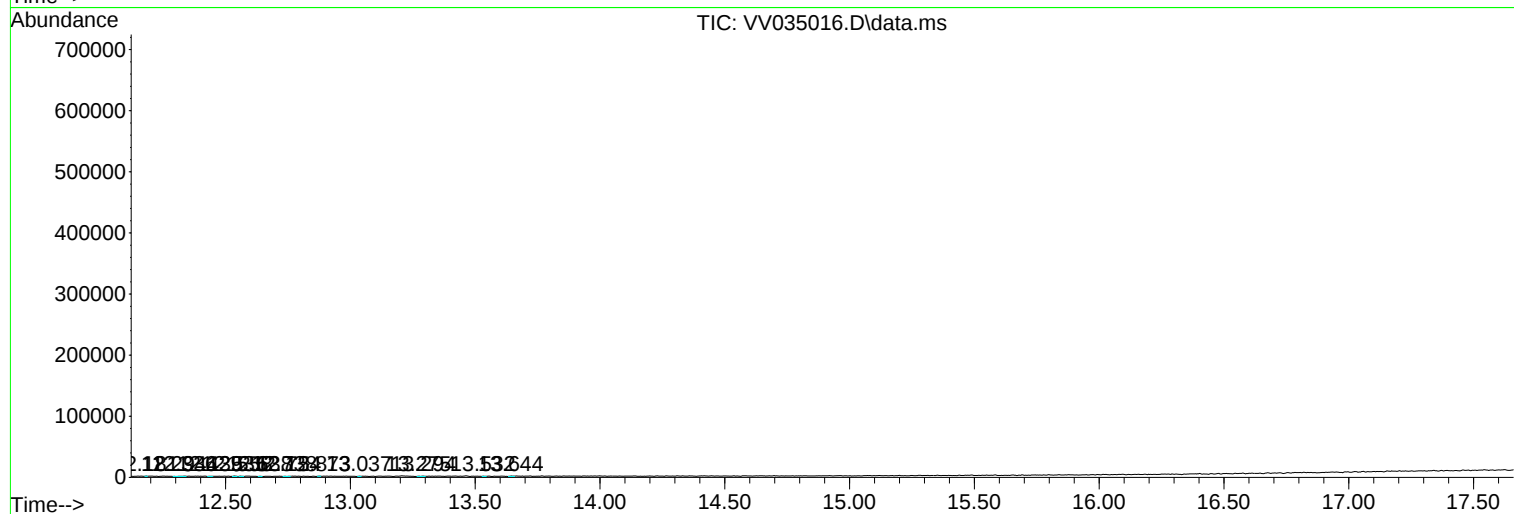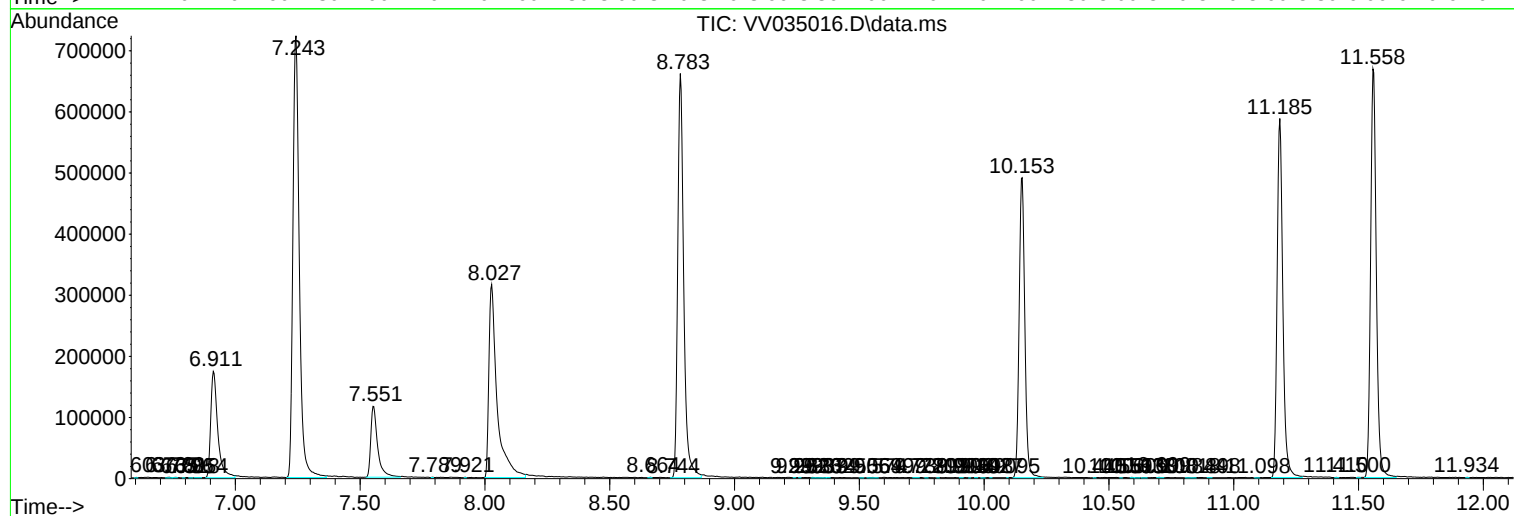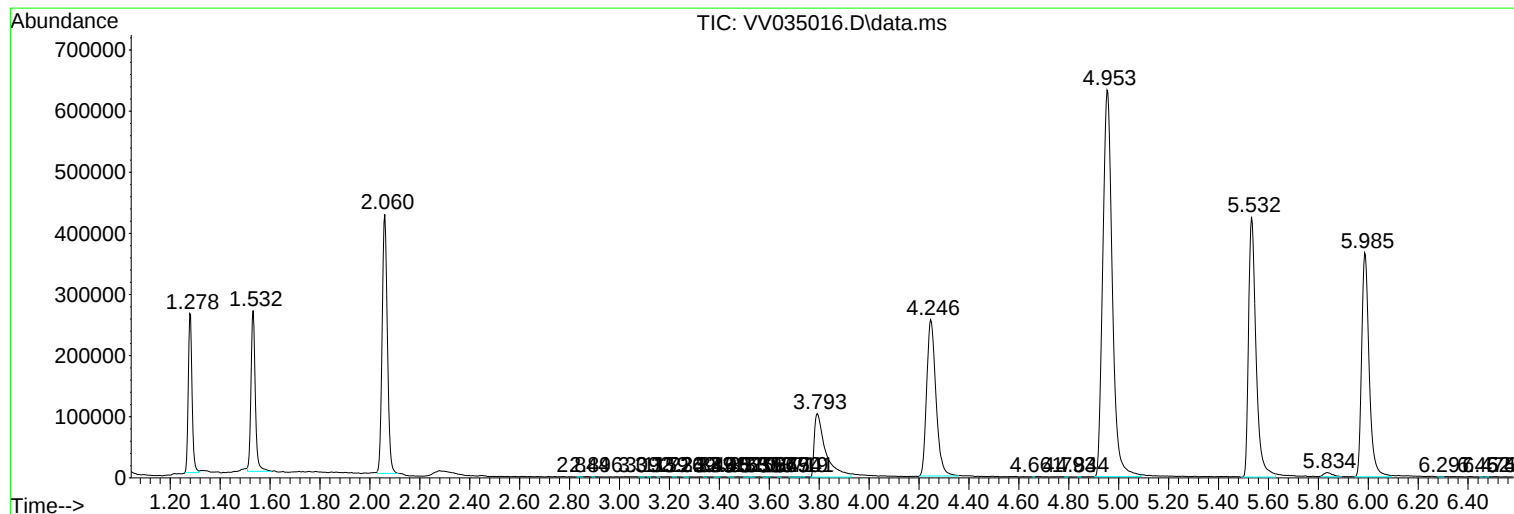

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035016.D
Acq On : 05 Apr 2024 19:19
Operator : SY/MD
Sample : P2006-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035016.D
Acq On : 05 Apr 2024 19:19
Operator : SY/MD
Sample : P2006-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
