

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035019.D
 Acq On : 05 Apr 2024 21:28
 Operator : SY/MD
 Sample : P2006-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	259324	279731	16.38%	2.288%
2	1.532	146	153	169	rVB	253197	294651	17.26%	2.410%
3	2.059	307	317	332	rBV	424276	616802	36.13%	5.045%
4	2.526	459	462	465	rVB2	553	341	0.02%	0.003%
5	2.548	468	469	470	rBV	522	193	0.01%	0.002%
6	2.793	540	545	549	rBV3	579	688	0.04%	0.006%
7	2.989	604	606	613	rVB4	630	737	0.04%	0.006%
8	3.027	613	618	623	rVB3	386	354	0.02%	0.003%
9	3.159	656	659	663	rVB2	722	394	0.02%	0.003%
10	3.191	667	669	672	rBV	345	189	0.01%	0.002%
11	3.211	672	675	678	rVB	401	243	0.01%	0.002%
12	3.233	678	682	687	rBV	361	332	0.02%	0.003%
13	3.262	687	691	693	rBV2	308	211	0.01%	0.002%
14	3.445	745	748	751	rVB3	306	208	0.01%	0.002%
15	3.477	755	758	760	rBV	391	247	0.01%	0.002%
16	3.590	787	793	796	rBV5	516	457	0.03%	0.004%
17	3.638	806	808	812	rVB2	507	250	0.01%	0.002%
18	3.657	812	814	816	rBV2	492	215	0.01%	0.002%
19	3.793	848	856	898	rBV	106442	335232	19.63%	2.742%
20	4.249	984	998	1033	rBV	260437	670647	39.28%	5.486%
21	4.883	1192	1195	1198	rVB3	417	204	0.01%	0.002%
22	4.953	1200	1217	1258	rBV2	636487	1707347	100.00%	13.965%
23	5.307	1325	1327	1330	rVB2	873	462	0.03%	0.004%
24	5.468	1375	1377	1379	rBV2	602	246	0.01%	0.002%
25	5.532	1386	1397	1423	rBV	434277	904278	52.96%	7.397%
26	5.834	1481	1491	1510	rBV3	12030	27471	1.61%	0.225%
27	5.937	1520	1523	1524	rBV3	452	210	0.01%	0.002%
28	5.985	1525	1538	1570	rVV	371961	775464	45.42%	6.343%
29	6.413	1666	1671	1673	rVB3	549	480	0.03%	0.004%
30	6.426	1673	1675	1677	rBV	465	289	0.02%	0.002%
31	6.452	1680	1683	1685	rVV2	609	281	0.02%	0.002%
32	6.577	1719	1722	1725	rVV3	360	267	0.02%	0.002%
33	6.648	1742	1744	1746	rBV	515	219	0.01%	0.002%
34	6.911	1816	1826	1854	rBV	177794	345642	20.24%	2.827%
35	7.243	1917	1929	1955	rBV	730557	1298906	76.08%	10.624%
36	7.551	2016	2025	2049	rBV	120148	226447	13.26%	1.852%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035019.D
 Acq On : 05 Apr 2024 21:28
 Operator : SY/MD
 Sample : P2006-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	7.812	2104	2106	2112	rVB4	886	656	0.04%	0.005%
38	7.963	2148	2153	2154	rBV3	468	408	0.02%	0.003%
39	7.992	2160	2162	2164	rBV2	505	238	0.01%	0.002%
40	8.027	2164	2173	2221	rBV2	320136	737157	43.18%	6.030%
41	8.529	2327	2329	2330	rBV	505	200	0.01%	0.002%
42	8.738	2391	2394	2396	rBV2	430	278	0.02%	0.002%
43	8.783	2396	2408	2443	rBV	672633	1126146	65.96%	9.211%
44	9.091	2501	2504	2505	rBV	493	270	0.02%	0.002%
45	9.143	2516	2520	2523	rBV4	532	366	0.02%	0.003%
46	9.185	2528	2533	2534	rBV2	580	384	0.02%	0.003%
47	9.230	2541	2547	2551	rBV2	651	683	0.04%	0.006%
48	9.278	2560	2562	2565	rVB2	522	226	0.01%	0.002%
49	9.297	2565	2568	2573	rVB4	469	386	0.02%	0.003%
50	9.336	2577	2580	2587	rVB4	455	507	0.03%	0.004%
51	9.426	2607	2608	2612	rBV3	493	294	0.02%	0.002%
52	9.493	2624	2629	2633	rBV4	541	549	0.03%	0.004%
53	9.545	2641	2645	2651	rBV4	509	560	0.03%	0.005%
54	9.731	2700	2703	2706	rBV3	308	268	0.02%	0.002%
55	9.796	2720	2723	2725	rBV	475	195	0.01%	0.002%
56	9.824	2730	2732	2734	rBV2	428	199	0.01%	0.002%
57	9.879	2746	2749	2752	rBV	605	438	0.03%	0.004%
58	9.921	2758	2762	2766	rBV3	492	445	0.03%	0.004%
59	9.947	2766	2770	2773	rBV3	430	419	0.02%	0.003%
60	10.030	2793	2796	2797	rBV2	403	194	0.01%	0.002%
61	10.040	2797	2799	2801	rVV2	474	208	0.01%	0.002%
62	10.149	2822	2833	2858	rBV	477678	771778	45.20%	6.313%
63	10.294	2874	2878	2882	rBV2	692	549	0.03%	0.004%
64	10.313	2882	2884	2888	rVV3	783	441	0.03%	0.004%
65	10.384	2903	2906	2909	rBV2	553	328	0.02%	0.003%
66	10.406	2909	2913	2917	rBV4	918	867	0.05%	0.007%
67	10.468	2929	2932	2935	rBV	301	227	0.01%	0.002%
68	10.500	2940	2942	2944	rBV2	347	214	0.01%	0.002%
69	10.705	2996	3006	3011	rBV3	721	1005	0.06%	0.008%
70	10.792	3029	3033	3037	rVB2	432	317	0.02%	0.003%
71	10.821	3039	3042	3046	rVB2	266	192	0.01%	0.002%
72	11.046	3106	3112	3114	rBV4	418	386	0.02%	0.003%
73	11.140	3133	3141	3144	rBV5	1206	1817	0.11%	0.015%
74	11.185	3144	3155	3182	rBV	609514	960321	56.25%	7.855%
75	11.503	3244	3254	3260	rVV4	9767	18601	1.09%	0.152%
76	11.558	3261	3271	3301	rVB	678430	1083731	63.47%	8.864%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035019.D
 Acq On : 05 Apr 2024 21:28
 Operator : SY/MD
 Sample : P2006-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.918	3381	3383	3385	rBV2	530	235	0.01%	0.002%
78	12.043	3420	3422	3424	rBV	403	244	0.01%	0.002%
79	12.133	3447	3450	3453	rBV3	476	349	0.02%	0.003%
80	12.184	3464	3466	3473	rBV2	464	452	0.03%	0.004%
81	12.229	3477	3480	3483	rBV	453	324	0.02%	0.003%
82	12.307	3496	3504	3509	rBV5	892	1403	0.08%	0.011%
83	12.329	3509	3511	3512	rBV	458	201	0.01%	0.002%
84	12.377	3522	3526	3528	rBV3	895	639	0.04%	0.005%
85	12.535	3572	3575	3577	rBV2	396	227	0.01%	0.002%
86	12.590	3586	3592	3601	rBV6	2025	2532	0.15%	0.021%
87	12.625	3601	3603	3605	rBV2	316	188	0.01%	0.002%
88	12.776	3648	3650	3652	rBV2	553	292	0.02%	0.002%
89	12.805	3656	3659	3663	rBV3	426	437	0.03%	0.004%
90	12.847	3668	3672	3676	rVV3	347	309	0.02%	0.003%
91	12.866	3676	3678	3683	rVB2	349	217	0.01%	0.002%
92	12.905	3687	3690	3693	rBV3	664	453	0.03%	0.004%
93	13.078	3742	3744	3746	rBV2	453	205	0.01%	0.002%
94	13.114	3753	3755	3757	rBV2	743	473	0.03%	0.004%
95	13.265	3800	3802	3806	rVB3	409	223	0.01%	0.002%
96	13.297	3810	3812	3815	rBV2	422	246	0.01%	0.002%
97	13.448	3851	3859	3873	rBV2	7422	12367	0.72%	0.101%
98	13.596	3903	3905	3908	rBV2	583	323	0.02%	0.003%
99	13.731	3945	3947	3950	rBV3	574	297	0.02%	0.002%
100	14.503	4185	4187	4189	rBV2	420	231	0.01%	0.002%

Sum of corrected areas: 12225650




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035019.D
Acq On : 05 Apr 2024 21:28
Operator : SY/MD
Sample : P2006-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

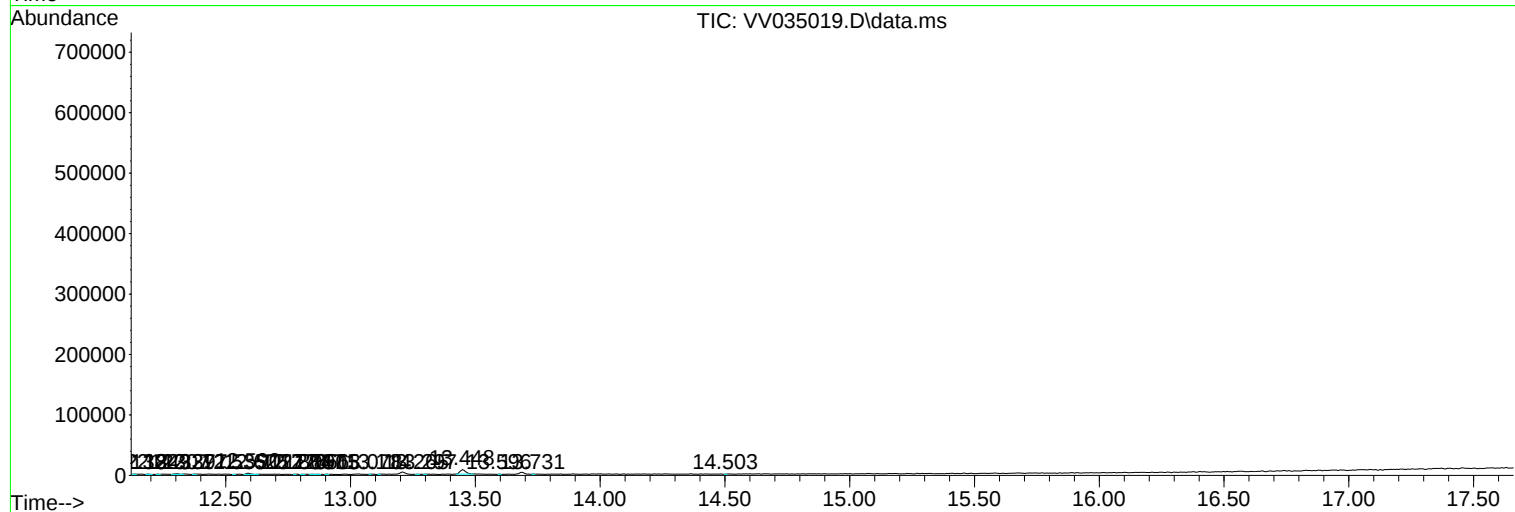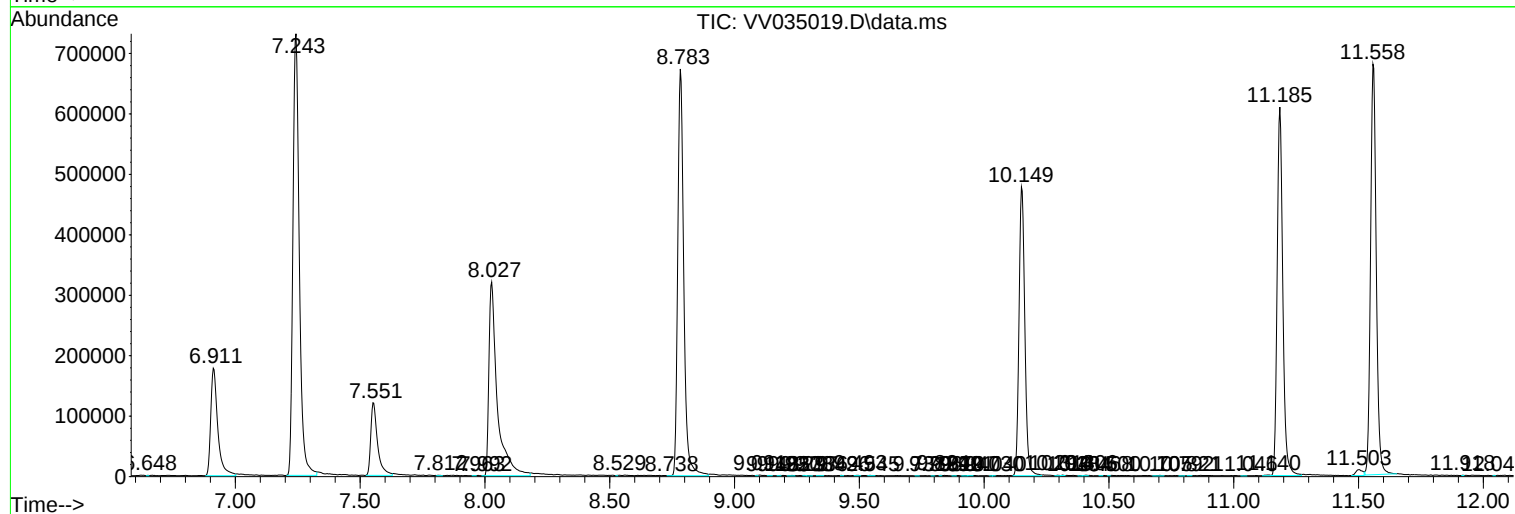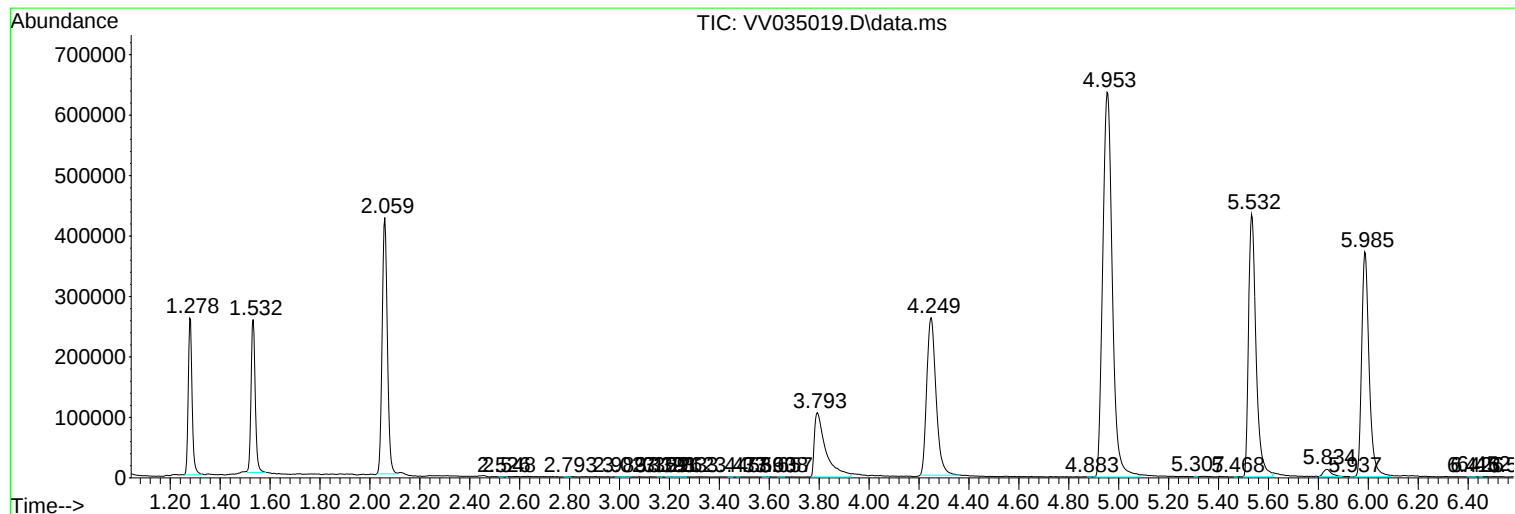

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035019.D
Acq On : 05 Apr 2024 21:28
Operator : SY/MD
Sample : P2006-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035019.D
Acq On : 05 Apr 2024 21:28
Operator : SY/MD
Sample : P2006-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------