

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040524\
 Data File : VV035020.D
 Acq On : 05 Apr 2024 21:52
 Operator : SY/MD
 Sample : P2006-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	61	rBV4	2534	4086	0.25%	0.035%
2	1.278	67	74	94	rVB	252221	268338	16.21%	2.267%
3	1.532	146	153	171	rVB	248962	285590	17.25%	2.413%
4	2.060	307	317	333	rBV	412629	599429	36.21%	5.064%
5	2.230	367	370	373	rBV3	989	852	0.05%	0.007%
6	2.446	433	437	440	rBV5	1321	1030	0.06%	0.009%
7	2.613	485	489	492	rBV3	613	432	0.03%	0.004%
8	2.693	510	514	516	rBV2	669	509	0.03%	0.004%
9	3.002	607	610	615	rBV3	492	475	0.03%	0.004%
10	3.114	640	645	650	rVB3	581	565	0.03%	0.005%
11	3.282	693	697	700	rVB3	402	322	0.02%	0.003%
12	3.307	700	705	706	rBV2	549	356	0.02%	0.003%
13	3.474	754	757	760	rBV2	477	360	0.02%	0.003%
14	3.619	798	802	805	rVB2	494	344	0.02%	0.003%
15	3.661	810	815	820	rBV3	449	512	0.03%	0.004%
16	3.793	847	856	893	rBV	107216	324119	19.58%	2.738%
17	4.246	981	997	1030	rBV	251147	653182	39.45%	5.518%
18	4.571	1095	1098	1102	rVB4	1059	748	0.05%	0.006%
19	4.590	1102	1104	1106	rBV	636	307	0.02%	0.003%
20	4.667	1123	1128	1130	rVV4	679	488	0.03%	0.004%
21	4.699	1136	1138	1145	rVB4	432	389	0.02%	0.003%
22	4.793	1162	1167	1168	rBV	478	371	0.02%	0.003%
23	4.844	1181	1183	1191	rVB4	567	500	0.03%	0.004%
24	4.886	1192	1196	1200	rBV2	400	295	0.02%	0.002%
25	4.953	1202	1217	1256	rBV2	620727	1655597	100.00%	13.987%
26	5.400	1353	1356	1358	rBV3	542	329	0.02%	0.003%
27	5.468	1375	1377	1381	rVB2	750	465	0.03%	0.004%
28	5.532	1386	1397	1434	rBV	414020	881059	53.22%	7.444%
29	5.834	1482	1491	1507	rBV4	8559	18884	1.14%	0.160%
30	5.986	1525	1538	1577	rVV	361072	760912	45.96%	6.429%
31	6.150	1586	1589	1591	rBV3	794	590	0.04%	0.005%
32	6.320	1640	1642	1647	rBV4	566	502	0.03%	0.004%
33	6.375	1654	1659	1663	rVB3	575	538	0.03%	0.005%
34	6.497	1692	1697	1700	rBV4	467	416	0.03%	0.004%
35	6.555	1711	1715	1717	rBV3	412	361	0.02%	0.003%
36	6.580	1721	1723	1727	rVB4	710	558	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035020.D
 Acq On : 05 Apr 2024 21:52
 Operator : SY/MD
 Sample : P2006-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.603	1727	1730	1732	rBV2	449	295	0.02%	0.002%
38	6.632	1736	1739	1741	rVV4	481	348	0.02%	0.003%
39	6.645	1741	1743	1748	rVV3	598	488	0.03%	0.004%
40	6.690	1752	1757	1758	rBV3	410	300	0.02%	0.003%
41	6.773	1779	1783	1786	rVB2	559	350	0.02%	0.003%
42	6.838	1799	1803	1808	rBV3	597	629	0.04%	0.005%
43	6.912	1810	1826	1853	rBV	173786	336916	20.35%	2.846%
44	7.243	1916	1929	1966	rBV	705045	1265945	76.46%	10.695%
45	7.551	2016	2025	2049	rBV	114341	217712	13.15%	1.839%
46	7.863	2119	2122	2127	rVB4	495	458	0.03%	0.004%
47	7.892	2127	2131	2132	rBV2	834	485	0.03%	0.004%
48	7.957	2146	2151	2154	rVB3	706	572	0.03%	0.005%
49	8.027	2164	2173	2214	rBV2	315890	730370	44.12%	6.171%
50	8.317	2261	2263	2266	rBV3	755	573	0.03%	0.005%
51	8.442	2299	2302	2304	rBV3	574	380	0.02%	0.003%
52	8.474	2309	2312	2313	rBV2	456	301	0.02%	0.003%
53	8.580	2342	2345	2349	rVB3	384	384	0.02%	0.003%
54	8.693	2377	2380	2388	rVB5	684	805	0.05%	0.007%
55	8.731	2388	2392	2395	rBV2	610	557	0.03%	0.005%
56	8.783	2397	2408	2435	rBV	645430	1071551	64.72%	9.053%
57	8.953	2459	2461	2464	rBV3	770	430	0.03%	0.004%
58	9.072	2497	2498	2503	rVB3	463	314	0.02%	0.003%
59	9.259	2554	2556	2561	rBV3	720	486	0.03%	0.004%
60	9.349	2580	2584	2587	rBV2	457	330	0.02%	0.003%
61	9.423	2603	2607	2612	rBV3	500	552	0.03%	0.005%
62	9.545	2643	2645	2648	rBV2	635	291	0.02%	0.002%
63	9.728	2699	2702	2707	rVB2	640	406	0.02%	0.003%
64	10.149	2819	2833	2858	rBV	473897	764369	46.17%	6.458%
65	10.484	2933	2937	2940	rBV	425	313	0.02%	0.003%
66	10.638	2979	2985	2994	rVB4	415	593	0.04%	0.005%
67	10.741	3010	3017	3025	rBV3	604	1034	0.06%	0.009%
68	10.792	3029	3033	3036	rVV2	464	381	0.02%	0.003%
69	10.866	3053	3056	3060	rVV2	592	469	0.03%	0.004%
70	10.895	3063	3065	3071	rBV4	444	425	0.03%	0.004%
71	11.008	3096	3100	3102	rBV3	502	335	0.02%	0.003%
72	11.095	3121	3127	3133	rBV4	512	674	0.04%	0.006%
73	11.127	3133	3137	3139	rBV3	773	678	0.04%	0.006%
74	11.185	3144	3155	3184	rBV	582170	911496	55.06%	7.701%
75	11.378	3213	3215	3218	rVB2	632	310	0.02%	0.003%
76	11.448	3232	3237	3240	rBV3	508	383	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035020.D
 Acq On : 05 Apr 2024 21:52
 Operator : SY/MD
 Sample : P2006-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.509	3246	3256	3260	rBV6	4968	8307	0.50%	0.070%
78	11.558	3260	3271	3293	rVV	646813	1031607	62.31%	8.716%
79	11.770	3335	3337	3341	rVB4	789	430	0.03%	0.004%
80	12.027	3414	3417	3420	rVB3	606	306	0.02%	0.003%
81	12.159	3455	3458	3463	rBV3	338	298	0.02%	0.003%
82	12.185	3464	3466	3471	rVB4	591	427	0.03%	0.004%
83	12.294	3495	3500	3504	rBV5	615	647	0.04%	0.005%
84	12.538	3574	3576	3583	rVB2	465	299	0.02%	0.003%
85	12.590	3587	3592	3597	rBV5	961	1098	0.07%	0.009%
86	12.673	3614	3618	3622	rVB3	354	340	0.02%	0.003%
87	12.850	3670	3673	3675	rBV3	500	352	0.02%	0.003%
88	13.133	3757	3761	3762	rBV3	449	298	0.02%	0.003%
89	13.204	3776	3783	3792	rVV6	2284	3359	0.20%	0.028%
90	13.313	3813	3817	3821	rBV3	585	596	0.04%	0.005%
91	13.452	3854	3860	3868	rVV3	3737	5268	0.32%	0.045%
92	13.622	3910	3913	3919	rVB3	649	573	0.03%	0.005%
93	13.661	3919	3925	3927	rBV4	728	746	0.05%	0.006%
94	13.992	4026	4028	4032	rVV2	683	405	0.02%	0.003%
95	14.802	4277	4280	4283	rVB3	666	432	0.03%	0.004%
96	14.915	4312	4315	4318	rBV3	940	596	0.04%	0.005%
97	15.111	4373	4376	4379	rBV3	1217	907	0.05%	0.008%
98	15.217	4406	4409	4411	rBV4	740	584	0.04%	0.005%
99	15.242	4415	4417	4419	rBV	860	480	0.03%	0.004%
100	15.696	4556	4558	4561	rBV4	1040	599	0.04%	0.005%




Sum of corrected areas: 11836452

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035020.D
Acq On : 05 Apr 2024 21:52
Operator : SY/MD
Sample : P2006-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

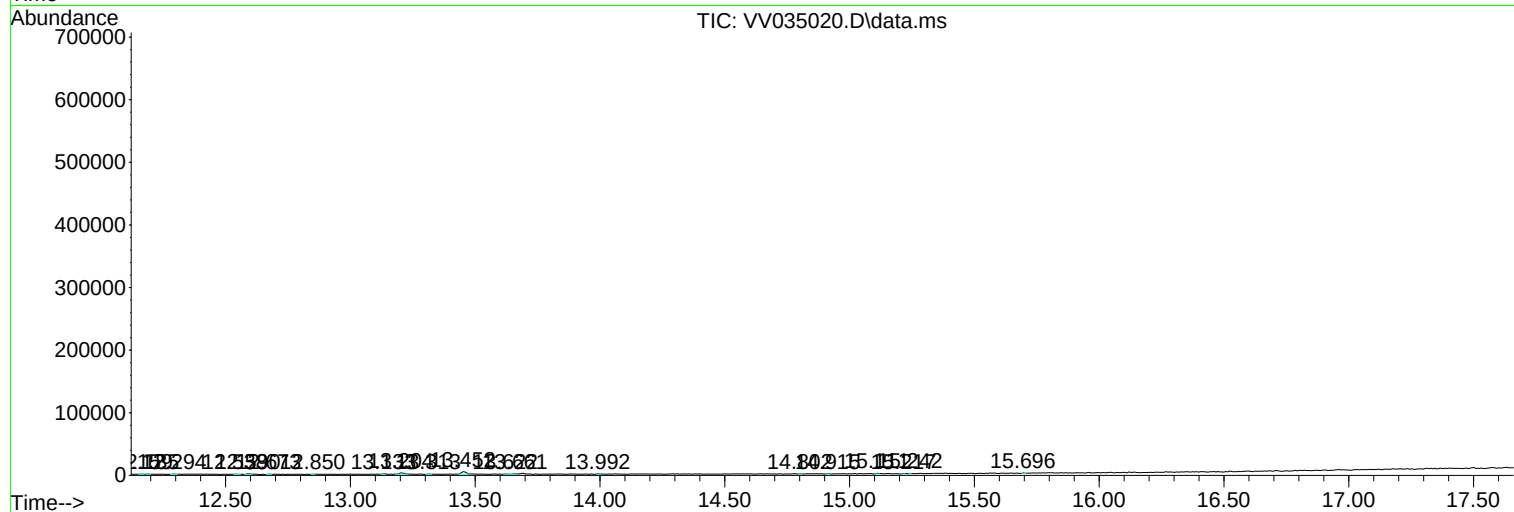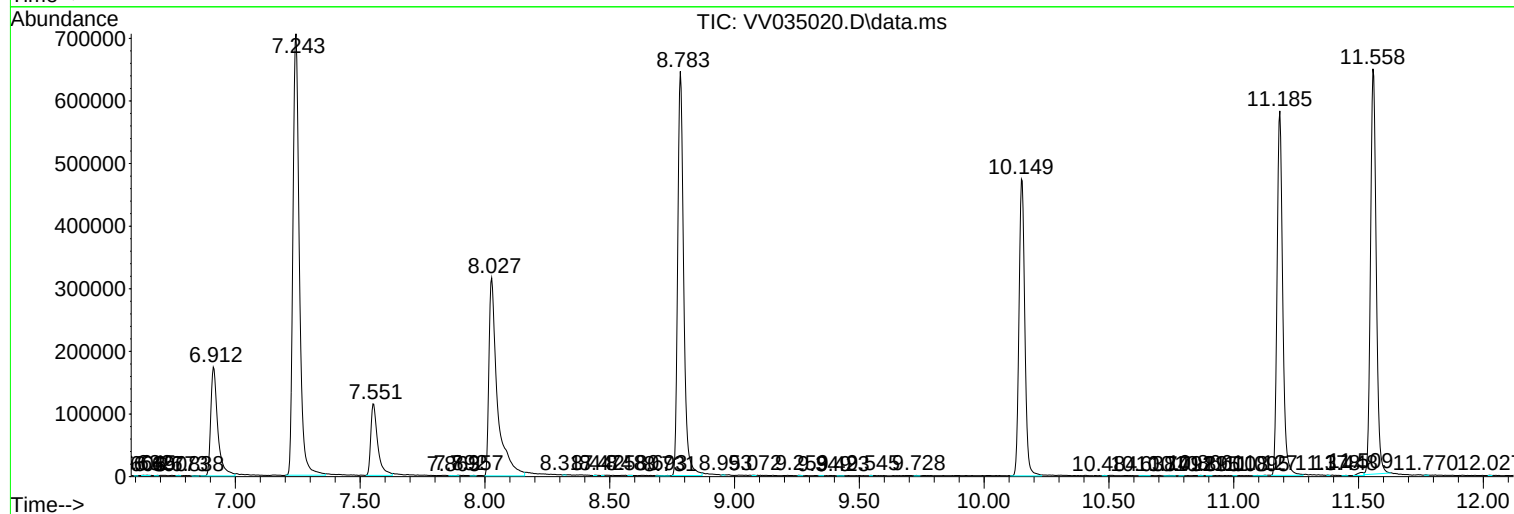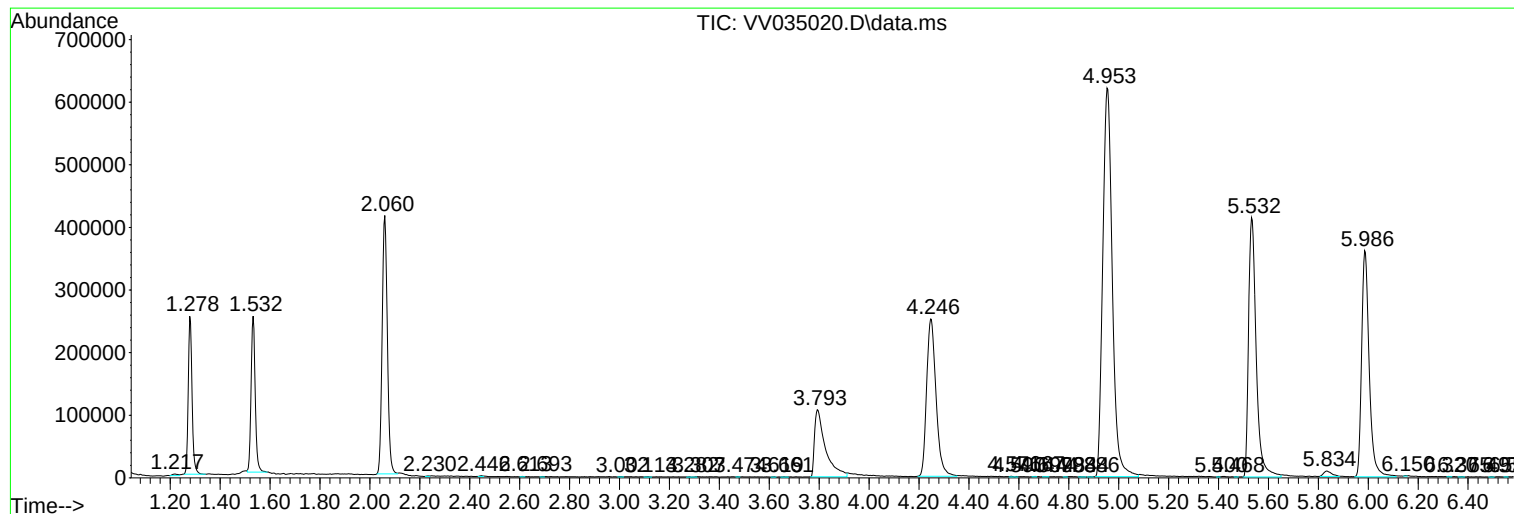

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035020.D
Acq On : 05 Apr 2024 21:52
Operator : SY/MD
Sample : P2006-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035020.D
Acq On : 05 Apr 2024 21:52
Operator : SY/MD
Sample : P2006-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------