

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035021.D
 Acq On : 05 Apr 2024 22:16
 Operator : SY/MD
 Sample : P2006-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	256116	274464	16.17%	2.288%
2	1.532	146	153	166	rVB	256962	293720	17.31%	2.449%
3	2.060	307	317	332	rBV	424395	615329	36.26%	5.131%
4	2.719	521	522	526	rBV3	352	224	0.01%	0.002%
5	2.976	600	602	604	rBV	373	164	0.01%	0.001%
6	2.992	604	607	608	rBV	385	167	0.01%	0.001%
7	3.076	630	633	636	rBV2	623	398	0.02%	0.003%
8	3.137	650	652	657	rBV3	369	273	0.02%	0.002%
9	3.159	657	659	662	rBV3	497	294	0.02%	0.002%
10	3.237	681	683	686	rVB	488	176	0.01%	0.001%
11	3.249	686	687	690	rBV	290	145	0.01%	0.001%
12	3.298	700	702	705	rVB	464	215	0.01%	0.002%
13	3.317	705	708	711	rBV2	435	321	0.02%	0.003%
14	3.378	725	727	729	rVV	391	167	0.01%	0.001%
15	3.404	733	735	738	rVB2	502	218	0.01%	0.002%
16	3.442	744	747	749	rBV2	350	199	0.01%	0.002%
17	3.497	760	764	765	rBV2	455	266	0.02%	0.002%
18	3.526	771	773	777	rVB3	351	199	0.01%	0.002%
19	3.548	777	780	782	rBV2	368	229	0.01%	0.002%
20	3.568	782	786	789	rVV2	376	294	0.02%	0.002%
21	3.616	799	801	803	rBV	316	160	0.01%	0.001%
22	3.626	803	804	805	rBV	323	120	0.01%	0.001%
23	3.683	817	822	827	rVB3	869	887	0.05%	0.007%
24	3.706	827	829	832	rBV2	547	271	0.02%	0.002%
25	3.722	832	834	838	rVB	756	389	0.02%	0.003%
26	3.745	838	841	842	rBV2	270	176	0.01%	0.001%
27	3.793	848	856	901	rBV	101080	321303	18.93%	2.679%
28	4.246	983	997	1027	rBV	258267	675739	39.82%	5.634%
29	4.838	1180	1181	1185	rBV2	664	353	0.02%	0.003%
30	4.954	1201	1217	1253	rBV2	639033	1697095	100.00%	14.150%
31	5.420	1360	1362	1364	rVB3	418	151	0.01%	0.001%
32	5.445	1368	1370	1373	rBV	649	438	0.03%	0.004%
33	5.532	1385	1397	1424	rBV	418321	882218	51.98%	7.356%
34	5.831	1480	1490	1512	rBV3	11765	27906	1.64%	0.233%
35	5.986	1526	1538	1567	rBV	365734	763266	44.97%	6.364%
36	6.249	1618	1620	1623	rBV3	537	293	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035021.D
 Acq On : 05 Apr 2024 22:16
 Operator : SY/MD
 Sample : P2006-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCOR78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.378	1658	1660	1663	rBV2	509	396	0.02%	0.003%
38	6.420	1671	1673	1675	rVB2	612	266	0.02%	0.002%
39	6.439	1675	1679	1680	rBV	510	330	0.02%	0.003%
40	6.474	1686	1690	1691	rBV4	718	482	0.03%	0.004%
41	6.500	1696	1698	1701	rBV3	674	455	0.03%	0.004%
42	6.564	1715	1718	1719	rBV2	651	334	0.02%	0.003%
43	6.732	1768	1770	1773	rVB3	487	224	0.01%	0.002%
44	6.748	1773	1775	1777	rBV2	326	203	0.01%	0.002%
45	6.841	1801	1804	1805	rBV	313	182	0.01%	0.002%
46	6.860	1808	1810	1813	rVB	372	168	0.01%	0.001%
47	6.912	1813	1826	1853	rBV	177032	343526	20.24%	2.864%
48	7.243	1918	1929	1961	rBV	721229	1292996	76.19%	10.781%
49	7.551	2016	2025	2048	rBV	119404	224698	13.24%	1.874%
50	7.950	2147	2149	2151	rBV2	318	171	0.01%	0.001%
51	7.992	2160	2162	2163	rBV	320	116	0.01%	0.001%
52	8.027	2163	2173	2211	rBV2	303845	698718	41.17%	5.826%
53	8.481	2311	2314	2315	rBV3	631	304	0.02%	0.003%
54	8.616	2354	2356	2361	rBV3	393	359	0.02%	0.003%
55	8.783	2397	2408	2439	rBV	646693	1078012	63.52%	8.988%
56	9.011	2477	2479	2482	rBV3	721	401	0.02%	0.003%
57	9.056	2490	2493	2495	rVB2	770	441	0.03%	0.004%
58	9.169	2526	2528	2533	rBV4	461	300	0.02%	0.003%
59	9.272	2559	2560	2563	rVB2	551	173	0.01%	0.001%
60	9.288	2563	2565	2569	rBV2	395	287	0.02%	0.002%
61	9.394	2596	2598	2602	rBV	432	320	0.02%	0.003%
62	9.420	2602	2606	2609	rBV2	358	320	0.02%	0.003%
63	9.516	2633	2636	2641	rVB3	456	387	0.02%	0.003%
64	9.542	2642	2644	2648	rVB2	414	288	0.02%	0.002%
65	9.567	2648	2652	2654	rBV3	328	310	0.02%	0.003%
66	9.584	2654	2657	2658	rBV	261	121	0.01%	0.001%
67	9.600	2658	2662	2664	rBV2	408	238	0.01%	0.002%
68	9.664	2680	2682	2685	rVB3	376	211	0.01%	0.002%
69	9.719	2697	2699	2704	rVB3	410	276	0.02%	0.002%
70	9.741	2704	2706	2709	rBV	385	186	0.01%	0.002%
71	9.799	2722	2724	2727	rVB	347	179	0.01%	0.001%
72	9.912	2756	2759	2762	rBV2	353	265	0.02%	0.002%
73	9.944	2765	2769	2770	rBV2	204	151	0.01%	0.001%
74	9.953	2770	2772	2773	rBV2	354	139	0.01%	0.001%
75	10.050	2800	2802	2803	rBV	302	130	0.01%	0.001%
76	10.149	2821	2833	2858	rBV	482417	765255	45.09%	6.381%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035021.D
 Acq On : 05 Apr 2024 22:16
 Operator : SY/MD
 Sample : P2006-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.625	2978	2981	2984	rBV2	286	236	0.01%	0.002%
78	10.728	3009	3013	3014	rBV2	509	316	0.02%	0.003%
79	10.863	3048	3055	3058	rBV3	513	641	0.04%	0.005%
80	10.879	3058	3060	3062	rVB	308	125	0.01%	0.001%
81	11.124	3134	3136	3139	rBV2	655	458	0.03%	0.004%
82	11.185	3144	3155	3184	rVV	579787	924299	54.46%	7.707%
83	11.442	3233	3235	3239	rBV2	531	334	0.02%	0.003%
84	11.506	3246	3255	3260	rBV7	6641	12093	0.71%	0.101%
85	11.558	3261	3271	3302	rVB	668642	1077902	63.51%	8.987%
86	11.924	3382	3385	3388	rBV2	436	326	0.02%	0.003%
87	11.963	3393	3397	3398	rBV	631	407	0.02%	0.003%
88	12.056	3423	3426	3427	rBV	460	286	0.02%	0.002%
89	12.153	3454	3456	3459	rBV2	450	258	0.02%	0.002%
90	12.252	3484	3487	3489	rBV	549	388	0.02%	0.003%
91	12.307	3497	3504	3507	rBV5	1632	1958	0.12%	0.016%
92	12.352	3516	3518	3523	rVB3	579	455	0.03%	0.004%
93	12.628	3602	3604	3606	rBV2	471	151	0.01%	0.001%
94	12.767	3645	3647	3649	rBV2	415	234	0.01%	0.002%
95	12.841	3668	3670	3673	rBV2	642	359	0.02%	0.003%
96	12.992	3713	3717	3724	rBV3	532	705	0.04%	0.006%
97	13.246	3794	3796	3799	rBV3	563	306	0.02%	0.003%
98	13.323	3818	3820	3821	rBV3	423	134	0.01%	0.001%
99	13.358	3829	3831	3833	rBV2	373	203	0.01%	0.002%
100	13.728	3944	3946	3948	rBV2	459	258	0.02%	0.002%




Sum of corrected areas: 11993377

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035021.D
Acq On : 05 Apr 2024 22:16
Operator : SY/MD
Sample : P2006-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

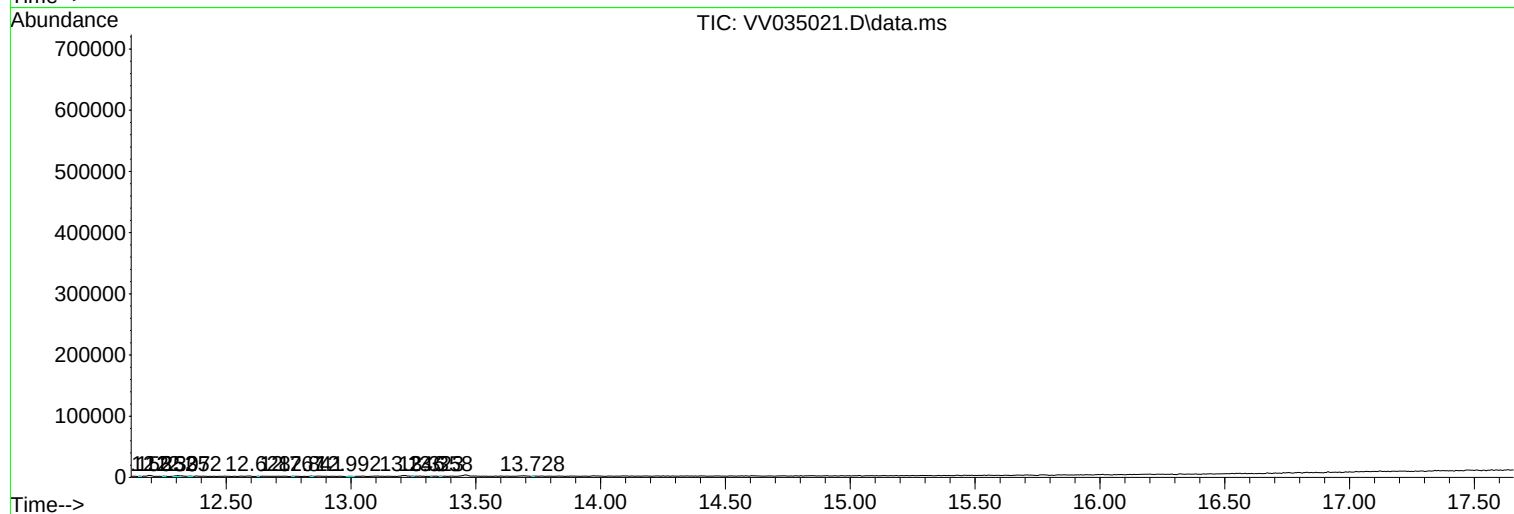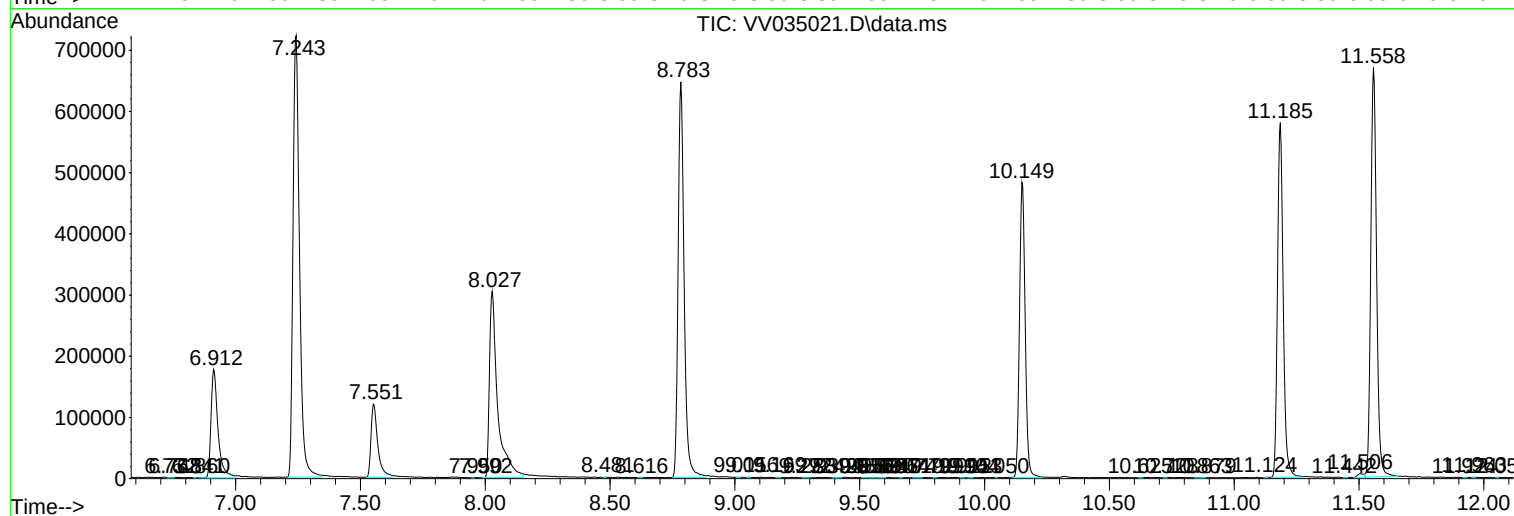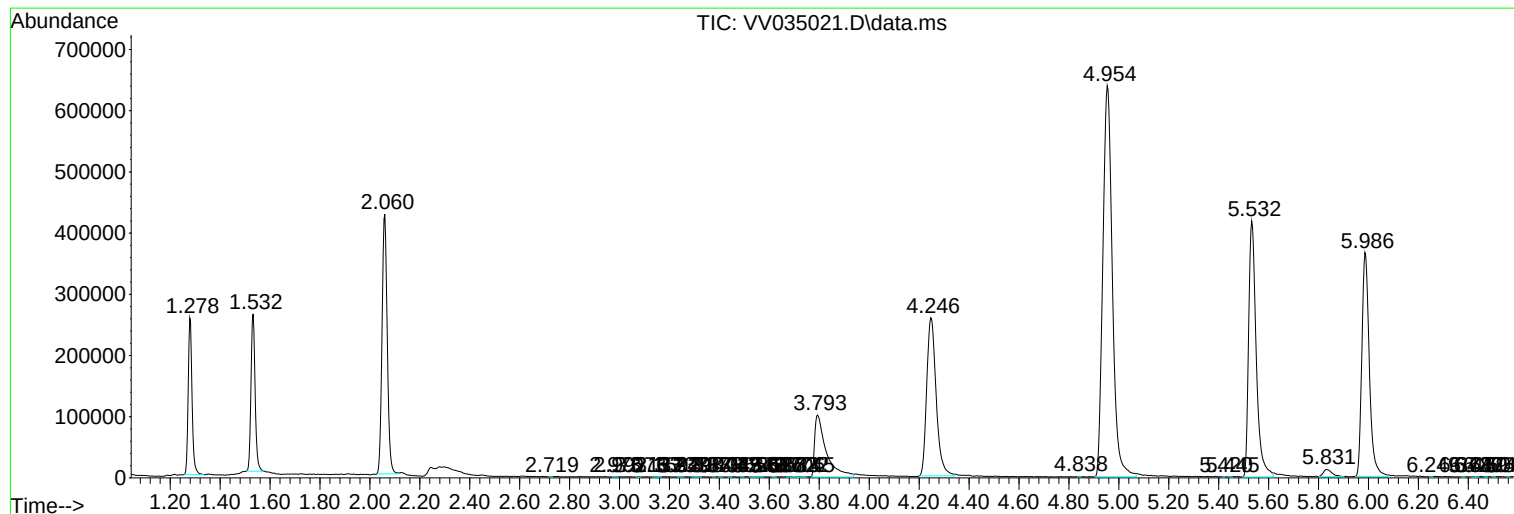

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035021.D
Acq On : 05 Apr 2024 22:16
Operator : SY/MD
Sample : P2006-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035021.D
Acq On : 05 Apr 2024 22:16
Operator : SY/MD
Sample : P2006-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc