

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035026.D
 Acq On : 06 Apr 2024 00:16
 Operator : SY/MD
 Sample : P2006-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	94	rVB	268651	286636	14.81%	1.662%
2	1.532	146	153	172	rVB	259725	299346	15.47%	1.735%
3	2.060	308	317	333	rVB	445106	640709	33.11%	3.714%
4	2.619	487	491	494	rBV2	575	528	0.03%	0.003%
5	2.757	532	534	536	rBV	503	306	0.02%	0.002%
6	3.066	628	630	632	rBV	392	173	0.01%	0.001%
7	3.217	672	677	678	rBV2	305	235	0.01%	0.001%
8	3.249	684	687	689	rBV	443	250	0.01%	0.001%
9	3.317	705	708	711	rBV2	337	243	0.01%	0.001%
10	3.355	718	720	721	rBV	326	137	0.01%	0.001%
11	3.426	739	742	745	rBV2	353	267	0.01%	0.002%
12	3.619	799	802	804	rBV2	353	221	0.01%	0.001%
13	3.664	813	816	823	rBV3	551	560	0.03%	0.003%
14	3.793	848	856	896	rBV	101650	323436	16.71%	1.875%
15	4.246	983	997	1033	rBV	270304	697944	36.06%	4.046%
16	4.642	1118	1120	1123	rBV3	452	236	0.01%	0.001%
17	4.661	1123	1126	1129	rVV4	548	315	0.02%	0.002%
18	4.953	1201	1217	1263	rBV2	671661	1858697	96.04%	10.775%
19	5.465	1373	1376	1377	rBV2	534	224	0.01%	0.001%
20	5.532	1386	1397	1423	rBV	477671	984759	50.88%	5.709%
21	5.841	1481	1493	1507	rBV4	9210	22190	1.15%	0.129%
22	5.931	1516	1521	1523	rBV4	1068	817	0.04%	0.005%
23	5.986	1526	1538	1572	rVV	386104	807081	41.70%	4.679%
24	6.387	1659	1663	1665	rVB3	523	360	0.02%	0.002%
25	6.410	1665	1670	1674	rBV4	929	999	0.05%	0.006%
26	6.429	1674	1676	1677	rBV	360	166	0.01%	0.001%
27	6.455	1682	1684	1688	rVB	444	264	0.01%	0.002%
28	6.500	1694	1698	1699	rBV	295	168	0.01%	0.001%
29	6.529	1705	1707	1708	rBV2	350	166	0.01%	0.001%
30	6.593	1723	1727	1730	rBV2	556	540	0.03%	0.003%
31	6.619	1734	1735	1737	rVB	624	207	0.01%	0.001%
32	6.722	1765	1767	1770	rBV	364	256	0.01%	0.001%
33	6.764	1777	1780	1781	rBV3	471	200	0.01%	0.001%
34	6.789	1784	1788	1790	rBV2	794	485	0.03%	0.003%
35	6.825	1797	1799	1805	rVB2	536	388	0.02%	0.002%
36	6.863	1806	1811	1812	rBV3	427	327	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035026.D
 Acq On : 06 Apr 2024 00:16
 Operator : SY/MD
 Sample : P2006-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.873	1812	1814	1816	rBV2	396	246	0.01%	0.001%
38	6.912	1816	1826	1859	rBV	196471	378718	19.57%	2.195%
39	7.243	1917	1929	1957	rBV	784851	1396708	72.17%	8.097%
40	7.551	2017	2025	2057	rBV	130897	244363	12.63%	1.417%
41	7.860	2119	2121	2123	rBV2	817	437	0.02%	0.003%
42	7.905	2133	2135	2140	rVB2	280	215	0.01%	0.001%
43	7.934	2142	2144	2145	rBV2	359	189	0.01%	0.001%
44	8.027	2159	2173	2212	rBV2	308277	718543	37.13%	4.165%
45	8.609	2352	2354	2357	rBV3	635	456	0.02%	0.003%
46	8.648	2363	2366	2368	rBV	289	173	0.01%	0.001%
47	8.670	2371	2373	2374	rBV	374	138	0.01%	0.001%
48	8.783	2397	2408	2444	rBV2	757002	1738233	89.82%	10.077%
49	9.165	2523	2527	2530	rBV4	425	390	0.02%	0.002%
50	9.365	2587	2589	2593	rBV3	475	335	0.02%	0.002%
51	9.410	2598	2603	2606	rBV2	510	486	0.03%	0.003%
52	9.497	2628	2630	2635	rVB2	495	349	0.02%	0.002%
53	9.519	2635	2637	2639	rBV3	386	178	0.01%	0.001%
54	9.558	2645	2649	2650	rBV	582	349	0.02%	0.002%
55	9.603	2662	2663	2666	rBV	201	122	0.01%	0.001%
56	9.625	2666	2670	2671	rVV2	345	186	0.01%	0.001%
57	9.638	2672	2674	2680	rVB	552	452	0.02%	0.003%
58	9.674	2682	2685	2686	rBV2	488	281	0.01%	0.002%
59	9.731	2700	2703	2707	rVB2	570	400	0.02%	0.002%
60	9.747	2707	2708	2710	rBV	248	131	0.01%	0.001%
61	9.760	2710	2712	2715	rVB2	479	169	0.01%	0.001%
62	9.796	2715	2723	2725	rVB3	434	482	0.02%	0.003%
63	9.815	2725	2729	2730	rBV	433	243	0.01%	0.001%
64	9.889	2750	2752	2754	rVB	501	185	0.01%	0.001%
65	9.905	2754	2757	2760	rBV2	422	362	0.02%	0.002%
66	10.008	2786	2789	2793	rBV	643	410	0.02%	0.002%
67	10.050	2800	2802	2806	rBV2	195	140	0.01%	0.001%
68	10.149	2821	2833	2862	rBV	511922	801932	41.44%	4.649%
69	10.403	2910	2912	2915	rBV3	389	190	0.01%	0.001%
70	10.419	2915	2917	2921	rVV3	590	412	0.02%	0.002%
71	10.484	2935	2937	2939	rBV3	417	170	0.01%	0.001%
72	10.497	2939	2941	2945	rVB3	542	367	0.02%	0.002%
73	10.516	2945	2947	2952	rVB4	538	374	0.02%	0.002%
74	10.545	2952	2956	2959	rBV2	427	315	0.02%	0.002%
75	10.561	2959	2961	2965	rVB3	540	292	0.02%	0.002%
76	10.593	2968	2971	2976	rBV2	409	314	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035026.D
 Acq On : 06 Apr 2024 00:16
 Operator : SY/MD
 Sample : P2006-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.619	2976	2979	2980	rBV2	402	204	0.01%	0.001%
78	10.767	3022	3025	3028	rVB2	326	171	0.01%	0.001%
79	10.783	3028	3030	3036	rVB3	634	521	0.03%	0.003%
80	10.828	3041	3044	3047	rVB2	407	195	0.01%	0.001%
81	10.873	3056	3058	3064	rVB4	394	367	0.02%	0.002%
82	10.902	3064	3067	3068	rBV	204	116	0.01%	0.001%
83	10.947	3078	3081	3082	rBV2	193	125	0.01%	0.001%
84	11.120	3126	3135	3145	rBV2	49322	81805	4.23%	0.474%
85	11.185	3145	3155	3188	rVB2	754721	1935326	100.00%	11.219%
86	11.561	3261	3272	3298	rVB2	831941	1838279	94.99%	10.657%
87	11.979	3399	3402	3403	rBV2	541	316	0.02%	0.002%
88	12.069	3428	3430	3433	rVB2	673	361	0.02%	0.002%
89	12.088	3433	3436	3437	rBV	248	151	0.01%	0.001%
90	12.310	3503	3505	3507	rBV2	386	123	0.01%	0.001%
91	12.345	3508	3516	3529	rVB9	3503	6977	0.36%	0.040%
92	12.693	3617	3624	3632	rBV7	2311	3385	0.17%	0.020%
93	12.841	3668	3670	3673	rBV	424	272	0.01%	0.002%
94	12.870	3678	3679	3681	rVB	395	137	0.01%	0.001%
95	12.988	3711	3716	3721	rBV3	627	713	0.04%	0.004%
96	13.050	3732	3735	3740	rVB3	658	453	0.02%	0.003%
97	13.194	3765	3780	3808	rBV	843764	1312384	67.81%	7.608%
98	13.677	3919	3930	3949	rBV	309290	492570	25.45%	2.855%
99	14.757	4253	4266	4281	rVB2	37323	69307	3.58%	0.402%
100	15.332	4434	4445	4464	rBV	176668	287370	14.85%	1.666%




Sum of corrected areas: 17249899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035026.D
Acq On : 06 Apr 2024 00:16
Operator : SY/MD
Sample : P2006-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

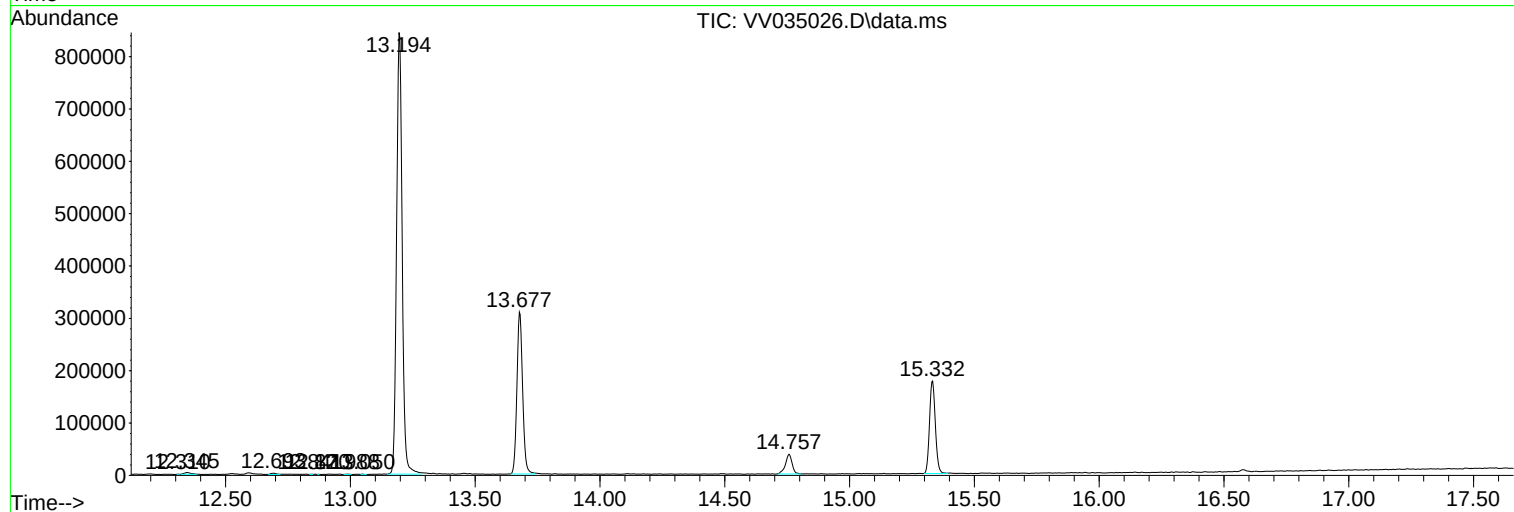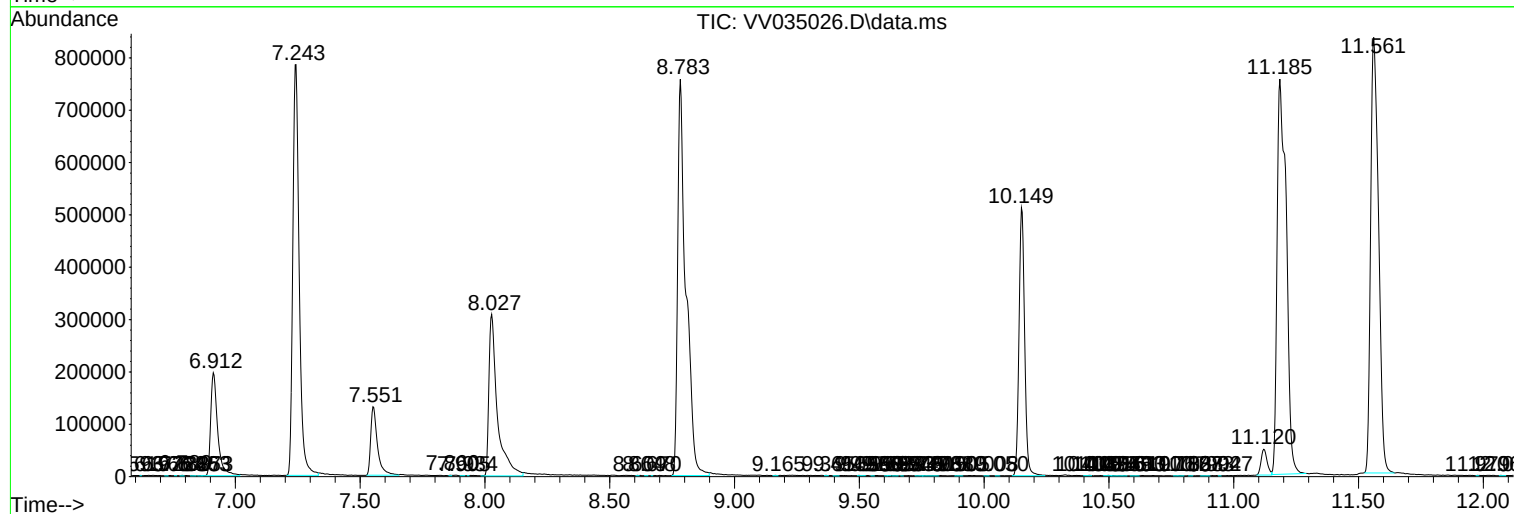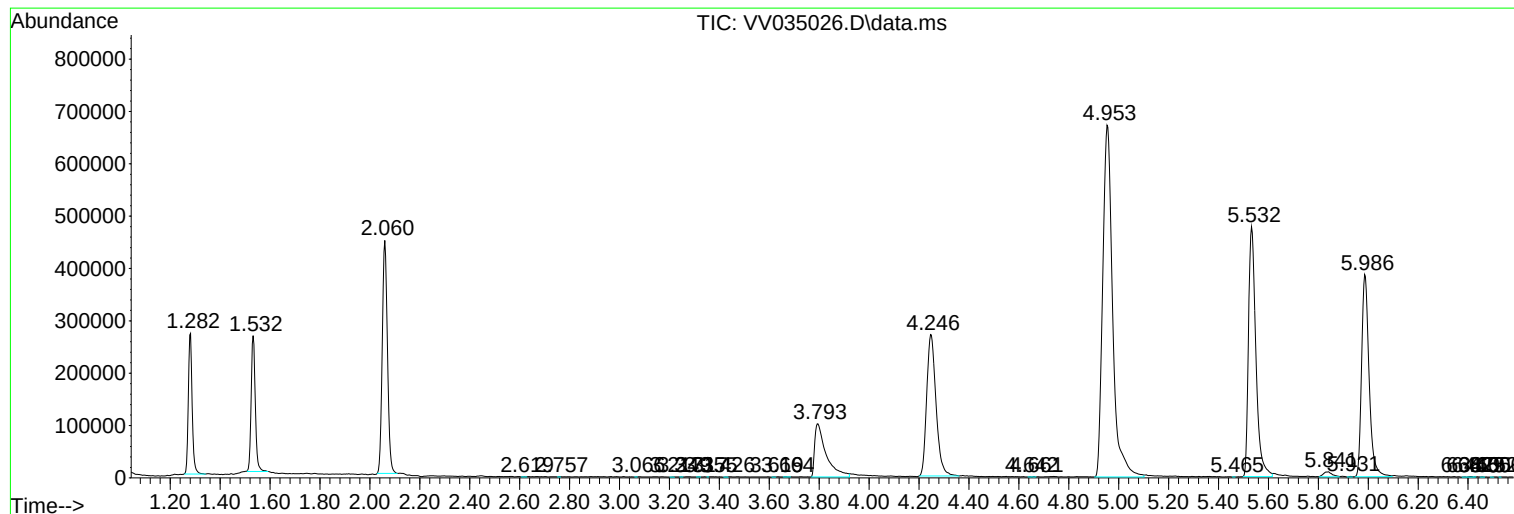

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035026.D
Acq On : 06 Apr 2024 00:16
Operator : SY/MD
Sample : P2006-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035026.D
Acq On : 06 Apr 2024 00:16
Operator : SY/MD
Sample : P2006-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------