

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035028.D
 Acq On : 06 Apr 2024 01:03
 Operator : SY/MD
 Sample : P2006-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	50	54	59	rBV6	3168	4416	0.16%	0.021%
2	1.278	68	74	93	rVB	277229	295525	10.45%	1.412%
3	1.532	146	153	164	rBV	254491	286889	10.14%	1.371%
4	2.059	307	317	344	rVB	463512	686154	24.26%	3.279%
5	2.452	434	439	444	rBV5	1203	1180	0.04%	0.006%
6	2.558	469	472	479	rBV5	644	661	0.02%	0.003%
7	2.609	485	488	492	rBV5	586	546	0.02%	0.003%
8	2.686	509	512	515	rVB	583	403	0.01%	0.002%
9	2.873	566	570	575	rVB4	764	716	0.03%	0.003%
10	3.149	653	656	660	rBV3	602	409	0.01%	0.002%
11	3.201	668	672	677	rVB3	390	450	0.02%	0.002%
12	3.227	677	680	683	rBV3	616	389	0.01%	0.002%
13	3.461	746	753	757	rBV3	566	819	0.03%	0.004%
14	3.712	829	831	837	rVB3	571	366	0.01%	0.002%
15	3.793	848	856	901	rBV	112293	353370	12.49%	1.689%
16	4.246	982	997	1036	rBV	275705	720600	25.48%	3.443%
17	4.493	1070	1074	1076	rBV4	675	476	0.02%	0.002%
18	4.657	1123	1125	1134	rVB4	530	655	0.02%	0.003%
19	4.722	1142	1145	1147	rBV2	892	618	0.02%	0.003%
20	4.815	1169	1174	1179	rVB5	651	530	0.02%	0.003%
21	4.956	1201	1218	1277	rBV2	691805	1964800	69.46%	9.388%
22	5.252	1307	1310	1317	rBV8	537	545	0.02%	0.003%
23	5.419	1359	1362	1365	rBV4	515	377	0.01%	0.002%
24	5.532	1381	1397	1430	rBV	497886	1046315	36.99%	5.000%
25	5.738	1458	1461	1464	rBV3	867	520	0.02%	0.002%
26	5.834	1481	1491	1504	rBV5	8871	19106	0.68%	0.091%
27	5.940	1518	1524	1526	rBV4	794	735	0.03%	0.004%
28	5.985	1526	1538	1571	rVV	397788	821643	29.05%	3.926%
29	6.133	1581	1584	1586	rBV4	787	510	0.02%	0.002%
30	6.214	1607	1609	1613	rVB4	889	508	0.02%	0.002%
31	6.288	1630	1632	1638	rVB3	525	429	0.02%	0.002%
32	6.352	1650	1652	1656	rVB4	959	565	0.02%	0.003%
33	6.381	1656	1661	1664	rBV4	563	534	0.02%	0.003%
34	6.448	1678	1682	1687	rVB3	656	595	0.02%	0.003%
35	6.635	1738	1740	1744	rVV5	624	446	0.02%	0.002%
36	6.657	1744	1747	1751	rVV4	631	564	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035028.D
 Acq On : 06 Apr 2024 01:03
 Operator : SY/MD
 Sample : P2006-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.690	1754	1757	1762	rVB4	659	480	0.02%	0.002%
38	6.796	1784	1790	1793	rBV3	520	574	0.02%	0.003%
39	6.911	1814	1826	1854	rBV	197784	391512	13.84%	1.871%
40	7.146	1897	1899	1903	rVB3	742	455	0.02%	0.002%
41	7.243	1917	1929	1956	rBV	808817	1436339	50.78%	6.863%
42	7.551	2016	2025	2052	rVV	131300	252098	8.91%	1.205%
43	7.738	2080	2083	2087	rVB5	1043	727	0.03%	0.003%
44	7.947	2142	2148	2149	rBV2	432	385	0.01%	0.002%
45	8.027	2162	2173	2220	rBV2	340029	793346	28.05%	3.791%
46	8.590	2344	2348	2353	rBV3	484	483	0.02%	0.002%
47	8.783	2396	2408	2413	rBV	806777	1284449	45.41%	6.137%
48	9.075	2494	2499	2504	rVB6	638	684	0.02%	0.003%
49	9.381	2591	2594	2600	rVB4	651	545	0.02%	0.003%
50	9.812	2725	2728	2732	rVB3	571	391	0.01%	0.002%
51	9.863	2741	2744	2746	rBV3	675	415	0.01%	0.002%
52	9.905	2754	2757	2760	rBV2	452	398	0.01%	0.002%
53	10.056	2802	2804	2808	rVB3	585	402	0.01%	0.002%
54	10.149	2821	2833	2862	rVV	531255	838313	29.64%	4.006%
55	10.490	2936	2939	2943	rVB3	609	441	0.02%	0.002%
56	10.660	2988	2992	2993	rBV2	662	415	0.01%	0.002%
57	10.705	3001	3006	3013	rVB4	625	761	0.03%	0.004%
58	10.744	3013	3018	3025	rBV2	585	758	0.03%	0.004%
59	10.895	3063	3065	3068	rVB3	821	368	0.01%	0.002%
60	10.931	3068	3076	3077	rBV4	929	991	0.04%	0.005%
61	10.982	3089	3092	3096	rBV3	1266	1018	0.04%	0.005%
62	11.004	3096	3099	3104	rVV5	640	654	0.02%	0.003%
63	11.120	3124	3135	3145	rBV	114293	188031	6.65%	0.898%
64	11.204	3145	3161	3188	rVB2	1142427	2814876	99.51%	13.450%
65	11.574	3261	3276	3300	rVB2	1238014	2828596	100.00%	13.516%
66	12.046	3420	3423	3425	rBV3	653	411	0.01%	0.002%
67	12.114	3439	3444	3450	rBV5	970	1143	0.04%	0.005%
68	12.159	3455	3458	3461	rBV3	638	481	0.02%	0.002%
69	12.204	3470	3472	3479	rVB4	1180	1081	0.04%	0.005%
70	12.239	3479	3483	3484	rBV3	963	601	0.02%	0.003%
71	12.297	3496	3501	3505	rBV4	692	684	0.02%	0.003%
72	12.339	3507	3514	3524	rVV6	4566	7212	0.25%	0.034%
73	12.406	3532	3535	3540	rBV5	513	420	0.01%	0.002%
74	12.490	3557	3561	3563	rBV2	496	432	0.02%	0.002%
75	12.512	3564	3568	3571	rBV4	1731	1572	0.06%	0.008%
76	12.586	3583	3591	3604	rBV5	5978	12234	0.43%	0.058%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035028.D
 Acq On : 06 Apr 2024 01:03
 Operator : SY/MD
 Sample : P2006-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.689	3614	3623	3634	rVB8	3355	6542	0.23%	0.031%
78	12.744	3637	3640	3642	rBV3	647	392	0.01%	0.002%
79	12.921	3690	3695	3696	rBV2	479	365	0.01%	0.002%
80	12.975	3707	3712	3716	rVB4	688	726	0.03%	0.003%
81	13.030	3723	3729	3732	rBV5	543	593	0.02%	0.003%
82	13.194	3764	3780	3809	rBV	1508192	2279363	80.58%	10.891%
83	13.458	3855	3862	3871	rVV5	1608	2496	0.09%	0.012%
84	13.496	3871	3874	3878	rVB5	716	481	0.02%	0.002%
85	13.596	3902	3905	3908	rBV3	874	687	0.02%	0.003%
86	13.680	3919	3931	3949	rBV	578685	916304	32.39%	4.378%
87	14.098	4053	4061	4077	rVB6	6290	13328	0.47%	0.064%
88	14.281	4116	4118	4121	rBV3	486	375	0.01%	0.002%
89	14.297	4121	4123	4127	rVV3	651	495	0.02%	0.002%
90	14.384	4145	4150	4151	rBV2	615	459	0.02%	0.002%
91	14.416	4156	4160	4164	rVB6	1185	1178	0.04%	0.006%
92	14.657	4228	4235	4239	rBV3	601	770	0.03%	0.004%
93	14.673	4239	4240	4245	rBV3	697	478	0.02%	0.002%
94	14.757	4250	4266	4278	rBV	67399	123709	4.37%	0.591%
95	14.969	4329	4332	4336	rVB5	902	673	0.02%	0.003%
96	15.062	4359	4361	4365	rVB3	748	439	0.02%	0.002%
97	15.271	4424	4426	4432	rVB3	908	745	0.03%	0.004%
98	15.332	4434	4445	4462	rVV	308718	496947	17.57%	2.375%
99	15.474	4487	4489	4496	rBV6	1146	1168	0.04%	0.006%
100	15.589	4522	4525	4527	rBV2	1027	747	0.03%	0.004%




Sum of corrected areas: 20928000

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035028.D
Acq On : 06 Apr 2024 01:03
Operator : SY/MD
Sample : P2006-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

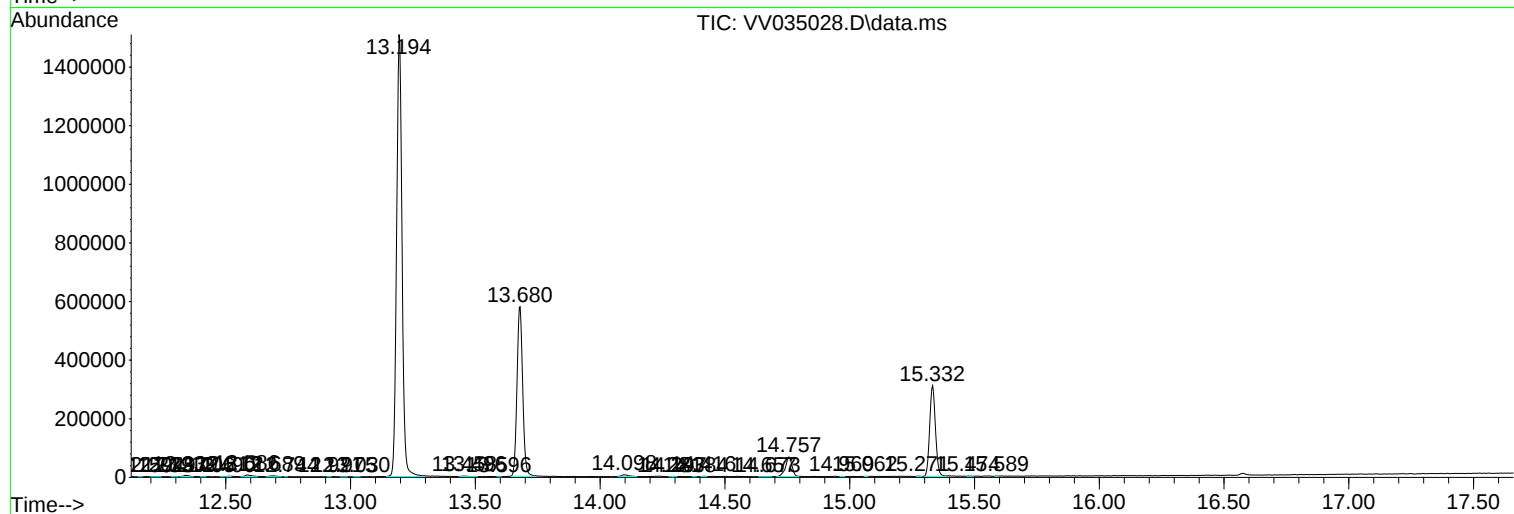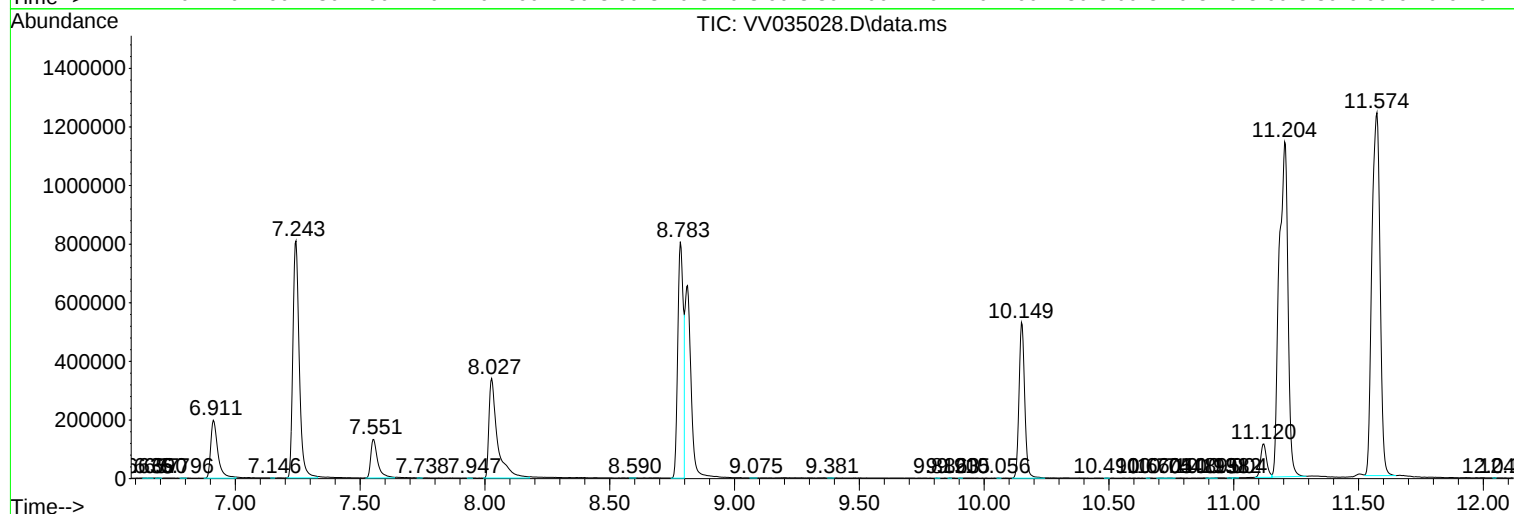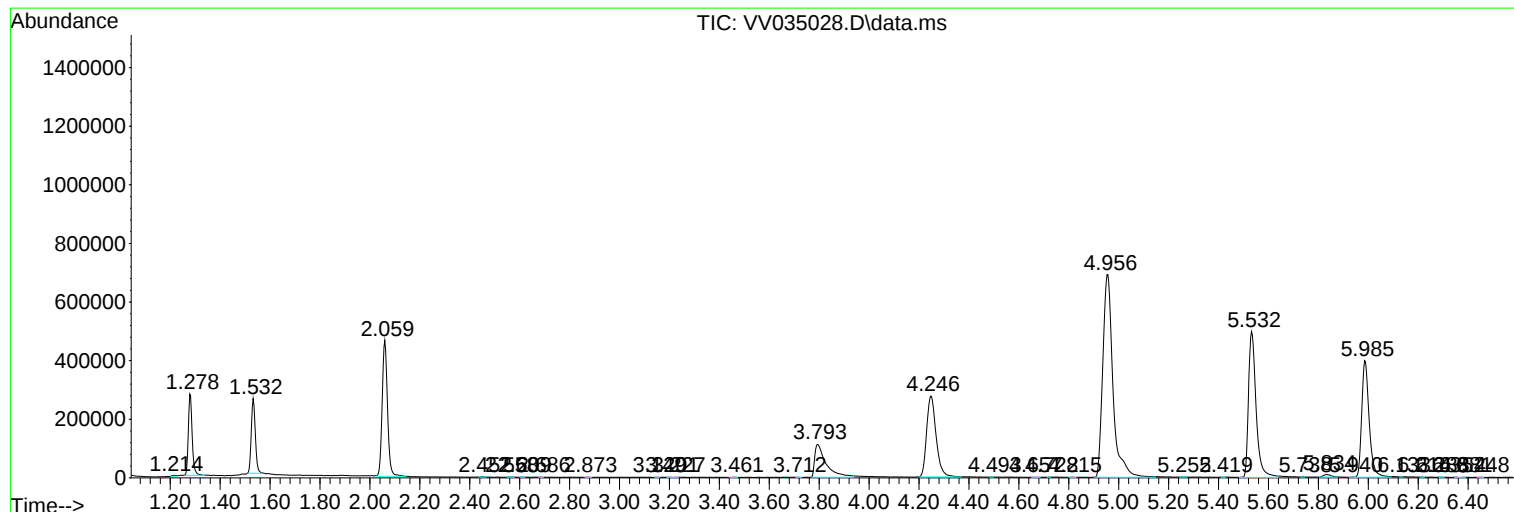

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035028.D
Acq On : 06 Apr 2024 01:03
Operator : SY/MD
Sample : P2006-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035028.D
Acq On : 06 Apr 2024 01:03
Operator : SY/MD
Sample : P2006-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------