

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035029.D
 Acq On : 06 Apr 2024 01:27
 Operator : SY/MD
 Sample : P2009-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	65	rBV2	6555	6913	0.36%	0.043%
2	1.281	67	75	91	rVB	290993	312174	16.20%	1.964%
3	1.532	146	153	169	rVB	267210	305095	15.83%	1.919%
4	2.060	306	317	335	rBV	468197	683581	35.47%	4.300%
5	2.349	405	407	413	rVB4	569	369	0.02%	0.002%
6	2.452	433	439	447	rVB7	1629	2495	0.13%	0.016%
7	2.532	461	464	469	rVB4	880	625	0.03%	0.004%
8	2.690	509	513	514	rBV3	1183	786	0.04%	0.005%
9	2.706	515	518	525	rVB6	1848	2258	0.12%	0.014%
10	3.082	628	635	639	rVB4	533	664	0.03%	0.004%
11	3.224	677	679	692	rVB4	747	1307	0.07%	0.008%
12	3.281	692	697	699	rBV	748	637	0.03%	0.004%
13	3.445	744	748	751	rBV3	477	349	0.02%	0.002%
14	3.468	751	755	759	rVB4	443	406	0.02%	0.003%
15	3.497	759	764	766	rBV2	401	335	0.02%	0.002%
16	3.568	780	786	789	rBV3	309	334	0.02%	0.002%
17	3.799	845	858	896	rBV3	127980	449470	23.32%	2.828%
18	4.246	981	997	1031	rBV	282597	734319	38.10%	4.620%
19	4.561	1092	1095	1099	rBV3	565	429	0.02%	0.003%
20	4.587	1099	1103	1108	rBV4	650	754	0.04%	0.005%
21	4.735	1144	1149	1150	rBV3	767	532	0.03%	0.003%
22	4.786	1161	1165	1170	rBV4	937	878	0.05%	0.006%
23	4.953	1202	1217	1269	rBV2	709240	1927255	100.00%	12.124%
24	5.288	1319	1321	1326	rBV3	577	520	0.03%	0.003%
25	5.429	1361	1365	1370	rBV5	644	665	0.03%	0.004%
26	5.477	1374	1380	1382	rBV2	686	508	0.03%	0.003%
27	5.532	1386	1397	1436	rBV	480823	1004794	52.14%	6.321%
28	5.731	1457	1459	1462	rBV3	635	336	0.02%	0.002%
29	5.767	1468	1470	1474	rVB3	675	460	0.02%	0.003%
30	5.834	1481	1491	1510	rBV6	11566	27721	1.44%	0.174%
31	5.985	1525	1538	1569	rBV	403948	843059	43.74%	5.304%
32	6.214	1607	1609	1616	rVB4	671	610	0.03%	0.004%
33	6.252	1616	1621	1623	rBV2	679	538	0.03%	0.003%
34	6.326	1642	1644	1647	rVV2	405	314	0.02%	0.002%
35	6.368	1655	1657	1660	rBV2	627	339	0.02%	0.002%
36	6.471	1685	1689	1692	rVB2	607	479	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035029.D
 Acq On : 06 Apr 2024 01:27
 Operator : SY/MD
 Sample : P2009-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.603	1726	1730	1734	rBV4	577	531	0.03%	0.003%
38	6.731	1766	1770	1774	rVB3	586	565	0.03%	0.004%
39	6.818	1794	1797	1801	rBV3	439	362	0.02%	0.002%
40	6.911	1815	1826	1853	rBV	201589	390078	20.24%	2.454%
41	7.243	1917	1929	1964	rBV	819710	1458521	75.68%	9.175%
42	7.551	2015	2025	2052	rBV	137061	256664	13.32%	1.615%
43	7.776	2091	2095	2101	rBV5	860	898	0.05%	0.006%
44	7.876	2122	2126	2127	rVV3	488	349	0.02%	0.002%
45	7.911	2135	2137	2142	rVB3	591	339	0.02%	0.002%
46	8.027	2163	2173	2225	rBV3	339262	803482	41.69%	5.055%
47	8.445	2300	2303	2306	rBV4	724	509	0.03%	0.003%
48	8.619	2353	2357	2360	rVV4	735	576	0.03%	0.004%
49	8.783	2394	2408	2440	rBV2	736634	1565630	81.24%	9.849%
50	9.079	2497	2500	2504	rBV4	784	632	0.03%	0.004%
51	9.210	2533	2541	2543	rBV5	762	763	0.04%	0.005%
52	9.304	2565	2570	2571	rBV4	624	399	0.02%	0.003%
53	9.317	2571	2574	2576	rVB4	663	383	0.02%	0.002%
54	9.342	2579	2582	2584	rBV3	783	508	0.03%	0.003%
55	9.487	2623	2627	2628	rBV4	575	397	0.02%	0.002%
56	9.686	2686	2689	2693	rBV2	523	323	0.02%	0.002%
57	9.747	2706	2708	2711	rBV3	521	357	0.02%	0.002%
58	9.866	2740	2745	2747	rBV3	595	496	0.03%	0.003%
59	9.960	2769	2774	2778	rVB3	501	476	0.02%	0.003%
60	9.992	2778	2784	2789	rVB4	281	364	0.02%	0.002%
61	10.034	2794	2797	2801	rVB3	424	368	0.02%	0.002%
62	10.091	2813	2815	2820	rBV2	350	314	0.02%	0.002%
63	10.149	2820	2833	2852	rBV	534054	842220	43.70%	5.298%
64	10.243	2860	2862	2867	rVB4	894	599	0.03%	0.004%
65	10.381	2900	2905	2907	rBV4	419	329	0.02%	0.002%
66	10.661	2990	2992	2998	rVB4	360	394	0.02%	0.002%
67	10.940	3075	3079	3081	rBV3	399	372	0.02%	0.002%
68	11.030	3104	3107	3110	rBV3	430	347	0.02%	0.002%
69	11.066	3114	3118	3120	rBV3	578	399	0.02%	0.003%
70	11.124	3126	3136	3144	rBV	34668	57543	2.99%	0.362%
71	11.185	3144	3155	3185	rVB2	715900	1599861	83.01%	10.065%
72	11.561	3260	3272	3298	rBV3	817719	1629759	84.56%	10.253%
73	11.792	3342	3344	3346	rBV	790	370	0.02%	0.002%
74	11.805	3346	3348	3350	rVB3	824	392	0.02%	0.002%
75	11.898	3374	3377	3380	rVB5	748	471	0.02%	0.003%
76	11.915	3380	3382	3385	rBV	644	384	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035029.D
 Acq On : 06 Apr 2024 01:27
 Operator : SY/MD
 Sample : P2009-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.169	3458	3461	3464	rVB4	675	315	0.02%	0.002%
78	12.191	3464	3468	3473	rBV2	807	666	0.03%	0.004%
79	12.339	3509	3514	3515	rBV4	914	484	0.03%	0.003%
80	12.374	3523	3525	3528	rBV2	437	327	0.02%	0.002%
81	12.458	3546	3551	3554	rBV4	384	390	0.02%	0.002%
82	12.480	3554	3558	3561	rVB4	518	387	0.02%	0.002%
83	12.586	3586	3591	3593	rBV3	824	607	0.03%	0.004%
84	12.689	3621	3623	3627	rVB4	971	597	0.03%	0.004%
85	12.818	3659	3663	3666	rVB2	514	409	0.02%	0.003%
86	12.940	3699	3701	3706	rVB2	507	357	0.02%	0.002%
87	12.969	3706	3710	3714	rBV2	361	378	0.02%	0.002%
88	13.197	3767	3781	3804	rBV	354817	568266	29.49%	3.575%
89	13.410	3845	3847	3850	rBV3	639	358	0.02%	0.002%
90	13.451	3854	3860	3861	rBV4	785	784	0.04%	0.005%
91	13.516	3877	3880	3884	rVB4	405	324	0.02%	0.002%
92	13.638	3912	3918	3919	rBV3	652	532	0.03%	0.003%
93	13.680	3920	3931	3949	rVV	131030	213161	11.06%	1.341%
94	13.956	4015	4017	4019	rBV	648	333	0.02%	0.002%
95	14.059	4046	4049	4053	rVB3	483	324	0.02%	0.002%
96	14.107	4062	4064	4067	rBV3	684	389	0.02%	0.002%
97	14.574	4206	4209	4211	rBV3	661	369	0.02%	0.002%
98	14.760	4253	4267	4278	rBV3	15924	27602	1.43%	0.174%
99	15.201	4402	4404	4407	rVB4	645	318	0.02%	0.002%
100	15.332	4433	4445	4461	rBV2	90252	148329	7.70%	0.933%




Sum of corrected areas: 15896038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035029.D
Acq On : 06 Apr 2024 01:27
Operator : SY/MD
Sample : P2009-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

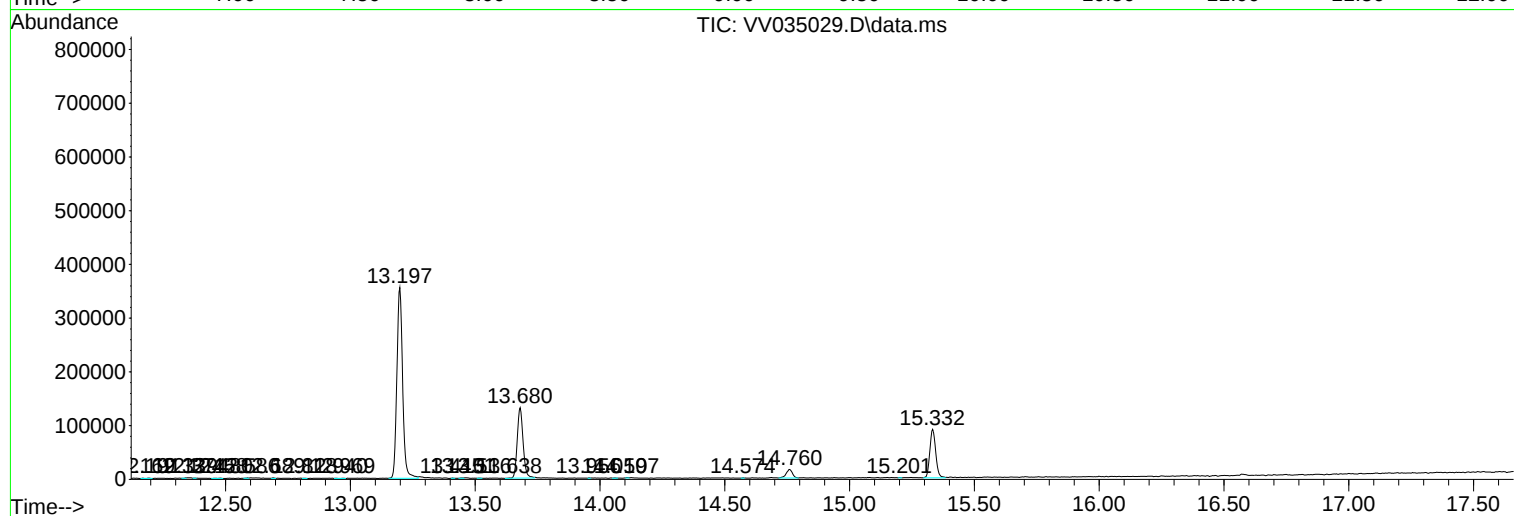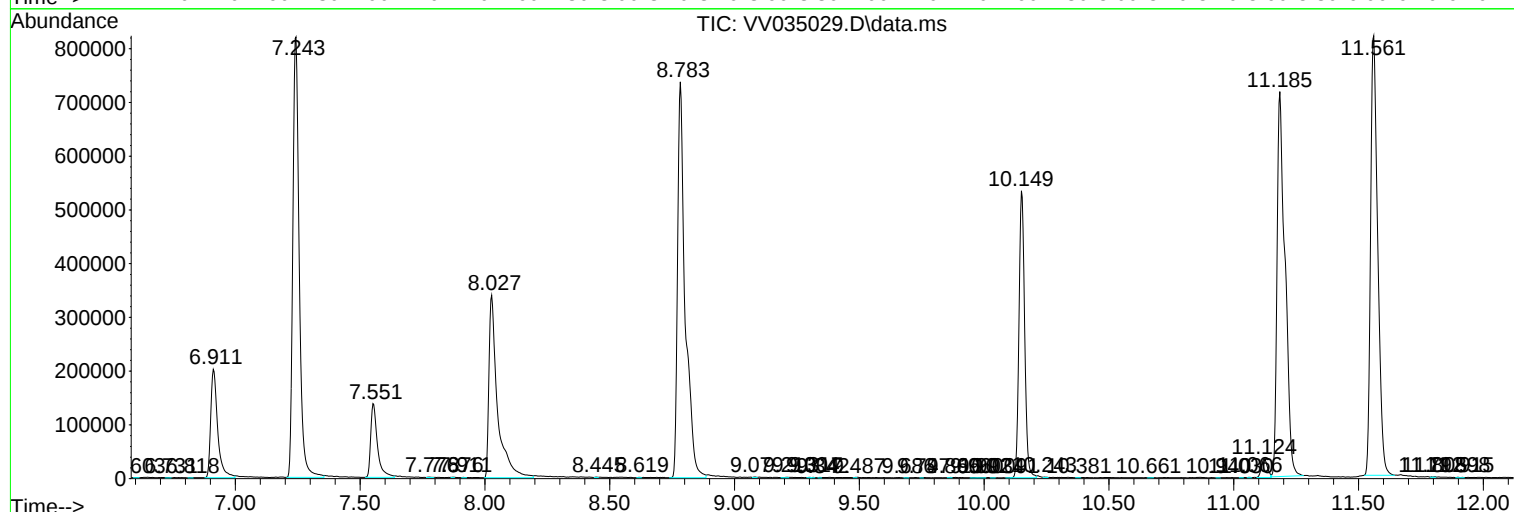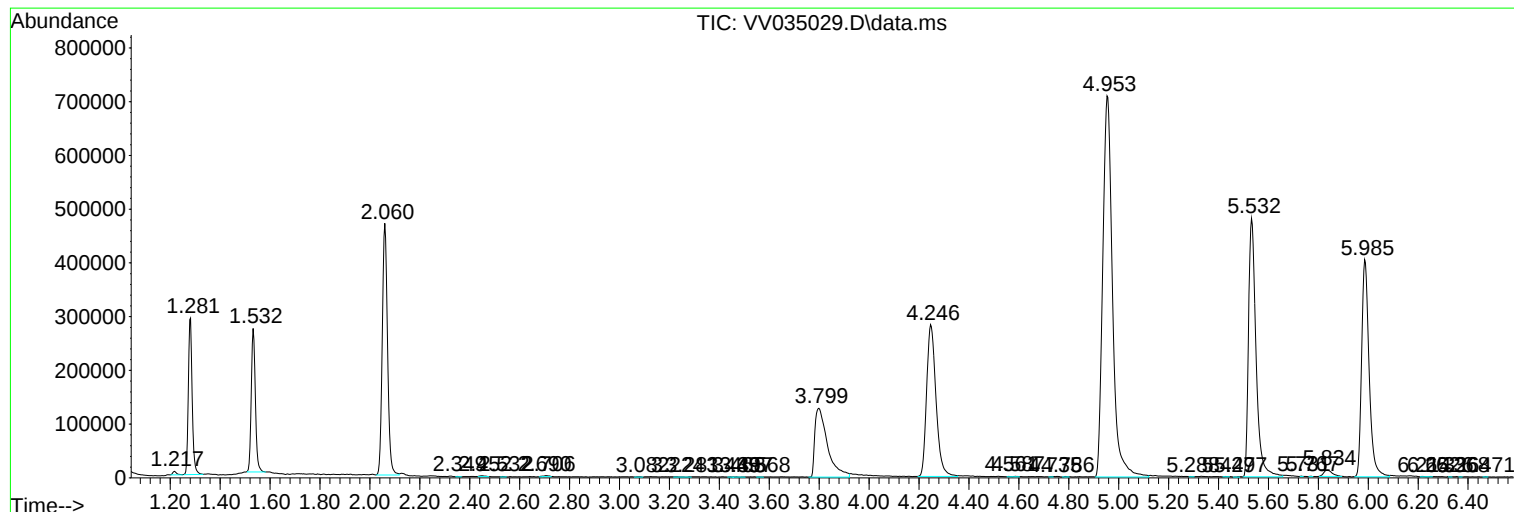

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035029.D
Acq On : 06 Apr 2024 01:27
Operator : SY/MD
Sample : P2009-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035029.D
Acq On : 06 Apr 2024 01:27
Operator : SY/MD
Sample : P2009-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc