

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035032.D
 Acq On : 06 Apr 2024 02:38
 Operator : SY/MD
 Sample : P2009-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	267782	287096	15.89%	1.942%
2	1.532	146	153	173	rVB	258563	298697	16.53%	2.021%
3	2.060	307	317	333	rBV	442246	640831	35.47%	4.336%
4	2.802	545	548	549	rBV2	544	275	0.02%	0.002%
5	2.954	593	595	597	rBV	475	310	0.02%	0.002%
6	3.092	637	638	642	rBV2	325	204	0.01%	0.001%
7	3.188	666	668	670	rBV	465	289	0.02%	0.002%
8	3.237	681	683	685	rBV2	462	178	0.01%	0.001%
9	3.249	685	687	689	rVV2	272	97	0.01%	0.001%
10	3.285	697	698	699	rBV2	152	43	0.00%	0.000%
11	3.298	699	702	706	rVV	323	285	0.02%	0.002%
12	3.327	709	711	712	rBV	183	58	0.00%	0.000%
13	3.397	731	733	736	rBV2	415	226	0.01%	0.002%
14	3.455	748	751	756	rBV3	429	379	0.02%	0.003%
15	3.526	770	773	778	rBV3	382	277	0.02%	0.002%
16	3.552	778	781	783	rVV3	325	190	0.01%	0.001%
17	3.709	827	830	834	rBV	279	207	0.01%	0.001%
18	3.732	834	837	838	rBV2	193	96	0.01%	0.001%
19	3.761	842	846	848	rBV2	371	252	0.01%	0.002%
20	3.793	848	856	893	rBV	108825	355795	19.69%	2.407%
21	4.246	983	997	1031	rBV	268547	693944	38.41%	4.695%
22	4.954	1201	1217	1253	rBV2	676425	1806628	100.00%	12.224%
23	5.532	1386	1397	1422	rBV	448837	931750	51.57%	6.304%
24	5.831	1476	1490	1524	rBV	739258	1507440	83.44%	10.199%
25	5.986	1527	1538	1570	rVB	387029	807735	44.71%	5.465%
26	6.310	1637	1639	1641	rBV2	400	141	0.01%	0.001%
27	6.397	1664	1666	1670	rVB2	267	151	0.01%	0.001%
28	6.423	1670	1674	1676	rBV4	517	350	0.02%	0.002%
29	6.436	1676	1678	1681	rBV3	339	239	0.01%	0.002%
30	6.532	1705	1708	1710	rBV3	360	264	0.01%	0.002%
31	6.603	1727	1730	1733	rBV2	589	420	0.02%	0.003%
32	6.783	1784	1786	1789	rVB2	318	167	0.01%	0.001%
33	6.812	1792	1795	1796	rBV	315	177	0.01%	0.001%
34	6.912	1815	1826	1859	rBV	193087	373347	20.67%	2.526%
35	7.146	1897	1899	1901	rBV2	892	476	0.03%	0.003%
36	7.240	1917	1928	1958	rBV	771275	1390352	76.96%	9.407%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035032.D
 Acq On : 06 Apr 2024 02:38
 Operator : SY/MD
 Sample : P2009-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	7.551	2016	2025	2058	rBV	129146	243946	13.50%	1.651%
38	7.915	2132	2138	2143	rVB6	1597	1936	0.11%	0.013%
39	8.027	2163	2173	2216	rBV3	307679	749954	41.51%	5.074%
40	8.728	2388	2391	2393	rBV2	656	468	0.03%	0.003%
41	8.783	2396	2408	2444	rBV	692092	1250450	69.21%	8.460%
42	9.076	2495	2499	2504	rBV4	785	679	0.04%	0.005%
43	9.233	2546	2548	2550	rBV3	555	283	0.02%	0.002%
44	9.301	2564	2569	2573	rBV3	558	482	0.03%	0.003%
45	9.442	2609	2613	2617	rBV3	466	488	0.03%	0.003%
46	9.532	2639	2641	2643	rBV	234	154	0.01%	0.001%
47	9.683	2686	2688	2692	rVB	577	357	0.02%	0.002%
48	9.712	2692	2697	2698	rBV2	415	295	0.02%	0.002%
49	9.831	2732	2734	2736	rVB2	305	104	0.01%	0.001%
50	9.902	2753	2756	2759	rBV3	503	327	0.02%	0.002%
51	9.931	2762	2765	2767	rBV	317	178	0.01%	0.001%
52	10.027	2792	2795	2796	rBV	303	139	0.01%	0.001%
53	10.149	2821	2833	2861	rBV	508477	805288	44.57%	5.449%
54	10.497	2938	2941	2945	rBV	610	490	0.03%	0.003%
55	10.584	2966	2968	2971	rVB2	537	263	0.01%	0.002%
56	10.625	2978	2981	2982	rBV2	647	297	0.02%	0.002%
57	10.709	3004	3007	3009	rBV	420	230	0.01%	0.002%
58	10.773	3024	3027	3028	rBV2	198	121	0.01%	0.001%
59	10.828	3042	3044	3045	rBV	322	128	0.01%	0.001%
60	10.854	3050	3052	3053	rBV	324	134	0.01%	0.001%
61	10.953	3081	3083	3091	rVB2	397	330	0.02%	0.002%
62	10.985	3091	3093	3095	rBV	294	126	0.01%	0.001%
63	11.085	3122	3124	3125	rBV	201	92	0.01%	0.001%
64	11.127	3129	3137	3144	rVV3	8538	14139	0.78%	0.096%
65	11.182	3144	3154	3183	rVV2	638255	1152666	63.80%	7.799%
66	11.558	3258	3271	3297	rBV	732499	1267923	70.18%	8.579%
67	11.792	3341	3344	3348	rBV5	699	576	0.03%	0.004%
68	11.892	3373	3375	3376	rBV2	509	153	0.01%	0.001%
69	12.130	3447	3449	3456	rBV3	513	461	0.03%	0.003%
70	12.172	3456	3462	3465	rBV3	497	605	0.03%	0.004%
71	12.191	3465	3468	3472	rBV4	509	548	0.03%	0.004%
72	12.345	3513	3516	3523	rVB4	515	474	0.03%	0.003%
73	12.436	3541	3544	3548	rBV2	412	350	0.02%	0.002%
74	12.458	3548	3551	3558	rVB4	630	598	0.03%	0.004%
75	12.538	3572	3576	3577	rBV2	403	210	0.01%	0.001%
76	12.599	3590	3595	3597	rBV2	558	439	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035032.D
 Acq On : 06 Apr 2024 02:38
 Operator : SY/MD
 Sample : P2009-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	12.616	3598	3600	3603	rVV	670	372	0.02%	0.003%
78	12.635	3603	3606	3609	rVV2	420	218	0.01%	0.001%
79	12.696	3623	3625	3628	rBV2	446	287	0.02%	0.002%
80	12.847	3671	3672	3676	rBV	280	151	0.01%	0.001%
81	12.876	3678	3681	3684	rVB2	451	320	0.02%	0.002%
82	13.085	3743	3746	3749	rBV2	579	437	0.02%	0.003%
83	13.201	3772	3782	3798	rBV	73967	122298	6.77%	0.827%
84	13.683	3923	3932	3953	rVB3	21949	36826	2.04%	0.249%
85	15.336	4438	4446	4457	rBV2	14532	22723	1.26%	0.154%




Sum of corrected areas: 14779879

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035032.D
Acq On : 06 Apr 2024 02:38
Operator : SY/MD
Sample : P2009-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

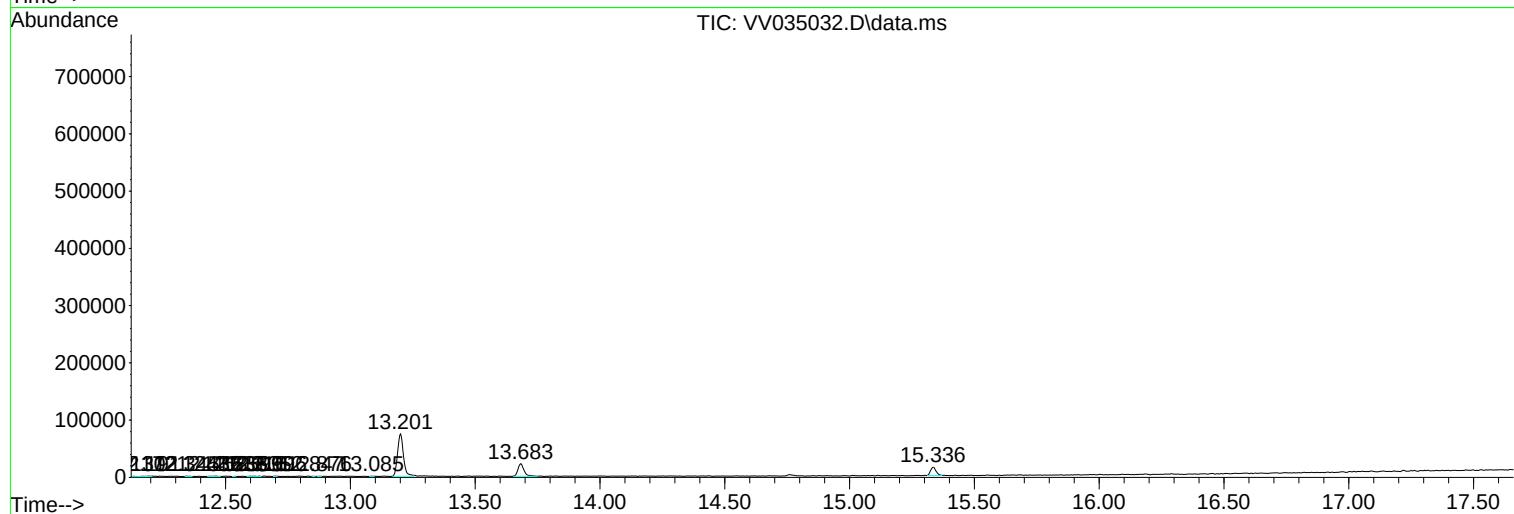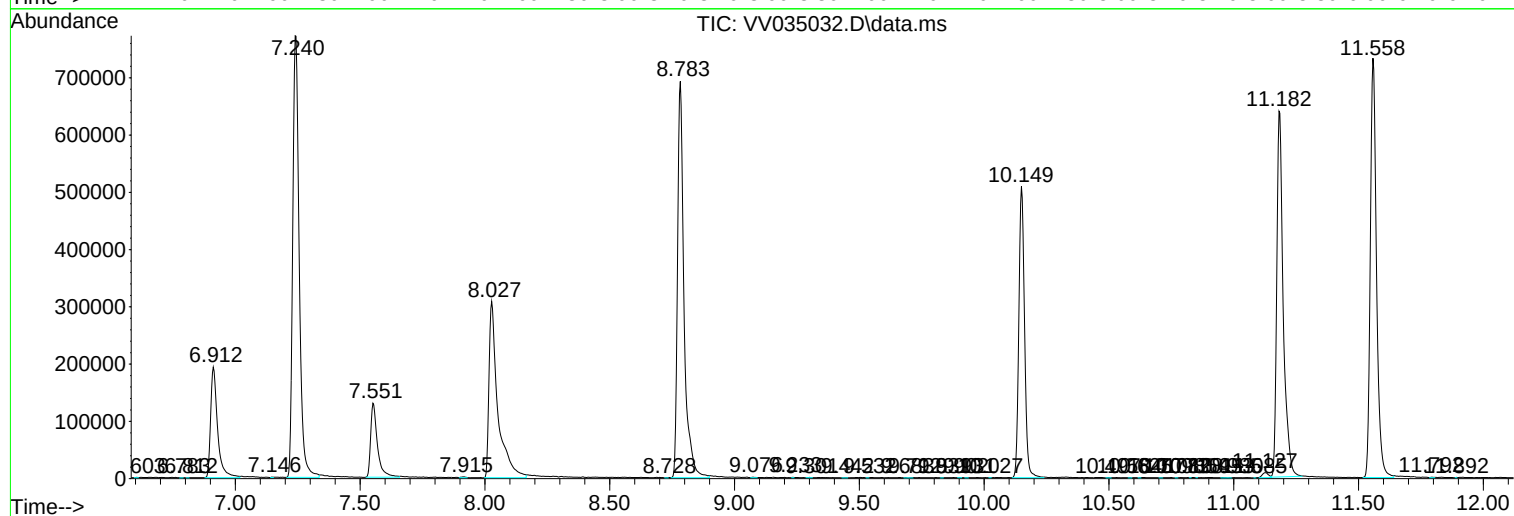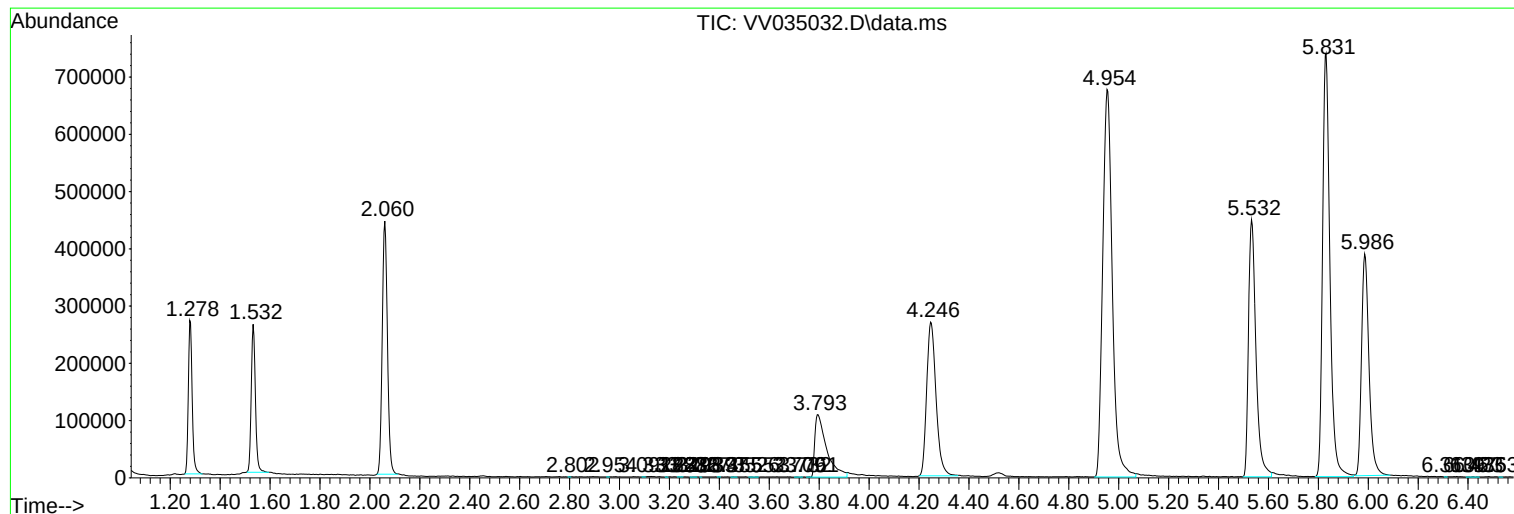

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035032.D
Acq On : 06 Apr 2024 02:38
Operator : SY/MD
Sample : P2009-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035032.D
Acq On : 06 Apr 2024 02:38
Operator : SY/MD
Sample : P2009-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
