

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035033.D
 Acq On : 06 Apr 2024 03:02
 Operator : SY/MD
 Sample : P2009-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	91	rVB	272242	286818	15.91%	2.161%
2	1.532	146	153	174	rVB	257225	297916	16.53%	2.244%
3	2.060	307	317	334	rBV	439273	636560	35.32%	4.795%
4	2.593	480	483	485	rBV2	435	308	0.02%	0.002%
5	2.850	560	563	565	rBV2	397	265	0.01%	0.002%
6	3.156	656	658	661	rBV2	316	251	0.01%	0.002%
7	3.323	708	710	712	rBV2	311	134	0.01%	0.001%
8	3.497	762	764	769	rVB	299	159	0.01%	0.001%
9	3.526	769	773	776	rBV2	577	573	0.03%	0.004%
10	3.577	785	789	791	rBV3	252	175	0.01%	0.001%
11	3.632	802	806	808	rBV3	508	380	0.02%	0.003%
12	3.735	833	838	842	rBV2	532	479	0.03%	0.004%
13	3.754	842	844	848	rBV2	218	156	0.01%	0.001%
14	3.793	848	856	886	rBV	110441	332114	18.43%	2.502%
15	4.246	983	997	1025	rBV	266441	686239	38.08%	5.170%
16	4.703	1136	1139	1141	rBV3	340	204	0.01%	0.002%
17	4.715	1141	1143	1145	rBV2	326	140	0.01%	0.001%
18	4.764	1155	1158	1160	rBV3	490	238	0.01%	0.002%
19	4.873	1190	1192	1196	rVB3	537	364	0.02%	0.003%
20	4.895	1196	1199	1202	rBV2	548	511	0.03%	0.004%
21	4.953	1202	1217	1263	rBV2	672079	1802310	100.00%	13.578%
22	5.429	1363	1365	1370	rVB3	639	500	0.03%	0.004%
23	5.532	1386	1397	1436	rBV	460929	958431	53.18%	7.220%
24	5.838	1479	1492	1519	rBV5	60779	147669	8.19%	1.112%
25	5.985	1525	1538	1567	rBV	384277	806081	44.72%	6.073%
26	6.442	1677	1680	1682	rBV2	635	385	0.02%	0.003%
27	6.503	1697	1699	1704	rVB3	632	379	0.02%	0.003%
28	6.526	1704	1706	1707	rVB3	288	93	0.01%	0.001%
29	6.535	1707	1709	1712	rVB	203	96	0.01%	0.001%
30	6.600	1724	1729	1732	rBV2	462	373	0.02%	0.003%
31	6.616	1732	1734	1735	rBV	429	199	0.01%	0.001%
32	6.651	1743	1745	1748	rVB3	537	225	0.01%	0.002%
33	6.667	1748	1750	1753	rBV2	348	216	0.01%	0.002%
34	6.693	1756	1758	1759	rBV2	344	151	0.01%	0.001%
35	6.715	1763	1765	1769	rBV3	441	368	0.02%	0.003%
36	6.841	1802	1804	1807	rVB	464	229	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035033.D
 Acq On : 06 Apr 2024 03:02
 Operator : SY/MD
 Sample : P2009-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.857	1807	1809	1812	rBV2	316	173	0.01%	0.001%
38	6.911	1814	1826	1854	rBV	190812	367212	20.37%	2.766%
39	7.243	1918	1929	1967	rBV	764437	1372259	76.14%	10.338%
40	7.551	2016	2025	2051	rBV	126431	239320	13.28%	1.803%
41	7.944	2144	2147	2148	rBV2	315	183	0.01%	0.001%
42	7.953	2148	2150	2152	rVB2	517	208	0.01%	0.002%
43	8.027	2164	2173	2224	rBV3	318404	778703	43.21%	5.866%
44	8.490	2315	2317	2323	rBV5	683	526	0.03%	0.004%
45	8.554	2332	2337	2343	rVB5	1033	1037	0.06%	0.008%
46	8.580	2343	2345	2347	rVB2	662	319	0.02%	0.002%
47	8.596	2347	2350	2354	rBV3	791	594	0.03%	0.004%
48	8.696	2379	2381	2382	rBV2	390	133	0.01%	0.001%
49	8.783	2397	2408	2441	rBV	700672	1246790	69.18%	9.393%
50	9.107	2507	2509	2510	rBV	277	150	0.01%	0.001%
51	9.117	2510	2512	2518	rVV3	1213	833	0.05%	0.006%
52	9.271	2556	2560	2564	rBV3	784	635	0.04%	0.005%
53	9.336	2577	2580	2582	rBV3	373	221	0.01%	0.002%
54	9.384	2593	2595	2596	rBV3	374	161	0.01%	0.001%
55	9.419	2602	2606	2609	rBV2	225	195	0.01%	0.001%
56	9.564	2648	2651	2652	rBV2	199	113	0.01%	0.001%
57	9.574	2652	2654	2657	rVB2	463	258	0.01%	0.002%
58	9.638	2671	2674	2676	rBV	367	181	0.01%	0.001%
59	9.661	2678	2681	2683	rBV2	355	167	0.01%	0.001%
60	9.680	2683	2687	2688	rBV3	239	119	0.01%	0.001%
61	9.689	2688	2690	2693	rVB	281	128	0.01%	0.001%
62	9.709	2693	2696	2701	rBV4	666	641	0.04%	0.005%
63	9.767	2711	2714	2717	rBV3	499	351	0.02%	0.003%
64	9.802	2722	2725	2727	rBV2	420	242	0.01%	0.002%
65	9.847	2737	2739	2743	rBV	374	230	0.01%	0.002%
66	9.905	2754	2757	2760	rBV	596	417	0.02%	0.003%
67	9.927	2760	2764	2766	rBV2	277	202	0.01%	0.002%
68	9.940	2766	2768	2772	rVV2	474	321	0.02%	0.002%
69	9.979	2778	2780	2781	rBV	218	108	0.01%	0.001%
70	10.056	2800	2804	2810	rBV3	622	716	0.04%	0.005%
71	10.082	2810	2812	2813	rBV	300	101	0.01%	0.001%
72	10.149	2818	2833	2856	rBV	517167	807693	44.81%	6.085%
73	10.419	2915	2917	2918	rBV	374	129	0.01%	0.001%
74	10.429	2918	2920	2921	rBV	276	150	0.01%	0.001%
75	10.493	2937	2940	2943	rBV3	257	264	0.01%	0.002%
76	10.532	2950	2952	2959	rVB3	613	557	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035033.D
 Acq On : 06 Apr 2024 03:02
 Operator : SY/MD
 Sample : P2009-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.564	2959	2962	2965	rBV2	387	256	0.01%	0.002%
78	10.773	3023	3027	3029	rBV2	437	398	0.02%	0.003%
79	11.005	3094	3099	3101	rBV2	405	363	0.02%	0.003%
80	11.027	3104	3106	3107	rBV2	310	125	0.01%	0.001%
81	11.088	3123	3125	3128	rVB3	386	207	0.01%	0.002%
82	11.130	3128	3138	3144	rBV6	7103	11790	0.65%	0.089%
83	11.185	3144	3155	3185	rVV	649312	1130435	62.72%	8.516%
84	11.468	3238	3243	3246	rBV3	446	363	0.02%	0.003%
85	11.558	3259	3271	3297	rBV	717277	1218979	67.63%	9.183%
86	11.937	3387	3389	3391	rBV2	349	174	0.01%	0.001%
87	12.098	3434	3439	3441	rBV3	413	427	0.02%	0.003%
88	12.307	3498	3504	3507	rBV3	698	825	0.05%	0.006%
89	12.329	3507	3511	3515	rVV2	509	468	0.03%	0.004%
90	12.429	3540	3542	3545	rBV3	470	284	0.02%	0.002%
91	12.467	3552	3554	3557	rBV2	482	261	0.01%	0.002%
92	12.541	3573	3577	3581	rBV2	557	535	0.03%	0.004%
93	12.586	3588	3591	3594	rBV2	405	320	0.02%	0.002%
94	12.837	3662	3669	3674	rBV3	459	702	0.04%	0.005%
95	12.873	3678	3680	3683	rVB3	280	101	0.01%	0.001%
96	12.908	3687	3691	3696	rBV2	540	542	0.03%	0.004%
97	13.146	3762	3765	3767	rVB3	413	223	0.01%	0.002%
98	13.201	3767	3782	3798	rBV2	56392	95034	5.27%	0.716%
99	13.638	3916	3918	3922	rBV2	384	286	0.02%	0.002%
100	13.683	3923	3932	3945	rVV3	16468	26696	1.48%	0.201%




Sum of corrected areas: 13274223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035033.D
Acq On : 06 Apr 2024 03:02
Operator : SY/MD
Sample : P2009-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

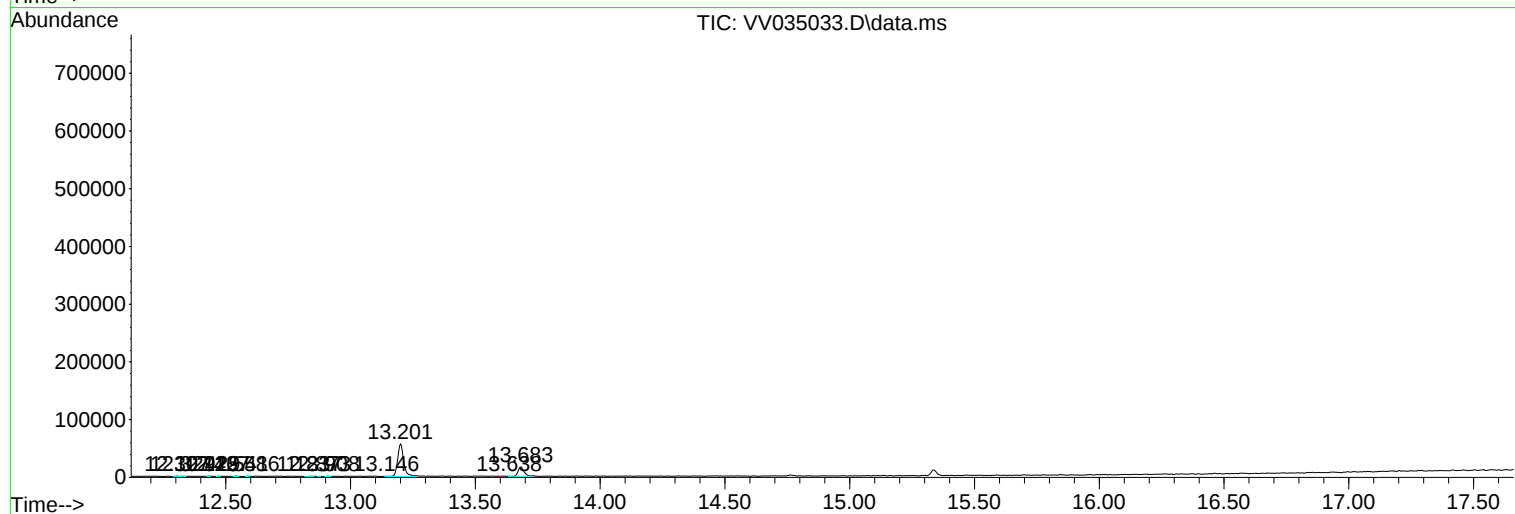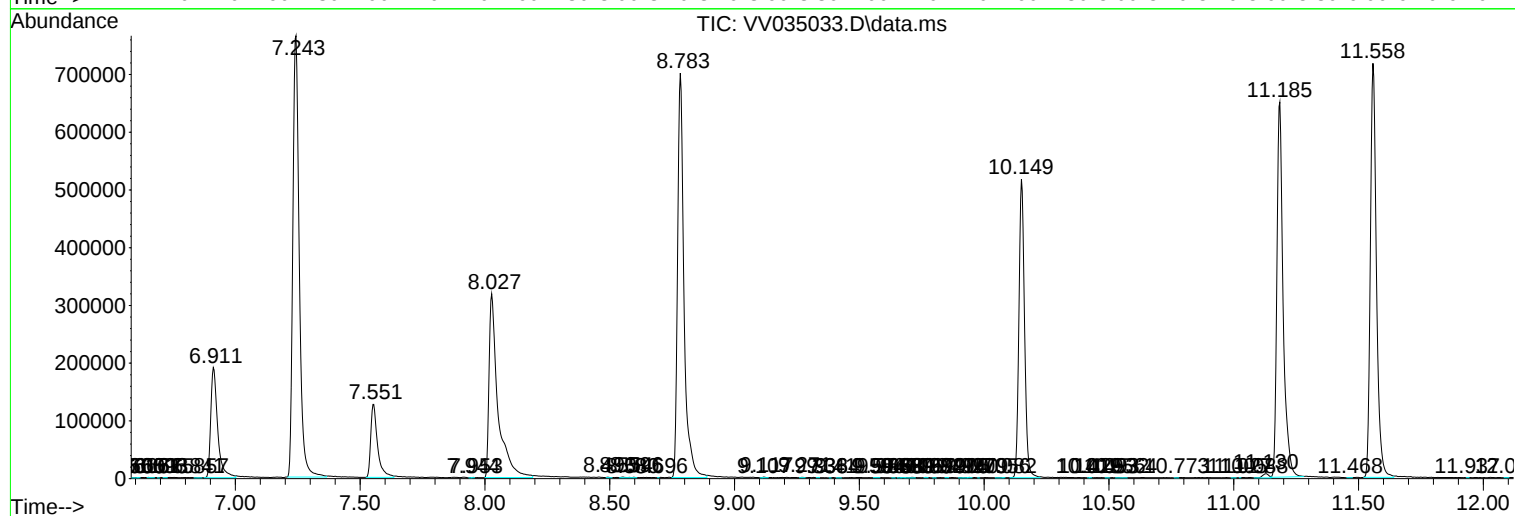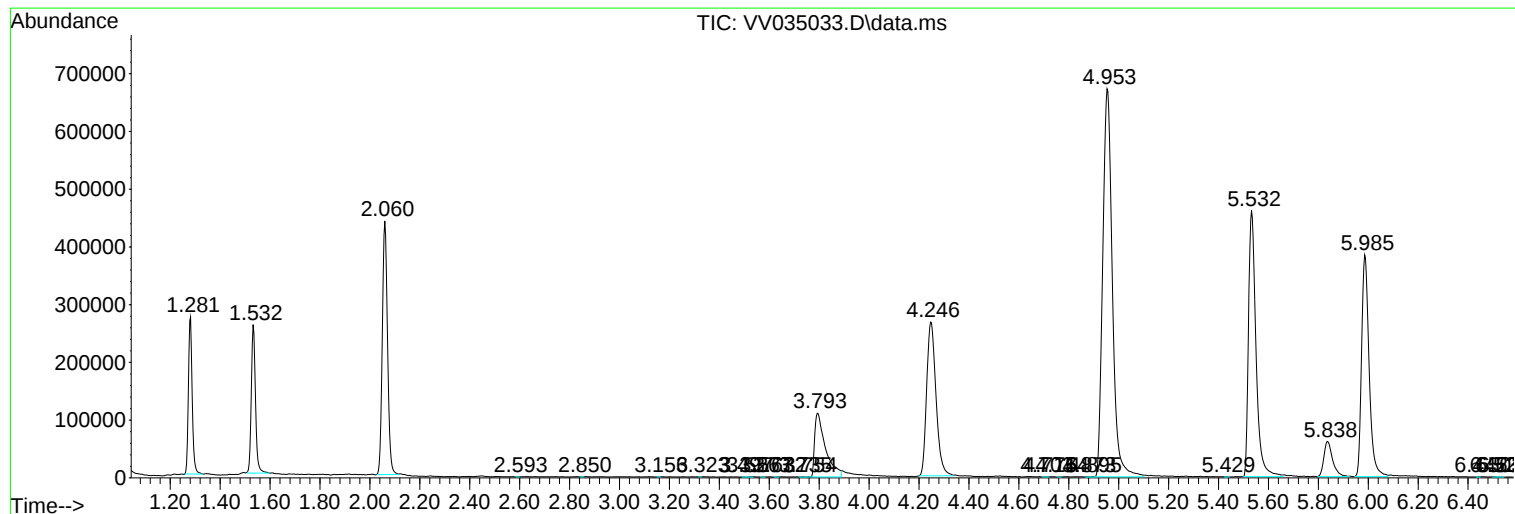

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035033.D
Acq On : 06 Apr 2024 03:02
Operator : SY/MD
Sample : P2009-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035033.D
Acq On : 06 Apr 2024 03:02
Operator : SY/MD
Sample : P2009-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------