

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035034.D
 Acq On : 06 Apr 2024 03:26
 Operator : SY/MD
 Sample : P2009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV	258917	277775	15.69%	2.128%
2	1.532	146	153	180	rVB	253069	299630	16.93%	2.295%
3	2.060	307	317	332	rBV	435675	630922	35.65%	4.833%
4	2.786	541	543	550	rVB2	612	597	0.03%	0.005%
5	2.815	550	552	554	rBV2	390	248	0.01%	0.002%
6	2.908	579	581	585	rVB2	731	289	0.02%	0.002%
7	2.979	600	603	607	rBV2	465	442	0.02%	0.003%
8	2.999	607	609	612	rVV2	525	295	0.02%	0.002%
9	3.015	612	614	617	rVB2	489	306	0.02%	0.002%
10	3.413	735	738	740	rBV2	283	155	0.01%	0.001%
11	3.494	760	763	765	rBV	304	169	0.01%	0.001%
12	3.651	810	812	815	rVB2	492	212	0.01%	0.002%
13	3.709	827	830	833	rVB	542	312	0.02%	0.002%
14	3.732	833	837	839	rBV2	484	296	0.02%	0.002%
15	3.796	848	857	900	rBV	106626	342658	19.36%	2.625%
16	4.246	983	997	1036	rBV	266910	689016	38.93%	5.278%
17	4.667	1125	1128	1130	rBV2	369	253	0.01%	0.002%
18	4.828	1172	1178	1180	rBV2	598	594	0.03%	0.005%
19	4.953	1202	1217	1254	rBV2	663308	1769885	100.00%	13.557%
20	5.452	1370	1372	1376	rBV3	471	348	0.02%	0.003%
21	5.532	1386	1397	1432	rBV	454783	945129	53.40%	7.240%
22	5.838	1480	1492	1518	rBV4	60740	142810	8.07%	1.094%
23	5.986	1526	1538	1567	rBV	382657	798397	45.11%	6.116%
24	6.281	1625	1630	1631	rBV3	623	528	0.03%	0.004%
25	6.404	1665	1668	1670	rBV2	521	348	0.02%	0.003%
26	6.420	1671	1673	1677	rVB3	488	235	0.01%	0.002%
27	6.497	1694	1697	1701	rVB3	572	280	0.02%	0.002%
28	6.526	1703	1706	1708	rBV2	405	307	0.02%	0.002%
29	6.574	1719	1721	1725	rVB2	367	237	0.01%	0.002%
30	6.600	1725	1729	1732	rBV3	663	648	0.04%	0.005%
31	6.625	1732	1737	1738	rBV2	557	434	0.02%	0.003%
32	6.728	1764	1769	1770	rBV3	401	326	0.02%	0.002%
33	6.828	1797	1800	1801	rBV2	323	172	0.01%	0.001%
34	6.912	1816	1826	1854	rBV	186512	363590	20.54%	2.785%
35	7.240	1918	1928	1962	rBV	765350	1361239	76.91%	10.427%
36	7.551	2017	2025	2056	rBV	125366	235157	13.29%	1.801%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035034.D
 Acq On : 06 Apr 2024 03:26
 Operator : SY/MD
 Sample : P2009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	7.767	2090	2092	2095	rBV3	738	360	0.02%	0.003%
38	7.870	2121	2124	2125	rBV	564	333	0.02%	0.003%
39	7.979	2154	2158	2159	rBV2	421	284	0.02%	0.002%
40	8.027	2164	2173	2222	rBV3	305458	765732	43.26%	5.865%
41	8.542	2330	2333	2336	rBV2	671	444	0.03%	0.003%
42	8.674	2370	2374	2376	rBV	448	362	0.02%	0.003%
43	8.735	2391	2393	2396	rVB3	563	265	0.01%	0.002%
44	8.783	2396	2408	2439	rBV	698820	1220739	68.97%	9.351%
45	9.120	2509	2513	2516	rBV3	426	379	0.02%	0.003%
46	9.159	2521	2525	2526	rBV3	479	314	0.02%	0.002%
47	9.188	2532	2534	2535	rBV	524	180	0.01%	0.001%
48	9.239	2548	2550	2552	rVB	440	194	0.01%	0.001%
49	9.268	2553	2559	2561	rBV2	517	411	0.02%	0.003%
50	9.297	2566	2568	2572	rVB2	406	286	0.02%	0.002%
51	9.326	2575	2577	2578	rBV	371	153	0.01%	0.001%
52	9.371	2588	2591	2593	rBV3	285	195	0.01%	0.001%
53	9.426	2606	2608	2611	rBV2	336	190	0.01%	0.001%
54	9.484	2624	2626	2628	rBV	387	235	0.01%	0.002%
55	9.535	2635	2642	2644	rBV2	547	538	0.03%	0.004%
56	9.596	2657	2661	2666	rBV3	389	413	0.02%	0.003%
57	9.654	2676	2679	2684	rVB3	516	485	0.03%	0.004%
58	9.683	2684	2688	2689	rBV	343	268	0.02%	0.002%
59	9.712	2695	2697	2700	rBV2	394	202	0.01%	0.002%
60	9.831	2732	2734	2737	rVB3	392	234	0.01%	0.002%
61	9.860	2740	2743	2744	rBV3	307	157	0.01%	0.001%
62	9.931	2762	2765	2770	rVB3	573	445	0.03%	0.003%
63	9.960	2770	2774	2776	rBV	443	322	0.02%	0.002%
64	9.995	2781	2785	2786	rBV3	389	240	0.01%	0.002%
65	10.021	2789	2793	2795	rBV2	582	379	0.02%	0.003%
66	10.072	2804	2809	2812	rBV3	482	477	0.03%	0.004%
67	10.149	2821	2833	2864	rBV	503986	800645	45.24%	6.133%
68	10.423	2915	2918	2923	rBV3	355	344	0.02%	0.003%
69	10.487	2936	2938	2940	rVB3	389	152	0.01%	0.001%
70	10.529	2948	2951	2953	rBV	301	203	0.01%	0.002%
71	10.561	2959	2961	2965	rVB	487	319	0.02%	0.002%
72	10.583	2965	2968	2970	rBV	522	406	0.02%	0.003%
73	10.706	3003	3006	3007	rBV	307	194	0.01%	0.001%
74	10.725	3007	3012	3016	rVV3	537	582	0.03%	0.004%
75	10.763	3021	3024	3025	rBV	615	349	0.02%	0.003%
76	10.876	3055	3059	3062	rBV2	393	370	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
 Data File : VV035034.D
 Acq On : 06 Apr 2024 03:26
 Operator : SY/MD
 Sample : P2009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.963	3084	3086	3090	rBV2	241	192	0.01%	0.001%
78	11.095	3123	3127	3129	rBV2	482	427	0.02%	0.003%
79	11.127	3129	3137	3144	rVV4	6002	9230	0.52%	0.071%
80	11.185	3144	3155	3182	rVV	634698	1085165	61.31%	8.312%
81	11.464	3239	3242	3244	rBV2	393	223	0.01%	0.002%
82	11.558	3259	3271	3299	rBV	704770	1191408	67.32%	9.126%
83	12.030	3415	3418	3423	rBV4	392	430	0.02%	0.003%
84	12.243	3481	3484	3489	rBV3	615	563	0.03%	0.004%
85	12.265	3489	3491	3494	rVB2	596	270	0.02%	0.002%
86	12.333	3509	3512	3516	rBV3	525	481	0.03%	0.004%
87	12.358	3518	3520	3526	rVV2	490	283	0.02%	0.002%
88	12.410	3532	3536	3541	rBV2	675	542	0.03%	0.004%
89	12.519	3564	3570	3574	rBV4	462	521	0.03%	0.004%
90	12.542	3574	3577	3579	rBV3	384	235	0.01%	0.002%
91	12.587	3588	3591	3592	rBV2	310	192	0.01%	0.001%
92	12.802	3654	3658	3661	rBV2	456	354	0.02%	0.003%
93	12.821	3661	3664	3666	rBV2	486	308	0.02%	0.002%
94	13.082	3742	3745	3748	rBV3	367	302	0.02%	0.002%
95	13.201	3773	3782	3797	rBV2	42216	68847	3.89%	0.527%
96	13.329	3819	3822	3826	rVB3	521	386	0.02%	0.003%
97	13.455	3859	3861	3863	rBV	475	288	0.02%	0.002%
98	13.683	3924	3932	3948	rVB2	12493	20757	1.17%	0.159%
99	14.255	4107	4110	4112	rVB2	729	378	0.02%	0.003%
100	15.339	4440	4447	4458	rBV6	6538	10277	0.58%	0.079%




Sum of corrected areas: 13055078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035034.D
Acq On : 06 Apr 2024 03:26
Operator : SY/MD
Sample : P2009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

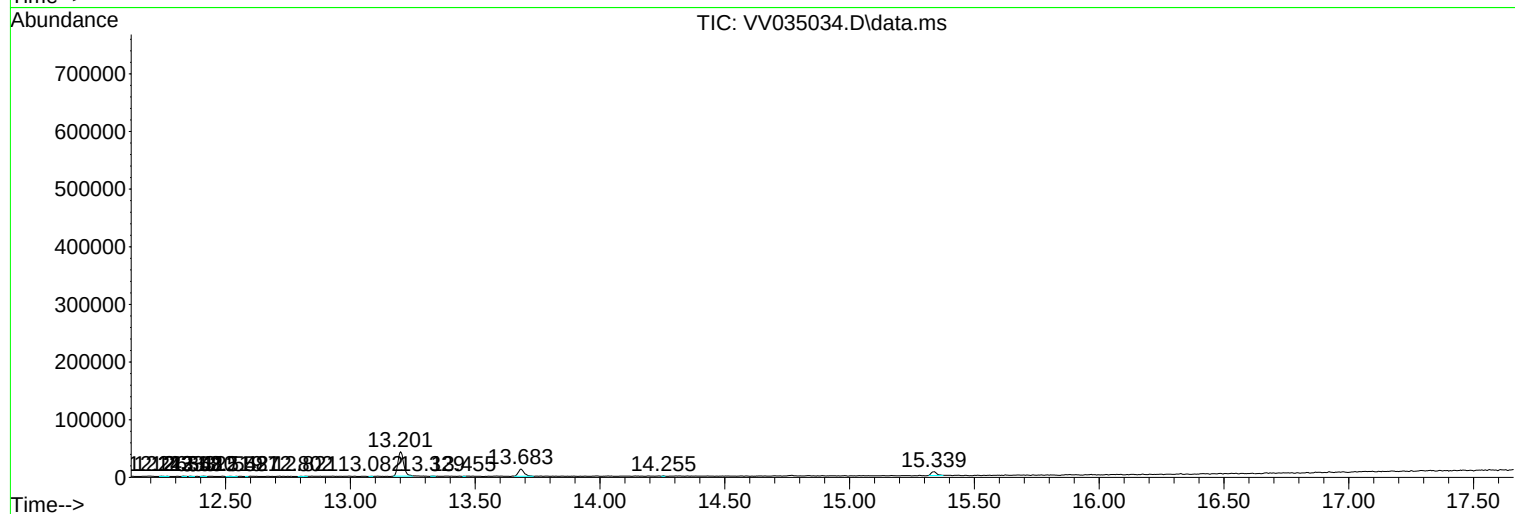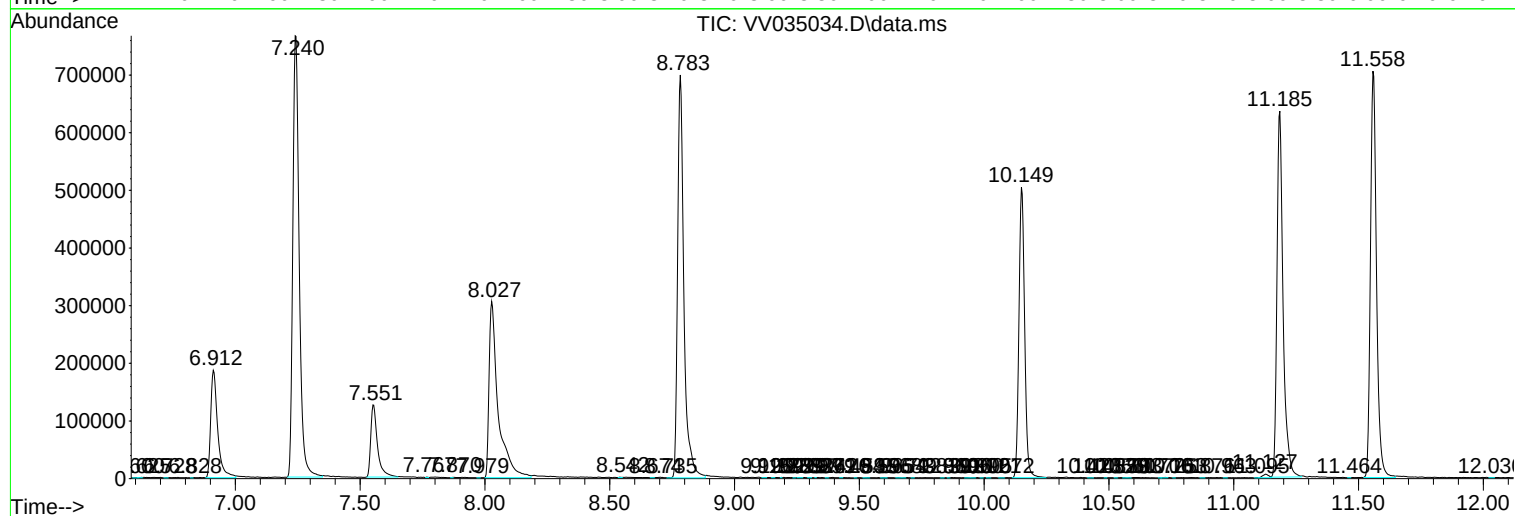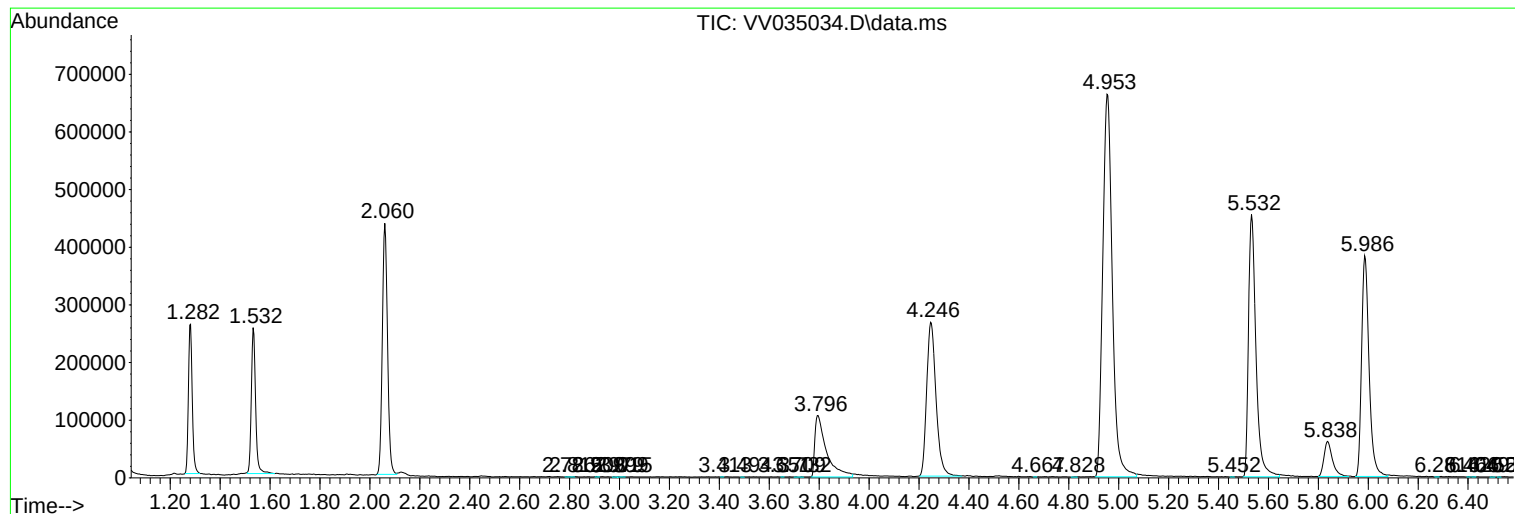

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035034.D
Acq On : 06 Apr 2024 03:26
Operator : SY/MD
Sample : P2009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV035034.D
Acq On : 06 Apr 2024 03:26
Operator : SY/MD
Sample : P2009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------