


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040524\
Data File : VV034990.D
Acq On : 05 Apr 2024 08:21
Operator : SY/MD
Sample : BFB281
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB281

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Sat Apr 06 02:25:24 2024

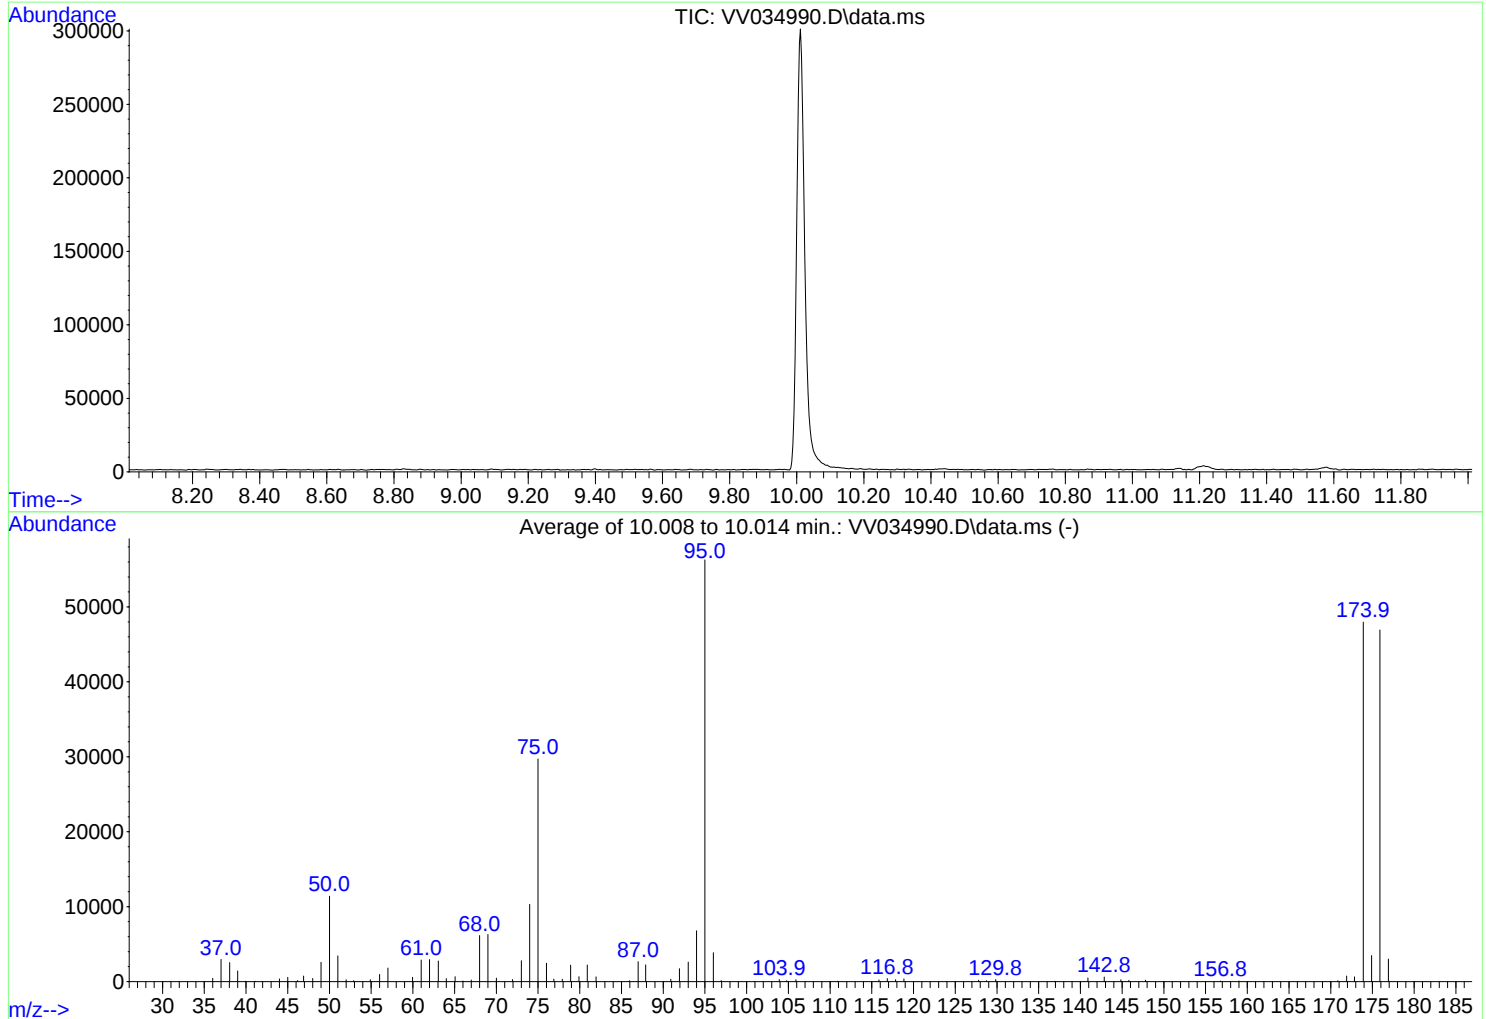

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	11410	PASS
75	95	30	80	52.8	29731	PASS
95	95	100	100	100.0	56283	PASS
96	95	5	9	6.9	3857	PASS
173	174	0.00	2	1.3	647	PASS
174	95	50	120	85.2	47981	PASS
175	174	5	9	7.3	3483	PASS
176	174	95	105	97.8	46925	PASS
177	176	5	10	6.4	3009	PASS

m/z	Abundance
40.00	1029.0
44.00	387.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	472.0
37.00	2912.0
38.00	2610.0
39.00	1391.0
40.00	1097.0
41.10	138.0
44.00	710.0
45.00	608.0
46.20	152.0
46.90	728.0
48.00	426.0
49.00	2532.0
50.00	11723.0
51.00	3483.0
52.00	264.0
52.90	105.0
54.80	245.0
56.00	964.0
57.00	1756.0
60.00	591.0
61.00	2789.0
62.00	2980.0
63.00	2797.0
64.00	434.0
65.00	673.0
67.00	196.0
68.00	6190.0
69.00	6146.0
70.00	430.0
71.90	266.0
73.00	2996.0
74.00	10467.0
75.00	30232.0
76.00	2646.0
76.90	327.0
77.90	331.0
78.90	2241.0
79.90	712.0
80.90	2280.0
82.00	654.0
86.00	138.0
87.00	2591.0
87.90	2376.0
90.90	307.0
92.00	1669.0
93.00	2661.0
94.00	6981.0
95.00	56864.0
96.00	3821.0
97.00	158.0
103.90	265.0
104.80	122.0
105.90	256.0
110.90	106.0
115.80	240.0
116.90	427.0
117.90	283.0
118.90	409.0
127.80	189.0
128.80	112.0
129.90	297.0
136.90	115.0
140.90	536.0
142.80	616.0
144.80	230.0
145.80	195.0
147.80	192.0
170.80	155.0
171.90	696.0
172.80	671.0
173.90	46472.0
174.90	3383.0
175.90	46264.0
176.90	3028.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	441.0
37.00	3091.0
38.10	2624.0
39.00	1511.0
40.00	1110.0
44.00	771.0
45.00	576.0
46.20	162.0
46.90	772.0
48.00	444.0
49.00	2682.0
50.00	11823.0
51.00	3574.0
52.00	268.0
52.90	143.0
54.90	264.0
56.00	1007.0
57.00	1913.0
60.00	599.0
61.00	2991.0
62.00	3043.0
63.10	2893.0
64.00	432.0
65.00	695.0
66.00	114.0
67.00	212.0
68.00	6346.0
69.00	6510.0
70.00	480.0
72.00	283.0
73.00	2852.0
74.00	10640.0
75.00	30696.0
76.00	2513.0
76.90	349.0
77.90	340.0
78.90	2293.0
79.90	683.0
80.90	2293.0
81.90	655.0
85.90	138.0
87.00	2813.0
87.90	2305.0
90.90	353.0
91.90	1786.0
93.00	2670.0
94.00	6980.0
95.00	58016.0
96.00	3999.0
96.90	148.0
103.90	287.0
104.80	135.0
105.90	245.0
110.90	114.0
115.90	256.0
116.80	410.0
117.90	261.0
118.90	387.0
127.80	189.0
128.70	132.0
129.80	303.0
140.90	505.0
142.80	650.0
144.90	244.0
145.80	179.0
147.80	214.0
156.80	122.0
159.00	110.0
170.90	142.0
171.90	778.0
172.90	664.0
173.90	49472.0
174.90	3599.0
175.90	48416.0
176.90	3137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	408.0
37.00	2892.0
38.10	2399.0
39.00	1378.0
39.90	1070.0
44.00	805.0
45.00	533.0
46.20	155.0
46.90	770.0
48.00	412.0
49.00	2546.0
50.00	10684.0
51.00	3275.0
52.00	224.0
52.90	164.0
55.00	256.0
56.00	919.0
57.00	1779.0
59.90	555.0
61.00	2864.0
62.00	2802.0
63.00	2572.0
64.00	365.0
65.10	635.0
66.00	129.0
67.00	227.0
68.00	5899.0
69.00	6228.0
70.00	520.0
72.00	287.0
73.00	2530.0
74.00	9844.0
75.00	28264.0
76.00	2243.0
76.90	355.0
77.90	288.0
78.90	2052.0
79.90	608.0
80.90	2117.0
81.90	607.0
85.90	125.0
87.00	2611.0
87.90	2044.0
90.90	308.0
91.90	1737.0
93.00	2510.0
94.00	6406.0
95.00	53968.0
96.00	3751.0
96.90	135.0
103.90	305.0
104.80	102.0
105.90	242.0
115.90	225.0
116.80	380.0
117.80	203.0
118.80	315.0
127.80	175.0
128.70	120.0
129.80	265.0
140.90	413.0
142.90	618.0
144.90	296.0
145.80	153.0
147.80	182.0
156.80	132.0
159.00	118.0
170.90	103.0
171.90	758.0
172.90	605.0
173.90	48000.0
174.90	3467.0
175.90	46096.0
176.90	2862.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281