


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040619\
 Data File : VV010142.D
 Acq On : 06 Apr 2019 09:36
 Operator : SY/MD
 Sample : BFB86
 Misc : 5.00G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
 Title : VOC Analysis
 Last Update : Tue Apr 09 07:35:38 2019

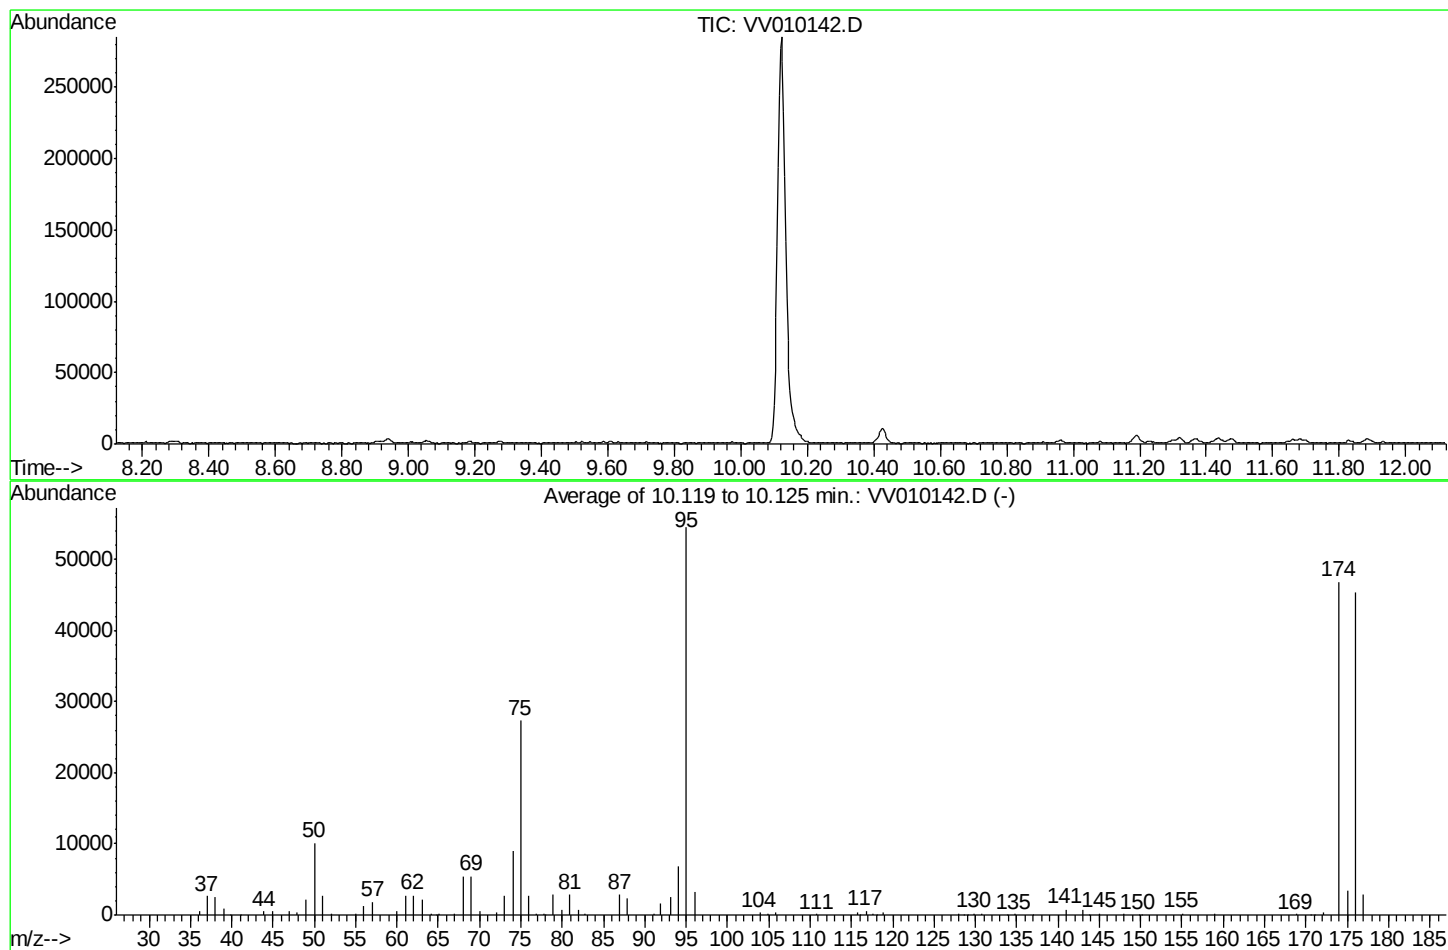

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	10147	PASS
75	95	30	80	50.1	27288	PASS
95	95	100	100	100.0	54506	PASS
96	95	5	9	5.9	3229	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.0	46866	PASS
175	174	5	9	7.5	3505	PASS
176	174	95	101	96.9	45432	PASS
177	176	5	9	6.3	2851	PASS

Scan 2795 (10.077 min): VV010142.D
BFB86

m/z	Abundance
39.10	105.0
40.00	130.0
43.90	282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.10	505.0
37.00	2751.0
38.00	2618.0
39.00	1014.0
39.90	245.0
43.90	849.0
45.00	498.0
46.90	498.0
48.00	215.0
49.00	2143.0
50.00	10010.0
51.00	2637.0
55.00	285.0
55.90	1182.0
57.10	1997.0
59.90	525.0
61.00	2847.0
62.00	2937.0
63.10	2267.0
64.20	255.0
64.80	102.0
65.20	103.0
67.10	170.0
68.00	5490.0
69.00	5485.0
70.10	484.0
72.00	339.0
73.00	2419.0
74.00	9677.0
75.00	27520.0
76.00	2733.0
76.90	256.0
77.80	226.0
78.90	2948.0
79.90	793.0
80.90	2717.0
81.90	644.0
82.90	134.0
87.00	3160.0
87.90	2311.0
91.10	294.0
92.00	1682.0
93.00	2522.0
94.00	6743.0
95.00	54008.0
96.00	3482.0
103.90	348.0
105.00	121.0
105.90	345.0
115.70	401.0
116.80	690.0
117.60	211.0
118.00	199.0
118.90	386.0
127.90	200.0
128.60	115.0
129.80	280.0
130.80	107.0
134.80	126.0
141.00	777.0
143.00	762.0
143.80	104.0
145.10	215.0
148.00	111.0
150.20	114.0
155.10	244.0
168.90	121.0
170.60	105.0
171.10	122.0
172.00	468.0
174.00	46552.0
175.00	3690.0
176.00	44712.0
177.00	2726.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.10	504.0
37.00	2761.0
38.00	2637.0
39.00	948.0
39.80	214.0
41.00	132.0
43.90	817.0
44.90	538.0
47.00	636.0
47.90	308.0
49.00	2219.0
50.00	10488.0
51.00	2765.0
52.10	156.0
55.00	278.0
55.90	1249.0
57.00	1935.0
59.90	482.0
61.00	2816.0
61.90	2879.0
63.00	2202.0
64.20	244.0
65.20	162.0
66.90	217.0
68.00	5692.0
69.00	5659.0
70.10	496.0
72.10	351.0
73.00	2677.0
74.00	9329.0
75.00	28064.0
76.00	2703.0
77.80	178.0
78.90	2989.0
80.00	818.0
80.90	2860.0
81.90	728.0
82.80	157.0
87.00	2952.0
87.90	2423.0
91.10	229.0
92.00	1674.0
93.10	2617.0
94.00	6962.0
95.00	56248.0
96.00	3275.0
104.00	372.0
104.90	145.0
105.90	292.0
110.80	141.0
115.70	333.0
116.10	229.0
116.80	616.0
117.70	259.0
118.80	395.0
127.90	248.0
129.90	256.0
130.80	138.0
133.90	117.0
134.80	156.0
141.00	754.0
143.00	718.0
143.80	108.0
145.10	205.0
147.90	168.0
149.70	116.0
150.10	107.0
155.00	216.0
159.00	145.0
168.90	186.0
170.70	112.0
172.00	447.0
174.00	48488.0
175.00	3589.0
176.00	46736.0
177.00	2922.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	449.0
37.00	2486.0
38.00	2446.0
39.00	982.0
39.80	211.0
41.00	151.0
44.00	795.0
44.90	550.0
47.00	707.0
47.90	365.0
49.00	2047.0
50.00	9945.0
51.00	2732.0
52.10	242.0
55.00	229.0
55.90	1112.0
57.00	1690.0
59.90	418.0
61.00	2590.0
61.90	2474.0
63.00	1981.0
64.20	187.0
65.10	229.0
66.90	211.0
68.00	5124.0
69.00	5290.0
70.00	441.0
72.10	286.0
73.00	2824.0
74.00	8217.0
75.00	26280.0
76.00	2485.0
76.90	199.0
78.00	130.0
78.90	2844.0
80.00	776.0
80.90	2848.0
81.90	807.0
82.70	152.0
87.00	2465.0
87.90	2131.0
91.10	293.0
91.90	1470.0
93.10	2387.0
94.00	6594.0
95.00	53264.0
96.00	2930.0
104.00	341.0
104.90	118.0
105.90	250.0
110.80	168.0
115.70	243.0
116.80	503.0
117.70	265.0
118.80	406.0
127.90	259.0
129.00	102.0
129.80	216.0
130.80	120.0
133.90	132.0
134.70	162.0
136.90	106.0
140.90	722.0
142.80	772.0
144.90	150.0
147.90	214.0
149.80	149.0
155.00	172.0
159.00	146.0
168.80	177.0
172.10	408.0
174.00	45560.0
175.00	3237.0
176.00	44848.0
177.00	2905.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86