

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020941.D
 Acq On : 06 Apr 2021 11:24
 Operator : SY/MD
 Sample : M1845-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	103	rVB2	891464	924557	31.10%	4.786%
2	1.571	157	165	180	rVB	195075	225596	7.59%	1.168%
3	2.108	323	332	359	rVB	468170	688471	23.16%	3.564%
4	2.265	379	381	382	rBV	655	200	0.01%	0.001%
5	2.371	412	414	420	rVB2	618	490	0.02%	0.003%
6	2.439	430	435	439	rBV4	1171	1134	0.04%	0.006%
7	2.516	452	459	467	rVB7	2957	5056	0.17%	0.026%
8	2.600	478	485	488	rBV3	681	818	0.03%	0.004%
9	2.641	496	498	500	rVV	385	171	0.01%	0.001%
10	2.667	504	506	511	rVB2	924	559	0.02%	0.003%
11	2.764	527	536	538	rBV3	4959	5701	0.19%	0.030%
12	2.854	562	564	566	rBV	554	319	0.01%	0.002%
13	2.867	566	568	570	rVV2	340	172	0.01%	0.001%
14	3.011	611	613	616	rVB	650	323	0.01%	0.002%
15	3.031	616	619	622	rVB2	576	323	0.01%	0.002%
16	3.092	636	638	641	rBV2	500	259	0.01%	0.001%
17	3.137	650	652	655	rVB2	370	153	0.01%	0.001%
18	3.169	659	662	664	rBV	307	201	0.01%	0.001%
19	3.182	664	666	667	rBV	491	173	0.01%	0.001%
20	3.330	710	712	714	rBV2	369	153	0.01%	0.001%
21	3.404	733	735	739	rVV2	484	268	0.01%	0.001%
22	3.429	741	743	750	rVB3	538	506	0.02%	0.003%
23	3.474	755	757	758	rBV	398	149	0.01%	0.001%
24	3.494	762	763	767	rVB2	561	252	0.01%	0.001%
25	3.522	770	772	774	rBV	526	345	0.01%	0.002%
26	3.612	798	800	802	rBV	312	180	0.01%	0.001%
27	3.658	812	814	819	rVB2	424	332	0.01%	0.002%
28	3.693	822	825	829	rVB2	415	339	0.01%	0.002%
29	3.715	829	832	838	rBV2	467	474	0.02%	0.002%
30	3.748	838	842	846	rVB2	622	536	0.02%	0.003%
31	3.831	866	868	871	rBV	576	458	0.02%	0.002%
32	3.912	877	893	923	rBV2	1171507	2973080	100.00%	15.389%
33	4.352	1014	1030	1061	rBV	360555	883170	29.71%	4.571%
34	4.821	1173	1176	1178	rBV2	513	343	0.01%	0.002%
35	4.850	1183	1185	1188	rBV2	602	442	0.01%	0.002%
36	4.866	1188	1190	1194	rBV	328	236	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040621\
 Data File : VW020941.D
 Acq On : 06 Apr 2021 11:24
 Operator : SY/MD
 Sample : M1845-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.886	1194	1196	1199	rBV2	296	180	0.01%	0.001%
38	4.902	1199	1201	1206	rVB3	527	361	0.01%	0.002%
39	4.931	1208	1210	1211	rBV	656	219	0.01%	0.001%
40	4.963	1217	1220	1221	rBV	308	173	0.01%	0.001%
41	5.050	1230	1247	1272	rBV2	791875	2024192	68.08%	10.478%
42	5.333	1333	1335	1338	rVV	634	315	0.01%	0.002%
43	5.352	1338	1341	1343	rVB3	884	467	0.02%	0.002%
44	5.442	1366	1369	1372	rBV2	609	349	0.01%	0.002%
45	5.619	1412	1424	1452	rBV	692512	1381235	46.46%	7.150%
46	5.911	1505	1515	1533	rBV2	22258	47016	1.58%	0.243%
47	6.024	1547	1550	1551	rBV2	602	366	0.01%	0.002%
48	6.072	1552	1565	1586	rVV	436398	880611	29.62%	4.558%
49	6.358	1652	1654	1656	rBV2	657	399	0.01%	0.002%
50	6.381	1660	1661	1663	rVB	611	154	0.01%	0.001%
51	6.452	1681	1683	1684	rBV	441	206	0.01%	0.001%
52	6.526	1704	1706	1707	rBV	350	170	0.01%	0.001%
53	6.583	1721	1724	1727	rBV3	1063	745	0.03%	0.004%
54	6.699	1757	1760	1761	rBV	542	213	0.01%	0.001%
55	6.741	1772	1773	1775	rBV	480	208	0.01%	0.001%
56	6.773	1778	1783	1784	rVV	385	310	0.01%	0.002%
57	6.873	1812	1814	1818	rVB2	771	438	0.01%	0.002%
58	6.902	1818	1823	1825	rBV2	802	760	0.03%	0.004%
59	6.934	1830	1833	1838	rBV3	655	458	0.02%	0.002%
60	6.989	1838	1850	1874	rBV	257783	470452	15.82%	2.435%
61	7.320	1941	1953	1971	rBV	978030	1673874	56.30%	8.664%
62	7.625	2037	2048	2067	rBV	181224	314928	10.59%	1.630%
63	7.879	2124	2127	2130	rVB3	578	312	0.01%	0.002%
64	7.937	2143	2145	2149	rVB2	611	265	0.01%	0.001%
65	8.046	2172	2179	2181	rBV4	756	789	0.03%	0.004%
66	8.095	2184	2194	2227	rBV	407659	806708	27.13%	4.176%
67	8.464	2305	2309	2312	rBV3	923	758	0.03%	0.004%
68	8.509	2321	2323	2327	rVB2	688	402	0.01%	0.002%
69	8.532	2328	2330	2333	rBV2	667	348	0.01%	0.002%
70	8.603	2349	2352	2355	rBV2	653	490	0.02%	0.003%
71	8.651	2366	2367	2369	rBV2	481	189	0.01%	0.001%
72	8.857	2418	2431	2467	rVV	1041164	1684063	56.64%	8.717%
73	9.246	2547	2552	2555	rVB3	551	518	0.02%	0.003%
74	9.451	2614	2616	2619	rBV2	578	310	0.01%	0.002%
75	9.844	2736	2738	2739	rBV	640	279	0.01%	0.001%
76	9.924	2761	2763	2765	rBV	363	176	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020941.D
 Acq On : 06 Apr 2021 11:24
 Operator : SY/MD
 Sample : M1845-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.024	2786	2794	2806	rBV7	6159	10439	0.35%	0.054%
78	10.069	2806	2808	2812	rBV2	511	347	0.01%	0.002%
79	10.088	2812	2814	2818	rVB2	435	231	0.01%	0.001%
80	10.133	2819	2828	2836	rBV5	4574	7148	0.24%	0.037%
81	10.220	2843	2855	2878	rBV	639389	1004480	33.79%	5.199%
82	10.480	2933	2936	2943	rBV3	568	575	0.02%	0.003%
83	10.538	2951	2954	2957	rBV3	774	568	0.02%	0.003%
84	10.567	2961	2963	2965	rBV2	910	449	0.02%	0.002%
85	10.625	2978	2981	2982	rBV2	471	235	0.01%	0.001%
86	10.963	3084	3086	3090	rVB3	866	505	0.02%	0.003%
87	10.988	3090	3094	3095	rBV2	659	386	0.01%	0.002%
88	11.107	3124	3131	3135	rBV4	984	1092	0.04%	0.006%
89	11.152	3138	3145	3155	rVB5	2244	3558	0.12%	0.018%
90	11.255	3165	3177	3196	rBV	1060873	1645301	55.34%	8.516%
91	11.631	3282	3294	3316	rBV	1026454	1628534	54.78%	8.430%
92	12.477	3554	3557	3558	rBV2	695	372	0.01%	0.002%
93	12.516	3566	3569	3571	rVB	826	418	0.01%	0.002%
94	12.641	3605	3608	3612	rBV3	526	366	0.01%	0.002%
95	12.898	3685	3688	3689	rBV2	549	291	0.01%	0.002%
96	13.336	3821	3824	3827	rBV2	857	703	0.02%	0.004%
97	13.593	3903	3904	3910	rBV3	570	482	0.02%	0.002%
98	13.628	3913	3915	3920	rBV2	821	787	0.03%	0.004%
99	13.670	3925	3928	3934	rBV3	656	721	0.02%	0.004%
100	13.786	3960	3964	3966	rBV	889	735	0.02%	0.004%




Sum of corrected areas: 19319068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020941.D
Acq On : 06 Apr 2021 11:24
Operator : SY/MD
Sample : M1845-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

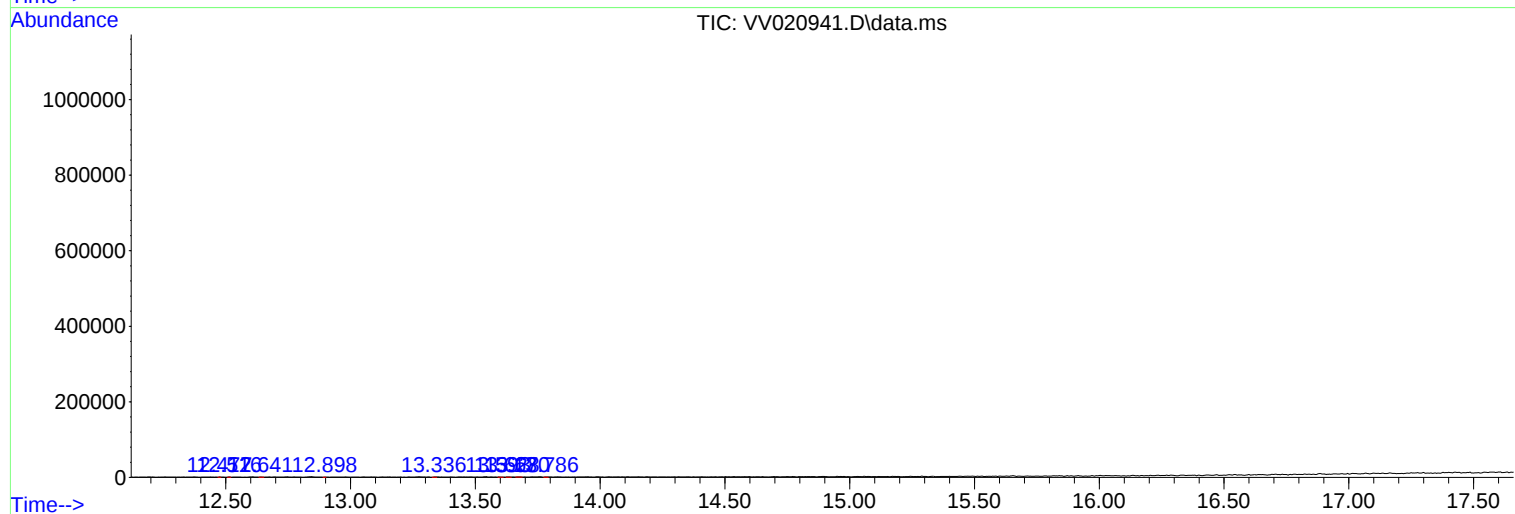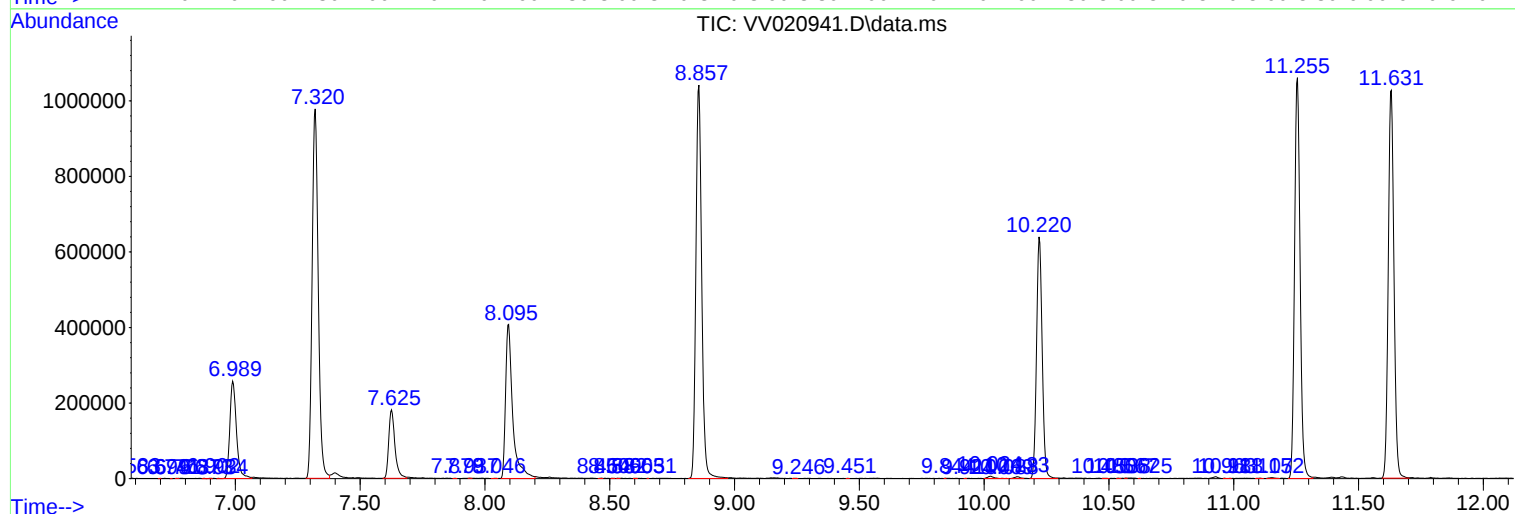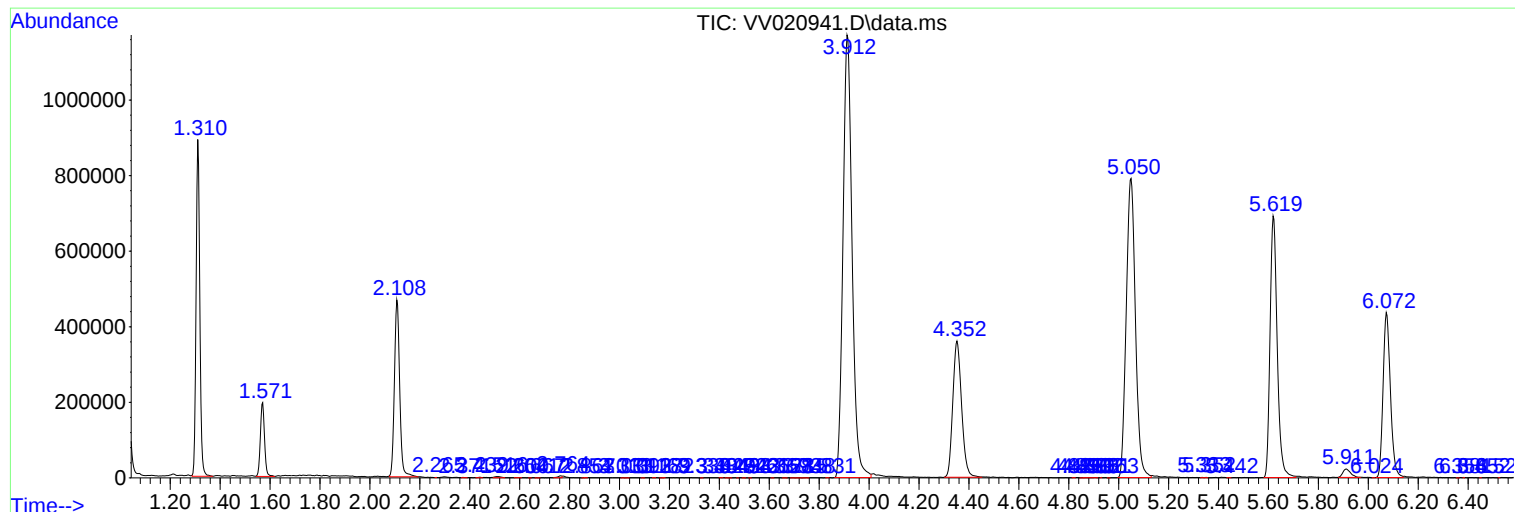

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020941.D
Acq On : 06 Apr 2021 11:24
Operator : SY/MD
Sample : M1845-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020941.D
Acq On : 06 Apr 2021 11:24
Operator : SY/MD
Sample : M1845-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
